



**HAL**  
open science

## Long-term stabilization of the length of an optical reference cavity

Gaëtan Hagel, Marie Houssin, Martina Knoop, Caroline Champenois, Michel Vedel, Fernande Vedel

► **To cite this version:**

Gaëtan Hagel, Marie Houssin, Martina Knoop, Caroline Champenois, Michel Vedel, et al.. Long-term stabilization of the length of an optical reference cavity. 2005. hal-00007728v2

**HAL Id: hal-00007728**

**<https://hal.science/hal-00007728v2>**

Preprint submitted on 29 Jul 2005 (v2), last revised 16 Sep 2005 (v3)

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

# Long-term stabilization of the length of an optical reference cavity

Gaëtan Hagel, Marie Houssin, Martina Knoop,\* Caroline Champenois, Michel Vedel, and Fernande Vedel  
*Physique des Interactions Ioniques et Moléculaires (CNRS UMR 6633), Université de Provence,  
Centre de Saint Jérôme, Case C21, 13397 Marseille Cedex 20, France*<sup>†</sup>

(Dated: July 29, 2005)

To obtain a high degree of length stabilisation of an optical reference cavity, its free-spectral range is locked by means of an accurate and stable frequency synthesizer. The locking scheme is twofold: a laser is locked on the  $N^{\text{th}}$  mode of a reference Fabry-Perot cavity and part of the laser light is shifted in frequency by an acousto-optical modulator (AOM) mounted in double-pass, matching half of the free spectral range of the reference cavity to be in resonance with the  $(N+1)^{\text{th}}$  mode of the cavity. The resulting absolute stabilization of the length of the cavity reaches the  $10^{-11}$  level per second limited by the lock transfer properties and the frequency stability of the AOM control synthesizer.

PACS numbers: 42.60.Lh Efficiency, stability, gain, and other operational parameters , 07.05.Dz Control systems

## I. INTRODUCTION

Today, the precision and stability of laser frequencies reaches beyond the  $10^{-14}$ -level, removing the last obstacles for an ultimate investigation of possible new frequency standards outpassing the performances of the actual cesium atomic clock by orders of magnitude [1]. Nevertheless, many experimental applications require lasers with less stringent performances, like a sub-MHz linewidth and an absolute frequency stability better than this spectral width for time scales up to a minute. In our experiment [2], probing of an atomic transition requires a narrow interrogation laser linewidth, which can be obtained in a straightforward way by stabilizing a laser on a Fabry-Perot cavity of high finesse. The use of the Pound-Drever-Hall (PDH) locking technique [3] permits to counteract rapid frequency fluctuations and allows to obtain laser linewidths largely inferior to 100 kHz.

To suppress frequency drifts, stabilisation of the length of the reference cavity of the interrogation laser is required. This can be realized by a maximum isolation from mechanical, acoustic and thermal perturbations, or by an absolute stabilisation on an atomic transition, generally by making use of an additional (diode) laser set-up. Stabilisation on an atomic transition is often made by the saturated absorption technique to avoid Doppler broadening effects in a gas at room temperature. The employed crossover transitions have spectral widths of about 10 MHz (for example Rb: 5.9 MHz, Cs: 14 MHz), limiting the attainable frequency stabilities to almost three orders of magnitude below these values.

Very few different techniques have been used to assure an absolute-length stabilisation of a reference cavity. They all compare the frequency difference between two eigenmodes of a reference cavity with an external rf frequency applied to a phase or frequency modulation de-

vice. The Dual-Frequency Modulation (DFM) technique with two phase modulators (EOM) in a row has been used in [4]. It has been applied in a slightly modified set-up to measure the frequency of molecular transitions with a uncertainty of  $2 \times 10^{-8}$  [5], where the change in free-spectral range (FSR) of an optical cavity is tracked by a servo on an EOM. Another implementation is reduced to the use of a single EOM [6]. Long-baseline interferometry uses double modulation techniques to assure length determination of the interferometer arms which can reach a relative uncertainty of  $10^{-11}$  [7].

In this manuscript we describe a new scheme for the use of a DFM method for the absolute-length stabilisation of an optical cavity. In order to avoid a mean-term drift of the laser we have chosen to stabilize the length of the cavity by locking the frequency difference between its  $N^{\text{th}}$  and its  $(N+1)^{\text{th}}$  longitudinal mode. The frequency difference is generated by an acousto-optical modulator at a fixed value matching half of the FSR of the reference cavity. The high accuracy and stability of a frequency synthesizer are thus transferred to the FSR. The use of acousto-optic modulators at frequencies largely beyond 100 MHz allows to stabilize short optical cavities. Furthermore, the described method is independent from the existence of nearby atomic transitions. We have demonstrated excellent frequency stability for periods up to a couple of hours.

## II. EXPERIMENTAL REALIZATION

The complete experimental set-up is pictured in figure 1. The 729-nm-laser is a broad-area diode laser mounted in an external cavity to assure single-mode lasing and to reduce its linewidth [8]. The diode is then stabilized onto a reference cavity by using the Pound-Drever-Hall lock [3]. Our present goal is to enhance the stability of this optical reference cavity. The cavity has a finesse of about 1000 and the spacer between the two mirrors is made out of Invar. This home-made cavity spacer has an outer diameter of 50 mm, an inner diameter of 10 mm,

\*Electronic address: Martina.Knoop@up.univ-mrs.fr

<sup>†</sup>URL: <http://www.up.univ-mrs.fr/ciml/>

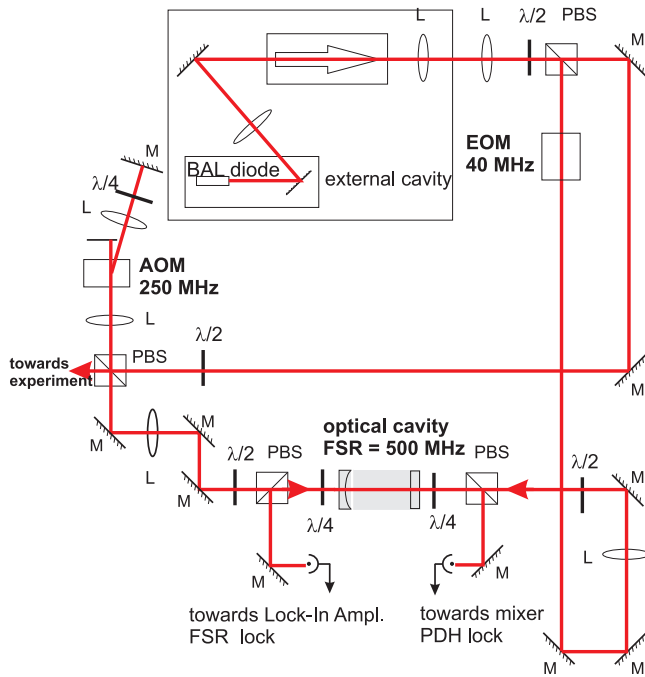


FIG. 1: Experimental setup of the described locking scheme. The lock signal for the PDH signal of the diode laser enters the cavity from the right, while the length stabilisation of the cavity is injected into the reference cavity from the left side, after a double-pass through the 250-MHz AOM. L designs the lenses used for efficient mode-matching, while mirrors are noted M, and polarization beam-splitters PBS. See text for detailed description.

and a length of about 300 mm. The cavity is formed by commercial broad-band mirrors (700-900 nm), a plane and a curved one (radius of curvature 2m). The plane mirror is mounted on a piezo-electric transducer (PZT) allowing to adjust the length of the cavity by application of a DC-voltage up to 150 V corresponding to a length variation of about 2  $\mu\text{m}$ . In the course of a day, the reference cavity undergoes a slow frequency drift mainly due to temperature variations, in a lab where the ambient temperature is stabilized to approximately one degree.

The instantaneous linewidth of the diode laser locked onto the reference cavity has been measured by an auto-correlation technique [9]. The beat signal of a part of the laser beam with a second part of the same beam which has passed through 10 km of optical fiber is shown in figure 2. This beat signal has been acquired with a HP ESA 1500A spectrum analyzer at a 3 kHz bandwidth. While the free-running laser (lower curve, open circles) has a linewidth of the order of several hundred kHz, which is a typical result for a broad-area diode laser in an external cavity, the linewidth of the locked laser is inferior to 25 kHz. This is achieved by feeding the frequency corrections of the PDH-signal to different elements in the diode laser cavity setup. While slow fluctuations (up to 200 Hz) are corrected by the piezo-electric element supporting the cavity grating, intermediate corrections (up

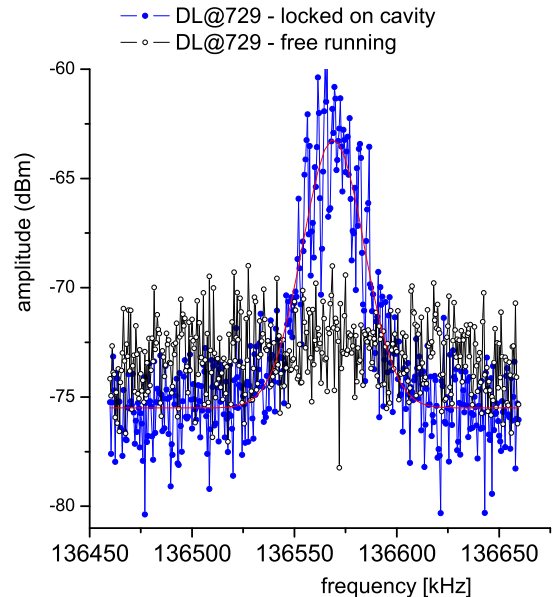


FIG. 2: Beat signal of one part of the 729 nm diode laser with another part of the same laser having passed through a 10 km optical fiber. The upper curve has been recorded for the diode laser being locked to the reference cavity, and results in a spectral linewidth lower than 25 kHz, while the lower curve has been measured with no lock at all resulting in a linewidth of several hundred kHz.

to 10 kHz) are applied via the diode laser current source, and rapid frequency corrections are made directly on the anode of the diode laser making use of an FET mounted as a passive voltage-current transductor [10].

To increase the stability of the reference cavity in order to avoid a mean-term drift of the laser we have chosen to stabilize the length of the cavity by locking the frequency difference between its  $N^{\text{th}}$  and its  $(N+1)^{\text{th}}$  longitudinal mode. The frequency difference is fixed by a highly stable frequency synthesizer driving the acousto-optical modulator at a frequency corresponding to the half of the FSR of the cavity.

In the described locking scheme, the frequency of the diode laser corresponds to the  $N^{\text{th}}$  multiple of the cavity's free spectral range

$$\nu_{DL} = (N + \varphi + \Phi) \cdot \nu_{FSR} \quad (1)$$

where  $N$  is the mode number,  $\varphi$  the Fresnel phase shift due to the curvature of the cavity mirrors, and  $\Phi$  the phase shift which occurs upon reflection due to the finite conductivity of the mirrors. In the following, we are only interested in the frequency difference of two neighboring modes, we may thus assume that these phase shifts are almost identical and can therefore be neglected.

In addition to the PDH lock of the diode onto the reference cavity, one part of the laser output which has double-passed an acousto-optical modulator is injected into

the cavity. Note that in our set-up this second beam enters the cavity from the opposite side of the PDH lock.

This beam has been offset in frequency by two times  $\nu_{AOM} = 249.82$  MHz fixing the FSR of the reference cavity.

$$\nu_{DL} + 2 \times \nu_{AOM} = (N + 1) \cdot \nu_{FSR} \quad (2)$$

The PDH lock relies on circular polarization of the laser light entering the cavity and prevents us from using separate polarizations for the two beams incident on the cavity. Therefore the two photodiodes generating the error signals are sensitive to both parts of the beam. It is thus imperative to separate the reactions of the two lock loops. In practice, this has been realized with a pure integrator in the length-stabilisation of the reference cavity and a resistor bias stabilization integrator [11] in the PDH lock (with a limited gain at zero frequency). As a consequence, at frequencies below the hertz, the corrections applied to the diode laser are negligible compared to those sent to the FSR lock.

One of the major points for a stable configuration of the locking scheme is to choose a frequency modulation  $f_m$  of the FSR lock larger than the second cut-off of the diode-lock ( $\approx 10$  kHz). At small frequency modulation values (e.g. 1 kHz) the gain of the PDH servo is too high (55dB) producing a strong reaction. As a consequence the lock of the laser on the reference cavity becomes unstable. For best results, we have chosen to modulate the driving frequency of the AOM at 22 kHz with an amplitude of 100 kHz. At this frequency the PDH gain is about 35 dB, which is at least an order of magnitude below the gain of the FSR stabilization.

To produce the counter-reaction, a photodiode detects the signal reflected by the cavity, which is then demodulated by a lock-in amplifier. The output of this lock-in is integrated (time constant of 1 s) before being sent to the PZT transducer controlling the length of the reference cavity.

The overall response of the lock is given by the resolution of the employed frequency synthesizer. In fact,

$$\frac{\Delta\nu_{DL}}{\nu_{DL}} = \frac{\Delta\nu_{FSR}}{\nu_{FSR}} = \frac{\Delta\nu_{synth}}{\nu_{synth}} \quad (3)$$

and the ratio of the FSR to diode frequency is, in our case,

$$\nu_{DL} \approx 0.8 \times 10^6 \nu_{FSR} = 1.6 \times 10^6 \nu_{synth} \quad (4)$$

We use an Aeroflex 2030-series frequency synthesizer with an internal frequency standard at 10 MHz (OCXO) having a 0.1 Hz accuracy and a fractional frequency stability at 1 minute of about  $5 \times 10^{-10}$  [12] to control the AOM output.

To test the stability of the cavity, the evolution of the diode laser frequency has been measured by a wavemeter, where the employed reference wavelength is a temperature stabilized HeNe transition at 632.8 nm. The

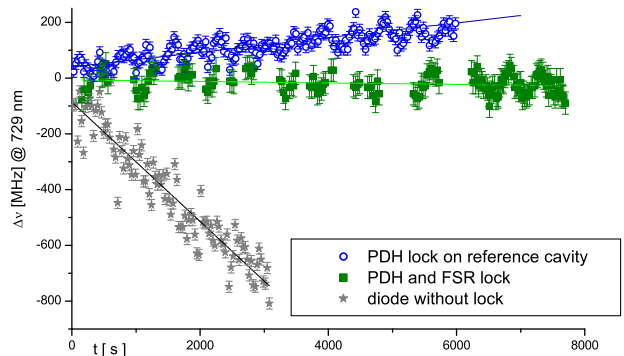


FIG. 3: Temporal evolution of the laser frequency for a free-running laser ( $\star$ ), the laser locked by PDH on the optical cavity ( $\circ$ ), and with the FSR of the cavity locked on the frequency synthesizer ( $\bullet$ ).

precision of the wavemeter is better than 40 MHz, which has been verified by the frequency resolution obtained on the atomic transition of a single calcium ion during periods of a couple of hours [13]. The temporal evolution of the diode laser frequency is reported in figure 3, the straight lines in this graph are linear fits to the acquired data, reflecting the long-term frequency drifts. On the considered time scales (10 minutes to three hours) the observed frequency variations have all presented a linear evolution.

The lower curve in figure 3 reflects the frequency of the diode laser in external cavity without any additional stabilisation. The frequency drift is almost 800 MHz per hour, mainly due to thermal drifts of the high-power diode-laser component and a very typical value for a non-stabilized laser. The upper curve shows the fluctuations of the diode frequency as it is stabilized onto the described Invar cavity. A reduction of the frequency drift to values below 100 MHz per hour can be observed. The center graph monitors the frequency of the diode locked to the reference cavity with the cavity's FSR stabilized by the synthesizer frequency. The apparent drift of the frequency has been reduced to less than 3 kHz per second, corresponding to a frequency variation per hour of less than 9 MHz limited by the frequency stability of the employed frequency synthesizer.

### III. CONCLUSION

We have presented a method to stabilize the length of an optical reference cavity implementing the lock of its FSR by an AOM. The corner stone of this method is a thorough frequency separation of the interaction of the two lock loops, the result is dependant of the quality of the locking schemes adopted. The stability reached by this method is only limited by the technical performance of the employed frequency synthesizer. The implemented

technique is a pure frequency lock, no phase condition has to be fulfilled. Compared to existing DFM methods which have been designed using phase modulators, the use of an acousto-optical modulator in our scheme allows application of the technique to cavities which are shorter than some tens of centimeters. Furthermore, the

presented method can be used in a wavelength regime where no atomic transitions are accessible. The stability performances described could be easily improved by using an external frequency standard with higher precision and stability for the frequency synthesizer fixing the length of the optical cavity.

- 
- [1] S. Diddams, T. Udem, J. Bergquist, E. Curtis, R. Drullinger, L. Hollberg, W. Itano, W. Lee, C. Oates, K. Vogel, and D. J. Wineland, *Science* **293**, 825 (2001).
- [2] C. Lisowski, M. Knoop, C. Champenois, G. Hagel, M. Vedel, and F. Vedel, *Appl. Phys. B* **81**, 5 (2005).
- [3] R. Drever, J. Hall, F. Kowalski, J. Hough, G. Ford, A. Munley, and H. Ward, *Appl. Phys. B* **31**, 97 (1983).
- [4] R. G. DeVoe and R. G. Brewer, *Phys. Rev. A* **30**, 2827 (1984).
- [5] L.-S. Ma, J. Ye, P. Dubé, and J. L. Hall, *J. Opt. Soc. Am. B* **16**, 2255 (1999).
- [6] P. Courteille, L. Ma, W. Neuhauser, and R. Blatt, *Appl. Phys. B* **59**, 187 (1994).
- [7] A. Araya, S. Telada, K. Tochikubo, S. Taniguchi, R. Takahashi, K. Kawabe, D. Tatsumi, T. Yamazaki, S. Kawamura, S. Miyoki, et al., *Applied Optics* **38**, 2848 (1999).
- [8] M. Houssin, P. Courteille, C. Champenois, M. Herbane, M. Knoop, M. Vedel, and F. Vedel, *Appl. Optics* **42**, 4871 (2003).
- [9] T. Okoschi, K. Kikuchi, and A. Nakayama, *Electron. Lett.* **16**, 630 (1980).
- [10] F. Schmidt-Kaler, private communication, 2003.
- [11] P. Horowitz and W. Hill, *The art of electronics* (Cambridge University Press, Cambridge, 1989).
- [12] Aeroflex Test Solutions, private communication, 2005.
- [13] M. Knoop, C. Champenois, G. Hagel, M. Houssin, C. Lisowski, M. Vedel, and F. Vedel, *Eur. Phys. J. D* **29**, 163 (2004).