



HAL
open science

Measurements of HNO₃ and N₂O₅ using Ion drift ? Chemical Ionization Mass Spectrometry during the MCMA ? 2006 Campaign

J. Zheng, R. Zhang, E. C. Fortner, L. Molina, A. C. Aiken, J. L. Jimenez, K.
Gäggeler, J. Dommen, S. Dusanter, P. S . Stevens, et al.

► To cite this version:

J. Zheng, R. Zhang, E. C. Fortner, L. Molina, A. C. Aiken, et al.. Measurements of HNO₃ and N₂O₅ using Ion drift ? Chemical Ionization Mass Spectrometry during the MCMA ? 2006 Campaign. Atmospheric Chemistry and Physics Discussions, 2008, 8 (2), pp.4877-4909. hal-00304024

HAL Id: hal-00304024

<https://hal.science/hal-00304024v1>

Submitted on 18 Jun 2008

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Measurements of HNO₃ and N₂O₅ using Ion drift – Chemical Ionization Mass Spectrometry during the MCMA – 2006 Campaign

J. Zheng¹, R. Zhang¹, E. C. Fortner^{1,*}, L. Molina², A. C. Aiken³, J. L. Jimenez³,
K. Gäggeler⁴, J. Dommen⁴, S. Dusanter⁵, P. S. Stevens⁵, and X. Tie⁶

¹Dept. Atmospheric Sciences, Texas A & M University, College Station, Texas 77843, TX, USA

²Molina Center for Energy and the Environment, La Jolla, CA, USA

³Dept. Chemistry and Biochemistry, University of Colorado, Boulder, CO, USA

⁴Laboratory of Atmospheric Chemistry, Paul Scherrer Institute, 5232 Villigen, Switzerland

⁵Dept. Chemistry, Indiana University, Bloomington, IN, USA

⁶Atmospheric Chemistry Division, National Center for Atmospheric Research, Boulder, CO, USA

*now at: Dept. Chemistry and Biochemistry, Montana State University, Bozeman, MT, USA

Received: 18 January 2008 – Accepted: 22 January 2008 – Published: 6 March 2008

Correspondence to: R. Zhang (zhang@ariel.met.tamu.edu)

Published by Copernicus Publications on behalf of the European Geosciences Union.

Nitric acid during
MCMA 2006

R. Zhang et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Abstract

An ion drift – chemical ionization mass spectrometry (ID-CIMS) was deployed in Mexico City between 5 and 31 March to measure HNO_3 and N_2O_5 during the 2006 Mexico City Metropolitan Area (MCMA) field campaign. The observation site, T0, was located at the Instituto Mexicano del Petróleo at the center of the Mexico City Basin with major emissions of pollutants from both domestic and industrial sources. Diurnally, HNO_3 was less than 200 parts per trillion (ppt) during the night and in the early morning, increased steadily from around 09:00 a.m. central standard time (CST), reached a peak value of 0.5 to 3 parts per billion (ppb) in the early afternoon, and declined sharply to less than half of the peak value near 05:00 p.m. CST. An inter-comparison between the ID-CIMS and an ion chromatograph/mass spectrometer (ICMS) showed a good correlation in the HNO_3 measurements ($R^2=0.75$). The HNO_3 mixing ratio was found to anti-correlate with aerosol nitrate, suggesting that the gaseous HNO_3 concentration was controlled by the gas-particle partitioning process. During most times of the MCMA 2006 field campaign, N_2O_5 was found to be under the detection limit (about 20 ppt for a 10 s integration time) of the ID-CIMS, because of high NO mixing ratio (>100 ppb) during the night. With one exception on 26 March 2006, about 40 ppt N_2O_5 was observed during the late afternoon and early evening hours under a cloudy condition, before NO built up at the surface site. The results revealed that during the 2006 MCMA field campaign HNO_3 was primarily produced by the reaction of OH with NO_2 and regulated by gas/particle partitioning, and HNO_3 production from N_2O_5 hydrolysis during the nighttime was small because of high NO and low O_3 concentrations near the surface.

1 Introduction

For decades, the Mexico City Metropolitan Area (MCMA), the biggest megacity in the world, has suffered from severe air pollution, especially in ozone (O_3) and particu-

Nitric acid during MCMA 2006

R. Zhang et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



**Nitric acid during
MCMA 2006**

R. Zhang et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

late matter (Molina and Molina, 2002; Molina et al., 2007). As the home of 20 million residents, 3.5 million vehicles, and 35 000 industries, the MCMA emits annually near 206 kilotons of nitrogen oxides ($\text{NO}_x = \text{NO} + \text{NO}_2$), 22.5 kilotons of sulfur dioxide (SO_2), and 1769 kilotons of volatile organic compounds (VOCs) (Molina and Molina, 2002) into the atmosphere, due to both domestic and industrial fossil fuel consump-
5 tions. Furthermore, the unique combination of geographical conditions, i.e. the basin topography, tropical solar radiation ($19^\circ 25' \text{N}$ and $99^\circ 10' \text{W}$), and high elevation (2240 m a.m.s.l.), makes air pollutants easier to accumulate in the MCMA and is favorable for photochemical production of O_3 and aerosols (Molina and Molina, 2002; Zhang et al., 2004a). Since 1988, this region annually experiences an hourly average O_3 concentra-
10 tion higher than 110 ppb for over 80% days and a peak O_3 concentration of frequently more than 300 ppb (Molina and Molina, 2002). Both VOCs and NO_x play critical roles during O_3 formation in the troposphere (Finlayson-Pitts and Pitts, 1999) and the variations in their concentrations and the ensuing effects on O_3 production rate can be
15 characterized as either NO_x -sensitive or VOC-sensitive (Sillman, 1999; Lei et al., 2004; Zhang et al., 2004b). Recently, based on a model study, Tie et al. (2007) suggested that the O_3 formation in the MCMA was VOC-limited. The lifecycle of NO_x and its budget in the MCMA is one of the critical pre-required information to develop effective O_3 control strategies (Lei et al., 2007). The dominant daytime sink of NO_x is through the
20 oxidation of NO_2 by the hydroxyl radical (OH) to form nitric acid (HNO_3),



which is removed from the atmosphere by dry and wet depositions (Finlayson-Pitts and Pitts, 1999). Generally, HNO_3 deposition is considered as an irreversible sink for NO_x , but recent studies have suggested that HNO_3 deposited on the surface can be recycled
25 back into the atmosphere as NO_x by heterogeneous reactions with NO (Saliba et al., 2001) and photolysis in the presence of water (Ramazan et al., 2006). Under certain meteorological conditions, HNO_3 can be transported over 1000 km downwind from the plume origin, and a HNO_3 enriched plume can potentially contribute to O_3 production far away from its origin.

During the nighttime, NO_x will titrate O_3 to form the nitrate radical (NO_3),



which can further react reversibly with NO_2 to form dinitrogen pentoxide (N_2O_5) (for Reaction 4, $K_{eq} = 4.5 \times 10^{-14} \exp[-1260/T] \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$, JPL, 2006). At night, NO_3 can exist in significant concentrations and undergo H-atom abstraction or addition reactions with hydrocarbons in a similar way as OH radicals during daytime (Suh et al., 2001). Comparing with NO_3 , N_2O_5 is relatively unreactive, but it can act as a reservoir of NO_3 and undergo heterogeneous hydrolysis to form HNO_3 (Zhang et al., 1995; Brown et al., 2006). Therefore, in-situ observations of HNO_3 and N_2O_5 are indispensable to fully characterize the NO_x chemistry and budget in the troposphere and to develop effective control strategies.

Several measurement techniques have been developed to measure gaseous HNO_3 in the troposphere, including a nylon filter (Anlauf et al., 1988), a mist chamber (Talbot et al., 1990), a denuder technique (Perrino et al., 1990; Simon et al., 1995), a luminol method (Hering et al., 1988), and chemical ionization mass spectrometry (CIMS) (Huey et al., 1998). Among the different approaches, the CIMS technique has the advantages of high sensitivity and fast time-response. Ambient HNO_3 mixing ratio varies considerably temporally and spatially, with the reported values ranging from a few tens of ppt in clean remote environment to tens of ppb in aged urban plumes (Furutani and Akimoto, 2002; Huey et al., 2004). Despite the importance of N_2O_5 in the nocturnal NO_x chemistry, only recently in situ N_2O_5 measurements have become possible. In situ measurements of N_2O_5 have been performed by a cavity ring-down spectroscopy technique (CRDS) (Brown et al., 2002) and a CIMS technique (Huey et al., 1995). The

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

observed N_2O_5 concentration ranges from a few ppt to hundreds of ppt (Brown et al., 2001; 2006; Slusher et al., 2004).

A series of field campaigns have been conducted MCMA such as the 2002, 2003 and 2006 field campaigns. The objectives of these campaigns are to fully characterize the up-to-date air quality, to investigate the underline chemical processes that are responsible for secondary air pollutants formations, and to develop effective control strategies. In this paper, we present measurements of HNO_3 and N_2O_5 during the MCMA 2006 campaign from a recently developed ion drift-chemical ionization mass spectrometry (ID-CIMS) technique and its first field deployment. The results provide insights into the production and gas/particle partitioning of HNO_3 in MCMA.

2 Experimental

2.1 ID-CIMS

The ID-CIMS method has been previously described (Fortner et al., 2004), and only details pertinent to this work are provided. Figure 1 shows a schematic diagram of the ID-CIMS that consists of an ion-drift tube, an ion source, and a quadrupole mass spectrometer. Also depicted in Fig. 1 is the HNO_3 calibration device, which consists of a U-shape 1-inch outer diameter (OD) and 7-inch long glass tube wrapped with a temperature-regulated heating jacket (the dashed line). The U-tube has two symmetrical compartments divided by a glass grid in the middle, with one side housing a 5.0-cm long Teflon permeation tube (VICI Metronics Inc.) and the other filled with 0.5-cm diameter glass beads. A corona discharge is used to produce the ion source; it consists of a stainless steel needle typically biased by about -1200 volts (V_1) and a grounded $1/4$ " OD stainless steel tube. A dry scroll pump (Varian) with a 500 liter per minute pumping speed draws the ambient air into the ID-CIMS system. A small portion of the air is introduced into the drift region through an orifice of about 0.5 mm. Within the drift tube, the reagent ion is produced and the ion-molecule reaction occurs to ionize

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



**Nitric acid during
MCMA 2006**

R. Zhang et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



the neutral species. The ion-drift tube is pumped by an Edwards E2M30 pump. A 10-ring drift tube sealed inside a heavy wall glass tube is used to guide the reagent ions and to control the ion-molecule reaction time. Each stainless steel ring is 7 mm thick and 40 mm OD and has a 14 mm diameter center hole. The rings are connected in series by three Teflon rods and isolated by 1/8" Nylon spacers. Neighboring rings are connected by a $1.0 \pm 5\%$ M Ω resistor. A negative voltage is typically set to develop an electronic field in the drift tube (V2). The reagent and product ions are introduced to the MS system through a pinhole of 400 μm , which is also biased negatively (V3). An Extrel 150-QS mass spectrometer is controlled by the Merlin 3.0 software (Extrel). Two high vacuum stages housing the quadrupole and the electron multiplier are pumped by two Varian TV-551 turbo molecular pumps with a Varian DS402 backing pump. During measurements, the dry scroll pump draws a flow of 200 standard liters per minute (slpm) ambient air into the inlet and only one liter air sample is sucked into the drift tube through the front orifice. A N₂ flow carrying the reagent ions is mixed with the air sample inside the drift tube and the ion-molecule reaction proceeds throughout the drift region. The typical pressure inside the drift tube is 2.8 torr. The reagent and the product ions are analyzed by the quadrupole mass spectrometer.

The unique character of the ID-CIMS lies in that it enables quantifications of neutral species by controlling the ion-molecule reaction time (Δt),



where A corresponds to the neutral species to be analyzed and quantified, R represents the reagent ion, k is the reaction rate constant, and P denotes the product ion. The concentration of the neutral species after the reaction time Δt is expressed,

$$[\text{A}] = \frac{[\text{P}^{(+\text{or}-)}]}{k \Delta t [\text{R}^{(+\text{or}-)}]} \quad (7)$$

where $[\text{P}^{(+\text{or}-)}]$ and $[\text{R}^{(+\text{or}-)}]$ correspond to the intensities of product and reagent ions measured by the mass spectrometer, respectively. k can be obtained by laboratory

measurements or theoretical calculations (Zhao et al., 2004). Δt is determined by the length of the drift tube and the velocity of the reagent ions, U . While moving along the drift region with the carrier gas at a flow velocity of (U_f), ions are also driven by a controllable electronic field to achieve a drift velocity (U_d), which is determined by

$$5 \quad U_d = \mu E \quad (8)$$

where μ is the ionic mobility and E is the electronic field intensity. μ can be calculated from the reduced ionic mobility, μ_0 ,

$$\mu = \mu_0(760/p)(T/273.16) \quad (9)$$

where p and T are the pressure and temperature inside the drift tube, respectively.

10 2.2 Ion chemistry

The ion chemistry used to detect HNO_3 is similarly to that described by Huey and Lovejoy (1996). The reagent ion, SiF_6^- , is produced in two steps. A flow of about 300 standard cubic centimeters per minute (sccm) N_2 doped with <0.1% SF_6 flows through the ion source region, where SF_6 is attached by one electron,



A trace amount of SiF_4 is introduced downstream of the ion source and reacts with SF_6^- through a fluoride transfer reaction to produce SiF_5^- . SiF_5^- subsequently reacts with HNO_3 at a rate of $(3.8 \pm 1) \times 10^{-10} \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$ (Huey and Lovejoy, 1996) to form $\text{SiF}_5^- \cdot \text{HNO}_3$ adduct. During the field campaign, both the isotope peak of the reagent ion ($^{30}\text{SiF}_5^-$, $m/e=125$) and the product ion, $\text{SiF}_5^- \cdot \text{HNO}_3$ ($m/e=186$) are recorded continuously.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



N_2O_5 is detected as the I^- reagent ion, which is generated inside the ion source through electron attachment reaction,



N_2O_5 subsequently reacts with I^- to produce NO_3^- , with a rate constant of $1.3 \times 10^{-9} \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$ (Huey et al., 1995).

The reduced ionic mobility μ_0 of SiF_5^- and I^- are determined according to Mason and McDaniel (1988),

$$\mu_0 = \frac{1.85 \times 10^4}{\bar{\Omega} \sqrt{T_{\text{eff}}}} \left(\frac{m+M}{mM} \right)^{1/2} \text{cm}^2 \cdot \text{V}^{-1} \cdot \text{s}^{-1}, \quad (15)$$

where T_{eff} is the effective temperature of the carrier gas (in K), m and M are the masses (in atomic mass units) of the ion (SiF_5^- or I^-) and the carrier gas (N_2), respectively, and $\bar{\Omega}$ is the momentum-transfer collision integral (in cm^2). T_{eff} is given by

$$\frac{3}{2} k_b T_{\text{eff}} = \frac{3}{2} k_b T + \frac{1}{2} m U_f^2 \quad (16)$$

where k_b is Boltzmann's constant and T is the temperature of the carrier gas. $\bar{\Omega}$ is obtained from the tabulated values (Viehland et al., 1975) based on ion-neutral interaction potentials. Because no experimental data are available to characterize the ion-neutral interactions in the $\text{SiF}_5^-/\text{N}_2$ or I^-/N_2 system, we perform ab initio calculations to obtain the ion-neutral interaction potentials using the Gaussian 03 software package on an SGI Origin 3800 supercomputer (Lei et al., 2000; Lei and Zhang, 2001). The geometry optimization and energy calculations at a series of center-to-center distances for $\text{SiF}_5^-/\text{N}_2$ and I^-/N_2 systems are conducted using density function method B3LYP/6-

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



31G(d,p) and B3LYP/LANL2DZ, respectively. The results are then fitted with a potential model

$$V(r) = \frac{B}{r^{12}} - \frac{C_6}{r^6} - \frac{C_4}{r^4} \quad (17)$$

where the B term represents the short-range repulsion energy, C_6 denotes the charge-induced quadrupole attraction plus the London dispersion attraction, and C_4 represents the attraction between the ion and the dipole induced in N_2 . Based on the calculated potential well depth, ε , and the minimum position, r_m , the corresponding value of \bar{Q} is obtained. Table 1 provides a summary of the calculations. The predicted values of μ_0 for SiF_5^- and I^- are 1.89 and $2.09 \text{ cm}^2 \cdot \text{V}^{-1} \cdot \text{s}^{-1}$, respectively.

2.3 Instrument calibrations

The ID-CIMS, in principle, can quantitatively determine the concentration of neutral species using Eq. (7). The accuracy of the calculation is affected by uncertainties associated with several parameters, including the reduced ionic mobility, the ion-molecule reaction rate constants, the transmission efficiencies of the quadrupole mass filter, fragmentation in the ion-molecule reaction, and etc. These parameters are invariant under given experimental conditions and their uncertainties are minimized by calibration with known concentration gas standards.

The HNO_3 calibration employs a permeation device, as shown in Fig. 1. The permeation device (Fig. 1a) is heated and maintained at 40.0°C . About 400 to 500 sccm N_2 carrier gas is fed into the side filled with glass beads and warmed to the same temperature as the entire device before entering the permeation tube side. After the permeation device, the concentrated HNO_3/N_2 stream is injected into a 1-inch OD Teflon tube in which they are mixed with a 20 to 150 slpm dilution flow. The concentrations of the exiting HNO_3 flow ranges between 0.25 and 2 ppb. Prior to each calibration, the permeation device is maintained at an operational condition for more than 6 h to achieve equilibrium.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



**Nitric acid during
MCMA 2006**

R. Zhang et al.

Due to the “sticky” nature of HNO_3 , it is necessary to verify the effective permeation rate under the normal operation condition to account for any possible wall loss during the preparation of the calibration standards. The procedure to verify the permeation rate is similar to the calibration process, but, instead of introducing the HNO_3 standards into the ID-CIMS for calibration, the HNO_3 standard is introduced to a glass bubbler containing a specific amount of pure water ($R > 17 \text{ M}\Omega$) for a specific time. All tubing is passivated by the HNO_3 standard for a few hours before the final solution is collected. The HNO_3 solution is analyzed by ion chromatography (DIONEX), which is calibrated by ultra pure sodium nitrate (Sigma-Aldrich) solutions. The measured permeation rate is $109 \pm 1.2 \text{ ng/min}$, within 10% of the manufacture certified value (116 ng/min).

Figure 2 shows a correlation between the volumetrically determined HNO_3 standard concentration and the calculated concentration using the procedure described in Sect. 2.1. The error bars represent the systematic variation in measurements. The value of the slope of Fig. 2 corresponds to the calibration factor used to compensate the difference between the true values and the adapted values of the calculation parameters, i.e., the ion-molecule reaction rate constant, reduced ionic mobility, quadrupole transmission efficiency, and etc. For five independent calibrations at 25°C , a calibration factor of 2.2 ± 0.2 is obtained.

N_2O_5 calibration is conducted with laboratory synthesized samples (Huey et al., 1995). N_2O_5 is formed through two sequential reactions (Reactions 3 and 4). O_3 and NO_2 are mixed in a sealed glass reactor and the produced N_2O_5 is collected in a cryotrap (-78.5°C) as white crystal. The first batch of N_2O_5 is discarded to remove the water residue inside the cryotrap. During calibration, pure N_2O_5 is kept in an octanol/dry ice bath (-57°C). A small amount of dry N_2 flows through the container and carries N_2O_5 vapor into a 10-cm long absorption cell inside a UV/VIS spectrometer (Perkin Elmer), where the absolute concentration of N_2O_5 is measured by its absorption at 215 nm ($\sigma = 2.95 \times 10^{-18} \text{ cm}^2 \text{ molecule}^{-1}$, JPL 2006). The concentrated N_2O_5 flow is diluted into a 140 slpm flow and analyzed by the ID-CIMS. Because N_2O_5 is in thermodynamic equilibrium with NO_2 and NO_3 (Reaction 4) and NO_3 can also be

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

detected, we estimate its potential interference and find that only less than 6% of initial N_2O_5 decomposes into NO_3 at room temperature. Figure 3 shows the plots of the N_2O_5 concentrations measured by ID-CIMS against the concentrations determined from UV absorption. The slope in Fig. 3 represents the calibration factor.

During the field measurements, HNO_3 background checks are performed once a few hours by directing the ambient air flow through a two-inch OD nylon filter. N_2O_5 background signal is checked by passing the ambient air mixed with several hundreds of ppb NO through a 12-in-long heated metal tubing. Detection limits of HNO_3 and N_2O_5 for 10 s integration time are estimated about 100 ppt and 20 ppt, respectively.

2.4 Field setup and characterization of the inlet

The ID-CIMS instrument was deployed at the T0 supersite, located at the Instituto Mexicano del Petr3leo (IMP) near the center of the Mexico City Basin ($19^\circ 29.400' \text{ N}$, $99^\circ 08.911' \text{ W}$). The ID-CIMS was housed inside an air-conditioned hut on the roof of Bldg. 32, which was about 30 m above the ground and among a cluster of buildings with the similar height. A 2.20 cm ID PFA tubing was used as the inlet, which had been proved to be the best inlet material (Neuman et al., 1999). In order to minimize the surface effect, ambient air was sampled from two feet above the hut ceiling, and the inlet length was about 12 feet to bring the air sample into the ID-CIMS, located a few inches away from the sampling window. During most times of the field campaign, the weather was dry and relatively cold. Because HNO_3 gas-aerosol partitioning was sensitive to temperature variations, no heating was applied to the HNO_3 inlet. Instead, the sampling flow rate was kept at 200 slpm to minimize the sampling residence time (0.42 s) and the entire inlet was kept under the ambient conditions.

In order to characterize the inlet performance, several tests were conducted by exposing the inlet to HNO_3 (performed at 760 torr, 25°C , $\text{RH}=50\%$). The front of the inlet was exposed to a solution of 68 wt% HNO_3 for less than one second and the ID-CIMS was set to collect data at 0.4 Hz. As shown in Fig. 4, a spike of about 40 ppb HNO_3 was detected by the ID-CIMS within 3 s and the HNO_3 signal immediately decreased

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

by about 80% after 9 s. The decay in the HNO_3 signal was well-fixed by an exponential decay function ($[\text{HNO}_3]=2.4+97.5 \exp(-0.237t)$), showing that the inlet had little memory effect. The influence between adjacent data points was less than 20% relative to each other, if data were collected within every 9 s.

The inlet for N_2O_5 measurements was also made from 2.2 cm ID Teflon tubing except that its length was only 2 ft to minimize surface loss.

An Aerodyne aerosol mass spectrometer (AMS) was used to measure the chemical composition of non-refractory aerosols from 35 nm to 1.5 μm in size. This version of AMS was equipped with a high-resolution time-of-flight mass analyzer and was capable of analyzing organic species and most nitrate and sulfate compounds of different elemental compositions at the same nominal m/z . More details about the AMS were described by DeCarlo et al. (2006).

An ICMS was set up at T0 to measure both gas and aerosol phase acids. Air was aspirated through a wet effluent diffusion denuder (WEDD) at 2 L/min to sample the gas phase acids. Water was continuously pumped through the denuder at a flow rate of 2 mL/min at counter flow to the air. The air to the aerosol collector (AC) first passed at 4 L/min through an activated charcoal denuder to remove the gas phase. The air stream was mixed with heated water vapor (100°C and a flow rate of 0.6 ml/min), which condensed on the aerosol particles. These droplets impacted on a cooled maze (Fisseha et al., 2006). The gas phase as well as the particle phase extracts were collected on a concentrator column (TAC-LP1, Dionex) and analyzed alternately using ion chromatography (conductivity detector) with a mass spectrometer in a quasi-continuous mode. The mass spectrometer (MSQ from Dionex) used electro-spray ionization and had a single quadrupole mass detector.

NO_x and O_3 data used in this work were measured by commercial instruments (Thermo Scientific). Both instruments were regularly calibrated during the campaign. The detection limits were 0.2 ppb for each species and the data were collected at 1-min interval.

**Nitric acid during
MCMA 2006**

R. Zhang et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[I◀](#)[▶I](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

3 Results and discussion

3.1 HNO₃ Measurements

The measurements of HNO₃ and N₂O₅ were conducted from 7 March to 30 March during the MCMA 2006. Due to a power supply failure, measurements from 13 March to 17 March were not available. The ID-CIMS was typically setup to measure HNO₃ during the daytime and after sunset it was switched to the N₂O₅ measurement. All data was collected at 0.1 Hz and presented in CST.

Figure 5 shows a diurnal profile of HNO₃ observed on 22 March, a sunny and hazy day. Due to its photochemical production nature, HNO₃ started to slowly accumulate right after sunrise. From 08:30 a.m. to 10:00 a.m., about 200 ppt HNO₃ was observed and no significant increase occurred before 11:00 a.m. After a steadily increase, HNO₃ reached near 3 ppb at 02:00 p.m., when the photochemical activity reached the maximum. From 02:00 p.m. to 04:00 p.m., HNO₃ reached a peak, and started to decrease sharply after 04:00 p.m. Within one and half hours, only about 400 ppt was observed. HNO₃ did not totally disappear even after it was completely dark, indicating that there were likely other HNO₃ sources sustaining its present. However, when the ID-CIMS was switched into the N₂O₅ mode, no detectable N₂O₅ was observed.

Figure 6 depicts another HNO₃ diurnal profile observed on 23 March, which was relatively cleaner and windier than the previous day. Before 09:00 a.m., HNO₃ was close the instrument detection limit. Shortly after, HNO₃ increased steadily to about 1 ppb at 11:30 a.m. and, then, started to decrease to 600 ppt at 01:00 p.m., when HNO₃ production was supposedly to be maximized. Around 02:45 p.m., HNO₃ started to increase again and reached a daily maximum 1.5 ppb. HNO₃ decreased steadily to 400 ppt at 04:00 p.m. Similar to the previous day observation, near 300 ppt HNO₃ was still observable at about 06:30 p.m. Also, when the ID-CIMS was switched into the N₂O₅ mode, no N₂O₅ was observable. Note that 22 March and 23 represented the typical polluted and clean conditions encountered during the field campaign, respectively.

Figure 7 shows the HNO₃ diurnal profile averaged over the entire campaign. Typ-

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



**Nitric acid during
MCMA 2006**

R. Zhang et al.

ically, no significant HNO_3 was observed before 08:00 a.m., and HNO_3 started to accumulate after 09:00 a.m. and reached daily high, 1 ± 0.65 ppb, between 02:00 to 03:00 p.m. After 04:00 p.m., HNO_3 decreased rapidly to less than 0.4 ppb at 06:00 p.m. and gradually approached 200 ppt, before the ID-CIMS was switched to N_2O_5 measurements. The occurrence of the HNO_3 daily peak was consistent with its photochemical production mechanism, however the magnitude of the HNO_3 peak was lower than that expected given the overwhelming NO_x emission inventory in the MCMA and the strong tropical solar radiation. Another interesting observation was that several hundred ppt HNO_3 was still detected several hours after sunset. Since no significant N_2O_5 was present, the nighttime production of HNO_3 from the hydrolysis of N_2O_5 (through Reactions 2 to 5) could not proceed.

It is evident that the gas-phase chemistry alone could not explain the observed slow rise in the HNO_3 diurnal profiles after sunrise and the residual HNO_3 amount after sunset during MCMA 2006. Heterogeneous processing of HNO_3 in the particle phase needs to be accounted for to explain the HNO_3 measurements (Zhang et al., 1993). It has been suggested that the heterogeneous reaction between HNO_3 and NH_3 in the particle-phase represents an important process to modulate the gaseous HNO_3 concentration (Seinfeld and Pandis, 1998),



Depending on the ambient relative humidity (RH), ammonium nitrate formed in Reaction 18 can exist as a solid or an aqueous solution of NH_4^+ and NO_3^- . The equilibrium constant, K_p , is dependent on the temperature,

$$\ln K_p = 84.6 - (24220/T) - 6.1 \times \ln(T/298) \quad (19)$$

For the measurements relevant to MCMA 2006, the RH was fairly low (<41% averaged over the campaign period). The dry environment at the MCMA prevented NH_4NO_3 from deliquescence and NH_4NO_3 was expected in a solid state. High ammonia (NH_3) concentration (>35 ppb in the early morning) was reported during the MCMA 2003

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[I◀](#)[▶I](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

campaign (Moya et al., 2004). Although no direct measurements of NH_3 was available at T0 during MCMA 2006, its concentration is expected to be high, given that both population and traffic activity inside the MCMA maintained an increasing trend since 2003.

Figure 8 shows a comparison between gaseous HNO_3 and aerosol nitrate (NO_3^-) mass concentration measured by an Aerodyne aerosol mass spectrometer (AMS) on 22 and 23 March. The calculated equilibrium constant (K_p) of Reaction 18 is also plotted in Fig. 8, which is a function of ambient temperature. There are several prominent features in Fig. 8. The aerosol nitrate NO_3^- started to increase right after sunrise and reached a maximum in the early morning. The aerosol nitrate peak occurred several hours earlier than that of the gaseous HNO_3 concentration. The aerosol nitrate dropped sharply after the morning peak and remained low throughout the afternoon and night hours. During each day, the measured HNO_3 concentration and the calculated K_p were anti-correlated with NO_3^- . On the other hand, there appeared to have a good correlation between the measured HNO_3 concentration and calculated K_p : both slowly increased at the morning hours and their peaks coincided. Hence, the slow rise in the measured HNO_3 concentration is likely explained by gas/aerosol partitioning. HNO_3 photochemically produced from Reaction 1 was scavenged from the gas phase by the particle-phase reaction with NH_3 to form aerosol nitrate, when ambient temperature was low and aerosol nitrate was favorable ($K_p < 6$). The gas/aerosol partitioning hence accounts for the delayed rise and daily maximum of measured HNO_3 compared to those of measured aerosol nitrate. As the temperature rose during the course of the day, the equilibrium favored gaseous HNO_3 . HNO_3 was released back to gas-phase from the evaporation of aerosol nitrate, even when its photochemical production decreased. After sunset, the HNO_3 photochemical production ceased, as reflected in the sharp decrease in measured HNO_3 , while a few hundreds of ppt HNO_3 were still measured. Since detectable NO_3^- was present and no detectable N_2O_5 was observed, the lingering nighttime HNO_3 likely originated from the residue ammonium nitrate aerosol, instead from the hydrolysis of N_2O_5 . Figure 8 also shows that on a daily basis higher

**Nitric acid during
MCMA 2006**

R. Zhang et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



aerosol nitrate corresponded to a higher HNO_3 peak, when the difference in K_p was insignificant. This explains the difference in the measurements of NO_3^- and HNO_3 between 22 and 23 March 2006. Therefore, we concluded that during MCMA 2006 at T0 gas/particle partitioning played a key role to account for the measurements in gaseous HNO_3 and aerosol nitrate.

The magnitude and diurnal cycle of aerosol nitrate during the MCMA 2003 was reported by Salcedo et al. (2006). In the morning, particulate nitrate increased and was consistent with the production of nitric acid. However, after 11:00 a.m. aerosol nitrate decreased while HNO_3 production continued. This observation was explained by the increase in the PBL height and temperature and the decrease in the RH as the day progressed. Also, it has been suggested that gas-particle partitioning plays a dominant role in the fate of aerosol nitrate over larger spatial scales (DeCarlo et al., 2007).

3.2 N_2O_5 measurements

The ID-CIMS instrument was typically switched to conduct N_2O_5 measurements after sunset during the 2006 MCMA campaign. During most times of the campaign, nighttime N_2O_5 was below the detection limit of the instrument. Because NO concentration frequently exceeded 100 ppb after 07:00 p.m. and O_3 was quickly depleted by the freshly emitted NO, Reactions 3 and 4 were inhibited at the surface level. Therefore, NO_3 and N_2O_5 did not play a major role during the nighttime chemistry on the surface. It was still likely that some HNO_3 might be formed above the planetary boundary layer (PBL) where the N_2O_5 chemistry was still occurring at night and mixed downward (Stutz et al., 2004). However, as an exception, two N_2O_5 peaks were observed in the late afternoon and early evening on March 26 (Fig. 9). There was a scattered shower started in the early afternoon and no HNO_3 was observed thereafter. At 04:00 p.m., the rain stopped and the sky remained cloudy, and O_3 and NO_2 were about 60 ppb and 20 ppb, respectively. Meanwhile, the NO concentration was less than 2 ppb. The ID-CIMS was switched to the N_2O_5 mode at 04:20 p.m. and continued the measurement until 09:40 p.m., when NO and NO_2 were about 40 ppb and 60 ppb but O_3 was

Nitric acid during MCMA 2006

R. Zhang et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[I◀](#)[▶I](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

only 3 ppb. Background checks were performed at the beginning and the end of the measurement. Two N_2O_5 peaks near 40 ppt were observed around 05:00 p.m. and 08:00 p.m., when both NO_2 and O_3 were still substantial, but no fresh NO emission was present. From 05:45 p.m. to 07:20 p.m., the T0 site was hit by another intermittent shower, and no N_2O_5 was observed and the NO_x and O_3 instruments were off-line for calibrations. After 07:30 p.m., O_3 was anti-correlated with NO_2 due to the NO titration. About 08:50 p.m., NO started to increase significantly and nearly all O_3 was depleted, as N_2O_5 disappeared. Although the ID-CIMS could also response to NO_3 radical as NO_3^- at the same $m/e=62$ peak, NO_3 radical was estimated to be less than 4% of the N_2O_5 signal assuming that Reaction 4 was under thermodynamic equilibrium and using the observed NO_2 and O_3 concentrations.

3.3 Inter-comparison with ICMS

An ICMS instrument was set up side-by-side with the ID-CIMS during the MCMA 2006 field campaign. The ICMS utilized a denuder to selectively collect gas phase HNO_3 into aqueous solutions, which were then analyzed by an electrospray mass spectrometer. The ICMS generated one data point about every two hours, thus its time series could not match with the temporal resolution of about 10 s from the ID-CIMS measurements. We compared the results between the two instruments for periods when both instruments were collecting data and the ID-CIMS data were averaged to represent the data during a similar period. The results were plotted in Fig. 10. A good correlation in performance was found ($R^2=0.75$) between the two techniques. We also performed a t -test for these two set of data and a P value of 0.68 further proved that statistically these two techniques reported the same results. The ID-CIMS data set was about 17% lower than the ICMS data set, and the intersection was well below the detection limit of either instrument.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



4 Conclusions

We deployed an ID-CIMS during the MCMA 2006 campaign to measure HNO_3 and N_2O_5 at the T0 site. The objective of this work is to characterize the NO_x chemistry and its budget in the MCMA. Diurnally, HNO_3 was less than 200 parts per trillion (ppt) during the night and in the early morning, increased steadily from around 09:00 a.m. CST, reached a peak value of 0.5 to 3 parts per billion (ppb) in the early afternoon, and declined sharply to less than half of the peak value near 05:00 p.m. CST. The HNO_3 mixing ratio was found to anti-correlate with aerosol nitrate, suggesting that the gaseous HNO_3 concentration was regulated by the gas-particle partitioning process. Inter-comparison between the ID-CIMS and the ICMS showed a good agreement ($R^2=0.75$) in HNO_3 measurements. During most times of the MCMA 2006 campaign, N_2O_5 was below the detection limit of the ID-CIMS due to high NO mixing ratio at the surface, with one exception of transient N_2O_5 peaks of 40 ppt were encountered on 26 March under cloudy conditions. The results reveal that during the MCMA 2006 campaign HNO_3 was primarily produced through the photochemical process and HNO_3 diurnal profile was largely controlled by the gas/particle partitioning process.

Acknowledgements. This research was funded by the Center for Atmospheric Chemistry and Environment at the Texas A & M University. The authors were grateful to N. A. Marley and J. S. Gaffney for providing the temperature and RH data.

References

- Anlauf, K. G., Mactavish, D. C., Wiebe, H. A., Schiff, H. I., and Mackay, G. I.: Measurement of atmospheric nitric-acid by the filter method and comparisons with the tunable diode-laser and other methods, *Atmos. Environ.*, 22, 1579–1586, 1988.
- Brown, S. S., Stark, H., Ciciora, S. J., and Ravishankara, A. R.: In-situ measurement of atmospheric NO_3 and N_2O_5 via cavity ring-down spectroscopy, *Geophys. Res. Lett.*, 28, 3227–3230, 2001.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



**Nitric acid during
MCMA 2006**

R. Zhang et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Brown, S. S., Stark, H., Ciciora, S. J., McLaughlin, R. J., and Ravishankara, A. R.: Simultaneous in situ detection of atmospheric NO_3 and N_2O_5 via cavity ring-down spectroscopy, *Rev. Sci. Instrum.*, 73, 3291–3301, 2002.

Brown, S. S., Ryerson, T. B., Wollny, A. G., Brock, C. A., Peltier, R., Sullivan, A. P., Weber, R. J., Dube, W. P., Trainer, M., Meagher, J. F., Fehsenfeld, F. C., and Ravishankara, A. R.: Variability in nocturnal nitrogen oxide processing and its role in regional air quality, *Science*, 311, 67–70, 2006.

DeCarlo, P. F., Kimmel, J. R., Trimborn, A., Northway, M. J., Jayne, J. T., Aiken, A. C., Gonin, M., Fuhrer, K., Horvath, T., Docherty, K. S., Worsnop, D. R., and Jimenez, J. L.: Field-deployable, high-resolution, time-of-flight aerosol mass spectrometer, *Anal. Chem.*, 78, 8281–8289, 2006.

DeCarlo, P. F., Dunlea, E. J., Kimmel, J. R., Aiken, A. C., Sueper, D., Crouse, J., Wennberg, P. O., Emmons, L., Shinozuka, Y., Clarke, A., Zhou, J., Tomlinson, J., Collins, D. R., Knapp, D., Weinheimer, A. J., Montzka, D. D., Campos, T., and Jimenez, J. L.: Fast airborne aerosol size and chemistry measurements with the high resolution aerosol mass spectrometer during the milagro campaign, *Atmos. Chem. Phys. Discuss.*, 7, 18269–18317, 2007.

Fisseha, R., Dommen, J., Gaeggeler, K., Weingartner, E., Samburova, V., Kalberer, M., and Baltensperger, U.: Online gas and aerosol measurement of water soluble carboxylic acids in zurich, *J. Geophys. Res.*, 111, D12316, doi:10.1029/2005JD006782, 2006.

Finlayson-Pitts, B. J. and Pitts, J. N.: *Chemistry of the upper and lower atmosphere : Theory, experiments and applications*, Academic Press, San Diego, Calif., xxii, 969 pp., 1999.

Fortner, E. C., Zhao, J., and Zhang, R. Y.: Development of ion drift-chemical ionization mass spectrometry, *Anal. Chem.*, 76, 5436–5440, 2004.

Furutani, H. and Akimoto, H.: Development and characterization of a fast measurement system for gas-phase nitric acid with a chemical ionization mass spectrometer in the marine boundary layer, *J. Geophys. Res.-Atmos.*, 107, 4016, doi:10.1029/2000JD000269, 2002.

Hering, S. V., Lawson, D. R., Allegrini, I., Febo, A., Perrino, C., Possanzini, M., Sickles, J. E., Anlauf, K. G., Wiebe, A., Appel, B. R., John, W., Ondo, J., Wall, S., Braman, R. S., Sutton, R., Cass, G. R., Solomon, P. A., Eatough, D. J., Eatough, N. L., Ellis, E. C., Grosjean, D., Hicks, B. B., Womack, J. D., Horrocks, J., Knapp, K. T., Ellestad, T. G., Paur, R. J., Mitchell, W. J., Pleasant, M., Peake, E., Maclean, A., Pierson, W. R., Brachaczek, W., Schiff, H. I., Mackay, G. I., Spicer, C. W., Stedman, D. H., Winer, A. M., Biermann, H. W., and Tuazon, E. C.: The nitric-acid shootout – field comparison of measurement methods, *Atmos. Environ.*,

22, 1519–1539, 1988.

Huey, L. G., Hanson, D. R., and Howard, C. J.: Reactions of SF_6^- and I^- with atmospheric trace gases, *J. Phys. Chem.*, 99, 5001–5008, 1995.

Huey, L. G. and Lovejoy, E. R.: Reactions of SiF_5^- with atmospheric trace gases: Ion chemistry for chemical ionization detection of HNO_3 in the troposphere, *Int. J. Mass. Spectrom.*, 155, 133–140, 1996.

Huey, L. G., Dunlea, E. J., Lovejoy, E. R., Hanson, D. R., Norton, R. B., Fehsenfeld, F. C., and Howard, C. J.: Fast time response measurements of HNO_3 in air with a chemical ionization mass spectrometer, *J. Geophys. Res.-Atmos.*, 103, 3355–3360, 1998.

Huey, L. G., Tanner, D. J., Slusher, D. L., Dibb, J. E., Arimoto, R., Chen, G., Davis, D., Buhr, M. P., Nowak, J. B., Mauldin, R. L., Eisele, F. L., and Kosciuch, E.: CIMS measurements of HNO_3 and SO_2 at the south pole during ISCAT 2000, *Atmos. Environ.*, 38, 5411–5421, 2004.

Huey, L. G.: Measurement of trace atmospheric species by chemical ionization mass spectrometry: Speciation of reactive nitrogen and future directions, *Mass Spectrom. Rev.*, 26, 166–184, 2007.

JPL: Chemical Kinetics and Photochemical Data for Use in Atmospheric Studies Evaluation Number 15, National Aeronautics and Space Administration, Jet Propulsion Laboratory, California Institute of Technology, Pasadena, Calif., 5–77, 2006.

Lei, W., de Foy, B., Zavala, M., Volkamer, R., and Molina, L. T.: Characterizing ozone production in the Mexico City metropolitan area: A case study using a chemical transport model, *Atmos. Chem. Phys.*, 7, 1347–1366, 2007, <http://www.atmos-chem-phys.net/7/1347/2007/>.

Lei, W. F., Derecskei-Kovacs, A., and Zhang, R. Y.: Ab initio study of oh addition reaction to isoprene, *J. Chem. Phys.*, 113, 5354–5360, 2000.

Lei, W. F. and Zhang, R. Y.: Theoretical study of hydroxylisoprene alkoxy radicals and their decomposition pathways, *J. Phys. Chem. A*, 105, 3808–3815, 2001.

Lei, W. F., Zhang, R. Y., Tie, X. X., and Hess, P.: Chemical characterization of ozone formation in the Houston-Galveston area: A chemical transport model study, *J. Geophys. Res.-Atmos.*, 109, D12301, doi:10.1029/2003JD004219, 2004.

Mason, E. A. and McDaniel, E. W.: Transport properties of ions in gases, Wiley, New York, xvi, 560 pp., 1988.

Molina, L. T., Molina, M. J., and Alliance for Global Sustainability: Air quality in the Mexico megacity: An integrated assessment, Alliance for global sustainability bookseries; 2, Kluwer

**Nitric acid during
MCMA 2006**

R. Zhang et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



**Nitric acid during
MCMA 2006**

R. Zhang et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Academic Publishers, Dordrecht; Boston, xxi, 384 pp., 2002.

Molina, L. T., Kolb, C. E., de Foy, B., Lamb, B. K., Brune, W. H., Jimenez, J. L., Ramos-Villegas, R., Sarmiento, J., Paramo-Figueroa, V. H., Cardenas, B., Gutierrez-Avedoy, V., and Molina, M. J.: Air quality in north America's most populous city—overview of the MCMA-2003 campaign, *Atmos. Chem. Phys.*, 7, 2447–2473, 2007, <http://www.atmos-chem-phys.net/7/2447/2007/>.

Moya, M., Grutter, M., and Baez, A.: Diurnal variability of size-differentiated inorganic aerosols and their gas-phase precursors during January and February of 2003 near downtown Mexico City, *Atmos. Environ.*, 38, 5651–5661, 2004.

Neuman, J. A., Huey, L. G., Ryerson, T. B., and Fahey, D. W.: Study of inlet materials for sampling atmospheric nitric acid, *Environ. Sci. Technol.*, 33, 1133–1136, 1999.

Perrino, C., Desantis, F., and Febo, A.: Criteria for the choice of a denuder sampling technique devoted to the measurement of atmospheric nitrous and nitric-acids, *Atmos. Environ. A-Gen.*, 24, 617–626, 1990.

Ramazan, K. A., Wingen, L. M., Miller, Y., Chaban, G. M., Gerber, R. B., Xantheas, S. S., and Finlayson-Pitts, B. J.: New experimental and theoretical approach to the heterogeneous hydrolysis of no₂: Key role of molecular nitric acid and its complexes, *J. Phys. Chem. A*, 110, 6886–6897, doi:10.1021/Jp056426n, 2006.

Saliba, N. A., Yang, H., and Finlayson-Pitts, B. J.: Reaction of gaseous nitric oxide with nitric acid on silica surfaces in the presence of water at room temperature, *J. Phys. Chem. A*, 105, 10 339–10 346, doi:10.1021/Jp012330r, 2001.

Salcedo, D., Onasch, T. B., Dzepina, K., Canagaratna, M. R., Zhang, Q., Huffman, J. A., DeCarlo, P. F., Jayne, J. T., Mortimer, P., Worsnop, D. R., Kolb, C. E., Johnson, K. S., Zuberi, B., Marr, L. C., Volkamer, R., Molina, L. T., Molina, M. J., Cardenas, B., Bernabe, R. M., Marquez, C., Gaffney, J. S., Marley, N. A., Laskin, A., Shutthanandan, V., Xie, Y., Brune, W., Leshner, R., Shirley, T., and Jimenez, J. L.: Characterization of ambient aerosols in Mexico city during the mcma-2003 campaign with aerosol mass spectrometry: Results from the cenica supersite, *Atmos. Chem. Phys.*, 6, 925–946, 2006, <http://www.atmos-chem-phys.net/6/925/2006/>.

Seinfeld J. H. and Pandis, S. N.: *From air pollution to climate change*, Wiley, New York, xxvii, *Atmos. Chem. Phys.*, 1326 pp., 1998.

Sillman, S.: The relation between ozone, NO_x and hydrocarbons in urban and polluted rural environments, *Atmos. Environ.*, 33, 1821–1845, 1999.

**Nitric acid during
MCMA 2006**

R. Zhang et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

- Simon, P. K. and Dasgupta, P. K.: Continuous automated measurement of gaseous nitrous and nitric-acids and particulate nitrite and nitrate, *Environ. Sci. Technol.*, 29, 1534–1541, 1995.
- Slusher, D. L., Huey, L. G., Tanner, D. J., Flocke, F. M., and Roberts, J. M.: A thermal dissociation-chemical ionization mass spectrometry (td-cims) technique for the simultaneous measurement of peroxyacyl nitrates and dinitrogen pentoxide, *J. Geophys. Res.-Atmos.*, 109, D19315, 2004.
- Stutz, J., Alicke, B., Ackermann, R., Geyer, A., White, A., and Williams, E.: Vertical profiles of NO_3 , N_2O_5 , O_3 , and NO_x in the nocturnal boundary layer: 1. Observations during the texas air quality study 2000, *J. Geophys. Res.*, 109, D12306, doi:10.1029/2003JD004209, 2004.
- Suh, I., Lei, W. F., and Zhang, R. Y.: Experimental and theoretical studies of isoprene reaction with NO_3 , *J. Phys. Chem. A*, 105, 6471–6478, 2001.
- Talbot, R. W., Vijgen, A. S., and Harriss, R. C.: Measuring tropospheric hno3 - problems and prospects for nylon filter and mist chamber techniques, *J. Geophys. Res.-Atmos.*, 95, 7553–7561, 1990.
- Tie, X. X., Madronich, S., Li, G. H., Ying, Z. M., Zhang, R. Y., Garcia, A. R., Lee-Taylor, J., and Liu, Y. B.: Characterizations of chemical oxidants in mexico city: A regional chemical dynamical model (wrf-chem) study, *Atmos. Environ.*, 41, 1989–2008, 2007.
- Viehland, L. A., Mason, E. A., Morrison, W. F., and Flannery, M. R.: Tables of transport collision integrals for (n, 6, 4) ion-neutral potentials, *Atom. Data Nucl. Data*, 16, 495–514, 1975.
- Zhang, R., Wooldridge, P. J., and Molina, M. J.: Vapor pressure measurements for the $\text{H}_2\text{SO}_4/\text{HNO}_3/\text{H}_2\text{O}$ and $\text{H}_2\text{SO}_4/\text{HCl}/\text{H}_2\text{O}$ systems: Incorporation of stratospheric acids into background sulfate aerosols, *J. Phys. Chem.*, 97, 8541–8548, 1993.
- Zhang, R. Y., Leu, M. T., and Keyser, L. F.: Hydrolysis of N_2O_5 and ClONO_2 on the $\text{H}_2\text{SO}_4/\text{HNO}_3/\text{H}_2\text{O}$ ternary solutions under stratospheric conditions, *Geophys. Res. Lett.*, 22, 1493–1496, 1995.
- Zhang, R. Y., Lei, W. F., Tie, X. X., and Hess, P.: Industrial emissions cause extreme urban ozone diurnal variability, *P. Natl. Acad. Sci. USA*, 101, 6346–6350, 2004a.
- Zhang, R. Y., Suh, I., Zhao, J., Zhang, D., Fortner, E. C., Tie, X. X., Molina, L. T., and Molina, M. J.: Atmospheric new particle formation enhanced by organic acids, *Science*, 304, 1487–1490, 2004b.
- Zhao, J. and Zhang, R. Y.: Proton transfer reaction rate constants between hydronium ion ($\text{H}_3\text{O}^{(+)}$) and volatile organic compounds, *Atmos. Environ.*, 38, 2177–2185, 2004.

**Nitric acid during
MCMA 2006**

R. Zhang et al.

Table 1. Ion-neutral potentials of $\text{SiF}_5^-/\text{N}_2$ and I^-/N_2 systems based on ab initio calculations.

	$\text{SiF}_5^-/\text{N}_2$	I^-/N_2
ε (eV)	0.050	0.057
r_m (Å)	4.82	4.06
B ($\text{eV}\cdot\text{Å}^{12}$)	8.62×10^6	5.29×10^5
C_6 ($\text{eV}\cdot\text{Å}^6$)	824.96	220.38
C_4 ($\text{eV}\cdot\text{Å}^4$)	20.98	8.39
$\bar{\Omega}$ (10^{-16}cm^2)	73.16	51.83

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

I◀

▶I

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



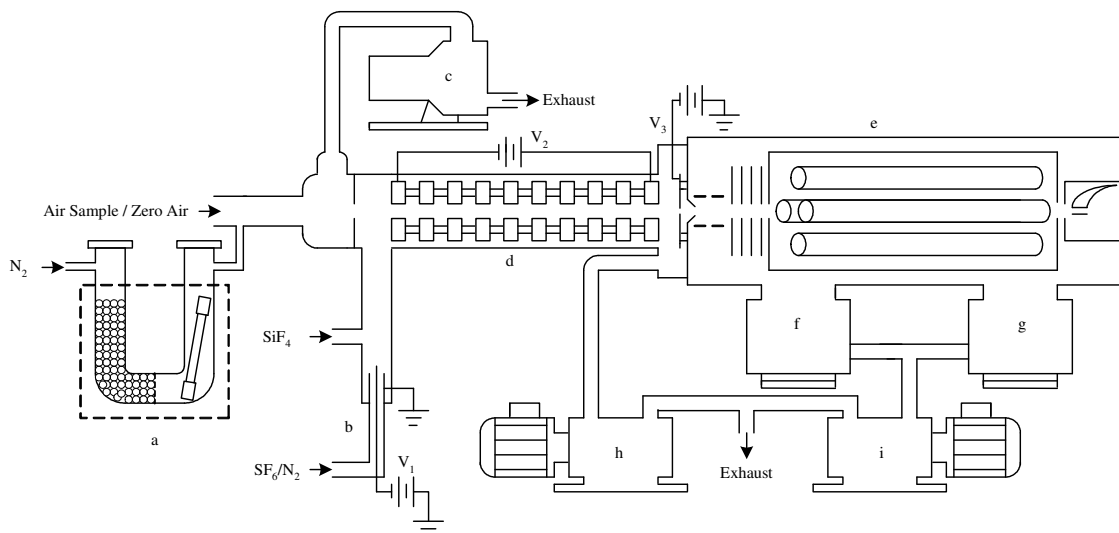


Fig. 1. Schematic diagram of the ID-CIMS: **(a)**, HNO₃ permeation device; **(b)**, ion source; **(c)**, dry scroll pump for air sampling; **(d)**, 10-ring drift tube; **(e)**, Extrel 150-QS mass spectrometer; **(f)** and **(g)**, Varian TV-551 turbo pumps; **(h)**, Edwards E2M30 oil pump; **(i)**, Varian DS402 oil pump.

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[◀](#)
[▶](#)
[◀](#)
[▶](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


Nitric acid during
MCMA 2006

R. Zhang et al.




Fig. 2. Plot of calculated versus volumetrically prepared HNO₃ concentrations. The slope corresponds to the calibration factor.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[I◀](#)[▶I](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Nitric acid during
MCMA 2006

R. Zhang et al.




Fig. 3. Plot of measured and calculated N₂O₅ vs. synthesized standards concentration. The slope corresponds to the calibration factor.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[I◀](#)[▶I](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Nitric acid during
MCMA 2006

R. Zhang et al.

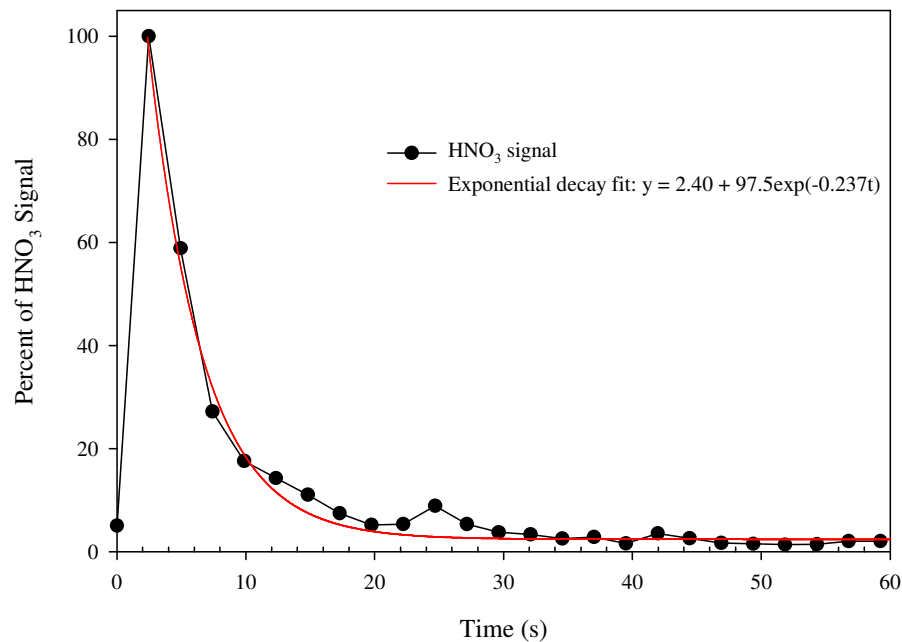


Fig. 4. Spike test of the inlet using a 68 wt % HNO₃ solution exposed to the 12 ft inlet for less than one second. The data was collected at 0.4 Hz.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

**Nitric acid during
MCMA 2006**

R. Zhang et al.




Fig. 5. Diurnal profile of HNO_3 observed on 22 March 2006. Backgrounds were checked at 08:36, 10:38, 12:30, 14:39, 16:35, 19:20, and 20:35 CST.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[I◀](#)[▶I](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

**Nitric acid during
MCMA 2006**

R. Zhang et al.




Fig. 6. Diurnal profile of HNO₃ observed on 23 March 2006. Backgrounds were checked at 08:00, 10:15, 13:00, 15:30, and 18:10 CST.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[I◀](#)[▶I](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Nitric acid during
MCMA 2006

R. Zhang et al.




Fig. 7. Averaged HNO₃ diurnal profile during the entire field campaign. Each point is based on 1755 data points and the error bars represent one standard deviation.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Nitric acid during
MCMA 2006

R. Zhang et al.

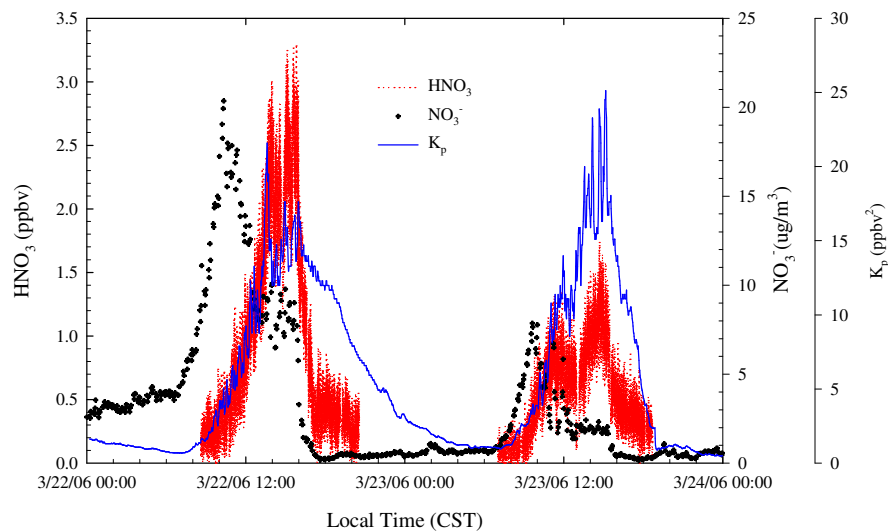


Fig. 8. Gaseous HNO_3 , aerosol nitrate (NO_3^-), and the calculated dissociation constant K_p of Reaction 18 for 22 and 23 March 2006.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Nitric acid during
MCMA 2006

R. Zhang et al.

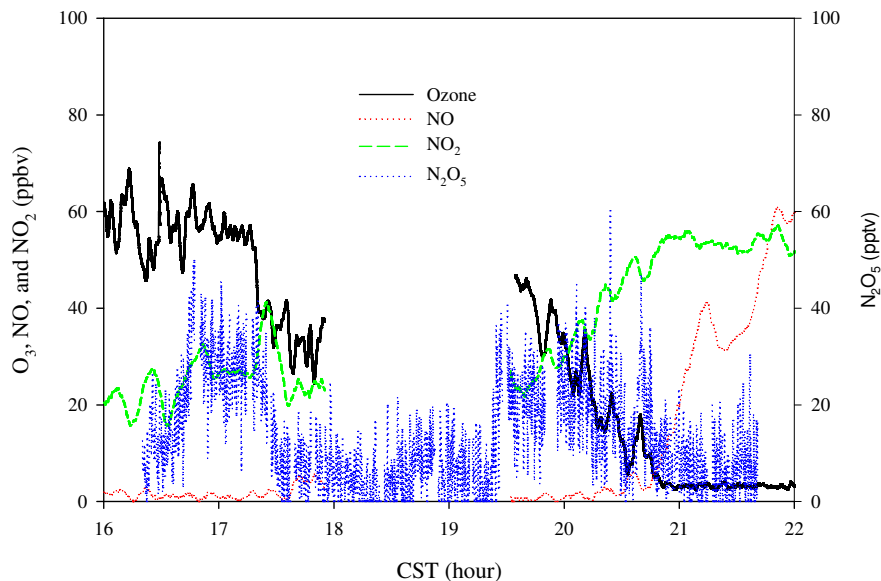


Fig. 9. N_2O_5 measured on 26 March. Also shown are plots of NO , NO_2 , and O_3 . The gap in the measurements was due to instrument calibrations.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

**Nitric acid during
MCMA 2006**

R. Zhang et al.

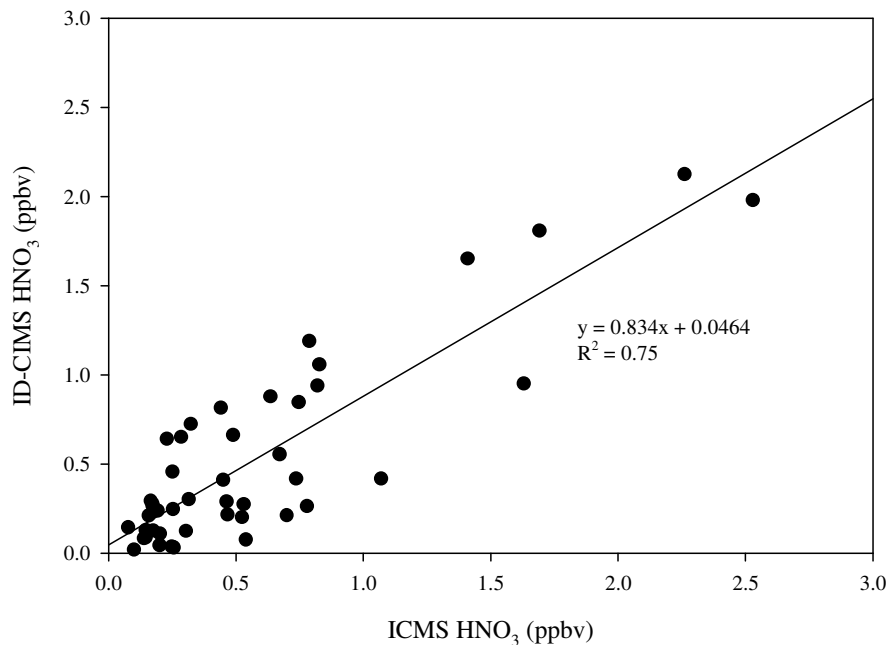


Fig. 10. Inter-comparison between the ID-CIMS and ICMS based on 45 overlapping data points collected from 8 to 29 March 2006.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[◀](#)[▶](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)