



**HAL**  
open science

## Leaving the lab: a portable and quickly tunable BCI

Aurélien van Langenhove, Marie-Hélène Bekaert, François Cabestaing

### ► To cite this version:

Aurélien van Langenhove, Marie-Hélène Bekaert, François Cabestaing. Leaving the lab: a portable and quickly tunable BCI. BCI Meets Robotics: Challenging Issues in Brain-Computer Interaction and Shared Control, MAIA'07, Nov 2007, Leuven, Belgium. hal-00521111

**HAL Id: hal-00521111**

**<https://hal.science/hal-00521111>**

Submitted on 25 Sep 2010

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

# Leaving the lab: a portable and quickly tunable BCI

A. Van Langenhove<sup>(1)</sup>, M.H. Bekaert<sup>(2)</sup>, F. Cabestaing<sup>(2)</sup>

<sup>(1)</sup> LAGIS, HEI, 13, rue de Toul, 59046 Lille. FRANCE (aurelienvlg@gmail.com)

<sup>(2)</sup> LAGIS, USTL, Bât. P2, Cité Scientifique, 59655 Villeneuve d'Ascq. FRANCE

## Context and goals

Although many systems for palliative communication based on non-invasive BCIs have been developed during the last few years, very few projects aim at leaving the research labs and hospitals for helping patients at home. Jon Wolpaw's team at the Wadworth Center<sup>1</sup> has developed a portable BCI that has now been used for more than one year on a daily basis by 5 people suffering from ALS. This experiment shows that highly handicapped people greatly benefit from such BCIs that they tend to use during long periods — between 5 and 8 hours a day — for communicating with their loved ones, for surfing the web, or reading and writing emails.


We also aim at being able to leave the lab with this now mature technology for screening handicapped people at home. This would allow checking easily if a patient can use efficiently a BCI without requiring him to come to the hospital or to a specialized laboratory. From the hardware point of view, this home-screening requires a BCI setup that can be used in any situation: portable, fully autonomous and battery powered. From the software point of view, the machine learning techniques that adapt the BCI to the individual must provide a "good" result within a few seconds rather than an "optimal" result after several minutes or hours of processing.

## Achievements and future work


This project started a few months ago, in April 2007 more precisely, and is therefore still under progress. The hardware setup — see figure (1) below — is composed of: (a) an EEG-signal amplifier (Guger Technologies<sup>2</sup> g.USBamp, 16 channels), (b) an EEG-cap, (c) a laptop computer with a dual-core processor for fast signal processing and efficient online classification, and (d) a separate LCD screen, for showing visual feedback to the user. This setup is powered by a battery (e). This system runs the widely used BCI2000 software [2].

A fast learning technique has been implemented for the matrix-based P300-speller paradigm [1]. It computes first and second order statistics of every sample of the EEG signals in the response to a visual stimulus in order to define the most discriminative ones. The pattern presented in figure (2) is a typical result of this learning procedure. The grey level of every sample ( $1 \dots 180$ ) on every electrode ( $1 \dots 8$ ) indicates its significance in terms of discrimination between a target and a non-target stimulus. Significant features — for example signal average on small temporal windows — can be determined from these patterns. This approach allows for very fast feature selection — in 2 or 3 seconds in our non optimized implementation — and is therefore well adapted to the home-screening application.

Since these statistics can be computed recursively, requiring a very small computing power, this learning procedure will also be implemented online. The proposed technique is the following: the user spells 3 to 5 characters in copy mode, which yields labeled responses used for the initial classifier training; then the interface is switched to free spelling mode and the online learning procedure adapts the set of features according to the constantly updated statistics. During this step, the operator indicates to the BCI if the letters spelled by the user are correct or not in order to provide a "ground truth" to the learning technique.

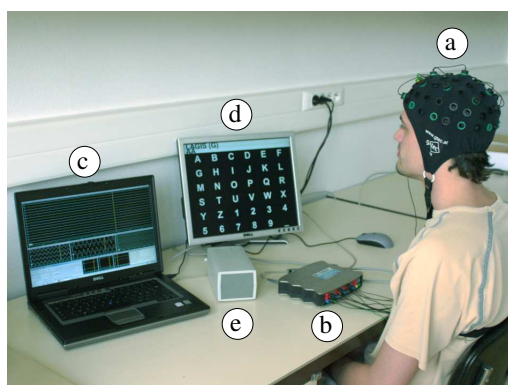

(1) hardware setup

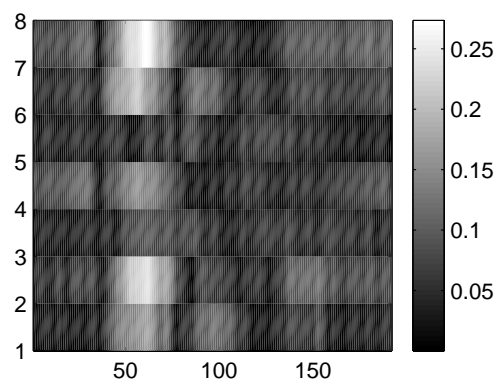

(2) classification pattern

## References

- [1] F. Cabestaing, T. Vaughan, D. M. Farland, and J. Wolpaw. Classification of evoked potentials by pearson's correlation in a brain-computer interface. *AMSE-journals (Barcelona, Spain), Modelling C*, 67:156–166, Feb. 2007.
- [2] G. Schalk, D. J. McFarland, T. Hinterberger, N. Birbaumer, and J. R. Wolpaw. BCI2000: A general-purpose brain-computer interface (BCI) system. *IEEE Transactions on Biomedical Engineering*, 51:1034–1043, 2004.

<sup>1</sup>Albany, NY, USA. <http://www.bciresearch.org/>

<sup>2</sup><http://www.gtec.at/>