



**HAL**  
open science

## **A Microfluidic Biochip Dedicated to Highly Parallelized Electrofusion**

Feriel Hamdi, Olivier Français, Julien Villemejeane, M Woytasik, Claire Dalmay,  
Lluis M. Mir, Elisabeth Dufour-Gergam, Bruno Le Pioufle

► **To cite this version:**

Feriel Hamdi, Olivier Français, Julien Villemejeane, M Woytasik, Claire Dalmay, et al.. A Microfluidic Biochip Dedicated to Highly Parallelized Electrofusion. MMB, 2011, Lucerne, Switzerland. <hal-00739182>

**HAL Id: hal-00739182**

**<https://hal.science/hal-00739182v1>**

Submitted on 13 Feb 2013

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



HAL Authorization

# A MICROFLUIDIC BIOCHIP DEDICATED TO HIGHLY PARALLELIZED ELECTROFUSION

F. Hamdi<sup>1,2</sup>, O. Français<sup>1</sup>, J. Villemejeane<sup>1,3,4</sup>, M. Woytasik<sup>2</sup>, C. Dalmay<sup>1</sup>, L.M. Mir<sup>3,4</sup>, E. Dufour-Gergam<sup>2</sup>, B. Le Pioufle<sup>1</sup>

<sup>1</sup> Ecole Normale Supérieure de Cachan, CNRS, SATIE, UMR 8029, Cachan, France

<sup>2</sup> Univ Paris-Sud, CNRS, Institut d'Electronique Fondamentale, UMR 8622, Orsay, France

<sup>3</sup> CNRS, UMR 8203, Institut Gustave-Roussy, Villejuif, France

<sup>4</sup> Univ Paris-Sud, UMR 8203, Orsay, France

## ABSTRACT

This paper deals with the development of a biochip dedicated to fusion between two types of cells, in a highly parallelized way. The fusion process is initiated by an electric field pulse applied to cells paired in fluidic traps. The paper will present different strategies for the capture and pairing of cells prior to the electrofusion, combining fluidic and electrical forces. The design is highly parallelized in order to fulfill our objective which is the high throughput production of hybrid cells.

The microfabrication process is described. Experimental results confirm the efficiency of the proposed device for cell trapping, pairing and fusion.

**KEY WORDS:** Microfluidics, Biochip, Electrofusion, Cell trapping

## INTRODUCTION

The electrofusion between a dendritic and a cancerous cell is one of the new techniques investigated for immunotherapy of cancer. Hybridomas produced massively might be reinjected *in vivo* as a vaccine [1]. Nowadays, electrofusion being performed in macroscopic chambers suffer of a poor efficiency. The miniaturized approach developed in this paper provides new avenues to enhance and control the different electrofusion steps, and go towards the high throughput production of hybrid cells.

To achieve parallel fusions on chip, three steps have to be integrated i) the trapping of cells flowing in the microfluidic channel ii) their pairing prior to fusion, iii) the electrofusion operation while cells are maintained at close contact. When the transmembrane voltage reaches 0.3V, membranes are permeabilized, and finally mixed leading to the formation of a hybrid cell including the cell content of the two mother cells.

## DESIGN

The design of the proposed biochip is derived from a device originally devoted to the mixing of droplets [2]. The pairing is performed in three steps i) cells type A are captured in location 1 thanks to the flow as shown on figure 1 ii) the flow is reversed, leading cells type A to move towards the facing fusion chamber in location 2 (see figure 1) iii) then cells type B are injected to be placed in location 2. Gold electrodes placed at both sides of the fusion chamber permit to apply the electric field (see figure 2) necessary to put into contact the cells of type A and B, and finally induce their fusion through an electropermeabilization pulse.

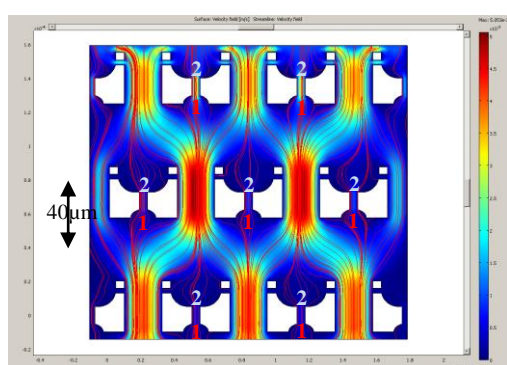


Figure 1: Comsol© simulation of the flow induced through the fluidic traps

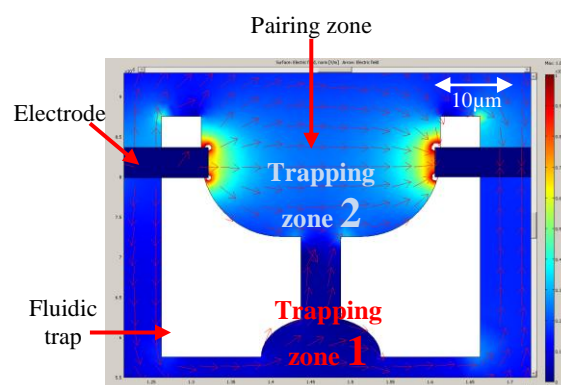


Figure 2: Comsol© simulation of the Electric field within the trap zone

## PROCESS OF FABRICATION

The microfluidic chip fabrication is based on photolithography process. Glass is used as substrate for the device in order to ensure the transparency that will permit the real time monitoring of the fusion operation. Gold is chosen as material for the electrodes, to insure the biocompatibility of the device. In classical microfluidic devices, structured PDMS composes the channels [3]. But in this method, a good alignment with the electrodes is not possible. To ensure

proper alignment, the microfluidic structures of the biochip presented (channels and fluidic traps) are fabricated using SU8-2025 ( $t=25\mu\text{m}$ ) thick photosensitive resist (figure 3).

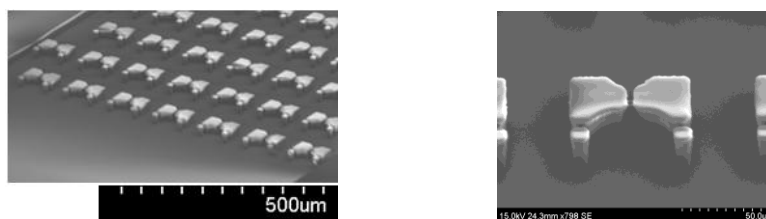


Figure 3: SEM view of the microfluidic traps

The packaging of the biochip is performed thanks to the bonding of a PDMS cover on the top of the SU8 fluidic structure. To do so, silanization of the photoresist after its hard baking (2 hours at  $175^\circ\text{C}$ ) is performed in liquid phase. After the silanization, the two surfaces (SU8 and PDMS) are activated with  $\text{O}_2$  plasma before being bonded on a hot plate. The microfabricated device is shown on figure 4.

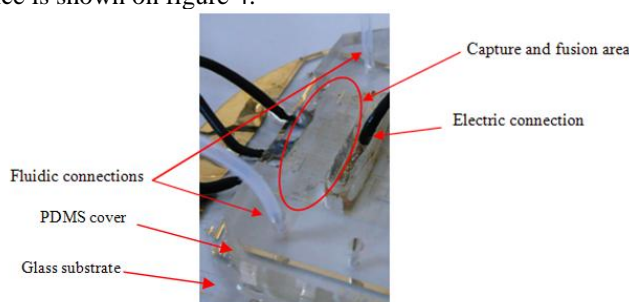


Figure 4: Packaged and connected electrofusion biochip

## RESULTS

B16F10 (mouse melanoma cells) with a concentration of  $10^6$  cells/ml in a Minimum Essential Media were used for the biological tests. In these initial tests a single cell type was used to analyze cells' placement in the microfluidic traps. The cells were injected in the biochip using a syringe pump and were paired using different patterned traps according to the 3 steps previously described (figures 5 and 6). Electric pulses were then applied using a Cliniporator™ generator (IGEA, Carpi, Italy) exposing the cells to  $100\mu\text{s}$  pulses of about  $2\text{kV}/\text{cm}$  amplitude. This demonstrates that a highly parallelized trapping and pairing of cells can be done prior to electrofusion on a microfluidic device. Analysis of the fusion efficiency and quality are underway.




Figure 5: Result of the microfluidic trapping of cells

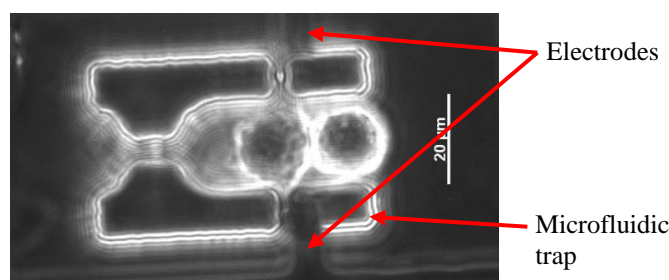


Figure 6: Paired cells under the application of electric pulses for the fusion

## ACKNOWLEDGEMENT

This work was performed thanks to the financial support of PRES Universud, CNANO'Ile de France, and the ANR PNANO Nanopulsbiochip

## REFERENCES

- [1] U. Trefzer and al, "Tumour-dendritic hybrid cell vaccination for the treatment of patients with malignant melanoma: immunological effects and clinical results", *Vaccine* 23 (2005) 2367–2373.
- [2] Y. Bai and al, "A double droplet trap system for studying mass transport across a droplet-droplet interface", *Lab on chip*, DOI: 10.1039/b925133b
- [3] T. Fujii and al, "PDMS-based microfluidic devices for biomedical applications", *Microelectronic Engineering*, Volumes 61-62, July 2002, pp. 907-914