



HAL
open science

Assessment of the effective attenuation coefficient of scattering media illuminated by a LED array : Effect of the beam size

Jean-Yves Le Pommellec, Vianney Piron, Mohamed-Lamine Askoura,
Jean-Pierre L'Huillier

► To cite this version:

Jean-Yves Le Pommellec, Vianney Piron, Mohamed-Lamine Askoura, Jean-Pierre L'Huillier. Assessment of the effective attenuation coefficient of scattering media illuminated by a LED array : Effect of the beam size. European Conferences on Biomedical Optics 2015, Jun 2015, Munich, Germany. pp.1-8, 10.1117/12.2183433 . hal-01202046

HAL Id: hal-01202046

<https://hal.science/hal-01202046>

Submitted on 18 Sep 2015

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Science Arts & Métiers (SAM)

is an open access repository that collects the work of Arts et Métiers ParisTech researchers and makes it freely available over the web where possible.

This is an author-deposited version published in: <http://sam.ensam.eu>
Handle ID: <http://hdl.handle.net/10985/10054>

To cite this version :

Jean-Yves LE POMMELLE, Vianney PIRON, Mohamed-Lamine ASKOURA, Jean-Pierre L'HUILLIER - Assessment of the effective attenuation coefficient of scattering media illuminated by a LED array : Effect of the beam size - In: European Conferences on Biomedical Optics 2015, Allemagne, 2015-06 - Proc. SPIE 9542, Medical Laser Applications and Laser-Tissue Interactions - 2015

Any correspondence concerning this service should be sent to the repository

Administrator : archiveouverte@ensam.eu

Assessment of the effective attenuation coefficient of scattering media illuminated by a LED array : Effect of the beam size

Jean-Yves Le Pommellec^{a*}, Vianney Piron^a, Mohamed-Lamine Askoura^b, Jean-Pierre L'Huillier^a

^aL'UNAM Ecole Nationale Supérieure des Arts et Métiers (ENSAM), Laboratoire Arts et Métiers ParisTech Angers (LAMPA), 2 Boulevard du Ronceray, BP 93525, 49035 Angers cedex 01, France.

^bL'UNAM Université, SFR 4207 QUASAV, Groupe ESA (Ecole Supérieure d'Agriculture), UPSP GRAPPE (Groupe de Recherche Agro-Alimentaire sur le Produit et Procédés), 55 Rue Rabelais-BP 30748, 49007 ANGERS Cedex 01, France.

ABSTRACT

The knowledge of the light fluence rate distribution inside a biological tissue irradiated by a Laser (or LED) is fundamental to achieve medical treatments. In this paper, a semi-infinite tissue model was considered, and the steady-state photon diffusion equation was solved by means of the 2-D Fourier Transform. This method can be applied to any irradiation source (radial symmetry or not) at the surface of the tissue. Two particular beam shapes are studied: planar irradiation and flat beam with finite radius. The total fluence rate along the depth in tissues was computed by adding the collimated and the diffuse components. The analytical solution was also used to study the effect of the beam radius on the light attenuation. Measurements were performed using a tank filled with a liquid-simulating medium (Milk), illuminated with a LED array (660 nm, 100mm×100mm). Several circular diaphragms were used to obtain uniform beams with well defined radii. An optical fibre (with an isotropic tip) was used to measure the fluence rate inside the medium. Preliminary experimental results are in agreement with theoretical predictions.

Key Words : Tissue-optics, Diffusion approximation, 2-D Fourier transform modelling, Effective attenuation coefficient, Beam size

1. INTRODUCTION

Irradiation of biological tissue by laser light has become an increasingly important tool used for both medical investigations and treatments. The therapeutic and diagnostic applications based upon light interaction in these fields depend mainly on how the energy fluence rate is distributed spatially within the tissue target. Clinical examples where the distribution of light inside various tissues plays a key role are typically Photodynamic tumor therapy¹, the photothermal treatments^{2,3}, and also fluorescence diagnostics with transillumination imaging.^{4,5}

Photon migration through highly scattering media such as biological tissues is well described by the radiative transfer equation (RTE)⁶. However the RTE is an integro-differential equation and it is often difficult to derive analytical solutions for solving the main bio-optical problems.

The Monte Carlo method⁷ provides accurate predictions of light transport, but suffers from large computation times and complex coding⁸ in case of heterogeneous tissue structure. For this reason, this stochastic method is predominantly useful for validation studies. Interestingly, under few assumptions (diffusion dominant over absorption, source-detector distances > 10 mm) the RTE can be simplified to a more tractable equation named diffusion equation^{9,10}. A large class of biological tissues, which are illuminated with light sources whose wavelength ranges from ~ 600 nm to ~ 900 nm¹¹, may advantageously be modeled using the diffusion equation. Finite Element Method (FEM) may be used to solve light propagation problem through turbid media¹² from the consideration of the diffusion approximation. However, semi-analytical expressions have been also proposed for cases of cylindrical beam sources.

*jean-yves.lepommelec@ensam.eu: +33 2 41 20 74 23

The Green's function method¹³ provides a solution for a tissue slab irradiated with a beam of finite radius. The determination of the eigen values of the problem involves finding the zeros of the transcendental functions, and then requires numerical implementation. Furthermore, the Hankel transform method^{14,15} gives another solution for a semi-infinite medium illuminated with a Gaussian beam.

The primary objective of this work was to present a general analytical model based on the 2-D Fourier Transform applied to the steady diffusion equation. This model can be used to determine the fluence rate at each point of a semi-infinite tissue model irradiated with any source beam source. Two particular cases are studied: planar irradiation and flat beam with finite radius. The effect of the source radius on the in-depth light attenuation was evaluated. Measurements were performed in a liquid-simulating phantom (Milk).

2. MATHEMATICAL STATEMENT

2-1. Photon diffusion equation

For the purpose of this study, the tissue is considered as a semi-infinite homogeneous medium. The incident radiation is assumed to be collimated and normal to the interface and the positive z direction corresponds to the tissue depth. The total fluence rate $\Phi(x, y, z)$ ($W.mm^{-2}$) at position (x, y, z) of the tissue is divided into collimated $\Phi_c(x, y, z)$ and diffuse components $\Phi_d(x, y, z)$ ^{11,14,15}

$$\Phi(x, y, z) = \Phi_c(x, y, z) + \Phi_d(x, y, z) \quad (1)$$

The collimated component satisfies Beer's law :

$$\Phi_c(x, y, z) = \Phi_c(x, y, 0) \exp[-\mu_t z] \quad (2)$$

Where $\Phi_c(x, y, 0)$ is the collimated photon flux at the point $(x, y, 0)$ of the surface of the medium, $\mu_t = \mu_a + \mu_s$ is the total attenuation coefficient, μ_a (mm^{-1}) is the absorption coefficient and μ_s (mm^{-1}) is the scattering coefficient.

The diffuse component $\Phi_d(x, y, z)$ is the solution of the diffusion equation :

$$\nabla^2 \Phi_d(x, y, z) - \mu_{eff}^2 \Phi_d(x, y, z) = -3\mu_s [\mu_s + g \mu_a] \Phi_c(x, y, 0) \exp(-\mu_t z) \quad (3)$$

where g is anisotropy factor and $\mu_{eff} = \sqrt{3\mu_s (\mu_a + (1-g)\mu_s)}$ is the effective attenuation coefficient.

2-2. Boundary conditions

For a semi-infinite medium under collimated irradiation, the indices of refraction are mismatched and no diffuse intensity enters the medium from outside. The boundary condition at the surface is^{11,15}

$$\Phi_d(x, y, 0) - 2AD \left. \frac{\partial \Phi_d(x, y, z)}{\partial z} \right|_{z=0} = -\frac{2Ag\mu_s}{\mu_a + (1-g)\mu_s} \Phi_c(x, y, 0) \quad (4)$$

where $D = 1/3[\mu_a + (1-g)\mu_s]$ is the diffusion coefficient.

The value of A is linked to the Fresnel coefficient $R_F(\theta)$ and consequently is a function of the refractive index of the scattering medium :

$$A = \frac{1 + 3 \int_0^{\pi/2} \sin \theta \cos \theta^2 R_F(\theta) d\theta}{1 - 2 \int_0^{\pi/2} \sin \theta \cos \theta R_F(\theta) d\theta}$$

For the computations , the value of the refractive index was set at 1.4 thus yielding $A = 2.949^{12}$.

2-3. Fourier transform formulation

The diffuse fluence rate due to a flat beam irradiation (radius r_0) is determined by solving Eq. 3 subject to the boundary condition (4), using the two dimensionnal Fourier transform defined as:

$$F[\Phi_d](k_x, k_y, z) = \iint \Phi_d(x, y, z) \exp[-2i\pi(k_x x + k_y y)] dx dy \quad (5)$$

The diffuse fluence rate can be easily computed if we work in cylindrical rather than Cartesian coordinates using the relations : $r = \sqrt{x^2 + y^2}$ and $\rho = \sqrt{k_x^2 + k_y^2}$.

$$\Phi_d(r, z) = 2\pi \int_0^{+\infty} \rho \left[\alpha(\rho) \exp(-\mu_t^* z) + \beta(\rho) \exp(-\sqrt{4\pi^2 \rho^2 + \mu_{eff}^2} \cdot z) \right] J_0(2\pi \rho r) d\rho \quad (6)$$

where

$$\alpha(\rho) = \frac{3\mu_s [\mu_t + g \mu_a] r_0 J_1(2\pi \rho r_0)}{(4\pi^2 \rho^2 + \mu_{eff}^2 - \mu_t) \rho} \quad (7)$$

$$\beta(\rho) = -\frac{\rho(1 + 2AD\mu_t) \alpha(\rho) + 6ADg\mu_s r_0 J_1(2\pi \rho r_0)}{(1 + 2AD\sqrt{4\pi^2 \rho^2 + \mu_{eff}^2}) \rho} \quad (8)$$

In Eq. (6) , J_0 is the Bessel function of first kind and zero - order, whereas in Eqs (7-8) J_1 is the Bessel function of first kind and one - order.

The Fourier-transform diffusion model was developed on the base of the software " Mathcad", and implemented on a personal computer.

In the case of $r_0 \rightarrow \infty$, the total fluence rate ($\Phi_c + \Phi_d$) is identical to that provided by Deulin and L'Huillier¹⁶ for the 1-D configuration (Planar irradiation). For a large penetration depth $\Phi(z) \sim \exp(-\mu_{eff} z)$. Consequently, μ_{eff} can be accurately assessed from measurement of the fluence rate inside tissues irradiated with a wide-plane collimated beam as reported by Choukeife and L'Huillier¹⁶

2-4. Fluence rate distribution measurement

The fluence rate distribution inside the tissue can be determined by displacing (step by step), along the beam axis, an isotropic-end optical fibre. For this probe, it has been shown (Star et al¹⁹) that the detected signal is proportional to the fluence rate in the medium.

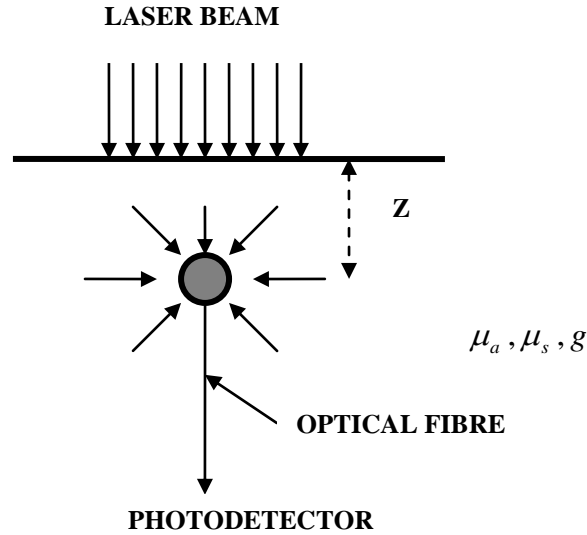


Figure 1: Measurement with an isotropic-end optical fibre

3 TYPICAL RESULTS

3-1. Theoretical results

Theoretical results are given for a tissue illuminated by a flat beam irradiation. The flux density collected by an isotropic optical fibre was calculated from equations (1), (2) and (6). In Figure 2, the logarithm of the normalized fluence rate : $\ln(\Phi(r=0, z)/\Phi(r=0, z=0))$ is plotted against depth for a semi-infinite tissue sample, irradiated with a collimated laser beam, with $\mu_a = 0.01 \text{ mm}^{-1}$, $\mu_s' = 1 \text{ mm}^{-1}$ and $g = 0.8$. The in-depth variations of the fluence rate is shown for a flat beam having three different radii : (5 mm, 10 mm and 20 mm). Close to the surface, the flux density increases by a factor depending on the field size. For large depths, the flux decreases as $\exp(-\alpha z)$ where α is the attenuation coefficient along the beam axis.

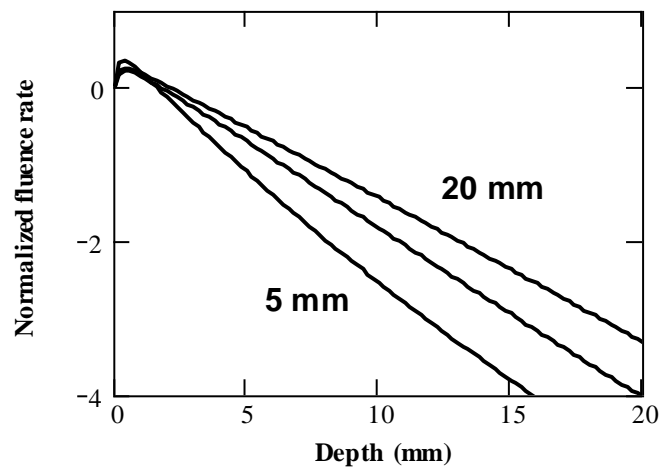


Figure 2 : Plots of the normalized fluence rate as a function of the depth inside the tissue

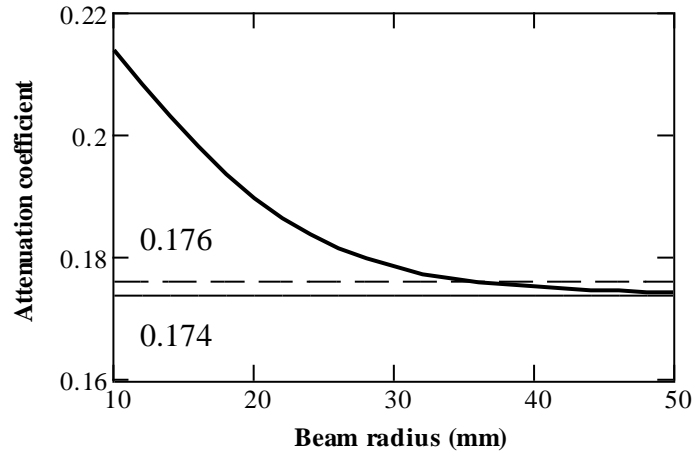


Figure 3 : Plots of the attenuation coefficient as a function of the beam radius

The effect of the incident beam size on the light attenuation along the beam axis is depicted in Figure 3. As shown, α decreases as the beam radius increases. Once the beam size reaches a large value (45 mm), this coefficient reaches the minimum value $\mu_{eff} = 0.174 \text{ mm}^{-1}$ corresponding to the 1-D solution.¹⁶ For a beam radius $r_0 = 35 \text{ mm}$ the attenuation is $\alpha = 0.176 \text{ mm}^{-1}$. The relative difference (%) between this value and the attenuation coefficient ($\mu_{eff} = 0.174 \text{ mm}^{-1}$) is equal to 1.2%. Consequently, the error on the μ_{eff} value is equal to 1.2% if the beam radius is $r_0 = 35 \text{ mm}$. Clearly, as this limit radius (called critical radius) is reached, the penetration of the beam is maximum.

3-2. Experimental results

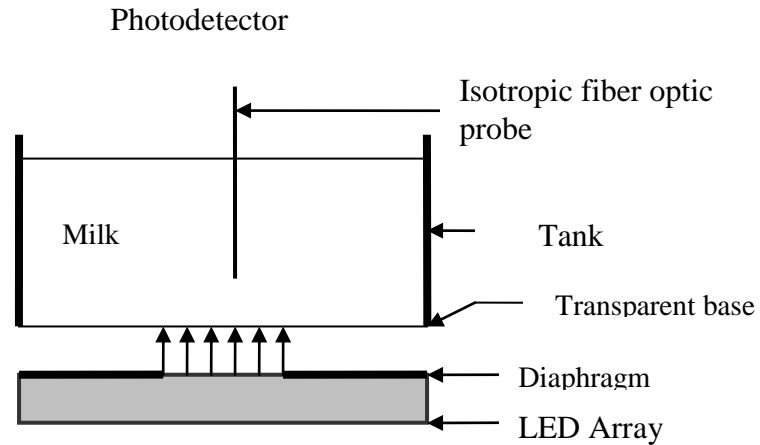


Figure 4 Experimental set up

Experiments were conducted to check the validity of the theoretical predictions. The measurements of the attenuation of the fluence rate in a scattering and absorbing medium as a function of depth are performed with the set up shown in Figure 4. A LED array (660 nm, 100mm×100 mm, 1.5 mW/mm²) is used to illuminate the transparent base of a tank filled with a tissue simulating "phantom" (Milk – UHT). Several circular diaphragms were used to obtain uniform circular beams with radii varying from 10 mm to 50 mm. The fluence rate was measured with an

isotropic light dosimetry probe (Optical fiber with an isotropic tip) connected to a photodiode and displaced by steps along the axis from the irradiation surface downward into the medium.

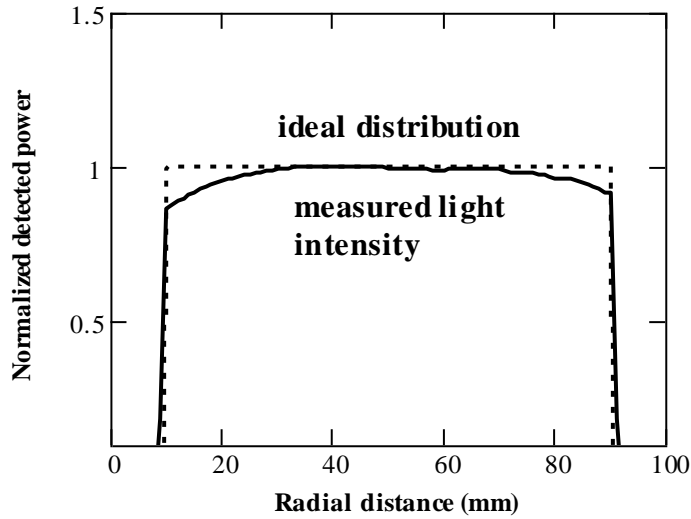


Fig 5 Light intensity distribution measured along the radius of a circular diaphragm

Figure 5 shows the light intensity distribution measured along the radius of a typical circular diaphragm ($r_0 = 40$ mm). As illustrated in this figure, the intensity generated appears as uniformly distributed over a large area except for radial distances close to the beam edge.

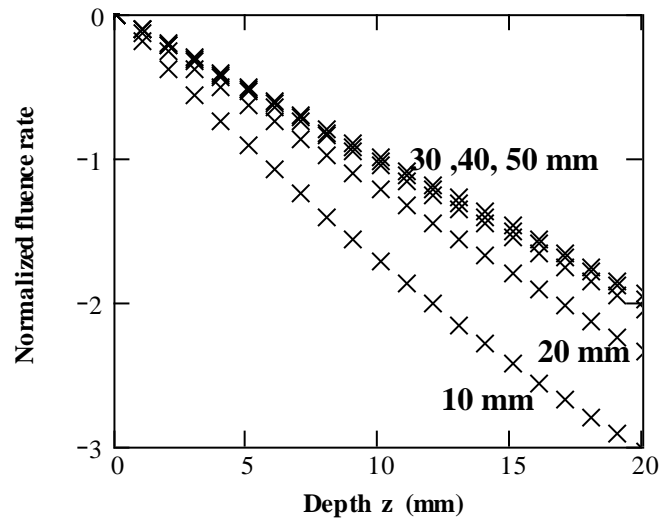


Figure 6 Experimental depth behaviour of the normalized fluence rate

The fluence rate was measured with an isotropic-end optical fibre displaced along the axis of the system. The logarithm of the normalized fluence rate is plotted (Figure 6) as a function of the distance between the fiber tip and the transparent base of the tank, for five circular diaphragms ($r_0 = 10, 20, 30, 40, 50$ mm). According to theoretical predictions, it appears that the logarithm of the fluence rate evolves linearly with respect to the depth z . Otherwise, it is still shown that the attenuation coefficient (defined as the slope of the curve) decreases as the radius increases and then tends to a minimum value for large beam size. For a broad incident beam (40 mm) the attenuation coefficient 0.098 mm^{-1} is close to the true effective attenuation coefficient 0.096 mm^{-1} .

4 CONCLUSION

In this paper, a semi-analytical model based on the two-dimensional Fourier Transform of the steady-state diffusion equation has been described. This model was used to compute the total Fluence rate in case of a semi-infinite tissue model illuminated with a uniform laser of finite radius or with a planar source. This approach is as versatile as the other techniques (Green's Function method or Hankel transform method), but has the advantage of being much faster. The simulations show that the effective attenuation coefficient of the studied tissue can be well assessed when a sufficient source radius is reached. Preliminary experiments allow us to calibrate theoretical specifications. Further investigations are now required to optimize such a procedure in cases of varied tissue-optical parameter sets.

REFERENCES

- [1] Wilson BC, Patterson MS. The physics, biophysics and technology of photodynamic therapy. *Phys Med Biol* 2008 ; 53: R61-R10
- [2]. Welch AJ, van Gemert MJC. *The Optical and Thermal Responses of Laser-Irradiated Tissue*. Plenum Press New York 1995
- [3]. L'Huillier JP. Theoretical analysis of the role played by tissue-optical parameters in the laser ablation process. *Proc SPIE* 1997; 3195: 151-165
- [4]. Leblond F., Davis SC. , Valdès PA., Pogue BW. Pre-clinical whole-body Fluorescence imaging : Review of instruments, methods and applications. *J.Photochem. Photobiol.B : Biology* 2010, 98, 77-94.
- [5]. L'Huillier JP., Vaudelle F. Improved localization of hidden fluorescent in highly scattering slab media based on a two-way transmittance determination. *Opt.Express*. 2006, 14(26), 12915-12929.
- [6]. Chandrasekhar S. *Radiative transfer*. Oxford UP New York 1960
- [7]. Wang L , Jacques S.L, Zheng L. Monte Carlo modelling of light transport in multi-layered tissues. *Computer methods and programs in Biomedecine* 1997; 47 : 131-146
- [8]. Mansouri C, L'Huillier JP, Kashou NH, Humeau A. Depth sensitivity analysis of functional near-infrared spectroscopy measurement using three-dimensional Monte Carlo modelling based magnetic resonance imaging. *Lasers in Med Sci* 2010 25:431-438.
- [9]. A Ishimaru. *Wave Propagation and scattering in Random Media*. Academic New York, 1978
- [10]. Prahl S.A. *Light transport in tissue*, Phd Thesis, University of Texas at Austin, 1988.
- [11]. Boulnois JL. Photophysical processes in recent medical laser developments : a review. *Lasers in Med Sci* 1986; 1 : 47-66.
- [12]. Deulin X, L'Huillier JP. Finite element approach to photon propagation modelling in semi-infinite homogeneous and multilayered tissue structures. *EPJ Appl Phys* 2006; 33 :133-146
- [13]. Reynolds L, Johnson C. Diffuse reflectance from a finite blood medium : applications to the modelling of the fiber optics catheters. *Applied Optics* 1976; 15 :2059-2067
- [14]. Grossweiner L.I., Karagiannes J.L, Johnson P.W, Zhang Z.Y, Gaussian-beam spread in biological tissues. *Applied Optics* 1990; 29 : 379-383
- [15]. Carp SA, Prahl SA, Venugopalan V. Radiative transport in the delta P1 approximation : accuracy of fluence rate and optical penetration depth predictions in turbid semi-infinite media. *J Biomed Opt* 2004; 9: 632-647

- [16]. Star W.M, Marijnissen PA. Calculating the response of isotropic light dosimetry probes as a function of the tissue refractive index. *Applied Optics* 1989; 28 : 2288-2291.
- [17]. Choukeife. JE., L'Huillier JP. Measurements of scattering effects within tissue-like media at two wavelengths of 632.8 nm and 680 nm. *Lasers Med Sci* 1999, 14:286-296.