



HAL
open science

Microwave Sensor within a Microfluidic Chip for Biological Applications

Abdelhatif El Fellahi, Thierry Bore, Lionel Rousseau, Bruno Le Pioufle,
Olivier Français

► **To cite this version:**

Abdelhatif El Fellahi, Thierry Bore, Lionel Rousseau, Bruno Le Pioufle, Olivier Français. Microwave Sensor within a Microfluidic Chip for Biological Applications. Eurosensors 2017, Sep 2017, Paris, France. pp.1-4, 10.3390/proceedings1040523 . hal-01592115

HAL Id: hal-01592115

<https://hal.science/hal-01592115>

Submitted on 31 Aug 2023

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Distributed under a Creative Commons Attribution 4.0 International License

Proceedings

Microwave Sensor within a Microfluidic Chip for Biological Applications †

Abdellatif El Fellahi ¹, Thierry Bore ^{1,2}, Lionel Rousseau ³, Bruno Le Pioufle ¹
and Olivier Français ^{3,*}

¹ SATIE, UMR CNRS 8029, ENS Cachan, University of Paris-Saclay, Cachan, France; abdelhatif.elfellahi@gmail.com (A.E.F.); bore.thierry@gmail.com (T.B.); bruno.lepioufle@satie.ens-cachan.fr (B.L.P.)

² School of Civil Engineering, University of Queensland, St Lucia, Australia

³ ESYCOM EA2552, Université Paris-Est, Paris, France; lionel.rousseau@esiee.fr

* Correspondence: olivier.francais@esiee.fr; Tel.: +33-145-926-694

† Presented at the Eurosensors 2017 Conference, Paris, France, 3–6 September 2017.

Published: 11 August 2017

Abstract: A miniaturized sensor operating in Radio Frequency region (RF) is proposed to address the need in picoliter liquid characterization. The sensor is based on a coplanar waveguide (CPW) combined with a microfluidic channel dedicated to microliter liquid characterization with perspectives for biology and single cell characterization. Using microtechnology process, the sensor has been designed on a 0.5 mm thick quartz wafer with Cr/Au electrodes. A prototype of the sensor has been fabricated and evaluated with ethanol/water mixtures at different molar fractions of ethanol. A good agreement between theoretical and measured electrical response of the sensor is observed.

Keywords: RF characterization; RF sensors; liquids; picoliter volumes; microfluidic; broadband; dielectric characterization

1. Introduction

Electromagnetic techniques have become popular in biomedical applications as they allow rapid, non-invasive and easily automated characterization. For these reasons, in the last decade intensive works have been devoted to develop RF and microwave sensors [1–6]. They are compatible with biological environments and allow characterizing very small volumes. Classically, the open-ended coaxial probe approach is most commonly used for complex permittivity [7]. However, this method requires relatively large sample volumes (few mL) and is not suitable to RF characterization at single cell scale. As an alternative, coplanar waveguide (CPW) sensors have been proposed [8–10], however the volumes involved are still too high. Here, a miniaturized sensor based a coplanar Ground-Signal-Ground waveguide and SU-8 microfluidic network dedicated to characterize picoliter volumes is proposed. The set up description is given in Section 2. Experimental results and a validation with water/ethanol mixtures are presented in section III.

2. Set-Up Description

The miniaturized sensor is a coplanar Ground-Signal-Ground waveguide as shown in Figure 1 which behaves like a miniaturized open-ended-probe. The tapered coplanar line topology (gold lines deposited onto quartz substrate) is designed up to 10 GHz to achieve a 20 μm -width signal line associated with a 2.5 μm -gap. Electromagnetic simulations based on (Ansys/HFSS[®]) demonstrate insertion losses less than 2 dB up to 10 GHz. The interaction between the electric field and the liquid under test is achieved thanks to an SU-8 microfluidic channel placed on top of the sensor. The cross-

section of the microfluidic channel is $50\ \mu\text{m}$ per $50\ \mu\text{m}$ and $50\ \mu\text{m}$ high (Figure 1). The volume of sample that can be analyzed is equal to 125 picoliters.

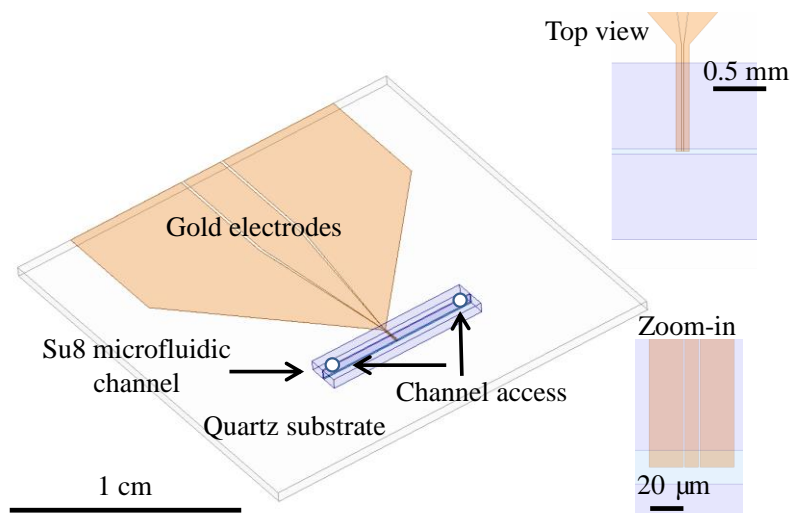


Figure 1. Schematic representation of the microwave/microfluidic sensor (HFSS picture), using gold electrodes in GSG (ground-Signal-Ground) configuration and SU8 microfluidic channel. The inset is a zoom-in.

An Anritsu Wiltron test fixture is used to connect the sensor to a Vector Network Analyzer and achieve reflection coefficient (S_{11}) measurement in the frequency range from 30 MHz to 3 GHz. The Figure 2 shows the photography of the test bench using a VNA (E5061B) with the miniaturized sensor.

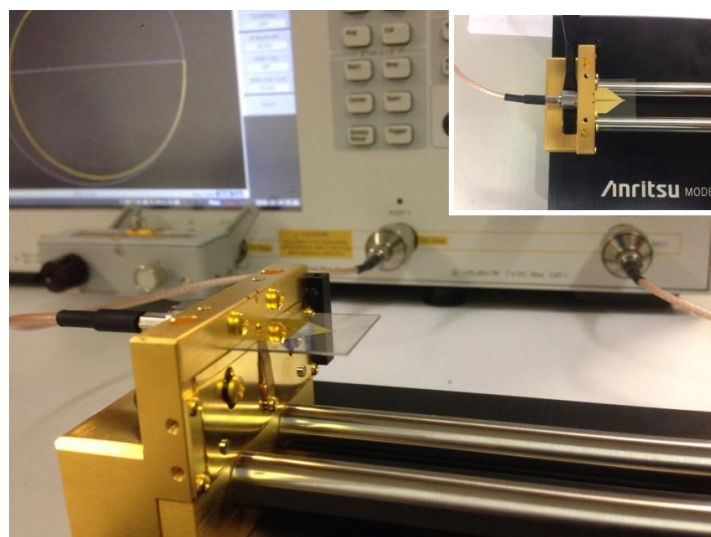


Figure 2. Photography of the test bench. The inset shows the top view.

3. RF Measurements

The fabrication of the miniaturized sensor is based on standard microtechnological processes. The device is fabricated using a $500\ \mu\text{m}$ -thick quartz wafer. The structure is a coplanar line technology and consists of three gold metal lines deposited on the substrate. The full chip dimensions are: width (w) = 15 mm and length = 20 mm. Finally, the SU-8 microfluidic channel is deposited at the end of the coplanar guide (Figure 1).

To characterize the device, we investigate water/ethanol mixtures. The solutions were prepared by Ethanol (CARLO ERBA) and Millipore water. We measured ethanol/water mixtures at the molar fractions of ethanol, $X_{EA} = 0.07, 0.17, 0.3, 0.7$ and 1 at $20\text{ }^{\circ}\text{C}$ in the frequency range 30 MHz to 3 GHz . These mixtures allow having solutions with a complex permittivity between 20 and 80 [12–16].

All measurements were obtained at room temperature from 30 MHz to 3 GHz (Figure 3). Each solution is measured using the average of 50 runs and input source is set to 0 dBm . The temperature of the liquids was also checked. As predicted, the difference in liquid properties can be clearly distinguished.

The analyte (volume = 125 pL) is placed in a SU-8 microfluidic channel. Figure 4 summarizes the reflection coefficient S_{11} measured for the different mixture at 1 GHz . We can note, that the module of reflection coefficient increased with the decreasing ethanol content. Thus, the imaginary part of S_{11} , decreased with the increasing ethanol concentration. Results demonstrate that the miniaturized sensor characterizes accurately picoliter volumes with high sensitivity to the complex permittivity evolution.

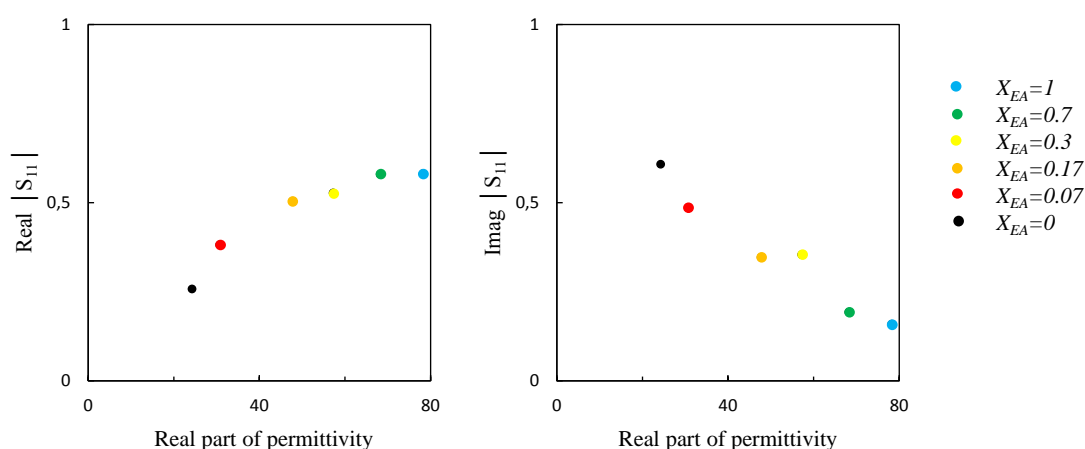


Figure 3. Experimental $|S_{11}|$ parameters of the sensor recorded at 1 GHz for ethanol/water mixtures retrieved at $20\text{ }^{\circ}\text{C}$ and mole fractions X_{EA} of ethanol.

4. Conclusions

In order to address the increasing need in characterization of picoliter liquids and biological cells, a miniaturized coplanar waveguide (CPW) sensor based on the interaction of a picoliter-range solution with the electromagnetic waves at gigahertz frequencies is developed. This sensor is designed using Electromagnetic simulations based on (Ansys/HFSS®). Experimental characterization of the device was carried out, highlighting its high sensitivity. The evolution of the real part and the imaginary part of the reflection coefficient S_{11} as a function of permittivity of different ethanol/water mixtures prove that the sensor is highly sensitive. These preliminary results show that the proposed instrumentation is a noninvasive solution to characterize picoliter volumes in a broadband range ($0.03\text{--}3\text{ GHz}$).

Acknowledgments: The authors acknowledge the Labex LaSIPS (ANR-10-LABX-0040-Lasips), the “Institut d’Alember”, the ESIEE-Paris Clean Room and the “CNRS” for project fundings.

Conflicts of Interest: The authors declare no conflict of interest.

References

1. Prodan, C. and Prodan, E. The dielectric behavior of living cell suspensions. *Phys. D Appl. Phys.* **1999**, *32*, 335–343.

2. Mateu, J.; Orloff, N.; Rinehart, M. and Booth, J. C. Broadband Permittivity of Liquids Extracted from Transmission Line Measurements of Microfluidic Channels. In Proceedings of the 2007 IEEE MTT-S International Microwave Symposium Digest, Honolulu, HI, USA, 3–8 June 2007; pp. 523–526.
3. Gabriel, S.; Lau, R. W. and Gabriel, C. The dielectric properties of biological tissues: Measurements in the frequency range 10 Hz to 20 GHz. *Phys. Med. Biol.* **1996**, *41*, 2251–2269.
4. Stuchly, M.A.; Kraszewski, A.; Stuchly, S. S. and Smith, A. M. Dielectric properties of animal tissues in vivo at radio and microwave frequencies: Comparison between species. *Phys. Med. Biol.* **1982**, *27*, 927–936.
5. Khan, U.; Al-Moayed, N.; Nguyen, N.; Obol, M.; Korolev, K.; Afsar, M. and Naber, S. High frequency dielectric characteristics of tumorous and non-tumorous breast tissues. In Proceedings of the 2007 IEEE MTT-S International Microwave Symposium Digest, Honolulu, HI, USA, 3–8 June 2007; pp. 1341–1344.
6. Seo, S.; Stintzing, T.; Block, I.; Pavlidis, D.; Rieke, M. and Layer, P. G. High frequency wideband permittivity measurements of biological substances using coplanar waveguides and application to cell suspensions. In Proceedings of the 2008 IEEE MTT-S International Microwave Symposium Digest, Atlanta, Georgia, 15–20 June 2008; pp. 915–918.
7. El Fellahi, A.; Bore, T.; Bensalem, S.; Bodenes, P.; Lopes, F.; Martincic, E.; Le Pioufle, B. and Francais, O. Monitoring of Microalgae Lipid Accumulation using RF Open Ended Biosensor. *IEEE Sens. Lett.* **2017**, *1*, 4500303.
8. Stuchly, S.S. and Bassey, C. E. Microwave coplanar sensors for dielectric measurements. *Meas. Sci. Technol.* **1998**, *9*, 1324–1329.
9. Seo, S.; Stintzing, T.; Block, I.; Pavlidis, D.; Rieke, M. and Layer, P. G. High frequency wideband permittivity measurements of biological substances using coplanar waveguides and application to cell suspensions. In Proceedings of the 2008 IEEE MTT-S International Microwave Symposium Digest, Atlanta, GA, USA, 15–20 June 2008; pp. 915–918.
10. Grenier, K.; Dubuc, D.; Poleni, P. E.; Kumemura, M.; Toshiyoshi, H.; Fujii, T. and Fujita, H. New broadband and contact less RF/microfluidic sensor dedicated to bioengineering. In Proceedings of the 2008 IEEE MTT-S International Microwave Symposium Digest, Boston, MA, USA, 7–12 June 2009.
11. Chen, T.; Dubuc, D.; Poupot, M.; Fournie, J.J. and Grenier, K., Accurate Nanoliter Liquid Characterization Up to 40 GHz for Biomedical Applications: Toward Noninvasive Living Cells Monitoring. *IEEE Trans. Microw. Theory Tech.* **2012**, *60*, 4171–4177.
12. Wagner, N.; Schwing, M. and Scheuermann, A. Numerical 3D FEM and experimental analysis of the open-ended coaxial line technique for microwave dielectric spectroscopy on soil. *IEEE Trans. Geosci. Remote Sens.* **2013**, *52*, 880–893.
13. Bore, T.; Yermán, L.; Serna, M.L.; Wall, H.; Torero, J.L. and Scheuerman, A. Dielectric spectroscopy of artificial faeces for smouldering applications. In Proceedings of the 2016 IEEE Sensors Applications Symposium (SAS), Catania, Italy, 20–22 April 2016; pp. 1–6.
14. Bore, T.; Wagner, N.; Cai, C. and Scheuermann, A. *Meas. Sci. Technol.* **2016**, *28*, 014016.
15. Petong, P.; Pottel, R. and Kaatze, U. Water-Ethanol Mixtures at Different Compositions and Temperatures. A Dielectric Relaxation Study. *J. Phys. Chem. A* **2000**, *104*, 7420–7428.
16. Sato, T. and Buchner, R. Dielectric Relaxation Processes in Ethanol/Water Mixtures. *J. Phys. Chem. A* **2004**, *108*, 5007–5015.

