



## Lower-limb lengths and angles in children older than six years: Reliability and reference values by EOS® stereoradiography

Virginie Rampal, Pierre-Yves Rohan, Ayman Assi, Ismat Ghanem, O. Rosello, A.-L. Simon, E. Gaumetou, V. Merzoug, Wafa Skalli, P. Wicart

### ► To cite this version:

Virginie Rampal, Pierre-Yves Rohan, Ayman Assi, Ismat Ghanem, O. Rosello, et al.. Lower-limb lengths and angles in children older than six years: Reliability and reference values by EOS® stereoradiography. *Orthopaedics & Traumatology: Surgery & Research*, 2018, 104 (3), pp.389-395. 10.1016/j.otsr.2017.10.007 . hal-02284306

**HAL Id: hal-02284306**

**<https://hal.science/hal-02284306>**

Submitted on 11 Sep 2019

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

**Original article****Lower-Limb Lengths and Angles in Children Older than Six Years: Reliability and Reference Values by EOS<sup>®</sup> Stereoradiography**

V. Rampal <sup>1,2</sup>, P.-Y. Rohan <sup>1</sup>, A. Assi <sup>3</sup>, I. Ghanem <sup>3</sup>, O. Rosello <sup>2</sup>, A.-L. Simon <sup>4</sup>, E. Gaumetou <sup>4</sup>, V. Merzoug <sup>5</sup>, W. Skalli <sup>1</sup>, P. Wicart <sup>6</sup>

<sup>1</sup>Institut de Biomécanique Humaine Georges Charpak, Arts et Métiers ParisTech, 151 boulevard de l'Hôpital, 75013 Paris, FRANCE

<sup>2</sup>Service d'orthopédie pédiatrique, Hôpitaux Pédiatriques de Nice CHU Lenval, 57 avenue de la Californie, 06000 Nice, FRANCE

<sup>3</sup>Laboratoire de biomécanique, Faculté de Médecine, Université de Saint Joseph, Beyrouth, LEBANON

<sup>4</sup>Service d'orthopédie pédiatrique, Hôpital Robert Debré, 48 Boulevard Serurier, 75019 Paris, FRANCE

<sup>5</sup>Service de radiologie, Hôpital Cochin et Hôpital Bicêtre, 27 rue du Faubourg Saint Jacques, 75014 Paris and 78 Rue du Général Leclerc, 94270 Le Kremlin-Bicêtre, FRANCE

<sup>6</sup>Service d'orthopédie pédiatrique, Hôpital Necker enfants Malades, 149 rue de Sèvres, 75015 Paris, FRANCE

**Corresponding author:** Virginie Rampal

rocher-rampal.v@pediatrie-chulenvall-nice.fr

Accepted Manuscript

## ABSTRACT

**Background:** Lower-limb alignment in children is classically assessed clinically or based on conventional radiography, which is associated with projection bias. Low-dose biplanar radiography was described recently as an alternative to conventional imaging. The primary objective of this study was to assess the reliability of length and angle values inferred from 3D reconstructions in children seen in everyday practice. The secondary objective was to obtain reference values for goniometry parameters in children.

**Hypothesis:** 3D reconstructions can be used to assess the lower limbs in children.

**Material and methods:** The paediatric reliability study was done in 18 volunteers who were divided into three groups based on whether they were typically developing (TD) children, had skeletal development abnormalities, or had cerebral palsy. The reference data were obtained in 129 TD children. Each study participant underwent biplanar radiography with 3D reconstruction performed by experts and radiology technicians. Goniometry parameters were computed automatically. Reproducibility was assessed based on the intra-class coefficient (ICC) and the ISO 5725 standard (standard deviation of reproducibility,  $SD_R$ ).

**Results:** For length parameters, the ICCs ranged from 0.94 to 1.00 and the  $SD_R$  from 2.1 to 3.5 mm. For angle parameters, the ICC and  $SD_R$  ranges were 0.60-0.95 and  $0.9^\circ$ - $4.6^\circ$ , respectively. No significant differences were found across experts or radiology technicians. Age-specific reference data are reported.

**Discussion:** These findings confirm the reliability of low-dose biplanar radiography for assessing lower-limb parameters in children seen in clinical practice. In addition, the study provides reference data for commonly measured parameters.

**Level of evidence:** IV

**Key Words:** Lower limb. Low-dose biplanar X-ray imaging. Paediatrics.

Accepted Manuscript

## 1. INTRODUCTION

Assessing lower-limb alignment is crucial in children to detect developmental abnormalities and to provide treatment guidance. However, few studies based on accurate measurement methods have provided data on normal paediatric values. Coronal lower-limb alignment in children is classically evaluated using semi-quantitative clinical [1] and radiological [2] methods. Radiography is associated with projection bias [2] but is nevertheless more accurate than clinical methods [3-6]. Salenius *et al.* [2] reported substantial uncertainty with tibio-femoral angle (TFA) values measured on conventional radiographs, particularly in children with combined axial abnormalities.

A reconstruction method based on low-dose biplanar calibrated images and a 3D model was validated recently as a tool for evaluating the radiological parameters of numerous anatomical structures [7-11]. This imaging and 3D reconstruction technique emerged as a promising alternative to the above-mentioned conventional procedures [12,13]. Gaumetou *et al.* established its reliability for evaluating segmental torsion of the lower limbs in children and adults [12].

Until now, studies of lower-limb parameters measured on low-dose biplanar radiographs focussed chiefly on differences between 2D and 3D values [14] or on comparing torsion measurements with those obtained by computed tomography [15]. Furthermore, most studies of reliability were conducted by research groups. Thus, whether low-dose biplanar radiography is reliable when performed in everyday practice by radiology technicians trained in conventional techniques has not been proven. Finally, according to a systematic literature review, available

studies focussed chiefly on the technical usefulness of the method, and clinical studies need to be performed [16].

The primary objective of this study was to assess the reliability of length and angle values inferred from 3D reconstructions in children seen in everyday practice. The secondary objective was to obtain reference values for goniometry parameters in children. The working hypothesis was that 3D reconstructions can be used to assess the lower limbs in children.

## **2. PATIENTS AND METHODS**

### **(2.1) Study participants**

This study was approved by the appropriate ethics committees (CPP 06001 for Arts et Métiers ParisTech and 2013-A01568-37, N°76 09 2013 for the Nice paediatric hospitals CHU-Lenval). Informed consent was obtained from the patients and parents before study inclusion.

In all, 141 participants were included. Among them, 18 were volunteers aged 6 to 15 years who were recruited at the outpatient clinic for the reliability study. Of these 18 participants, 6 were typically developing (TD) children in whom radiographs were prescribed for non-orthopaedic medical reasons, 6 were non-TD (NTD) children with minor orthopaedic abnormalities that did not affect the study parameters, and 6 had cerebral palsy (CP). All 18 children were able to stand without help.

The collection of reference data was done in 129 TD children aged 6 to 15 years (including the 6 in the reliability study). Recruitment was during a paediatric orthopaedics visit, which allowed the exclusion of patients with axial, rotational, and/or length abnormalities. Both

lower limbs of each participant were included, for a total of 258 lower limbs. The 129 participants were divided into four age groups as shown in Table 1 [12].

## **(2.2) Methods**

Each participant underwent low-dose biplanar radiography using the EOS<sup>®</sup> system (EOS<sup>®</sup> Imaging, Paris, France), at one of two study sites (Arts et Métiers-ParisTech in Paris, n=82; and CHU-Lenval in Nice, n=59). The participant was standing in the shifted feet position [10]. Using biplanar images acquired within a calibrated environment and STEREOS software version 1.6.4.7977 [10, 12], the operator identified anatomical landmarks on the antero-posterior and lateral views, to obtain geometric parameters describing the lower limb. Based on these geometric parameters, the software automatically generated a pre-personalised 3D reconstruction, which was then back-projected onto the coronal and sagittal radiographs. The operator adjusted the contours of the 3D model to match the radiographic views. Based on the geometric parameters and specific points on the 3D model, the software automatically computed 3D angles and distances. For this study, the 3D angles were projected onto the coronal and sagittal planes to allow comparisons of 2D measurements with those reported previously. The following radiographic parameters were computed automatically: femoral mechanical angle (FMA), tibial mechanical angle (TMA), hip-knee-shaft angle (HKS), femoro-tibial angle (FTA), femoral head diameter (FHD), femoral neck length (FNL), and neck-shaft angle (NSA). The ratio of femoral over tibial length (F/T) was computed.

## **(2.3) Analysis method**



For the reliability study, reconstructions of each lower limb were obtained twice, in each of three independent paediatric orthopaedics centres. One reconstruction was done by an expert (orthopaedic surgeon with an in-depth understanding of the method) and by a radiology technician trained in the reconstruction technique and everyday use of the software. Thus, for each lower limb of each of the 18 participants, 6 reconstructions were obtained.

#### **(2.4) Statistical analysis**

The intra-class coefficient (ICC) and standard deviation of reproducibility ( $SD_R$ ) were computed. For the  $SD_R$ , the ISO 5725 standard was used [17]. Reliability was then assessed based on a 95% confidence interval (95%CI) of  $2 \cdot SD_R$ . Finally, the values obtained by experts and technicians were compared.

The mean and standard deviation (SD) of each parameter were computed for the 129 participants in the reference data study and for the 6 NTD patients and 6 CP patients. Distribution normality was assessed using the Kolmogorov-Smirnov test. For each parameter, the mean and SD served to define normal channels ( $\text{mean} \pm 1 \text{ SD}$ ), high and low subnormal channels (between  $\text{mean} \pm 1 \text{ SD}$  and  $\text{mean} \pm 2 \text{ SD}$ ), and high and low abnormal channels ( $>$  or  $<$   $\text{mean} \pm 2 \text{ SD}$ ). Differences across age groups and between experts and technicians were evaluated using Student's *t* test (Statistica<sup>®</sup> software, Francisco Partners, San Francisco, CA, USA), with *p* values  $< 0.05$  considered significant.

### **3. RESULTS**

#### **Reliability (Table 2)**

For length parameters, the ICC values ranged from 0.94 to 1.00 and the  $SD_R$  values from 2.1 to 3.5 mm. The corresponding values for angle parameters were 0.60-0.95 and  $0.9^\circ$ - $4.6^\circ$ . No significant differences were found between experts and technicians for these parameters ( $p>0.5$ ).

### **Reference data for lower-limb 3D radiological parameters**

The values of all parameters were normally distributed. Table 1 reports the means and SDs of each parameter in each age group and Figures 1 to 4 the changes according to age. F/T was the most stable parameter, with a mean of  $1.1\pm0.03$  in all age groups. FNL was the parameter showing the greatest age-related changes, with a range of  $131^\circ\pm5^\circ$  to  $136^\circ\pm7^\circ$  across age groups.

Tables 3 and 4 report the normal, high and low subnormal, and abnormal values for each parameter. Data from the NTD and CP groups are shown in Table 5 and Figures 1 to 4.

## **4. DISCUSSION**

To our knowledge, this is the first study establishing the reliability of lower-limb 3D reconstruction in children seen in everyday clinical practice. In addition, except for a study focussed on rotational parameters [12], no other studies have provided reference values for lengths and angles determined in children using 3D images.

The main limitation of this study is that the design was cross-sectional and not longitudinal. Females predominated, particularly in the 6- and 7-year-olds (Table 1). However, in this youngest age group, overall morphology shows no marked differences between girls and boys. On the other hand, the sex ratio imbalance precluded a reliable comparison of parameter

values between females and males. For this study, we elected to consider only chronological age, as no difference with bone age was to be expected in our population of healthy children. Obtaining radiographs for bone age determination in the absence of a clinical indication would have been ethically debatable. Finally, the lower age limit of 6 years reflects a limitation of the EOS<sup>®</sup> system: the patient must stand immobile for about 10 s, which is difficult for children younger than 6 years.

The primary objective of this study was to assess the reliability of angle and length parameter values derived from 3D reconstructions in children seen in everyday practice. To this end, we determined both the ICC and the SD<sub>R</sub> values. The ICC provides an overall estimate of the correlation between measurements by different observers but does not quantitatively evaluate the degree of uncertainty. Bland and Altman pointed out that correlations linking data values were not the most relevant assessment because, in clinical practice, quantitative values and information about uncertainty are required to establish a diagnosis (relative to normal channels) and for monitoring a patient over time [19]. The ISO 5725-2 standard describes “the basic method for the determination of repeatability and reproducibility of a standard measurement method” [17]. Consequently, in addition to ICC values, we computed SD<sub>R</sub> values. Inter-observer reproducibility and 95% CIs of length parameters, although slightly less favourable than in research studies [10,11,18], are sufficient for clinical purposes. Reproducibility for angle parameters is comparable to previous data [10, 11, 18] (Table 2). Finally, compared to manual or automated measurements on conventional radiographs, reproducibility is better in our study [20].

The secondary objective of this study was to obtain reference values for lower-limb radiological parameters in healthy children. The availability of reference values is crucial to the

optimal management of lower-limb abnormalities. To the best of our knowledge, no reference data for lower-limb length parameters, the NSA, or the HKS angle in children have been reported. Thus, our study provides original data.

### **Length parameters**

FHD and FNL increased, as expected, throughout growth, and their values in the oldest age group (13 to 15 years) were similar to those reported in adults [21]. F/T remained stable throughout growth, with very little variability (SD,  $\pm 0.03$ ). The F/T value is closely similar to that reported by Than *et al.* [21] in adults (1.2). This finding is of special interest, since evaluating the ratio of femoral and tibial lengths, for instance when planning limb lengthening, is of the utmost importance. In addition, in constitutional bone disorders, metaphyseal and epiphyseal abnormalities negatively affect bone growth, and reference to a normal F/T ratio is useful for correcting the abnormalities.

### **Angle parameters**

The FMA and TMA values in our study are slightly higher than those reported by Sabarwal *et al.* (87°-88° and 88°-90°, respectively). This difference is probably ascribable to the use in our study of 3D measurements, which eliminates problems related to measurements on a 2D projection of a 3D object when standard radiographs are used [22]. The decrease in valgus angulation after 7 years of age is consistent with reported data [2,3,22,23].

### **Patients in the NTD and CP groups**

Although evaluating abnormal lower limbs was not our objective, our study shows that the parameters whose values remained unchanged across age groups in the TD children (FMA, TMA, FTA, NSA, and F/T) were also unchanged in our NTD and CP children able to walk unassisted.

In conclusion, to our knowledge this is the first study focussing the key issue of the objective evaluation in everyday practice of coronal lower-limb alignment based on 3D reconstructions from low-dose biplanar X-ray images. The results confirm that the EOS<sup>®</sup> system can be used in everyday practice to assess the lower limbs of children, including those with orthopaedic deformities or cerebral palsy. The absence of statistically significant differences between values obtained by experienced orthopaedic surgeons and radiology technicians established that properly trained radiology techniques can perform the reconstructions.

In addition, the reference data provided here are parts of a continual effort to assist physicians in assessing lower-limb alignment, with the goal of improving patient monitoring or planning treatment strategies.

**Acknowledgements**

We thank the radiology technicians Pascal CARON, Edith VETTER, Valerie BERNASCONI, and Delphine CELEA for their assistance with the reconstructions.

**Disclosure of interest:** None of the authors has any conflicts of interest to disclose.

## References

1. Jacquemier M, Jouve JL, Jimeno MT, et al. Lower limb morphotypes. A clinical study in 1401 children. *Rev Chir Orthop* 1997;83:531-9.
2. Salenius P, Vankka E . The development of the tibiofemoral angle in children. *J Bone Joint Surg* 1975;57-A:259-61.
3. Fabry G. Clinical practice. Static, axial, and rotational deformities of the lower extremities in children. *Eur J Pediatr*. 2010;169:529-34.
4. Heath CH, Staheli LT. Normal limits of knee angle in white children--genu varum and genu valgum. *J Pediatr Orthop* 1993;13:259-62.
5. Hinman RS, May RL, Crossley KM. Is there an alternative to the full-leg radiograph for determining knee joint alignment in osteoarthritis? *Arthritis Rheum* 2006;15; 55:306-13.
6. Kraus VB, Vail TP, Worrell T, et al. A comparative assessment of alignment angle of the knee by radiographic and physical examination methods. *Arthritis Rheum* 2005;52:1730-5.
7. Pomero V, Mitton D, Laporte S, et al. Fast accurate stereoradiographic 3D-reconstruction of the spine using a combined geometric and statistic model. *Clin. Biomech* 2004;19, 240–7.
8. Sabourin M, Jolivet E, Miladi L, et al. Three-dimensional stereoradiographic modeling of the rib cage before and after spinal growing rod procedures in early onset scoliosis. *Clin Biomech (Bristol, Avon)* 2010;25:284-91
9. Lebailly F, Lima L.V, Clairemidi A, et al. Semi-automated stereoradiographic upper limb 3D reconstructions using a combined parametric and statistical model: a preliminary study. *Surg. Radiol. Anat* 2011;34, 757–65.

10. Chaibi Y, Cresson T, Aubert B, et al.. Fast 3D reconstruction of the lower limb using a parametric model and statistical inferences and clinical measurements calculation from biplanar X-rays. *Comput Methods Biomech Biomed Engin* 2012;15:457-66.
11. Quijano S, Serrurier A, Aubert B, et al. Three dimensional reconstruction of the lower limb from biplanar calibrated radiographs. *Med Eng Phys* 2013;35:1703-12
12. Gaumétou E, Quijano S, Ilharreborde B, et al. EOS analysis of lower extremity segmental torsion in children and young adults. *Orthop Traumatol Surg Res* 2014;100:147-51.
13. Meyrignac O, Moreno R, Baunin C, et al. Low-dose biplanar radiography can be used in children and adolescents to accurately assess femoral and tibial torsion and greatly reduce irradiation. *Eur Radiol* 2015;25:1752-60
14. Gheno R, Nectoux E, Herbaux B, et al. Three-dimensional measurements of the lower extremity in children and adolescents using a low-dose biplanar X-ray device. *Eur Radiol.* 2012;22:765-71.
15. Roszkopf AB, Ramseier LE, Sutter R, et al. Comparison of 3D models based on low-dose biplanar radiography and low-dose CT. *Am J Roentgenol.* 2014;202:W285-W291.
16. McKenna C, Wade R, Faria R, et al. EOS 2D/3D X-ray imaging system: a systematic review and economic evaluation. *Health Technol Assess* 2012;16:1-188.
17. ISO5725-2:1994: ISO 5725-2 Accuracy (Trueness and Precision) of Measurements Methods and Results.—Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method, International Organisation for Standardisation, Geneva, Switzerland



18. Assi A, Chaibi Y, Presedo A, et al. Three-dimensional reconstructions for asymptomatic and cerebral palsy children's lower limbs using a biplanar X-ray system: a feasibility study. *Eur J Radiol* 2013;82:2359-64.
19. Bland JA, Altman DG. Statistical methods for assessing agreement between two methods of clinical measurements. *The Lancet* 1986; 8: 307-10
20. Nowicki PD, Vanderhave KL, Farley FA, et al. Reliability of digital radiographs for pediatric lower extremity alignment. *J Pediatr Orthop* 2012;32:631-5.
21. Than P, Szuper K, Somoskeöy S, et al. Geometrical values of the normal and arthritic hip and knee detected with the EOS imaging system. *Int Orthop* 2012;36:1291-7.
22. Sabharwal S, Zhao C, Edgar M. Lower limb alignment in children: reference values based on a full-length standing radiograph. *J Pediatr Orthop* 2008;28:740-6.
23. Saini UC, Bali K, Sheth B, et al. Normal development of the knee angle in healthy Indian children: a clinical study of 215 children. *J Child Orthop* 2010;4:579-86.

**Table 1.** Main characteristics of the 129 study participants, by age group

|                                | Group I<br>6 - 7 years | Group II<br>8 - 9 years | Group III<br>10 - 12 years | Group IV<br>13 - 15 years |
|--------------------------------|------------------------|-------------------------|----------------------------|---------------------------|
| Number of participants         | 18                     | 21                      | 56                         | 34                        |
| Females/Males                  | 16/2                   | 13/8                    | 43/13                      | 20/14                     |
| <b>Angles (°), mean±SD</b>     |                        |                         |                            |                           |
| FMA                            | 93 ± 2                 | 93 ± 2                  | 93 ± 2                     | 93 ± 2                    |
| TMA                            | 89 ± 2                 | 88 ± 2                  | 89 ± 2                     | 87 ± 2                    |
| FTA                            | 178 ± 2                | 179 ± 3                 | 174 ± 4                    | 177 ± 5                   |
| NSA                            | 137 ± 8                | 131 ± 6                 | 134 ± 5                    | 132 ± 7                   |
| HKS                            | 2 ± 1                  | 3 ± 2                   | 5 ± 1                      | 5 ± 2                     |
| <b>Longueurs (mm), mean±SD</b> |                        |                         |                            |                           |
| FHD                            | 30 ± 2                 | 34 ± 3                  | 37 ± 3                     | 42 ± 3                    |
| FNL                            | 33 ± 5                 | 40 ± 5                  | 44 ± 5                     | 52 ± 6                    |

FMA, femoral mechanical angle; TMA, tibial mechanical angle; FTA, femoro-tibial angle; NSA, neck-shaft angle; HKS, hip-knee-shaft angle; FHD, femoral head diameter; FNL, femoral neck length

**Table 2.** Intra-class coefficient (ICC) and standard deviation of reproducibility (SD<sub>R</sub>) of the radiological parameters studied and comparison with previously reported data

| Parameter           | SD repeatability | SD reproducibility | 95%CI  | ICC  | Chaibi et al. [10] | Chaibi et al. [10] | Quijano et al. [11] | Assi et al. [18] | Assi et al. [18] |
|---------------------|------------------|--------------------|--------|------|--------------------|--------------------|---------------------|------------------|------------------|
|                     |                  |                    |        |      | Fast 3D            | Full 3D            |                     | TD               | PC               |
|                     |                  |                    |        |      | 95%CI              | 95%CI              | 95%CI               | 95%CI            | 95%CI            |
| <b>Lengths (mm)</b> |                  |                    |        |      |                    |                    |                     |                  |                  |
| FHD                 | 1.0 mm           | 0.9 mm             | 2.1 mm | 0.96 | 1.6                | 1.4                | 1.6                 |                  |                  |
| FNL                 | 1.7 mm           | 1.5 mm             | 3.4 mm | 0.95 |                    |                    |                     |                  |                  |
| FL                  | 1.2 mm           | 1.1 mm             | 2.4 mm | 1.0  | 2.4                | 1.8                | 1.9                 |                  |                  |
| TL                  | 1.6 mm           | 1.6 mm             | 3.3 mm | 0.99 | 2.3                | 2.3                | 2.2                 |                  |                  |
| <b>Angles (°)</b>   |                  |                    |        |      |                    |                    |                     |                  |                  |
| FMA                 | 1.2 °            | 1.2 °              | 2.5 °  | 0.81 | 2.7                | 1.3                | 2.3                 | 0.7              | 0.7              |
| TMA                 | 2.1 °            | 2.0°               | 4.2 °  | 0.61 | 3.6                | 2.6                | 1.3                 | 1.5              | 2.0              |
| HKS                 | 0.5 °            | 0.4 °              | 0.9 °  | 0.90 | 1.1                | 0.8                | 0.7                 | 0.5              | 0.4              |
| NSA                 | 2.3 °            | 2.1 °              | 4.6 °  | 0.87 | 3.7                | 3.0                | 2.9                 | 1.5              | 2.2              |
| FTA                 | 0.8 °            | 0.7 °              | 1.6 °  | 0.95 |                    |                    | 1.0                 |                  |                  |

FHD, femoral head diameter; FNL, femoral neck length; FL, femoral length; TL, tibial length;

FMA, femoral mechanical angle; TMA, tibial mechanical angle; HKS, hip-knee-shaft angle; NSA, neck-shaft angle; FTA, femoro-tibial angle

**Table 3.** Mean, subnormal, and abnormal values of parameters that did not change with age

|                    |                   | Abnormal<br>low<br><-2 SD | Subnormal low<br>-1 to -2 SD | Normal<br>$\pm 1$ SD | Subnormal<br>high<br>1 to 2 SD | Abnormal<br>high<br>>2 SD |
|--------------------|-------------------|---------------------------|------------------------------|----------------------|--------------------------------|---------------------------|
| FMA ( $^{\circ}$ ) | I-IV <sup>a</sup> | <89                       | 89 - 91                      | 91 - 95              | 95 - 98                        | > 98                      |
| F/T ratio          | I-IV <sup>a</sup> | <1.1                      |                              | 1.1 – 1.2            | > 1.2                          |                           |

FMA, femoral mechanical angle; F/T ratio, ratio of femoral over tibial length

<sup>a</sup>The Roman numerals refer to the age groups described in Table 1.

**Table 4.** Mean, subnormal, and abnormal values of parameters that did changed with age

|          |                       | Abnormal<br>low<br><-2 SD | Subnormal low<br>-1 to -2 SD | Normal<br>±1 SD | Subnormal<br>high<br>1 to 2 SD | Abnormal<br>high<br>>2 SD |
|----------|-----------------------|---------------------------|------------------------------|-----------------|--------------------------------|---------------------------|
| ATM (°)  | I-II-III <sup>a</sup> | <84                       | 84 to 87                     | 87 to 91        | 91 to 93                       | >93                       |
|          | IV <sup>a</sup>       | <82                       | 82 to 85                     | 85 to 90        | 90 to 92                       | >92                       |
| AFT (°)  | I <sup>a</sup>        | <174                      | 174 to 176                   | 176 to 180      | 180 to 182                     | >182                      |
|          | II <sup>a</sup>       | <173                      | 173 to 176                   | 176 to 182      | 182 to 185                     | >185                      |
|          | III <sup>a</sup>      | <166                      | 166 to 170                   | 170 to 178      | 178 to 182                     | >182                      |
|          | IV <sup>a</sup>       | <168                      | 168 to 172                   | 172 to 182      | 182 to 187                     | >187                      |
| HKS (°)  | I <sup>a</sup>        | <-1                       | -1 to 1                      | 1 to 4          | 4 to 6                         | >6                        |
|          | II <sup>a</sup>       | <-3                       | -3 to 2                      | 2 to 12         | 12 to 16                       | >16                       |
|          | III-IV <sup>a</sup>   | <2                        | 2 to 4                       | 4 to 6          | 6 to 8                         | >8                        |
| ACD (°)  | I <sup>a</sup>        | <121                      | 121 to 129                   | 129 to 145      | 145 to 152                     | >152                      |
|          | II <sup>a</sup>       | <119                      | 119 to 125                   | 125 to 137      | 137 to 143                     | >143                      |
|          | III <sup>a</sup>      | <123                      | 123 to 129                   | 129 to 140      | 140 to 145                     | >145                      |
|          | IV <sup>a</sup>       | <118                      | 118 to 125                   | 125 to 139      | 139 to 146                     | >146                      |
| DTF (mm) | I <sup>a</sup>        | <25                       | 25 to 27                     | 27 to 32        | 32 to 35                       | >35                       |
|          | II <sup>a</sup>       | <28                       | 28 to 31                     | 31 to 37        | 37 to 40                       | >40                       |
|          | III <sup>a</sup>      | <31                       | 31 to 34                     | 34 to 40        | 40 to 43                       | >43                       |
|          | IV <sup>a</sup>       | <35                       | 35 to 39                     | 39 to 45        | 45 to 48                       | >48                       |
| LC (mm)  | I <sup>a</sup>        | <23                       | 23 to 28                     | 28 to 38        | 38 to 43                       | >43                       |
|          | II <sup>a</sup>       | <29                       | 29 to 34                     | 34 to 45        | 45 to 50                       | >50                       |
|          | III <sup>a</sup>      | <33                       | 33 to 38                     | 38 to 50        | 50 to 55                       | >55                       |
|          | IV <sup>a</sup>       | <41                       | 41 to 47                     | 47 to 58        | 58 to 64                       | >64                       |

TMA, tibial mechanical angle; FTA, femoro-tibial angle; HKS, hip-knee-shaft angle; NSA, neck-shaft angle; FHD, femoral head diameter; FNL, femoral neck length

<sup>a</sup>The Roman numerals refer to the age groups described in Table 1.


**Table 5.** Mean $\pm$ SD of the lower-limb parameters in non-typically developing (NTD) children and children with cerebral palsy (CP)

|     | NTD<br>N=12 limbs | CP<br>N=12 limbs |
|-----|-------------------|------------------|
| FMA | 94 $\pm$ 3        | 92 $\pm$ 2       |
| TMA | 88 $\pm$ 3        | 89 $\pm$ 2       |
| FTA | 178 $\pm$ 4       | 180 $\pm$ 2      |
| NSA | 134 $\pm$ 6       | 134 $\pm$ 6      |
| HKS | 3 $\pm$ 2         | 4 $\pm$ 1        |
| FHD | 35 $\pm$ 6        | 30 $\pm$ 3       |
| FNL | 38 $\pm$ 11       | 36 $\pm$ 4       |
| F/T | 1.1 $\pm$ 0.0     | 1.1 $\pm$ 0.0    |


FMA, femoral mechanical angle; TMA, tibial mechanical angle; FTA, femoro-tibial angle; NSA, neck-shaft angle; HKS, hip-knee-shaft angle; FHD, femoral head diameter; FNL, femoral neck length; F/T, ratio of femoral over tibial length

**FIGURE LEGENDS****Figure 1**

Changes across age groups in mean values of the femoral mechanical angle (FMA), tibial mechanical angle (TMA), femoro-tibial angle (FTA), and neck-shaft angle (NSA) (all angles in degrees)

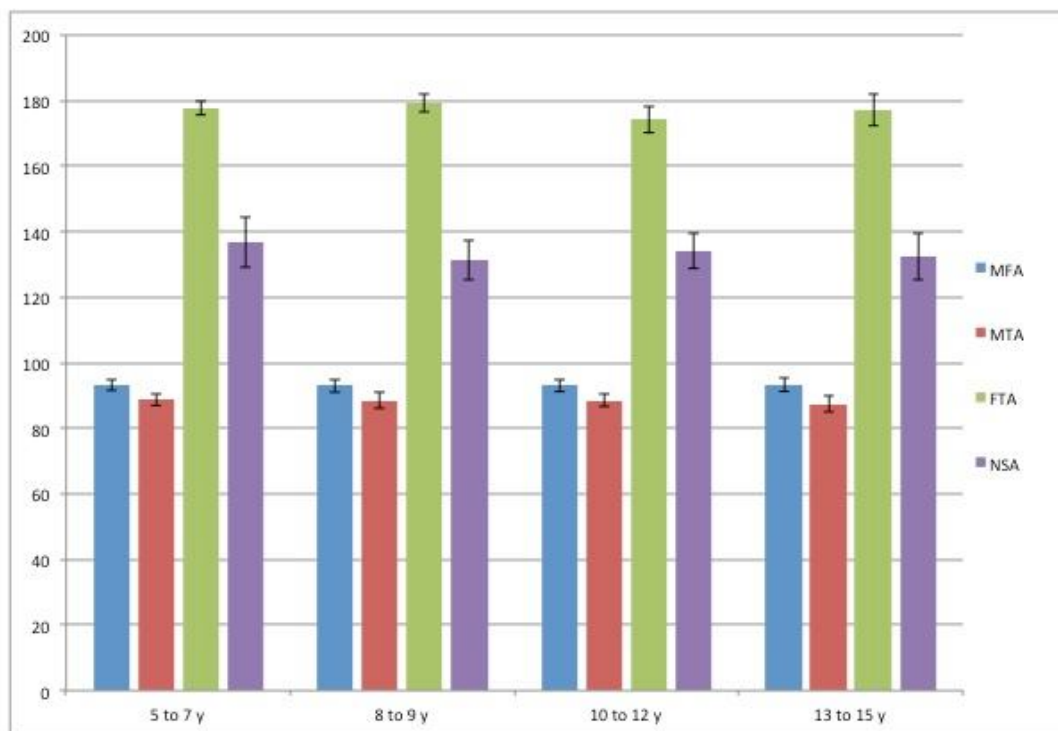**Figure 2**


Changes across age groups in mean values of the ratio of femoral over tibial length ratio

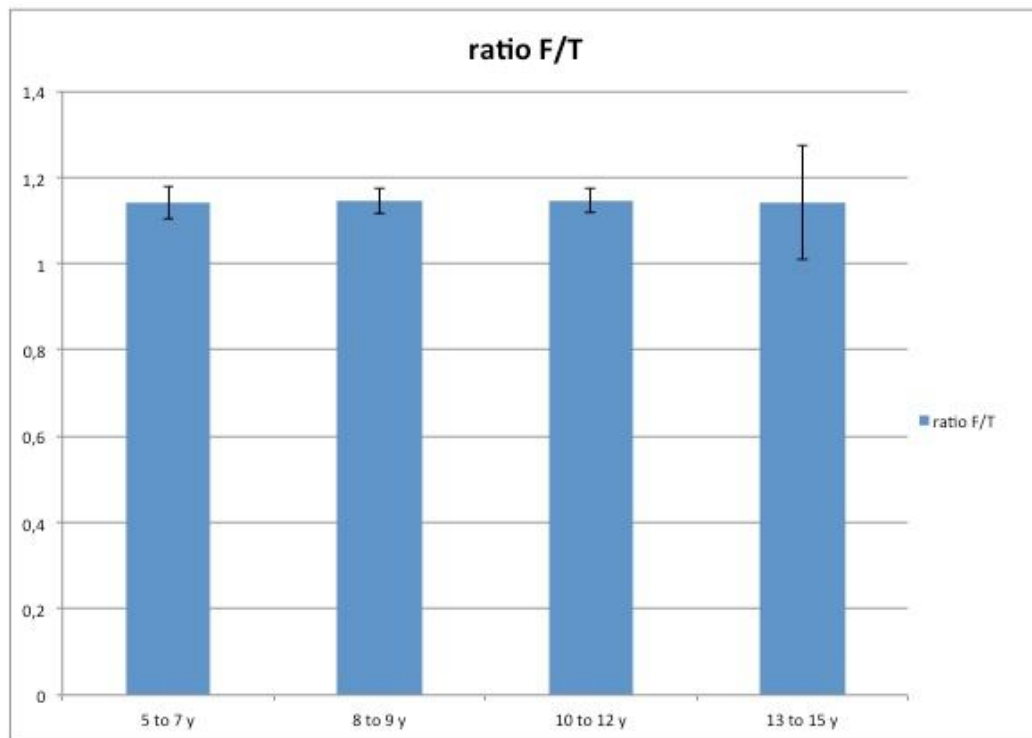

**Figure 3**

Changes across age groups in mean values of femoral head diameter (FHD, mm) and femoral neck length (FNL, mm)



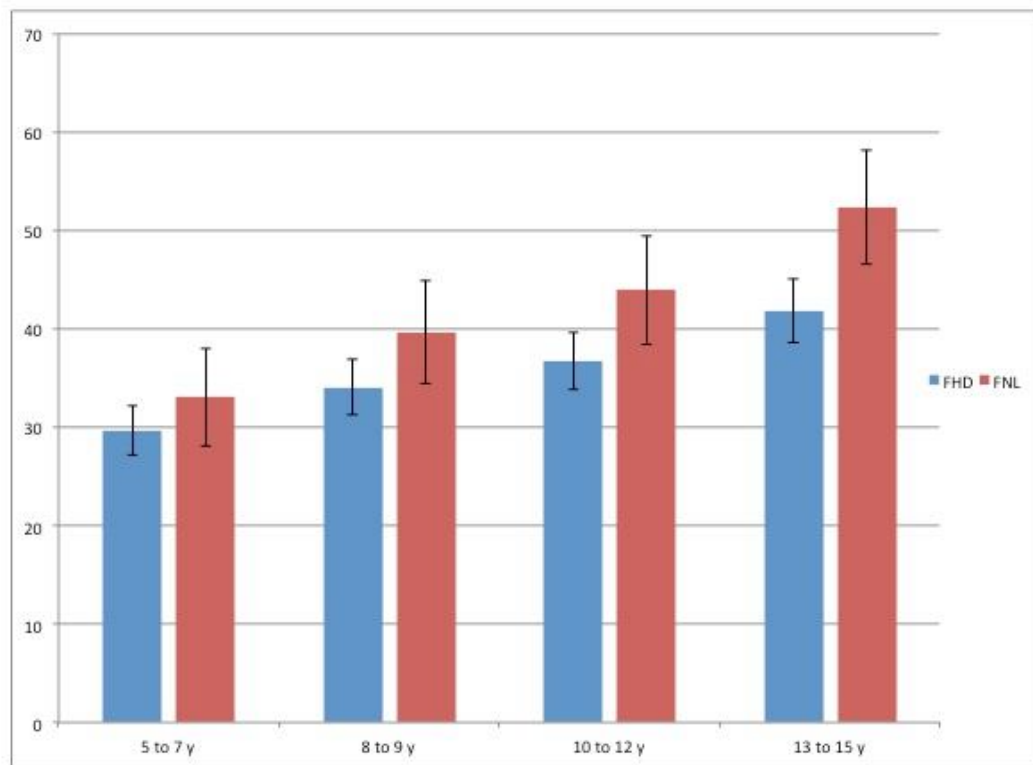

**Figure 4**

Changes across age groups in mean values of the hip-knee-shaft angle (HKS, in degrees))

