



HAL
open science

Simultaneous assay of ascorbate and urate antioxidants in human blood serum using PEDOT-based electrochemical microsensor

Fadhila Sekli-Belaidi, Anne Galinier, Pierre Gros

► **To cite this version:**

Fadhila Sekli-Belaidi, Anne Galinier, Pierre Gros. Simultaneous assay of ascorbate and urate antioxidants in human blood serum using PEDOT-based electrochemical microsensor. *Combinatorial Chemistry and High Throughput Screening*, 2013, 16 (2), pp.84-91. 10.2174/1386207311316020002 . hal-02355061

HAL Id: hal-02355061

<https://hal.science/hal-02355061>

Submitted on 8 Nov 2019

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Open Archive TOULOUSE Archive Ouverte (OATAO)

OATAO is an open access repository that collects the work of Toulouse researchers and makes it freely available over the web where possible.

This is an author-deposited version published in : <http://oatao.univ-toulouse.fr/>
Eprints ID : 8948

To link to this article : DOI:10.2174/1386207311316020002
URL : <http://dx.doi.org/10.2174/1386207311316020002>

To cite this version :
Sekli-Belaidi, Fadhila and Galinier, Anne and Gros, Pierre
Simultaneous assay of ascorbate and urate antioxidants in human blood serum using PEDOT-based electrochemical microsensor.
(2013) *Combinatorial Chemistry & High Throughput Screening*,
vol. 16 (n° 2). pp. 84-91. ISSN 1875-5402

Any correspondence concerning this service should be sent to the repository administrator: staff-oatao@listes.diff.inp-toulouse.fr

Simultaneous Assay of Ascorbate and Urate Antioxidants in Human Blood Serum Using PEDOT- Based Electrochemical Microsensor

Fadhila Sekli-Belaidi¹, Anne Galinier² and Pierre Gros^{*1}

¹Université de Toulouse, Laboratoire de Génie Chimique UMR CNRS/INP/UPS 5503, Université Paul Sabatier, 31062 Toulouse Cedex, France

²Laboratoire de biochimie, CHU Rangueil, 31059 Toulouse cedex 9, France

Abstract: An electrochemical microsensor has been developed for the simultaneous assay of ascorbate (AA) and urate (UA) antioxidants in human blood serum. The electrode surface was modified by means of electropolymerized conductive poly(3,4-ethylenedioxythiophene) PEDOT organic films. Highly selective responses (detection potential difference more than 250 mV) were obtained for both biomarkers by optimizing the PEDOT thickness. Contrary to most previous studies the analytical performances were recorded by testing the microsensor directly in blood serum without any pretreatment of the samples. Using differential pulse voltammetry (DPV) the sensitivity and detection limit were $0.481 \mu\text{A } \mu\text{M}^{-1} \text{cm}^{-2}$ and $4.2 \mu\text{mol L}^{-1}$ for AA and $1.815 \mu\text{A } \mu\text{M}^{-1} \text{cm}^{-2}$ and $2.0 \mu\text{mol L}^{-1}$ for UA. The calibration curves were linear in the concentration range $5\text{--}200 \mu\text{mol L}^{-1}$ for AA and $3\text{--}700 \mu\text{mol L}^{-1}$ for UA. The accuracy of the sensor was satisfactorily compared with the reference analytical methods provided that the synergic effect between both antioxidants was considered. The sensor response was unmodified in the presence of the major biochemical interfering species.

Keywords: Antioxidants, ascorbic and uric acids, blood serum analysis, EC' mechanism, electrochemical microsensor, interfering species, PEDOT film.

1. INTRODUCTION

Oxidative stress has been one of the most widely studied biochemical processes for several years. It is the consequence of an excessive production of highly reactive oxygen (ROS) and nitrogen (RNS) species like superoxide anion $\text{O}_2^{\bullet-}$, hydrogen peroxide H_2O_2 , hydroxyl radical OH^{\bullet} , nitric oxide NO, or peroxynitrite ONOO^- [1] and leads to the oxidation of lipids, proteins and nucleic acids, which contributes to cellular dysfunction and death [2]. Oxidative stress is known to be involved in aging processes and has been proposed as one of the potential causes for cataract, cancers, cardiovascular and degenerative diseases (Parkinson, Alzheimer) and even infertility in men [3-5]. One of the main antioxidant defence systems involves low molecular weight antioxidants, i.e. ascorbic acid (AA), uric acid (UA), glutathione, β -carotene, α -tocopherol, coenzyme Q_{10} , which reduce ROS and RNS by oxido-reduction reactions [6]. Among them, AA and UA are present in highest concentrations in most biological fluids (plasma, serum, urine, tears, cerebrospinal fluids...) and may thus be considered as biochemical markers in a lot of pathologies (preeclampsia disease, neonatal hypoxia, coronary heart diseases...) where oxidative stress is involved [7-9]. Particularly AA is a powerful water soluble antioxidant at physiological levels. In synergic action with other circulating antioxidants, vitamin C plays a key role in protecting living cells against oxidative injury and prevents lipid peroxidation [10]. It is currently used clinically for the treatment and

prevention of scurvy, common cold, mental illness, cancer, AIDS or coronary artery disease [11]. AA deficit (less than $11 \mu\text{mol L}^{-1}$ in blood serum) is the principal cause of scurvy whose incidences increase because of the societal and economic current living conditions. For instance the prevalence of serum hypovitaminosis C was found to be only 0.95% among French healthy volunteers [12] but arise to 16 and 25% in UK low income/materially female and male respectively [13]. It also concerned 47.3% of hospitalized adult patients [14] and 70% of children with cancer upon diagnosis [15]. Consequently a biological assay is of great interest to quickly determine the diagnosis and thus avoid additional expensive examinations. In contrast, the role of UA in conditions associated with oxidative stress is not entirely clear. While commonly regarded as an indicator of gout, epidemiological studies suggest that high UA levels in serum represent also a risk factor for cardiovascular diseases [8] or Lesch-Nyhan syndrome [16]. Thus the selective and convenient detection of AA and UA is very important for biological researches as well as for routine analysis.

Numerous analytical methods have been developed for the quantitative determination of AA and UA in biological samples. They are generally based on enzymatic methods [17], spectrofluorometry [18], HPLC analysis [19] or electrophoretic microchip [20]. However these methods suffer from costly materials and complex experimental protocols, require sample pretreatment and are generally time consuming. For instance the reference method for biological assay of AA involved HPLC coupled with a fluorometric detection and requires the serum to be previously deproteinized (see section 2.5 below). Comparatively electrochemical techniques present several advantages such as simplicity, low cost, fast analysis and

*Address correspondence to this author at the Université de Toulouse, Laboratoire de Génie Chimique UMR CNRS/INP/UPS 5503, Université Paul Sabatier, 31062 Toulouse Cedex, France; Tel: 33 5 61 55 82 69; Fax: 33 5 61 55 61 39; E-mail: gros@chimie.ups-tlse.fr

good selectivity [21]. Moreover, analysis can be realized in short time scales and in relative complex and resistive media by using microelectrodes. However, a major problem is that AA and UA require generally high overpotentials on usual non-modified bare electrodes. Furthermore both antioxidants are in these conditions oxidized at very close potentials which make their simultaneous detection and quantitative determination difficult [22].

Chemically modified electrodes have been largely developed to solve these problems and to discriminate between the electrochemical responses of AA and UA oxidation. Several electrode modification processes have been proposed, using highly oxidized metal electrodes [23], metallic films [24] and nanoparticles [25, 26] electrodeposition, metal complexes [27], electrochemically reduced diazonium salts [28], single [29] or multiwalled carbon nanotubes [30-33], carbon-surface [34-37] and carbon-paste [38] electrodes, self-assembled thiol monolayer [39] or conducting polymers [40-43]. In this latter case, attention has been devoted since the mid-1990s to poly(3,4-ethylenedioxythiophene) (PEDOT) [44] which induces uniform and adherent polymer film on most electrode materials, shows quite high conductivity in its oxidized state, presents good stability in aqueous electrolyte and above all biocompatibility with biological media [45]. Moreover PEDOT was found to be resistant to fouling by the AA oxidation products [46], thus indicating PEDOT to be very promising in the design of amperometric sensors [47-49]. Nevertheless the analytical performances of all these sensors were systematically determined in model solutions whatever the modification procedure chosen. Moreover the analysis of real biological samples like human urine and blood serum, when considered, was mostly presented as a feasibility study realized in particular experimental conditions, i.e. considering AA and UA as interfering species for the assay of neurotransmitters like dopamine, or in presence of AA in large excess which does not reflect the healthy human situation (the concentration of AA in blood serum being one order of magnitude lower than that of UA in physiological conditions [50]). Consequently AA was either assayed separately to UA, or just detected and not assayed while its quantification represents a task of interest as well important as UA in clinical analysis. Finally AA was in other papers not detected in the original sample but added amounts were assayed by means of standard adding method.

In our previous studied [51] we evaluated PEDOT-modified electrodes to selectively detect and simultaneously assay ascorbic and uric acids under similar concentrations in aqueous solution. Particularly we reported the influence of PEDOT electropolymerization parameters on the amperometric response of the resulting microsensor. However most results were obtained in synthetic aqueous solutions and only one test was realized in blood serum. It is now essential to evaluate such modified electrode in biological medium in order to validate its analytical performances in real conditions and to apply the resulting sensor in the field of clinical biology analysis. The present paper experiences the voltammetric sensor in blood serum analysis. The analytical performances have been determined and discussed by considering the matrix effects of such complex medium. The accuracy of the sensor was evaluated by comparison with the reference analytical methods (HPLC

for AA and enzymatic assay for UA). The influence of the major interfering species present in blood was also studied. Finally the efficiency of the microsensor was proved by analyzing 14 human blood serum samples.

2. MATERIALS AND METHODS

2.1. Chemicals

3,4-ethylenedioxythiophene (EDOT), potassium ferricyanide $K_3Fe(CN)_6$ and metaphosphoric acid HPO_3 were purchased from Aldrich. Ascorbic acid, uric acid, dopamine, xanthine, hypoxanthine, glutamic acid, cysteine, N-Acetyl-L-cysteine (NAC), β -D glucose, albumin, uricase (E.C. 1.7.3.3) from *Bacillus fastidiosus* and peroxidase (E.C. 1.11.1.7) from horseradish were purchased from Sigma. Tetrabutylammonium perchlorate (TBAPC), potassium dihydrogenophosphate KH_2PO_4 , di-potassium hydrogenophosphate K_2HPO_4 , acetonitrile and N,N-bis(4-sulfobutyl) 3,5-dimethylaniline (MADB) were purchased from Acros. All reagents were of analytical grade and used as received. The aqueous solutions were prepared with doubled distilled water. High pure nitrogen was used for deaeration. Human blood serum samples were kindly given by the Laboratoire de Biochimie from Hôpital Rangueil – Toulouse and stored at $-20^\circ C$ before being used.

2.2. Materials

All electrochemical experiments were performed with an Autolab II Metrohm potentiostat (Eco-Chimie) interfaced to a microcomputer and using the GPES 4.9 software. A three-electrode system was used. A 50 μm diameter gold wire purchased from Goodfellow (Lille, France) was chosen as working microelectrode. The fabrication process involved glass capillaries from Clark Electromedical Instruments (Phymep, Paris, France), a microelectrode puller (Model PC 10) and a microgrinder (Model EG44) purchased from Narishige (London, UK). A 1 mm diameter platinum wire (1 cm length) was used as auxiliary electrode. All potentials reported in the text are referred to a saturated calomel reference electrode (SCE) ($Hg/Hg_2Cl_2/KCl_{sat}$) connected to the cell by a Luggin capillary. AA analysis was performed with a Dionex liquid chromatograph coupled to a fluorimetric detector. An isocratic pump and an autosampler were also used. Enzymatic assay of UA used an automate Olympus AU 2700 spectrophotometer.

2.3. Fabrication and Preparation of PEDOT-Modified Gold Microelectrodes

Microelectrodes were fabricated and characterized according to the procedure described by Ruffien-Ciszak *et al.* [52]. Briefly, the gold wire was inserted in the glass capillary. The capillary was pulled in two microelectrodes with the microelectrode puller. A tapered end was produced and warmed up again in order to consolidate the cohesion between glass and gold. Then this tip was polished on the diamond particle whetstone microgrinder at an angle of 90° for several minutes. The resulting microelectrodes presented disk geometry with total radius less than 120 μm .

The PEDOT electrodeposition process was similar to that previously reported [51]. A gold disk microelectrode was

polished with alumina slurry and rinsed with distilled water. The polished surface was then pretreated by cycling the electrode potential between -0.88 V and 1.5 V for 10 min at 10 mV s^{-1} in 20 mL deaerated acetonitrile containing 0.1 mol L^{-1} TBAPC as supporting electrolyte. Deaeration was obtained by purging the solution with nitrogen during 10 min; moreover a nitrogen atmosphere was maintained over the solution during the experiments. The electropolymerization was performed by cycling the electrode potential between -0.88 V and 1.5 V at 250 mV s^{-1} in the previous electrolytic solution also containing 2.5 mmol L^{-1} EDOT monomer. The amount of polymer synthesized corresponded to an anodic charge of 12 mC cm^{-2} (about $6.10 \cdot 10^{-8} \text{ mol cm}^{-2}$) and was previously optimized for the simultaneous detection of AA and UA in synthetic aqueous solution [51]. The modified electrode was then rinsed with acetonitrile and distilled water successively to remove any physically adsorbed monomer. This modified electrode is hereafter referred to as $\mu\text{Au-PEDOT}$.

2.4. Electrochemical Detection of AA and UA

The $\mu\text{Au-PEDOT}$ was immersed in a three-electrode cell where a nitrogen flux was constantly maintained. Experiments were performed in 250 μL unstirred and undiluted blood serum without adding any supplementary electrolyte. The sample was left to come at room temperature before analysis. Electrochemical measurements were performed by differential pulse voltammetry (DPV) since this electrochemical method induced higher currents than those recorded by cyclic voltammetry [46]. The experimental conditions were optimized with respect to the determination of AA [53]: pulse amplitude 50 mV, step potential 6 mV, pulse time 119 ms, interval time 1s, potential scan rate 6 mV s^{-1} . AA and UA assays were performed by standard addition method.

2.5. AA and UA Assay Using Reference Analytical Methods


AA concentration was determined indirectly from the assay of its oxidized form dehydroascorbic acid (DHA) obtained after addition of $\text{K}_3\text{Fe}(\text{CN})_6$ 0.3 mmol L^{-1} . Serum samples were previously deproteinized with 0.5 mol L^{-1} metaphosphoric acid/methanol (75/25 v/v) and centrifugated at 3500 rpm at 4°C during 10 min. DHA analysis was accomplished in the supernatant by chromatography [54] using an isocratic elution on a Phenomenex Onyx C18 $100 \times 4.6 \text{ mm}$ column thermoregulated at 25°C . The mobile phase consisted of 0.05 mol L^{-1} phosphate buffer solution (PBS)/methanol (90/10 v/v) pH 7.8 whose flow rate was kept constant at 1.6 mL min^{-1} . The fluorimetric detection was performed after addition of 4 mmol L^{-1} orthophenylenediamine in the sample with an exciting and emission wavelength set at 350 nm and 420 nm, respectively. Each assay involved two chromatographic runs, the first one to determine the initial concentration of DHA in blood serum and the second one after oxidative treatment of the sample. The concentration of ascorbate in serum was calculated by subtraction of DHA to the total vitamin C. The calibration and intralaboratory assays were estimated by using calibrator and internal standards delivered by CromSystem Instruments. The limit of quantification was 5

$\mu\text{mol L}^{-1}$. The repeatability and reproductibility for two levels of total vitamin C (36.9 and $119.23 \mu\text{mol L}^{-1}$) were 2.5 and 9%, and 3.6 and 8%, respectively.

UA assay was performed as previously described [55]. Briefly UA was oxidized into allantoin in a first reaction catalyzed by uricase:



Hydrogen peroxide was then reduced by MADB in a second reaction catalyzed by peroxidase to give the blue color quinoneimine:



All reactions were realized at 37°C . 25 μL of serum sample was added to 1 ml of phosphate buffer solution (PBS) 0.042 mol L^{-1} pH 7.5 containing 0.15 mmol L^{-1} MADB, 0.3 mmol L^{-1} 4-aminophenazone, 5.9 kU L^{-1} peroxidase and 0.25 kU L^{-1} uricase. Detection of the quinoneimine chromophor was performed spectrophotometrically at 660 nm. Calibration was obtained by the external standard method. The limit of quantification was $2 \mu\text{mol L}^{-1}$. The repeatability and reproductibility were 1.11 and 1.71% for a concentration of UA equal to $171 \mu\text{mol L}^{-1}$ and 2.44% for $388 \mu\text{mol L}^{-1}$ and 0.73 and 2.12% for $1362 \mu\text{mol L}^{-1}$.

3. RESULTS AND DISCUSSION

3.1. DPV in Blood Serum

Fig. (1) shows differential pulse voltammograms (DPVs) recorded with a bare-gold microelectrode (dashed line) and the $\mu\text{Au-PEDOT}$ modified electrode (solid line) immersed in 250 μL undiluted blood serum sample.

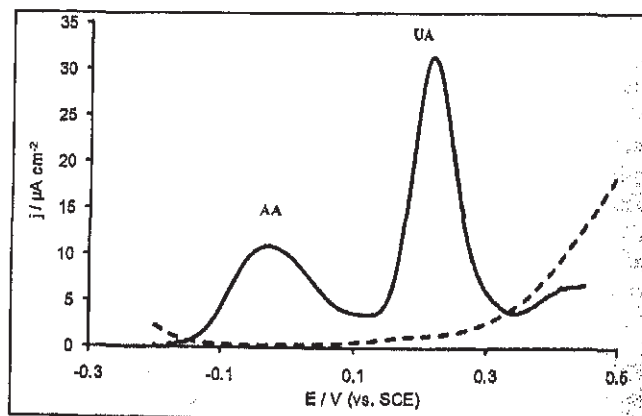


Fig. (1). DPVs recorded with a $50 \mu\text{m Au}$ microelectrode (dashed line) and a $\mu\text{Au-PEDOT}$ (solid line) in blood serum sample containing $13.8 \mu\text{mol L}^{-1}$ AA and $225 \mu\text{mol L}^{-1}$ UA. PEDOT film was electropolymerized between -0.88 V and 1.5 V vs SCE at 250 mV s^{-1} in 0.1 mol L^{-1} TBAPC-acetonitrile containing EDOT 2.5 mmol L^{-1} . Electrochemical parameters are indicated in section 2.4.

Whatever the electrode, it has been previously verified that no significant signal was observed in PBS pH 7.0 except for the electro-oxidation of gold starting at about 0.8 V (result not shown). The oxidation of AA and UA on the unmodified electrode resulted in a broad and non exploitable wave starting at about 0.2 V. This result is in agreement with

previous works making evidence that both antioxidant species cannot be detected selectively on non-modified electrodes [22]. In contrast, two well-defined and distinct anodic peaks were recorded with the μAu -PEDOT electrode. By adopting the experimental conditions previously described for PEDOT electrodeposition (section 2.3) and for DPV parameters (section 2.4), it was possible to shift the peak potentials to lower values, i.e. -0.03 V and 0.23 V for AA and UA oxidation, respectively. This potential shift thus makes the sensor less sensitive to possible interfering species present in blood sample (see below). The potential difference was more than 250 mV , thus allowing the simultaneous detection of both species with the same modified electrode. The peak separation was attributed to different surface accumulations of each antioxidant on the polymer surface. It is known that the interactions between PEDOT and AA are essentially of electrostatic type (AA being anionic and the polymer backbone being positively charged at the pH used) [56] whereas UA is concentrated at the polymer mainly by means of hydrophobic interaction [57]. These interactions certainly explain also why the currents recorded at μAu -PEDOT were strongly higher compared to those obtained on the unmodified electrode, thus improving the sensitivity of the sensor. On the other hand both potential difference and amperometric responses were lower than those obtained previously in synthetic model solutions [51]. In the present case the voltammogram was plotted in blood serum without any dilution or pretreatment of the sample. The matrix effect certainly explains these results. It is noteworthy that the current depletion is more important for UA than for AA. In the aqueous solution UA was the most hydrophobic species whereas several other hydrophobic compounds (like lipids) are present in blood. These latter could adsorb on the polymer surface and thus prevent UA from being efficiently oxidized at the modified electrode. Anyway the PEDOT modified electrode clearly demonstrates a catalytic activity for the oxidation of both antioxidant species.

3.2. Analytical Performances

Fig. (2A, B) exhibit the DPVs recorded with the μAu -PEDOT electrode in blood serum under increasing concentrations of AA and UA, respectively. Although using high concentrated AA (resp. UA) stock solutions, the successive additions in such a low ($250\ \mu\text{L}$) sample volume induced not only an increase in the corresponding peak current but also a decrease in the UA (resp. AA) oxidation signal. The resulting calibration curves are also shown (inset). Both exhibited a linear variation of the peak current as a function of the concentration of the corresponding antioxidant species. Complementary experiments showed that the linearity for AA was observed in the concentration range $5\text{--}200\ \mu\text{mol L}^{-1}$. The detection limit was $4.2\ \mu\text{mol L}^{-1}$ ($S/N=3$). Similarly the UA oxidation current density varied linearly with the concentration in the range $3\text{--}700\ \mu\text{mol L}^{-1}$ and a detection limit of $2.0\ \mu\text{mol L}^{-1}$ ($S/N=3$) was reached. It is interesting to notice that both limits of quantification are very close to those of the reference methods (see section 2.5). The sensor sensitivities were $0.481\ \mu\text{A}\ \mu\text{M}^{-1}\ \text{cm}^{-2}$ and $1.815\ \mu\text{A}\ \mu\text{M}^{-1}\ \text{cm}^{-2}$ for AA and UA, respectively. It is noteworthy that the sensitivity was sensibly higher for UA than for AA. This difference resulted not only from the

specific interactions of each antioxidant with the polymer as previously discussed; it was also the consequence of an EC' mechanism resulting from a chemical reaction in solution coupled to the electrochemical step [58] as demonstrated previously in our laboratory with synthetic aqueous solutions containing a mixture of AA and UA [59]. The apparent standard potential of the (ascorbyl radical/ascorbate ion) redox system being lower than that of the (alloxan/urate) one (0.28 V and 0.59 V at pH 7.0, respectively [60, 61]), a spontaneous oxidoreduction reaction between AA and the UA oxidation product takes place, thus regenerating the reduced form of UA at the vicinity of the modified electrode surface. Consequently an obvious change was observed in the sensitivity of the microsensor for UA oxidation current depending on whether AA was present in the sample or not [59]. This phenomenon was never considered before certainly because AA was in most studies in excess compared to UA. Consequently the regeneration process was constant and the calibration curve corresponding to UA assay was the same whatever the AA concentration. In contrast it is of particularly importance when AA and UA concentrations are in the same order of magnitude since even a little variation of AA concentration would modify sensibly the UA anodic current. For all real samples AA has thus to be assayed before UA, the calibration curve of UA taking account of the presence of AA and the consecutive synergic effect between both antioxidants. The relative standard deviations (R.S.D.) were 5.2% and 4.8% ($n = 3$ successive measurements) for AA and UA, respectively. The reproducibility was estimated at 7.4% for AA and 5.4% for UA on the basis of 4 independent measurements. It is noteworthy that these analytical performances are worse than those recorded in aqueous synthetic solutions. This is particularly true for the sensitivity which was found to be equal to $0.87\ \mu\text{A}\ \mu\text{M}^{-1}\ \text{cm}^{-2}$ for AA and $4.05\ \mu\text{A}\ \mu\text{M}^{-1}\ \text{cm}^{-2}$ for UA in the latter case [51]. This significant decrease in the sensor sensitivity is no doubt the consequence of the modifications of the electrode surface state during measurements which are induced by matrix effects almost systematically present with real complex samples. However all these performances are well suited to the assay of both antioxidants in biologic fluids like blood serum, as well as under physiological conditions (the physiological concentrations in blood serum are between 11 and $79\ \mu\text{mol L}^{-1}$ for AA and between 180 and $420\ \mu\text{mol L}^{-1}$ for UA [50]) as in the presence of one of the two acids at high concentrations. Table 1 indicates the analytical performances of recently reported electrochemical microsensors based on modified electrodes which were applied to the assay or detection of AA and UA in biological fluids. From these data one could rapidly conclude that the microsensor developed in this work presents the worse analytical performances. Comparison is not so easy since we have previously shown that PEDOT-modified electrode provided amongst the best results when used in model aqueous solution [51].

Actually most results reported in Table 1 were obtained in synthetic buffered solutions and the sensors were tested once in urine or blood serum. Furthermore works devoted to the simultaneous assay of AA and UA are very scarce. In these studies AA were very often considered as an interfering species or introduced in large excess, this latter

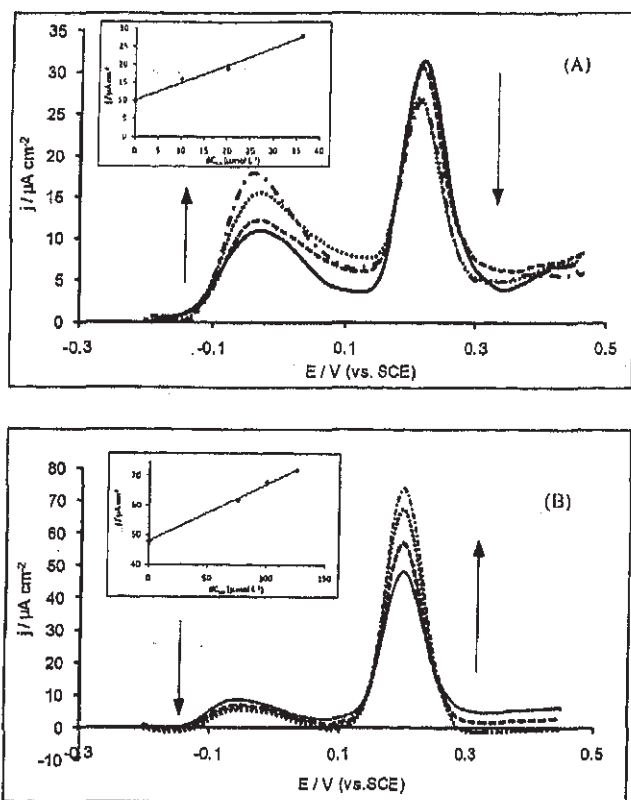


Fig. (2). DPVs recorded with the $\mu\text{Au-PEDOT}$ in blood serum sample initially containing $13.8 \mu\text{mol L}^{-1}$ AA and $225 \mu\text{mol L}^{-1}$ UA (solid line) and after successive additions of AA (Fig. 2A) or UA (Fig. 2B). (A) addition of AA : $10 \mu\text{mol L}^{-1}$ (dashed line); $20 \mu\text{mol L}^{-1}$ (dotted line); $36 \mu\text{mol L}^{-1}$ (dashed dotted line). (B) addition of UA : $75 \mu\text{mol L}^{-1}$ (dashed line); $100 \mu\text{mol L}^{-1}$ (dotted line); $125 \mu\text{mol L}^{-1}$ (dashed dotted line). Inset: calibration curves.

case not reflecting the healthy human conditions. Consequently AA was generally only detected but not assayed. In our study the analytical performances of the microsensor were exclusively evaluated in blood serum and both antioxidant concentrations were determined simultaneously as it is currently the case in clinic biology analysis with other costly techniques. To the best of our knowledge it is the first time that such study was performed exclusively in real biologic sample with PEDOT-modified electrode.

The sensor accuracy was evaluated by comparing the results of the voltammetric sensor (taking account of the calibration curves) with those obtained by using the reference methods (see section 2.5 for experimental protocols). Fig. (3) shows the results recorded with several blood samples for AA (Fig. 3A) and UA (Fig. 3B) assay. In both cases an excellent correlation was observed in the physiological concentration range studied as both slopes (0.951 and 0.993 for AA and UA, respectively) and correlation coefficients (0.997 and 0.998) were close to 1. The electrochemical microsensor thus provides analytical results very similar to those of the reference methods while implying relatively cheaper apparatus. Furthermore results are obtained in quasi real time (DPVs are recorded in less than 1 min).

3.3. Interfering Species

The analytical performances of the voltammetric microsensor have also been evaluated in the presence of the main common co-existing substances which could interfere with the detection of AA and UA in blood serum. In this respect the effect of dopamine, xanthine, glutamic acid, cysteine, glucose and albumin was examined. The concentrations were chosen in order all the electroactive species to be clearly identified in the voltammogram. Supplementary addition of interfering species was realized if necessary. Fig. (4) shows the DPVs obtained with a blood sample containing all these species. Compared to the curve obtained with only AA and UA (Fig. 1, solid line) no significant change was observed in the oxidation peak potentials of both antioxidant species (-0.065 V instead of -0.030 V for AA and 0.260 V instead of 0.230 V for UA). In this potential range, glutamic acid was not detected and glucose presented no electrochemical activity.

Table 2 reports AA and UA anodic currents recorded in the absence and in the presence of the different compounds. The values were not affected except in the presence of xanthine. In this latter case the peak current density corresponding to UA oxidation increased during the second potential sweep when the potential reached 0.70 V in the first scan, thus allowing the electrochemical oxidation of xanthine into uric acid [57]. In consequence, the potential range of the $\mu\text{Au-PEDOT}$ voltammetric sensor was reduced from -0.2 V to 0.4 V in order to obtain selective and reliable results. Finally the presence of albumin induced a slight negative shift of about 30 mV in the oxidation peak potentials of all the electrochemically detected species and a decrease in both AA and UA anodic currents of about 10%.

3.4. Analysis of Blood Serum Samples

The voltammetric sensor has been tested with 14 blood serum samples and the results compared with the reference analytical methods. Data are reported in Table 3. In all cases the electrochemical assays of AA and UA were confirmed by referent procedures. It is noteworthy that the microsensor allowed the detection of both antioxidants in a single measurement without any pretreatment or dilution of the sample. Furthermore, it was possible to proceed with the calibration using the standard addition method and a single calibration point per antioxidant species as the responses of the sensor were linear in a large concentration range.

4. CONCLUSION

Modification of gold microelectrode surface by means of PEDOT electropolymerization has proved to be efficient to elaborate a voltammetric sensor for the assay of AA and UA in human blood serum. The $\mu\text{Au-PEDOT}$ electrode exhibited an efficient electrocatalytic behavior which makes possible to detect both antioxidant species in human blood serum without any pretreatment of the sample nor dilution or addition of any electrolyte. Contrary to most previous studies the analytical performances of the microsensor were adapted to the simultaneous determination of both concentrations in physiological conditions. Even if the sensitivity of the sensor was significantly lower in blood serum than in aqueous

Table 1 Comparison of the Analytical Performances of Different Electrochemical Microsensors for the Determination of Ascorbate (AA) and Urate (UA) Antioxidants in Physiological Samples

Modification Method	ΔE_p , mV	Linear Range/ μM		Detection Limit/ μM		Sensitivity/ $\mu\text{A } \mu\text{M}^{-1} \text{cm}^{-2}$		Sample		Ref.
		AA	UA	AA	UA	AA	UA	AA	UA	
PVA	130	10-250	2-50	7.6	0.6	0.89	3.1	NR	urine	[34]
PMPy/Pd _{nano}	440	50-1000	0.5-20	7	0.027	0.006	0.28	NR	urine	[40]
AgHCFNPs	400	4-78	2-150	0.42	0.08	0.152	1.22	NR	serum	[25]
GNP/LC	320	3-2500	0.5-300	1	0.2	0.36	-	-	serum	[26]
PEDOT	372	500-3500	20-130	7.4	1.4	0.004	0.136	NR	serum	[41]
PG-activated	375	25-500	2.5-30	13	1.4	0.012	1.52	NR	serum	[35]
MWCNT	355	15-800	0.55-90	7.7	0.42	0.041	0.34	AA tablets	serum	[30]
PMT/Pd _{nano}	520	10-160	NR	7	NR	0.013	NR	serum	NR	[43]
ETPG	390	NR	0.05-10	NR	0.001	NR	32.75	NR	serum	[37]
TNCPE	240	1-100	0.4-100	0.5	0.08	NR	NR	AA tablets	serum	[38]
CILE	295	50-7400	2-220	20	1	NR	NR	NR	urine	[36]
Fe(III)P/MWCNT	460	14-2500	6-1300	3	0.3	0.081	0.059	ND	serum	[31]
PPD	345	2-2000	50-1600	0.4	2.5	0.007	0.005	ND	serum	[42]
Baelbp/Cu	223	5-160	5-300	2	2	0.49	0.51	serum	serum	[27]
PEDOT	403	5-300	2-600	2.5	1.5	0.875	4.05	synthetic solutions		[51]
PEDOT	250	5-200	3-700	4.2	2.0	0.481	1.815	serum	serum	This work

Note. PVA: poly (vinyl alcohol); P/PMPy/Pd_{nano}: poly (N-methylpyrrole)/Pd-nanoclusters; AgHCFNPs: silver hexacyanoferrate nanoparticles; GNP/LC: gold nanoparticles self-assembled; PEDOT: poly(3,4-ethylenedioxythiophene); PG-activated: pyrolytic graphite activated; MWCNT: multi walled carbon nanotubes; PMT/Pd_{nano}: poly(3-methylthiophene)/Pd nanoparticles; ETPG: electrochemically treated pencil graphite; TNCPE: thionine-nafion carbon paste modified electrode; CILE: carbon ionic liquid electrode; Fe(III)P/MWCNT: Non-covalent iron(III)-porphyrin functionalized multi-walled carbon nanotubes; PPD: para-phenylenediamine; Baelbp/Cu: 2-[bis(2-aminoethyl)amino]ethanol, 4,40-bipyridine bridged dicopper(II); ND: not determined; NR: not reported.

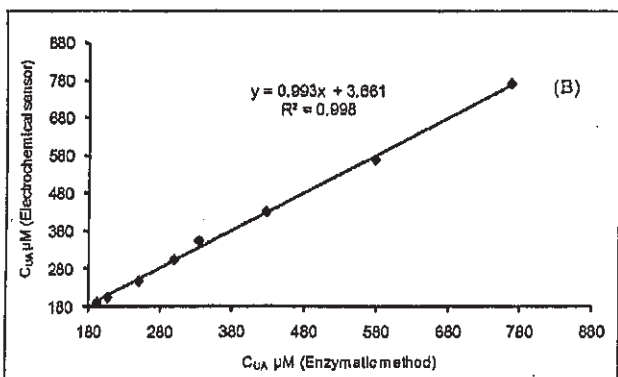
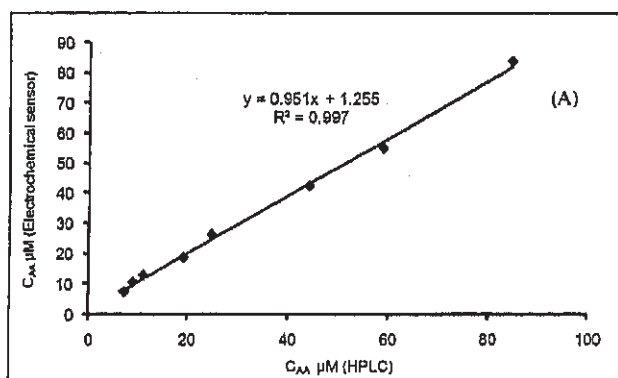


Fig. (3). Comparison of the analytical results obtained with the μAu -PEDOT microsensors with those recorded with the reference methods for AA (Fig. 3A) and UA (Fig. 3B) assays (see section 2.5. for experimental details).

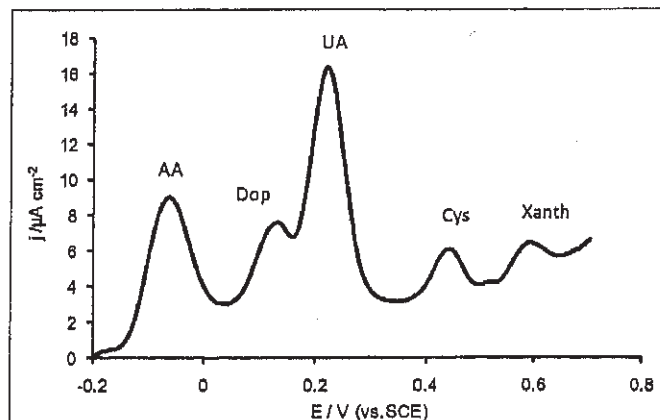


Fig. (4). DPV recorded with the μAu -PEDOT in blood serum sample containing ascorbic acid $10.7 \mu\text{mol L}^{-1}$, dopamine $50 \mu\text{mol L}^{-1}$, uric acid $19.2 \mu\text{mol L}^{-1}$, cysteine $200 \mu\text{mol L}^{-1}$, xanthine $100 \mu\text{mol L}^{-1}$, glutamic acid $500 \mu\text{mol L}^{-1}$, glucose 5.5mmol L^{-1} and albumin 2g L^{-1} .

solution due to matrix effects, the amperometric responses were not modified by the presence of the major biochemical interfering species. The sensor thus provided results in good agreement with those obtained with reference methods with an analytical procedure involving only one calibration point per antioxidant. Disposable sensors being preferable in clinical biology in order to avoid contamination between samples, works are in progress in our laboratory to evaluate the stability of the sensor under storage conditions.

Table 2. Effect of Interfering Species on AA and UA Anodic Peak Currents Recorded at -0.05 V and 0.23 V, Respectively. Blood Serum Initially Containing 10.7 $\mu\text{mol L}^{-1}$ AA and 19.2 $\mu\text{mol L}^{-1}$ UA

Interfering Species	Concentration	Peak Current ($\mu\text{A cm}^{-2}$)	
		AA	UA
No interfering	-	10.4	20
Dopamine (μM)	50	10.2	19.85
Cysteine (μM)	200	10.3	20.1
N-acetyl-cysteine (μM)	100	10.4	20.1
Glucose (mM)	5.5	10.5	19.97
Glutamic acid (μM)	500	10	20.2
Xanthine (μM)	100	10.4	20
			22*
Hypoxanthine (μM)	100	9.98	20.1
Albumin (g/L)	2	9.46	18.2

*UA oxidation current recorded during the second DPVs.

Table 3. Determination of AA and UA Concentration in Blood Serum Samples with the Voltammetric Microsensor and the Reference Analytical Methods. AA and UA were Detected on the μAu -PEDOT at -0.05 V and 0.23 V, Respectively

Sample	AA/ $\mu\text{mol L}^{-1}$		UA/ $\mu\text{mol L}^{-1}$	
	μAu -PEDOT	Ref. Method	μAu -PEDOT	Ref. Method
1	42.5	43.9	431	429
2	18.7	19.2	205	208
3	22.0	25.8	192	193
4	13.8	12.3	248	251
5	42.3	44.2	569	579
6	7.4	7.3	355	335
7	26.2	24.8	336	304
8	4.2	5.6	304	301
9	83.7	84.8	442	413
10	18.4	16.3	769	769
11	10.7	9.0	368	365
12	55.0	58.9	228	232
13	34.2	32.6	436	433
14	15.9	17.2	252	251

CONFLICT OF INTEREST

Authors declare that they have no conflict of interest by any means with respect to the instant research manuscript.

ACKNOWLEDGEMENTS

The authors would like to thank Laure Latapie from the Laboratoire de Génie Chimique and the Laboratoire de Biochimie for technical support.

REFERENCES

- [1] Lowenstein, C.J.; Snyder, S.H. Nitric oxide, a novel biologic messenger. *Cell*, 1992, 70, 705-707.
- [2] Ames, B.N.; Shigenaga, M.K.; Hagen, T.M. Oxidants, antioxidants and the degenerative diseases of aging. *Proc. Natl. Acad. Sci.*, 1993, 90, 7915-7922.
- [3] Halliwell, B.; Gutteridge, J. *Free radicals in biology and medicine*, 3rd ed.; Oxford University Press: New York, 1999.
- [4] Bast, A.; Haenen, G.R.M.M.; Doelman, C.J.A. Oxidants and antioxidants: state of the art. *Am. J. Med.*, 1991, 91, 2-13.
- [5] Colagar, A.H.; Marzony, E.T. Ascorbic acid in human seminal plasma: determination and its relationship to sperm quality. *J. Clin. Biochem. Nutr.*, 2009, 45, 144-149.
- [6] Favier, A. Le stress oxydant : intérêt de sa mise en évidence en biologie médicale et problèmes posés par le choix d'un marqueur. *Ann. Biol. Clin.*, 1997, 55, 9-16.
- [7] Arrigoni, O.; Tullio, M. Ascorbic acid: much more than just an antioxidant. *Biochim. Biophys. Acta*, 2002, 1569, 1-9.
- [8] Alderman, M.H. Uric acid and cardiovascular risk. *Curr. Opin. Pharmacol.*, 2002, 2, 126-130.
- [9] Afzal-Ahmed, I.; Mann, G.E.; Shennan, A.H.; Poston, L.; Naftalin, R.J. Preeclampsia inactivates glucose-6-phosphate dehydrogenase and impairs the redox status of erythrocytes and fetal endothelial cells. *Free Radic. Biol. Med.*, 2007, 42, 1781-1790.
- [10] Exner, M.; Hermann, M.; Hofbauer, R.; Hartmann, B.; Kapiotis, S.; Gmeiner, B. Thiocyanate catalyzes myeloperoxidase-initiated lipid oxidation in LDL. *Free Radic Biol Med.*, 2004, 37, 146-155.
- [11] Li, Y.; Schellhorn, H.E. New developments and novel therapeutic perspectives for vitamin C. *J. Nutr.*, 2007, 10, 2171-2184.
- [12] Faure, H.; Preziosi, P.; Roussel, A.M.; Bertrais, S.; Galan, P.; Sereberg, S.; Favier, A. Factors influencing blood concentration of retinol, α -tocopherol, vitamin C, and β -carotene in the French participants of the SU.VI.MAX trial. *Eur. J. Clin. Nutr.*, 2006, 60, 706-717.
- [13] Mosdøl, A.; Erens, B.; Brunner, E.J. Estimated prevalence and predictors of vitamin C deficiency within UK's low-income population. *J. Pub. Health*, 2008, 30, 456-460.
- [14] Fain, O.; Paries, J.; Jacquart, B.; Le Moël G.; Kettaneh, A.; Stirnermann, J.; Heron, C.; Sitbon, M.; Taleb, C.; Letellier, E.; Betari, B.; Gattegno, L.; Thomas, M. Hypovitaminosis C in hospitalized patients. *Eur. J. Int. Med.*, 2003, 14, 419-425.
- [15] Lima de Araújo, L.; Maciel Barbosa, J.; Gomes Ribeiro, A.P.; Oliveira Dos Santos, A.C.; Pedrosa, F. Nutritional status, dietary intake and serum levels of vitamin C upon diagnosis of cancer in children and adolescents. *Nutr. Hosp.*, 2012, 27, 496-503.
- [16] Jinnah, H.A. Lesch-Nyhan disease: from mechanism to model and back again. *Dis. Models. Mech.*, 2009, 2, 116-121.
- [17] Zhao, Y.; Yang, X.; Lu, W.; Liao, H.; Liao, F. Uricase based methods for determination of uric acid in serum. *Microchim Acta*, 2009, 164, 1-6.
- [18] Feng, S.L.; Wang, J.; Chen, X.G.; Fan, J. Kinetic spectrofluorimetric determination of trace ascorbic acid based on its inhibition on the oxidation of pyronine Y by nitrite. *Spectrochim. Acta. Part A*, 2005, 61, 841-844.
- [19] Kand'ar, R.; Drabkova, P.; Hampl, R. The determination of ascorbic acid and uric acid in human seminal plasma using an HPLC with UV detection. *J. Chromatogr. B*, 2011, 879, 2834-2839.
- [20] Liang, R.P.; Gan, G.H.; Qiu, J.D. Surface modification of poly(dimethylsiloxane) microfluidic devices and its application in simultaneous analysis of uric acid and ascorbic acid in human urine. *J. Sep. Sci.*, 2008, 31, 2860-2867.
- [21] Strohckova, E.M.; Tur'yan, Y.I.; Kuselman, I.; Shenhar, A. Simultaneous voltammetric determination of uric and ascorbic acids in urine. *Talanta*, 1997, 44, 1923-1928.

- [22] Zheng, D.; Ye, J.; Zhou, L.; Zhang, Y.; Yu, C. Simultaneous determination of dopamine, ascorbic acid and uric acid on ordered mesoporous carbon/Nafion composite film. *J. Electroanal. Chem.*, 2009, *625*, 82-87.
- [23] Premkumar, J.; Khoo, S.B. Electrocatalytic oxidations of biological molecules (ascorbic acid and uric acid) at highly oxidized electrodes. *J. Electroanal. Chem.*, 2005, *576*, 105-112.
- [24] Matos, R.C.; Augelli, M.A.; Lago, C.L.; Angnes, L. Flow injection analysis-amperometric determination of ascorbic and uric acids in urine using arrays of gold microelectrodes modified by electrodeposition of palladium. *Anal. Chim. Acta*, 2000, *404*, 151-157.
- [25] Noroozifar, M.; Khorasani-Motlagh, M.; Taheri, A. Preparation of silver hexacyanoferrate nanoparticles and its application for the simultaneous determination of ascorbic acid, dopamine and uric acid. *Talanta*, 2010, *80*, 1657-1664.
- [26] Hu, G.; Guo, Y.; Shao, S. Simultaneous determination of dopamine and ascorbic acid using the nano-gold self-assembled glassy carbon electrode. *Electroanalysis*, 2009, *21*, 1200-1206.
- [27] Wang, M.Y.; Xu, X.Y.; Yang, F.; Zhang, S.Y.; Yang, X.J. Development of an amperometric sensor for simultaneous determination of uric acid and ascorbic acid using 2-[bis(2-aminoethyl)amino]ethanol, 4,40-bipyridine bridged dicopper(II) complex. *J. Appl. Electrochem.*, 2008, *38*, 1269-1247.
- [28] Nassef, H.M.; Radi, A.E.; O'Sullivan, C. Simultaneous detection of ascorbate and uric acid using a selectively catalytic surface. *Anal. Chim. Acta*, 2007, *583*, 182-189.
- [29] Yue, Y.; Hu, G.; Zheng, M.; Guo, Y.; Cao, J.; Shao, S. A mesoporous carbon nanofiber-modified pyrolytic graphite electrode used for the simultaneous determination of dopamine, uric acid and ascorbic acid. *Carbon*, 2012, *50*, 107-114.
- [30] Habibia, B.; Pourmaghi-Azarb, M.H. Simultaneous determination of ascorbic acid, dopamine and uric acid by use of a MWCNT modified carbon-ceramic electrode and differential pulse voltammetry. *Electrochim. Acta*, 2010, *55*, 5492-5498.
- [31] Wang, C.; Yuan, R.; Chai, Y.; Chen, S.; Zhang, Y.; Hu, F.; Zhang, M. Non-covalent iron(III)-porphyrin functionalized multi-walled carbon nanotubes for the simultaneous determination of ascorbic acid, dopamine, uric acid and nitrite. *Electrochim. Acta*, 2012, *62*, 109-115.
- [32] Zare, H.R.; Shishehbore, M.R.; Nematollahi, D. A highly sensitive and selective sensor on the basis of 4-hydroxy-2-(triphenylphosphonio)phenolate and multi-wall carbon nanotubes for electrocatalytic determination of folic acid in presence of ascorbic and uric acid. *Electrochim. Acta*, 2011, *58*, 654-661.
- [33] Yang, S.; Li, G.; Yang R.; Xia, M.; Qu, L. Simultaneous voltammetric determination of dopamine and uric acid in the presence of high concentration of ascorbic acid using multi-walled carbon nanotubes with methylene blue composite film-modified electrode. *J. Solid State Electrochem.*, 2011, *15*, 1909-1918.
- [34] Li, Y.; Lin, X. Simultaneous electroanalysis of dopamine, ascorbic acid and uric acid by covalently modified glassy carbon electrode. *Sens. Actuators B*, 2006, *115*, 134-139.
- [35] da Silva, R.P.; Lima, A.W.O.; Serrano, S.H.P. Simultaneous voltammetric detection of ascorbic acid, dopamine and uric acid using a pyrolytic graphite electrode modified into dopamine solution. *Anal. Chim. Acta*, 2008, *613*, 89-98.
- [36] Safavi, A.; Maleki, N.; Moradlou, O.; Tajabadi, F. Simultaneous determination of dopamine, ascorbic acid and uric acid using carbon ionic liquid electrode. *Anal. Biochem.*, 2006, *359*, 224-229.
- [37] Özcan, A.; Sahin, Y. Preparation of selective and sensitive electrochemically treated pencil graphite electrodes for the determination of uric acid in urine and blood serum. *Biosens. Bioelectron.*, 2010, *25*, 2497-2502.
- [38] Shahrokhian, S.; Ghalkhani, M. Simultaneous voltammetric detection of ascorbic acid and uric acid at a carbon-paste modified electrode incorporating thionine-nafion ion-pair as an electron mediator. *Electrochim. Acta*, 2006, *51*, 2599-2606.
- [39] Dey, R.S.; Gupta, S.; Pairs, R.; Chen, S.M.; Raj, C.R. Flow injection amperometric sensing of uric acid and ascorbic acid using the self-assembly of heterocyclic thiol on Au electrode. *J. Solid State Electrochem.*, 2012, *16*, 173-178.
- [40] Atta, N.F.; El-Kady, M.F.; Galal, A. Simultaneous determination of catecholamines, uric acid and ascorbic acid at physiological levels using poly(N-methylpyrrole)/Pd nanoclusters sensors. *Anal. Biochem.*, 2010, *400*, 78-88.
- [41] Jeyalakshmi, S.R.; Kumar, S.S.; Mathiyarasu, J.; Phani, K.L.N.; Yegnarman, V. Simultaneous determination of ascorbic acid, dopamine and uric acid using PEDOT polymer modified electrodes. *Indian. J. Chem., Sect. A.*, 2007, *46*, 957-961.
- [42] Mazloum-Ardakani, M.; Sheikh-Mohseni, M.A.; Benvidi, A. Electropolymerization of thin film conducting polymer and its application for simultaneous determination of ascorbic acid, dopamine and uric acid. *Electroanalysis*, 2011, *23*, 2822-2831.
- [43] Atta, N.F.; El-Kady, M.F. Novel poly(3-methylthiophene)/Pd, Pt nanoparticles sensor: synthesis, characterization and its application to the simultaneous analysis of dopamine and ascorbic acid in biological fluids. *Sens. Actuators B*, 2010, *145*, 299-310.
- [44] Roncali, J. Conjugated poly(thiophenes): synthesis, functionalization and applications. *Chem. Rev.*, 1992, *92*, 711-738.
- [45] Guimard, N.K.; Gomez, N.; Schmidt, C.E. Conducting polymers in biomedical engineering. *Prog. Polym. Sci.*, 2007, *32*, 876-921.
- [46] Kumar, S.S.; Mathiyarasu, J.; Phani, K.L.; Jain, Y.K.; Yegnarman, V. Determination of uric acid in the presence of ascorbic acid using poly(3,4-ethylenedioxythiophene)-modified electrode. *Electroanalysis*, 2005, *17*, 2281-2286.
- [47] Balamurugan, A.; Chen, S.M. Poly(3,4-ethylenedioxythiophene-co-(5-amino-2-naphthalenesulfonic acid)) (PEDOT-PANS) film modified glassy carbon electrode for selective detection of dopamine in the presence of ascorbic acid and uric acid. *Anal. Chim. Acta*, 2007, *596*, 92-98.
- [48] Vasantha, V.S.; Chen, S.M. Synergistic effect of a catechin-immobilized poly(3,4-ethylenedioxythiophene)-modified electrode on electrocatalysis of NADH in the presence of ascorbic acid and uric acid. *Electrochim. Acta*, 2006, *52*, 665-674.
- [49] Lupu, S.; Mucci, A.; Pigani, L.; Seeber, R.; Zanardi, C. Polythiophene derivative conducting polymer modified electrodes and microelectrodes for determination of ascorbic acid. Effect of possible interferents. *Electroanalysis*, 2002, *14*, 519-525.
- [50] Polidori, M.C.; Stahl, W.; Eichler, O.; Niestroj, I.; Sies, H. Profiles of antioxidants in human plasma. *Free Rad. Biol. Med.*, 2001, *30*, 456-462.
- [51] Sekli-Belaidi, F.; Temple-Boyer, P.; Gros P. Voltammetric microsensor using PEDOT-modified gold electrode for the simultaneous assay of ascorbic and uric acids. *J. Electroanal. Chem.*, 2010, *647*, 159-168.
- [52] Ruffien-Ciszak, A.; Gros, P.; Comtat, M.; Schmitt, A.M.; Questel, E.; Casas, C.; Redoules, D. Exploration of the global antioxidant capacity of the stratum corneum by cyclic voltammetry. *J. Pharm. Biomed. Anal.*, 2006, *40*, 162-167.
- [53] Bello, A.; Gianneto, M.; Mori, G.; Seeber, R.; Terzi, F.; Zanardi, C. Optimization of the DPV potential waveform for determination of ascorbic acid on PEDOT-modified electrodes. *Sens. Actuators B*, 2007, *121*, 430-435.
- [54] Speck, A.-J.; Schrijver, J.; Scheur, W.-H. Fluorimetric determination of total vitamin C in whole blood by high performance liquid chromatography with pre-column derivatization. *J. Chromatogr.*, 1984, *305*, 53-60.
- [55] Barham, D.; Trinder, P.; An improved colour reagent for the determination of blood glucose by the oxidase system. *Analyst*, 1972, *97*, 142-145.
- [56] Martin, C.R.; Van Dyke, L.S. In: *Mass and Charge Transport in Electronically Conductive Polymers*; R. W. Murray, Ed.; Wiley: New York, 1992, pp. 403-424.
- [57] Schöpf, G.; Kößmehl, G. *Electrically Conductive Polymers*; Springer-Verlag: Berlin, 1997, p. 80.
- [58] Bard, A.J.; Faulkner, L.R. *Electrochimie: principes, méthodes et applications*; Masson: Paris, 1983, p. 486.
- [59] Sekli-Belaidi, F.; Evrard, E.; Gros P. Evidence of an EC' mechanism occurring during the simultaneous assay of ascorbic and uric acids on poly(3,4-ethylenedioxythiophene) modified gold microsensor. *Electrochem. Commun.*, 2011, *13*, 423-425.
- [60] Buettner, G.R.; Jurkiewicz, B.A. In: *Handbook of antioxidants*; E. Cadenas, L. Packer, Ed.; M. Dekker: New-York, 1996, pp. 91-115.
- [61] Jacob, C.; Giles, G.I.; Giles, N.M.; Sies, H. Sulfur and selenium: the role of oxidation state in protein structure and function. *Angew. Chem. Int. Ed.*, 2003, *42*, 4742-4758.