



HAL
open science

Development of an ultra thin beam profiler for charged particle beams

B. Boyer, R. Cornat, E. Delagnes, Y. Geerebaert, O. Gevin, F. Haddad, Charbel Koumeir, F. Magniette, P. Manigot, F. Poirier, et al.

► **To cite this version:**

B. Boyer, R. Cornat, E. Delagnes, Y. Geerebaert, O. Gevin, et al.. Development of an ultra thin beam profiler for charged particle beams. 14th Pisa Meeting on Advanced Detectors, May 2018, La Biodola-Isola d'Elba, Italy. pp.29-30, 10.1016/j.nima.2018.09.134 . hal-02475944

HAL Id: hal-02475944

<https://hal.science/hal-02475944>

Submitted on 25 Oct 2021

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Distributed under a Creative Commons Attribution - NonCommercial 4.0 International License

NIMA POST-PROCESS BANNER TO BE REMOVED AFTER FINAL ACCEPTANCE

Development of an ultra thin beam profiler for charged particle beams

B. Boyer^a, R. Cornat^c, E. Delagnes^d, Y. Geerebaert^a, O. Gevin^d, F. Haddad^{b,c}, C. Koumeir^b, F. Magniette^a, P. Manigot^a, F. Poirier^b, M. Rubio Roy^f, N. Servagent^c, C. Thiebaut^a, M. Verderi^a

^aLLR, Ecole polytechnique, CNRS/IN2P3, 91128 Palaiseau, France

^bGIP ARRONAX, Saint-Herblain, CNRS DR17, Rennes France

^cLaboratoire SUBATECH, IMT Atlantique, CNRS/IN2P3, Université de Nantes, France

^dIRFU, CEA, Université Paris-Saclay, F-91191 Gif-sur-Yvette, France

^eLaboratoire de Physique Nucléaire et des Hautes Energies, Sorbonne Université - CNRS/IN2P3

^fUniv. Grenoble Alpes, CNRS, CEA, Grenoble INP, INAC-SPINTEC, Grenoble, France

Abstract

Beam profiling during patient treatment in protontherapy requires ultra-thin monitors to preserve the high beam quality. For detectors upstream in the line, a material budget as low as $\sim 15 \mu\text{m}$ water-equivalent is needed. In addition, the current trend of dose escalation to treat highly resistant tumors implies challenging requirements on monitor radiation hardness and dynamic range. We propose a new type of beam profiler, PEPITES, using secondary electron emission (SEE) and built with thin-film techniques. The beam is profiled by crossing a pattern or a series of patterns which emit the SEE signal and can be made ultra-thin as SEE originates from the few nanometers next to the surface. The patterns are deposited on membranes, which, in contrast with common systems like ionization chambers, are free from mechanical constraints and can then afford higher absorbed doses and be as thin as achievable. A simple demonstrator prototype has been built and successfully operated with a proton beam at the ARRONAX cyclotron at St Herblain in a wide range of currents (100 fA to 10 nA) and several energies (30 - 68 MeV). Beam profiling results from these tests are presented, and our plans for the next prototypes are mentioned.

Keywords: , beam profiler, thin film, protontherapy

1. Motivation and detector principle

Protontherapy exploits the property of protons to deliver the maximum dose at the end of their track, resulting in the highest level of damages in the stopping area, deep in the tissues, called the Bragg peak. The depth can be adjusted by adapting the beam energy (between 70 and 230 MeV for medical cyclotrons). It is a benefit compared to gamma beams which deliver dose all along their paths. Moreover, with low lateral scattering in the tissues, proton beams remain focused on the tumor. The main medical indications are resistant, inoperable or pediatric cancers. Dose delivery requires a continuous and precise measurement of beam intensity, position and profile. When crossing the monitor material thicknesses, the beam undergoes a dispersion that should lead to a maximum sub-millimeter lateral spreading at the patient to be tolerable. The continuous presence of the monitor in the line also requires good resistance to radiation. The current trend of dose escalation to treat very resistant tumors with high intensity beams increases the

demand on monitors radiation tolerance and on their dynamic range.

We propose a 10 μm Water Equivalent Thickness beam monitor with high durability, wide dynamic range and easy operation. The device uses secondary electron emission (SEE) phenomenon. As a surface process, SEE allows very thin active layers: 5 nm of matter are sufficient to generate the full signal. Secondary electrons have very low energies (few eV) which implies to work in vacuum, in compliance with our use-case. The SEE yield is proportional to the dE/dx of the beam particles ([1], [2]) and is independent of the beam intensity up to currents far beyond the medical needs. The device contains one or several segmented electrodes which emit the signal when crossed by the beam. Their pattern is adapted to the beam to be profiled and is composed of conductive elements read independently. Patterns are deposited by metal evaporation or by sputtering onto thin non-conductive substrate and can be strips, pads, etc. Their thickness has to be large enough to allow elec-

37 trical conduction, which requires ~ 30 nm for a metal. The
 38 baseline monitor consists in two strip-based electrodes to measure
 39 the beam along the X and Y axes, perpendicular to its direction,
 40 and collection electrodes. Gold strips onto organic thermostable
 41 polymers have been used so far.

42 2. Experimental setup

43 We built a prototype profiler consisting of two electrodes
 44 (emission and collection) separated by a 1 cm gap. The emission
 45 electrode allows to test two different material combinations.
 46 The first one consists of gold strips (50 nm thick, 1.6 mm
 47 width, 0.35 mm interstrip, 6 cm length) on a 6 μ m PEEK foil
 48 substrate. The second part is a 100 nm thick, 1.4 x 1.4 cm²,
 49 Si₃N₄ membrane with one large gold strip (50 nm thick). The
 50 collection electrode is a 100 nm gold layer onto a 8 μ m, 6x6
 51 cm², Kapton[®] foil. Gold metallization was made by chemical
 52 vapor deposition on the polymers and sputtering on the Si₃N₄
 53 membrane. A +100V potential is applied to the collection elec-
 54 trode. A single low noise pico-ammeter (Keithley 6517B) is
 55 used for the signal readout. It is connected to the strips through
 56 a switch matrix to sequentially select the read strips. Command
 57 control and data acquisition are handled by the Pyrame frame-
 58 work developed at the LLR [3]. The detector is installed in a 25
 59 cm diameter cylindrical vacuum chamber placed on a transla-
 60 tion table for alignment with respect to the beam line exit about
 61 1 meter away. The chamber is equipped with 60 mm diameter
 62 entrance/exit beam windows made of a 3 mm sapphire glass in
 63 a first run (2016/09) and 230 μ m Kapton[®] foils in a second run
 64 (2017/03), to decrease the beam dispersion and the activation
 65 of the system. SRIM [4] has been used to calculate the beam
 66 energy loss from the beam line exit to the detector.

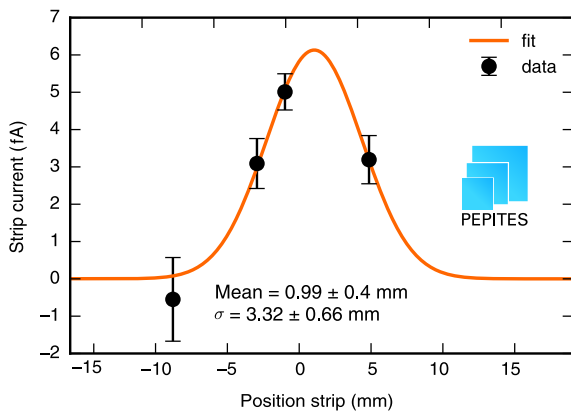


Figure 1: Profile with protons 60 MeV, $I_{beam} = 170$ fA, 4 strips connected

69 3. Results and discussion

70 Measurements have been carried out at the ARRONAX cy-
 71 clotron at St Herblain[5]. Profiles have been determined for

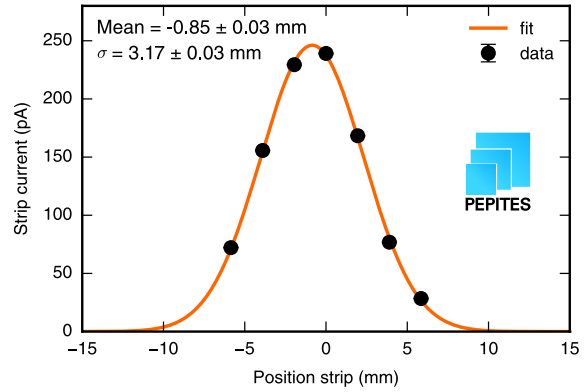


Figure 2: Profile with protons 66 MeV, $I_{beam} = 10$ nA, 7 strips connected

72 a wide range of protons beam currents: 170 fA up to 10 nA
 73 (Fig 1 and 2) and for several beam energies: 66, 60 and 27.9
 74 MeV. In addition, the beam profile at $I_{beam} = 100$ pA has been
 75 compared to the one measured by the DOSION[6] monitor, and
 76 found compatible. Signal with Si₃N₄+ gold sample has also
 77 been observed for different beam currents.

78 4. Conclusion

79 The principle of an ultra-thin beam monitor using SEE and
 80 based on thin film techniques has been validated. The next steps
 81 include studies on radiation tolerance, alternative patterns and
 82 materials, the development of a low noise electronic ASIC, to
 83 finally achieve a fully functional prototype of at least 2x8 chan-
 84 nels.

85 5. Acknowledgments

86 The authors wish to acknowledge Denis Tondelier (LPICM),
 87 Denis Bernard (LLR) and the HsFoils company. This project
 88 is funded by the ANR (ANR-17-CE31-0015) and the labex
 89 P2IO. It has been also, in part, supported by a grant from the
 90 French National Agency for Research called "Investissements
 91 d'Avenir", Equipex Arronax-Plus (ANR-11-EQPX-0004) and
 92 Labex IRON (ANR-11-LABX-18-01).

- 93 [1] E. J. Sternglass, Theory of secondary electron emission by high-speed ions,
 94 Phys. Rev. 108 (1957) 1–12. doi:10.1103/PhysRev.108.1.
 95 [2] J. Schou, Transport theory for kinetic emission of secondary electrons
 96 from solids by electron and ion bombardment, Nuclear Instruments and
 97 Methods 170 (1) (1980) 317 – 320. doi:https://doi.org/10.1016/0029-
 98 554X(80)91032-0.
 99 [3] F. Magniette, M. Rubio-Roy, F. Thiant, Pyrame, a rapid-prototyping frame-
 100 work for online systems, Journal of Physics, Conference Series Vol 664.
 101 [4] J. F. Ziegler, M. D. Ziegler, J. P. Biersack, SRIM - The stopping and range
 102 of ions in matter (2010), Nuclear Instruments and Methods in Physics Re-
 103 search B 268 (2010) 1818–1823. doi:10.1016/j.nimb.2010.02.091.
 104 [5] F. Poirier, S. Girault, S. Auduc, C. Huet, E. Mace, J.-L. Delvaux, F. Had-
 105 dad, THE C70 ARRONAX AND BEAM LINES STATUS, in: IPAC11,
 106 San Sebastian, Spain, 2011.
 107 URL <https://hal.archives-ouvertes.fr/hal-01378849>
 108 [6] G. Boissonnat, et al., Characterization and performances of DOSION, a
 109 dosimetry equipment dedicated to radiobiology experiments taking place
 110 at GANIL, Nucl. Instrum. Meth. A856 (2017) 1–6. arXiv:1607.06645,
 111 doi:10.1016/j.nima.2016.12.040.