



HAL
open science

A Uranium Atlas, from 365 to 505 nm

Amanda J. Ross, Patrick Crozet, Allan Adam, Dennis W. Tokaryk

► **To cite this version:**

Amanda J. Ross, Patrick Crozet, Allan Adam, Dennis W. Tokaryk. A Uranium Atlas, from 365 to 505 nm. *Journal of Molecular Spectroscopy*, 2020, 369, pp.111270. 10.1016/j.jms.2020.111270 . hal-02500613

HAL Id: hal-02500613

<https://hal.science/hal-02500613>

Submitted on 6 Mar 2020

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

A Uranium Atlas, from 365 to 505 nm

Amanda J. Ross¹, Patrick Crozet¹, Allan G. Adam² and Dennis W. Tokaryk³

¹Université de Lyon, Université Claude Bernard Lyon 1, CNRS, Institut Lumière Matière, F-69622, Villeurbanne, France

²Department of Chemistry and Centre for Laser, Atomic, and Molecular Sciences, University of New Brunswick, Fredericton, NB E3B 5A3, Canada


³Department of Physics and Centre for Laser, Atomic, and Molecular Sciences, University of New Brunswick, Fredericton, NB E3B 5A3, Canada

Abstract

A Fourier-transform spectrum of the emission from a commercial Uranium hollow-cathode lamp 19800 – 27400 cm^{-1} is proposed, in ascii format, as a possible aid to calibration of laser excitation spectra.

Corresponding Author : Dr Amanda Ross, amanda.ross@univ-lyon1.fr

Graphical Abstract

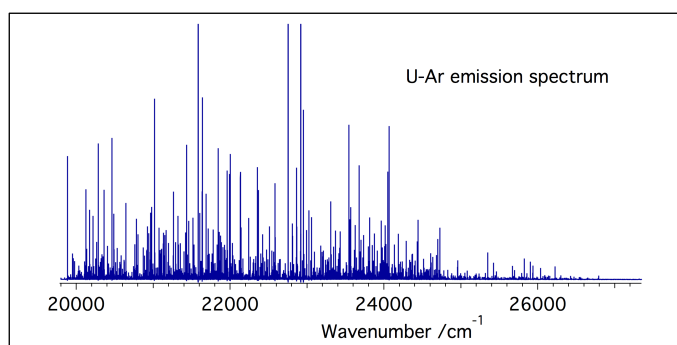

Introduction

It can sometimes be convenient to compare spectral reference signals with an original reference spectrum, rather than matching peaks with a list of peak positions from an atlas. This work was motivated by difficulties encountered in calibrating laser excitation spectra taken in short (1 cm^{-1}) scans with a ring dye laser around 438 nm, using optogalvanic lines from a uranium + argon hollow-cathode lamp as reference. Uranium has a rich spectrum in this region; a modest selection of transitions between 15,870 and 25,900 cm^{-1} was published from spectra recorded at

Laboratoire Aimé Cotton in France in 1977 [1], followed by a much more extensive catalogue of lines 11,000 – 25,900 cm^{-1} recorded at Los Alamos in 1980 [2] presented as a spectral atlas, and recommended for optogalvanic calibration[3]. Because the peaks of the weaker features are not quoted in these sources, short pieces of excitation spectra sometimes fall between secure calibration lines. To remedy this, we have recorded the spectrum from a U + Ar hollow-cathode lamp 19,800 – 27,400 cm^{-1} , covering shorter wavelengths than the (much richer) digital I₂ atlas [4] recorded for much the same purpose. This U + Ar spectrum

is available in ascii format (supplementary material). It is a convenient extension to the recent work of Sarmiento and co-workers [5], who advocate the use of uranium (in preference to thorium) hollow-cathode lamps for calibration of high-resolution astronomical spectrographs operating in the near IR and visible. Ref. [5] covered the spectral bandwidth of the CARMENES instrument (500–1700 nm), and the 25 vacuum wavenumbers for peaks in the region common to both match to within quoted uncertainties, and with average difference 0.0004 cm^{-1} . Redman and co-workers have examined uranium hollow-cathode lamp emission still further to the infrared [6, 7], also in the context of calibration of astronomical instruments where frequency comb standards are not available.

Experiment

We recorded emission from a commercial (Cathodeon) Uranium + argon hollow-cathode lamp running at 135 V, 50 mA. The spectrum was recorded in two pieces on a Fourier transform spectrometer (Bomem DA3) using a quartz beamsplitter optimised for the visible spectrum, and a trialkali photomultiplier (EMI 9558QB) as detector. The longer wavelength section, $19800 - 23000\text{ cm}^{-1}$ was recorded through two optical filters, one blue-green band pass (CS 4-76 from Corning Glass), the other $\lambda < 500\text{ nm}$ (Corion Inc). The second part was recorded through a $\lambda < 450\text{ nm}$ sharp cut filter (Corion Inc) using higher photomultiplier sensitivity to compensate lower signals in this region. The optical path difference for the FT spectrometer was chosen to give an apodised resolution of

0.04 cm^{-1} . Interferograms were re-processed (correcting for phase errors and zero-padding to interpolate between data points) with in-house software [8] to improve on line shapes.

The wavenumber scales were also processed to match a selection of some 150 peaks tabulated in the existing atlases of refs [1] and [2]. The spectrum recorded at Laboratoire Aimé Cotton [1] came from a liquid nitrogen-cooled hollow cathode, with full-width half-maximum linewidths less than 0.02 cm^{-1} . The peaks were on average 0.002 cm^{-1} lower than those from the Los Alamos work (in which the authors gave an estimated accuracy of 0.003 cm^{-1}), taken with a water-cooled commercial lamp. After making small corrections to our raw wavenumber scale, (-0.003 cm^{-1} at $20,000\text{ cm}^{-1}$, increasing to 0.014 cm^{-1} at $27,000\text{ cm}^{-1}$, probably resulting from imperfect setting of the entrance aperture for the instrument), the two pieces were spliced together, merging just below $23,200\text{ cm}^{-1}$. The resulting spectrum is illustrated in Figure 1. The inset highlights the region at shorter wavelength not covered in ref. [2]; in which ref. [1] reports just 7 transitions.

Measured linewidths are between 0.05 and 0.075 cm^{-1} , comparable with the effective resolution at the short wavelength region in ref. [2]; peak positions should be determined to better than 0.005 cm^{-1} . To illustrate consistency with the earlier works, Figure 2 depicts the deviations of peak positions determined from this composite spectrum with respect to our selection of transitions listed in the literature.

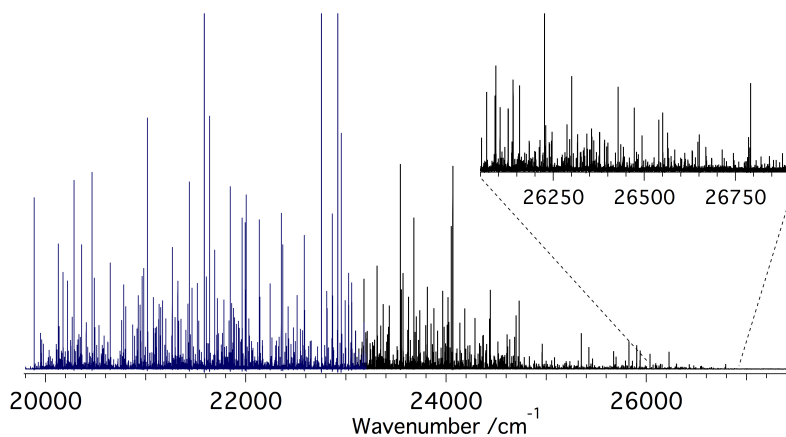


Figure 1 (colour online). Emission from a uranium+argon hollow-cathode lamp, with no correction for instrumental intensity response. Different optical filters were used below and above $23,200\text{ cm}^{-1}$ (see text). The inset shows the region beyond the spectrum of ref. [2].

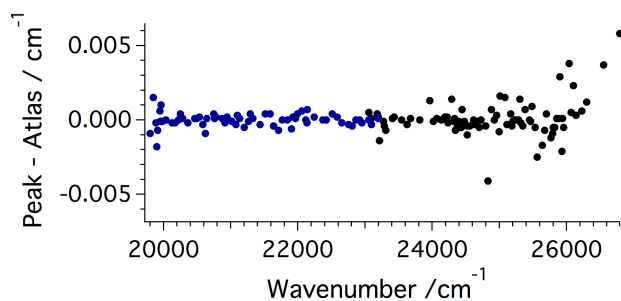


Figure 2. Scatter plot showing differences in cm^{-1} between peak positions taken from this spectrum and a selection of peak positions listed in existing atlases, mostly from ref. [2], but including peaks from ref. [5] below $19,900 \text{ cm}^{-1}$ and from ref. [1] above $25,000 \text{ cm}^{-1}$.

The complete composite spectrum of the uranium + argon lamp is available to download in Ascii format (supplementary data), or may be obtained on request to the authors. We believe it matches the estimated accuracy of the Los Alamos atlas (0.003 cm^{-1}) at least up to $26,000 \text{ cm}^{-1}$. At shorter wavelengths, performance may be degraded, but differences with other sources remain within 0.005 cm^{-1} .

Acknowledgements.

Financial support for this work came from NSERC, Canada, and from CNRS, France. AA wishes to acknowledge funding from Université Claude Bernard as visiting professor in October 2019, and from the Harrison McCain foundation in Canada.

Supplementary material can be found online, (<https://doi.org/10.1016/j.jms.2020.111270>)

References

- 1 Uranium and iodine standards measured by means of Fourier-transform spectroscopy; S. Gerstenkorn, P. Luc, A. Perrin and J. Chauville; *Astronomy & Astrophysics*, **58**, 255-66, (1977);
- 2 AN ATLAS OF URANIUM EMISSION INTENSITIES IN A HOLLOW CATHODE DISCHARGE; B. A. Palmer, R. A. Keller and R. Engleman Jr; Los Alamos informal report, *LA 8251-MS*, (1980); the wavenumbers quoted in this atlas are shifted with respect to the raw spectrum available on the Kitt Peak historical archive (<https://www.nso.edu/data/historical-archive>).
- 3 Atlas for optogalvanic wavelength calibration; R. A. Keller, R. Engleman and B. A. Palmer; *Appl. Opt.*, **19**, 836-37, (1980); doi.org/10.1364/ao.19.000836
- 4 A molecular iodine atlas in ascii format; H. Salami and A. J. Ross; *J. Mol. Spectrosc.*, **233**, 157-59, (2005); doi.org/10.1016/j.jms.2005.06.002
- 5 Comparing the emission spectra of U and Th hollow cathode lamps and a new U line list; L. F. Sarmiento, A. Reiners, P. Huke, F. Bauer, E. W. Guenter, U. Seemann and U. Wolter; *Astronomy & Astrophysics*, **618**, (2018); doi.org/10.1051/0004-6361/201832871
- 6 A high-resolution atlas of uranium-neon in the H band; S. L. Redman, G. G. Ycas, R. Terrien, S. Mahadevan, L. W. Ramsey, C. F. Bender, S. N. Osterman, S. A. Diddams, F. Quinlan, J. E. Lawler and G. Nave; *Astrophys. J. Supp. Ser.*, **199**, (2012); doi.org/10.1088/0067-0049/199/1/2
- 7 THE INFRARED SPECTRUM OF URANIUM HOLLOW CATHODE LAMPS FROM 850 nm to 4000 nm: WAVENUMBERS AND LINE IDENTIFICATIONS FROM FOURIER TRANSFORM SPECTRA; S. L. Redman, J. E. Lawler, G. Nave, L. W. Ramsey and S. Mahadevan; *Astrophys. J. Supp. Ser.*, **195**, (2011); doi.org/10.1088/0067-0049/195/2/24
- 8 An alternative approach to interferogram collection and processing for a vintage Bomem DA3 Fourier transform spectrometer; B. G. Guislain, R. A. R. Harvey, D. W. Tokaryk, A. J. Ross, P. Crozet and A. G. Adam; *J. Mol. Spectrosc.*, **364**, (2019); doi.org/10.1016/j.jms.2019.111181