



HAL
open science

A data-driven classification solution for the timed-up and go test in risk falling assessment

Levy Batista, Mathieu Milhem, Thierry Bastogne, Fabien Clanché, Gabin Personeni, Jean-Philippe Jehl, G r me Gauchard

► **To cite this version:**

Levy Batista, Mathieu Milhem, Thierry Bastogne, Fabien Clanch , Gabin Personeni, et al.. A data-driven classification solution for the timed-up and go test in risk falling assessment. 42nd Engineering in Medicine and Biology Conference, EMBC 2020, Jul 2020, Montr al, Canada. hal-02568440

HAL Id: hal-02568440

<https://hal.science/hal-02568440v1>

Submitted on 9 May 2020

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destin e au d p t et   la diffusion de documents scientifiques de niveau recherche, publi s ou non,  manant des  tablissements d'enseignement et de recherche fran ais ou  trangers, des laboratoires publics ou priv s.

A data-driven classification solution for the Timed-Up and Go test in Risk Falling Assessment

Levy Batista, Mathieu Milhem, Thierry Bastogne, Fablien Clanché, Gabin Personeni, Jean-Philippe Jehl and G r me Gauchard

Abstract— This study presents a new version of the TUG test used to diagnose the falling risk in elderly persons. Patients are equipped with wearable inertial sensors and a classification algorithm is implemented to predict the risk.

Clinical Relevance— This new test would allow clinicians to improve the diagnostic efficiency of the TUG test while preserving its simplicity of application.

I. INTRODUCTION

The present study addresses the issue of automated classification methods of healthy and risky subjects based on the Timed-Up and Go test. This test was introduced in 1991 by Podsiadlo and Richardson [1] and since many other studies have proposed to improve its diagnostic performances. However, Barry *et al.* have shown in 2014 the poor performances of the current test [2] with a sensitivity of only 32%. In this study, our goal is to keep the simplicity of the test while improving its sensitivity performances by analyzing signals recorded during the tests by inertial wearable sensors.

II. METHODS

An age simulation suit was used by four different subjects who performed the TUG test in triplicate with and without the simulation suit. Each subject was equipped with five wearable inertial sensors at five specific positions: neck, belt, right wrist, left and right foot. The inertial sensors used for the test were MetaMotionR sensors developed by Mientlab Inc. This technology is composed of a BMI160 6-axis Accelerometer + Gyroscope, a BMM150 3-axis Magnetometer, a BOSCH 9-axis Sensor Fusion, a 8MB Flash Memory and a lithium-ion rechargeable battery. 9 signals (accelerometry, gyrometry and magnetometry) were measured during each run.

The implemented method is decomposed as follows: time synchronization, axis recovery, pitch and roll estimation by a Kalman filter, followed by the yaw angle reconstruction, the probabilistic estimation of two statistics: direction and motion, the motion decomposition into four phases, feature extraction (duration, vertical accelerometry magnitude and frequency)

*Research supported by MAIF Foundation.

L Batista, M Milhem, and T. Bastogne are with CYBERnano, 193 avenue Paul Muller, 54180, Villers-l s-Nancy, FRANCE.

T. Bastogne is with the Universit  de Lorraine, CNRS, CRAN, and the INRIA BIGS, F-54000 Nancy, FRANCE.

J-P Jehl is with the Universit  de Lorraine, CNRS, IJL, F-54000 Nancy, FRANCE

F Clanch , G. Personeni, and G Gauchard are with the Universit  de Lorraine, DevAH, F-54000 Nancy, France.

for each motion phase, and finally motion classification. The latter step was based on a logistic regression model using 12 motion features as discrimination variables. A total of 24 runs were carried out using a full factorial design of experiments.

III. RESULTS

For four different positions of the sensor, the logistic model was able to discriminate positive and negative runs with 100% of sensitivity and specificity, except for the use on the wrist. That position was not able to provide informative signals for the TUG test. The logistic model was only composed of two motion features: duration of the turn round and duration of the return phase.

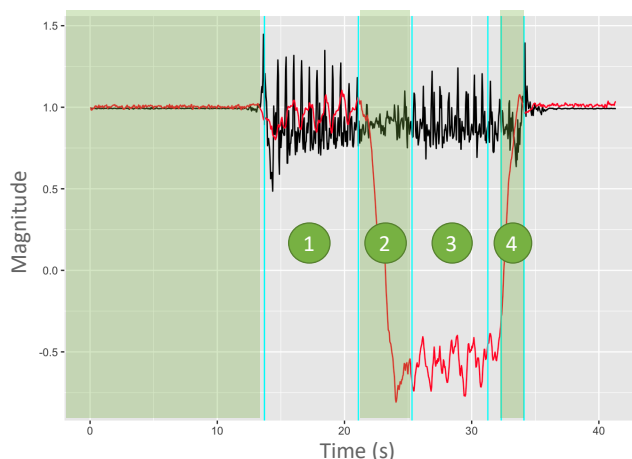


Figure 1. Automatic TUG Motion Segmentation. 4 phases of the TUG test during a pilot trial. Black: vertical accelerometry. Red: yaw angle

IV. DISCUSSION & CONCLUSION

This pilot study has shown the proof of concept of an improved TUG test using inertial wearable sensors associated with a sensor fusion method and a logistic regression model. An automatic TUG motion segmentation was successfully tested and two discriminant motion features were identified. New experiments are ongoing on real patients to confirm the performances obtained with the age simulation suit.

REFERENCES

- [1] PODSIADLO, Diane et RICHARDSON, Sandra. The timed ‘‘Up & Go’’: a test of basic functional mobility for frail elderly persons. *Journal of the American geriatrics Society*, 1991, vol. 39, no 2, p. 142-148.
- [2] BARRY, Emma, GALVIN Rose, KEOGH Claire, HORGAN Frances, FAHEY Tom. Is the timed up and go test a useful predictor of risk of falls in community dwelling older adults: a systematic review and meta-analysis. *BMC Geriatrics*, 14(1):14, 2014.