



HAL
open science

Antibacterial properties of metal and PDMS surfaces under weak electric fields

Yuzhen Lou, Pascal Thebault, Fabrice Burel, Nasreddine Kébir

► **To cite this version:**

Yuzhen Lou, Pascal Thebault, Fabrice Burel, Nasreddine Kébir. Antibacterial properties of metal and PDMS surfaces under weak electric fields. *Surface and Coatings Technology*, 2020, 394, pp.125912. <10.1016/j.surfcoat.2020.125912>. <hal-03017754>

HAL Id: hal-03017754

<https://hal.science/hal-03017754v1>

Submitted on 22 Aug 2022

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire HAL, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Distributed under a Creative Commons CC BY-NC 4.0 - Attribution - Non-commercial use - International License

Antibacterial properties of metal and PDMS surfaces under weak electric fields

Yuzhen LOU¹, Pascal THEBAULT², Fabrice BUREL¹, Nasreddine KEBIR¹

¹Normandie Université, INSA Rouen Normandie, Laboratoire PBS, UMR CNRS 6270 & FR 3038, Avenue de l'Université, 76801 Saint Etienne du Rouvray, France.

²Normandie Université, UNIROUEN, Laboratoire PBS, UMR CNRS 6270 & FR 3038, 76821 Mont-Saint-Aignan, France.

Correspondence to:

Nasreddine KEBIR (E-mail: nasreddine.kebir@insa-rouen.fr)

Pascal THEBAULT (E-mail: pascal.thebault@univ-rouen.fr)

Abstract:

The adhesion of several species of bacteria on two parallel rectangular electrodes under weak electric fields was studied. The electrodes were based on native metal or PDMS coated Cu. After 2 hours of contact at a voltage of 0.2 to 1V without any current, the Zn cathode showed a bacterial repellent effect with a difference in bacterial adhesion of about 1.5 to 2 log CFU/cm² on the anode. Al electrodes were inactive due to their passivation by the alumina layer. At 1V, both Zn and Al exhibited more than 80% mortality of suspended bacteria. The Cu electrodes showed a very high bactericidal effect even at 0V, and the bacterial adhesion on its surface was too weak to see a difference between the two electrodes. A similar study carried out on PDMS surfaces, covering Cu electrodes, revealed that a difference of 1 log CFU/cm² of bacterial adhesion between the cathode and anode surfaces can be obtained by applying a voltage ranging from 10 to 30V. This cathodic repellent effect was specific to staphylococcus species, suggesting that in the presence of a PDMS coating, the electrostatic forces on the surface are too low to be the main factor governing bacterial adhesion.

Keywords: Electrical field; Bacterial adhesion; PDMS; Metallic surface; Bactericidal effect.

1. Introduction

Microbial contamination of surfaces often leads to the formation of a biofilm, resulting in serious problems for human health (e.g. device-related infections, healthcare-related infections) as well as for industrial sectors (e.g. corrosion of metal surfaces, food contamination, deterioration of pipes...), leading to a negative socio-economic impact [1-3].

However, it should be noted that bacteria in their biofilms require antibiotic concentrations 100 to 1000 times higher than those of planktonic bacteria to achieve effective eradication [4]. Therefore, the development of materials capable of preventing the adhesion of bacteria and/or the formation of biofilms on their surface is a key element to avoid contamination. Gottenbos *et al.* have reported that the initial attachment of bacteria depends on the result of non-specific interactions such as Van der Waals, electrostatic, acid-base interactions and Brownian motion forces [5]. Dunne *et al* also reported that once the bacteria approach surfaces at a critical distance (usually less than 1 nm), adhesion is determined by the net sum of attractive or repulsive forces, including electrostatic and hydrophobic interactions, steric hindrance, van der Waals forces etc [6].

Three types of antibacterial surfaces are described in the literature: anti-adhesive surfaces, contact-killing surfaces and release-based surfaces [7].

Anti-adhesive surfaces are designed to repel bacteria by optimizing their physico-chemical properties such as the surface charge (negative charges), the wettability or the topography (micro/nano-patterned surfaces) [8-11]. However, they cannot affect the viability of pathogen that can be released to contaminate others. Furthermore, the use of physical surface modifications (particularly surface topography) as non-specific methods to prevent the bacterial adhesion is much more complex than we can imagine [12].

Contact-killing surfaces which are generally based on cationic biocidal agents covalently bonded to substrate surfaces that attract negatively charged bacteria and kill them by disrupting their cell membrane [13-15]. However, these surfaces quickly become inactive after being buried under a layer of dead bacteria.

Released-based surfaces are designed to leach antibacterial agents that kill not only adhered bacteria but also planktonic bacteria [16-18]. The disadvantage of this kind of surfaces is its limited activity owing to the limited amount of the loaded antibacterial compounds. However, excessive use of antibiotics may lead to the phenomenon of bacterial resistance [19].

It is noteworthy that the use of an electrical method to prevent infection of medical devices, without traumatising the patient by removal of the device, is of great interest. In addition, over time, bacteria should not adapt as well with electrical treatment as with antibiotics [20]. Direct and alternating currents [21, 22] as well as acoustic (by piezo-electric actuators) [23] and radio frequency wave [24] treatments have already proven to be effective techniques to prevent initial bacterial adhesion and growth, through *in vitro* and *in vivo* experiments. On the other hand, the electrical current has been found to increase the efficacy of antibiofilm agents in a synergistic action called 'the bioelectric effect' [25-29], which can lead to a dramatic decrease in the concentration of the antibiofilm compounds used. Thus, the development of electrically stimulated surfaces that prevent bacterial adhesion and biofilm formation is an emergent and attractive pathway.

Busalmen *et al.* [30] have studied, using an optical microscope, the influence of an electrical field on the adhesion of *Pseudomonas fluorescens* onto the surface of gold electrodes, under flow conditions at two different ionic strengths (0.01 and 0.1 M NaCl; pH 7). By applying negative electric potentials (-0.5 and -0.2V relative to a reference electrode [Ag/AgCl-KCl saturated solution]), they have evidenced a decrease in bacterial adhesion of one Log (CFU/mm²) after 15 min of contact, compared to adhesion at a potential of 0.2V. In another work [31], using the same system, they demonstrated the impact of this electrical field on the growth of planktonic cells and biofilms of *Pseudomonas fluorescens* (cell morphology, size at cell division, time to division, and biofilm structure). Gall *et al.* [32] have studied, using Quartz Crystal Microbalance with Dissipation analysis (QCM-D), the effect of applying an electrical field, perpendicular to the flow of a *Pseudomonas fluorescens*

suspension, on the adhesion of bacterial cells to the gold electrode. Surprisingly, they demonstrated that the tested bacteria were rigidly attached to the negatively charged surface, unlike to the positively charged one, suggesting that the applied electric potential could influence the conformation of the bacterial cell surface, allowing the cells to overcome the electrostatic energy barrier.

In this study, we investigated the adhesion of different bacterial species, in a static mode (without flow), on metallic and PDMS surfaces under an electrical field (without any current), generated by two parallel metal electrodes (as in a capacitor) immersed in an aqueous suspension of bacteria. The impact of the applied electrical field on bacterial survival has also been studied.

2. Materials and methods

Materials

Sylgard[®] 184 was purchased from DOW chemical company (USA) and was used as the coating material. Copper, zinc and aluminum blades (10×100×1.5 mm³, Jeulin, France) were used as electrodes. *Staphylococcus aureus* (ATCC 29213), *Staphylococcus epidermidis* (ATCC 35984), *Enterococcus faecalis* (ATCC 29212), *Pseudomonas aeruginosa* (PA14) and *Escherichia coli* (K12 MG1655) strains were stored as frozen aliquots in brain heart infusion broth (BHI, Bacto, France) and 30% of glycerol at -20°C. Ultrapure water, obtained from a Milli-Q system (Siemens, France), was used in all cases.

Preparation of PDMS-coated copper or zinc electrodes

15 g of the two parts of Sylgard[®] 184, i.e. silicone elastomer base and curing agent, in a ratio of 10:1 (w/w) were mixed and casted into a low-density polyethylene petri dish square (120×120×17 mm³). Then, the mixture was degassed under vacuum, until all air bubbles were removed, and cured at 70 °C for 3 h to form a first PDMS layer. Six blades were then put on top of this layer and covered with a second layer of PDMS (20 g) using the same process. The resulting PDMS-coated electrodes (12×3.5×40 mm³) were cut out by using a scalpel. The thickness of the coating was around 1 mm.

Preparation of Bacterial suspensions

For each experiment, all bacterial species were pre-cultured in BHI at 37°C under shaking at 140 rpm for approximately 16 h. Then, bacteria were harvested by centrifugation (Sigma® 3-16KL, rotor 19776, Germany) under 1600 g for 15 minutes at 20°C and resuspended at a concentration of $10^7 \sim 10^8$ CFU/ml in Milli-Q water to avoid the influence of charged particles in BHI or Phosphate Buffered Saline (PBS, Gibco, UK).

Zeta potential measurements

Zeta potentials of bacteria were measured with a Zetasizer Nano-ZS system (Malvern Panalytical, Ltd., UK) at 25 °C in Milli-Q water solution at $10^7 \sim 10^8$ CFU/ml. Three measurements were carried out for each bacterial suspension.

Assessment of bacteria attachment onto PDMS and metallic blade surfaces under an electric field

The process used to evaluate the attachment of bacteria to the surface of metallic or PDMS-coated electrodes is shown in Figure 1. The PDMS-coated electrodes were sterilized in 70% ethanol overnight and washed twice with Milli-Q water before use. Uncoated electrodes were sterilized in 70% ethanol for 20 min, followed by sonication for 30 min, and washed twice with Milli-Q water before use.

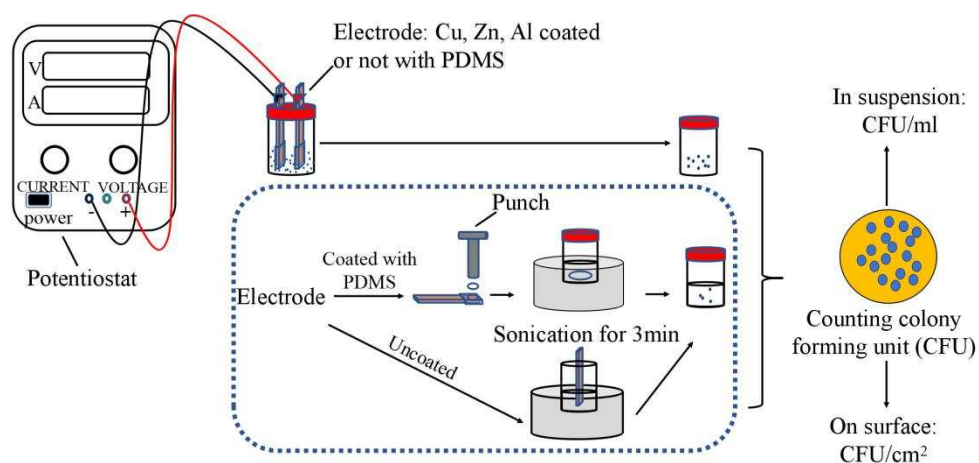


Figure 1. Process used to evaluate the adhesion of bacteria to the surface of metallic or PDMS-coated electrodes

The bacterial adhesion was studied in a system of parallel plates with a distance of 1 cm between the two electrodes connected to the potentiostat (0-30 V,

Velleman[®]). The electrodes were immersed (1 cm) in 7 ml of the previous prepared bacterial suspension during 2 h. Then, to remove unattached bacteria, these electrodes were washed in 15 ml of sterile Milli-Q water under slight shaking while the potentiostat was still on. They were then detached from the potentiostat. To recover the bacteria fixed to the surface, metallic electrodes were directly immersed in 7 mL of PBS solution, under sonication for 3 min. For PDMS-coated electrodes, a sample of PDMS was taken with a circular punch ($\varnothing=1$ cm) and was immersed in 3 ml of PBS solution under sonication for 3 min. Decimal dilutions of the resulting bacterial suspensions, containing bacteria detached from the surface, as well as those where the experiments were conducted, containing unattached surviving bacteria, were spread (20 μ l or 100 μ l) on BHI agar plates and incubated at 37°C for 24 h before colony counting. All experiments were performed in at least triplicate.

3. Results and discussion

Bacterial adhesion onto a surface is often explained by the Derjaguin, Landau, Verwey and Overbeek (DLVO) theory of colloidal stability. It describes initially repulsive electrical double layer interactions (electrostatic repulsion) between bacteria and similarly charged surfaces. At the same time, bacteria are attracted by van der Waals forces and approach surface contact as soon as they cross the electrostatic energy barrier by decreasing the interfacial distance. [5,6]

In this work, we aimed to use an electrical field to increase electrostatic forces between bacteria and cathodic (negatively charged) surfaces, in order to decrease bacterial adhesion and colonization. Thus, we have used two parallel electrodes, as in a capacitor, immersed in an aqueous suspension of bacteria (Figure 2). Cu, Al and Zn were used as models for metallic electrodes; PDMS was used as representative electrodes for plastic-based biomaterials.

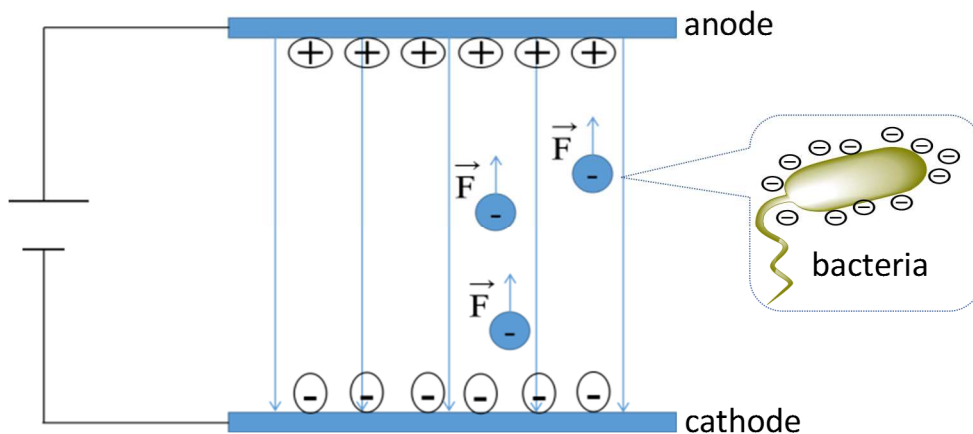


Figure 2. Schematic principle of antibacterial action of cathode.

3.1. Bacterial adhesion to metal electrodes

The results of the enumeration of live *S. aureus* adhering to electrodes of Cu, Zn and Al, after immersion in bacterial suspensions for 2 hours at an electrical voltage of 0 to 1 V, are shown in Figure 3 (A1). Above 1 V, the presence of current and electrolysis reactions can be observed, making it unnecessary to study electrostatic interactions. The survival of suspended bacteria was also monitored before and after immersion of the electrodes (Figure 3 (A2)).

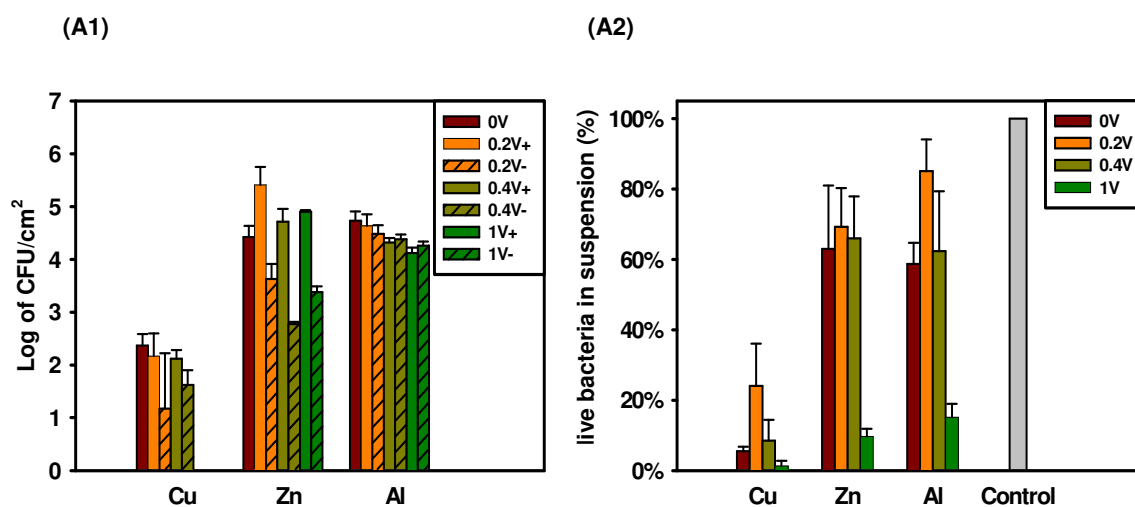


Figure 3. Adhesion of *S. aureus* onto the surface of Cu, Zn and Al after 2h of contact under 0, 0.2, 0.4 and 1V: (A1) live bacteria adhered to the surface; (A2) live bacteria in suspension; control: live bacteria in suspension without any electrode.

For copper electrodes at 0 V, the concentration of adhered *S. aureus* was only about 2 log of CFU/cm² (Figure 3 (A1)). This low adhesion can be explained by the well-known bactericidal properties of copper [33-35], which is confirmed by the percentage of bacterial surviving in solution (Figure 3 (A2)). Indeed, less than 20 % of bacteria in solution are still alive (or cultivable) after 2 h. However, a slight difference in bacterial adhesion between anode (positively charged) and cathode (negatively charged) at 0.2 and 0.4 V was observed. Furthermore, the increase of voltage to 1 V, suppressed the adhesion of *S. aureus* onto the surface and increased the suspended bacterial mortality to more than 95 %. These results suggest that the bactericidal effect of copper could be enhanced by the application of an electric field and are consistent with the "bioelectric effect" [25-29].

For the two other electrodes, a bacterial adhesion of approximately 4.5 log of CFU/cm² was achieved at 0 V. In the case of Al, no difference in bacterial adhesion between cathode and anode was observed regardless of the applied voltage. This could be explained by the well-known passivation of the aluminum surface by oxidation leading to the formation of a thin layer of alumina, which is an ionic salt (Al₂O₃). The electrical properties of this layer are very different from those of its pure metal, and its electrochemical static polarization is more difficult to achieve. For Zn electrodes, at all applied voltages, there was a decrease in the adhesion of *S. aureus* on the cathode compared to bacterial adhesion at 0V. At the same time, a slight increase on the anode was observed inducing a difference of more or less 2 log of CFU/cm² between these two electrodes. This result suggests that electrostatic interactions are, in this case, quite predominant. Therefore, this result also indicates that bacterial adhesion could be modulated on the Zn electrodes by the use of an electric field. Moreover, for a voltage ranging from 0 to 0.4V, an insignificant decrease, of about 10 to 40%, of live bacteria in suspension was observed for both Al and Zn electrodes. However, at 1 V, a decrease in the live bacteria population in solution of about 80 % was observed for both electrodes. Soumya *et al.* [36] reported that potentials at about 0.9 V would affect the redox potential across the cell membrane and disrupt redox

homeostasis, thereby accelerating the production of endogenous reactive oxygen species (ROS) and inhibiting bacterial growth. In summary, these results show that the nature of the electrode and the voltage values have an impact on the adhesion of *S. aureus* to the surface as well as on suspended bacterial mortality.

On the other hand, in order to determine whether the structure of the external membrane of bacteria cells has any influence on these results, we studied the adhesion of *E. coli*, as a model of Gram-negative bacteria, to zinc electrodes under voltage values ranging from 0 to 1 V.

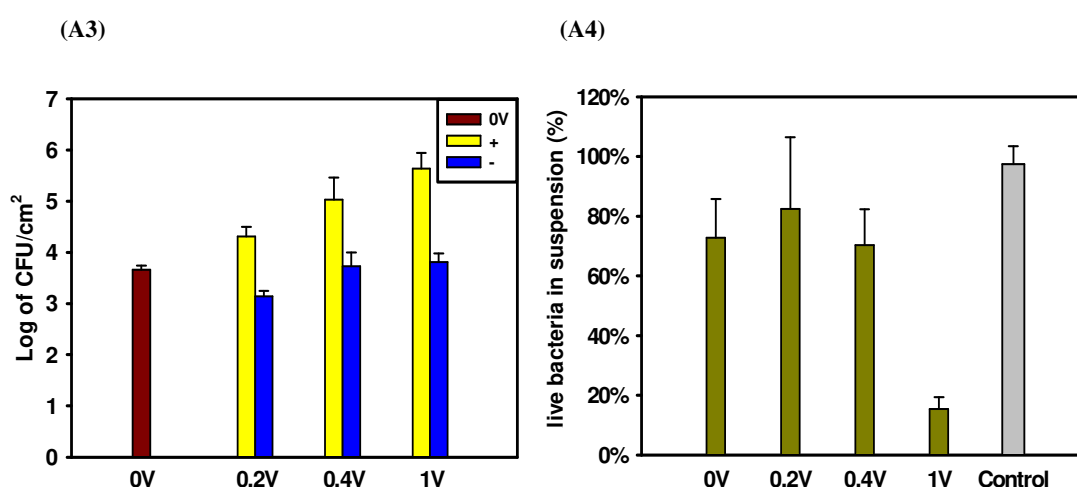


Figure 4. Adhesion of *E. coli* to the surface of zinc electrodes after 2h of contact at voltage values between 0 and 1 V: (A3) live bacteria adhered to the surface; (A4) live bacteria in suspension; control: live bacteria in suspension without any electrode.

Figure 4 shows that *E. coli* behaves almost similarly to *S. aureus* in terms of adhesion to the Zn electrodes after 2 h of contact. Indeed, a difference in *E. coli* adhesion of about 1.5 to 2 log of CFU/cm² between the anode and cathode was observed. In addition, the percentage of killing of *E. coli* in suspension was also quite similar to that of *S. aureus*, i.e. low for a voltage of 0, 0.2 or 0.4 V, and higher than 80% at 1 V.

Experiments were then carried out with different types of bacteria to verify whether these results are universal or not on zinc electrodes. The bacteria chosen are the most representative species involved in the phenomenon of contamination in the hospital environment. *S. epidermidis* and *E. faecalis* are Gram-positive bacteria and mainly cause skin and endocardial infections, respectively [37, 38]. Gram-negative bacteria such as *P. aeruginosa* and *E. coli* account for more than 30 % of nosocomial

infections [37]. *P. aeruginosa* causes several infections in human organs such as the urinary, blood, respiratory and gastrointestinal systems [40]. *E. coli* can also cause urinary or bloodstream infections for example [41]. These experiments were performed only at 0 and 0.2 V.

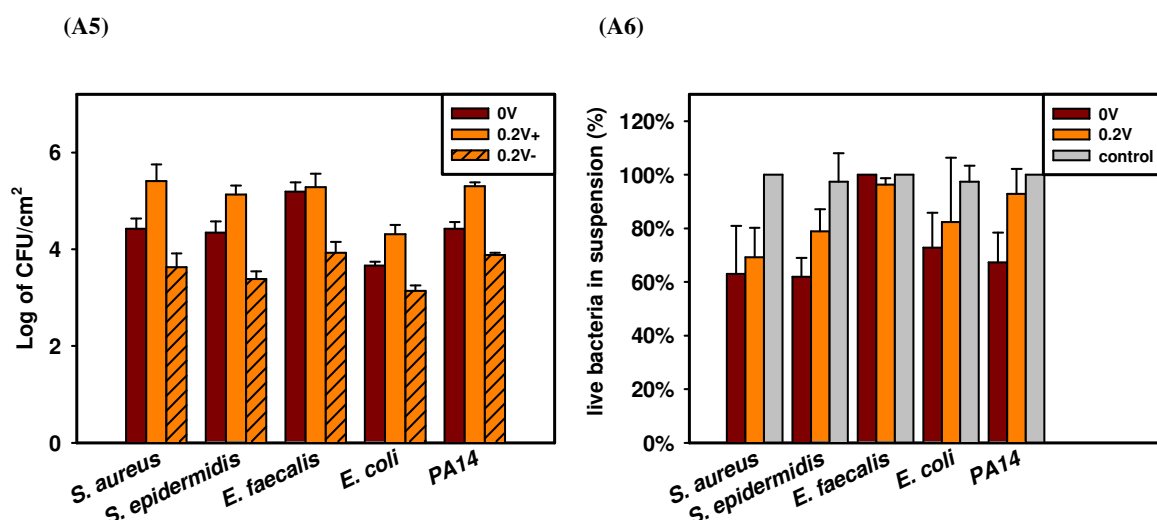


Figure 5. Adhesion of different bacterial species to the surface of zinc after 2h of contact at voltage values of 0 and 0.2 V: (A5) live bacteria adhered to the surface; (A6) live bacteria in suspension, control: live bacteria in suspension without any electrode.

As shown in Figure 5, at 0.2 V, a difference of bacterial adhesion was obtained between the cathode and the anode for each strain, with a lower adhesion on the cathode. These results suggest that bacterial adhesion could be controlled under an electric field whatever the bacterial species. Furthermore, no significant decrease of bacterial concentration in solution was observed for all tested species.

3.2. Bacterial adhesion to the surface of PDMS under an electrical field

In a second part, we studied the bacterial adhesion, under the effect of an electric field, on the surface of PDMS, which is a material widely used as biomaterial. Previous copper electrodes were coated with a PDMS layer of a thickness around 1 mm and used as electrodes. The applied voltage ranged from 0 to 30 V, which is the maximum voltage provided by the potentiostat. The copper electrodes were chosen because they can easily reveal whether the metal surface was completely covered by

the PDMS or not due to the disappearance of the bactericidal activity of the Cu in suspension.

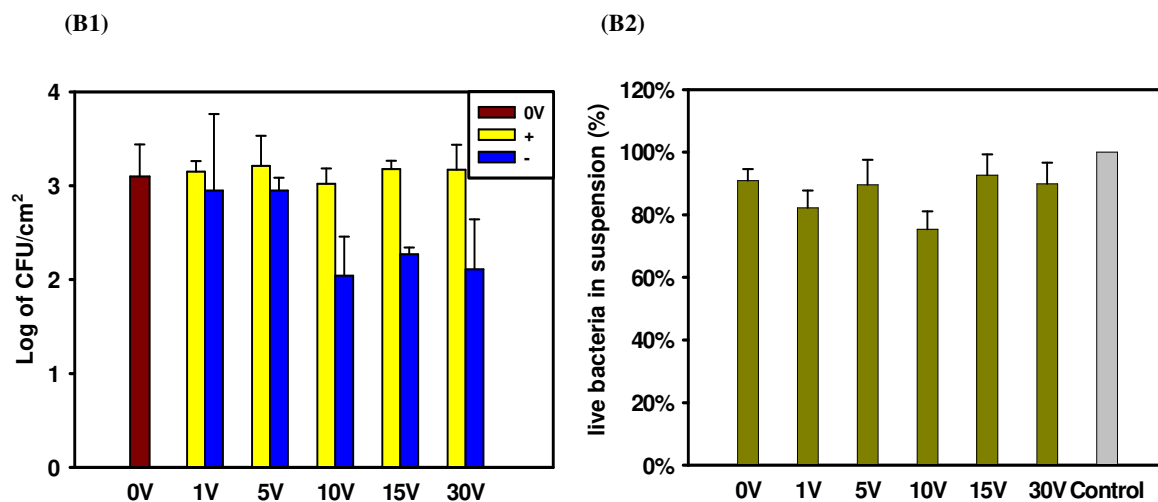


Figure 6. Adhesion of *S. aureus* to the PDMS-coated copper surface (1mm) after 2 hours of contact at voltage values between 0 and 30 V: (B1) live bacteria adhering to the surface; (B2) live bacteria in suspension; control: live bacteria in suspension without electrode.

The results of the adhesion of *S. aureus* to the surface of the PDMS under an electric field are shown in Figure 6. It can be seen that without an electrical voltage, the bacterial adhesion was about 3 log CFU/cm², which is higher than its value on the surface of the uncoated copper (Figure 3). The difference in bacterial adhesion between cathode and anode at 1 and 5 V was not significant. On the other hand, at higher applied voltages (10 to 30 V), a lower bacterial adhesion on the cathode, around 2 log CFU/cm², was observed, probably due to the electrostatic repulsion between the negative charges on the surface of the PDMS and the negatively charged bacterial cells. In addition, the percentage of live bacteria in suspension was approximately 90% regardless of the applied voltage, which is quite consistent with the percentage observed in milli-Q water. These results show that the PDMS coating on the copper electrodes leads to (i) the disappearance of the bactericidal effect of copper in the bacterial suspension, meaning that the electrodes were fully coated, and (ii) no significant bacterial stress at applied high voltage, probably due to the chemical and electrical insulating properties of PDMS. Consequently, the applied voltage must be increased above 30 V to achieve a greater anti-adhesion effect.

The study of adhesion of different bacterial species onto PDMS surfaces was also carried out at 30 V (Figure 7). No copper bactericidal activity was detected for all species. However, *S. epidermidis* appears to be quite sensitive to the applied electric field and showed a reduction of about 50% in the concentration of live bacteria in suspension. For surface adhesion, only *S. epidermidis* showed the same behaviour as *S. aureus* with a difference of about 1 log CFU/cm² between cathode and anode. This result is in contradiction with the previous result on the zinc electrodes at 0.2V. To understand this specificity of the Staphylococcus genus, measurements of the zeta potential of the bacterial membrane were performed (Table 1).

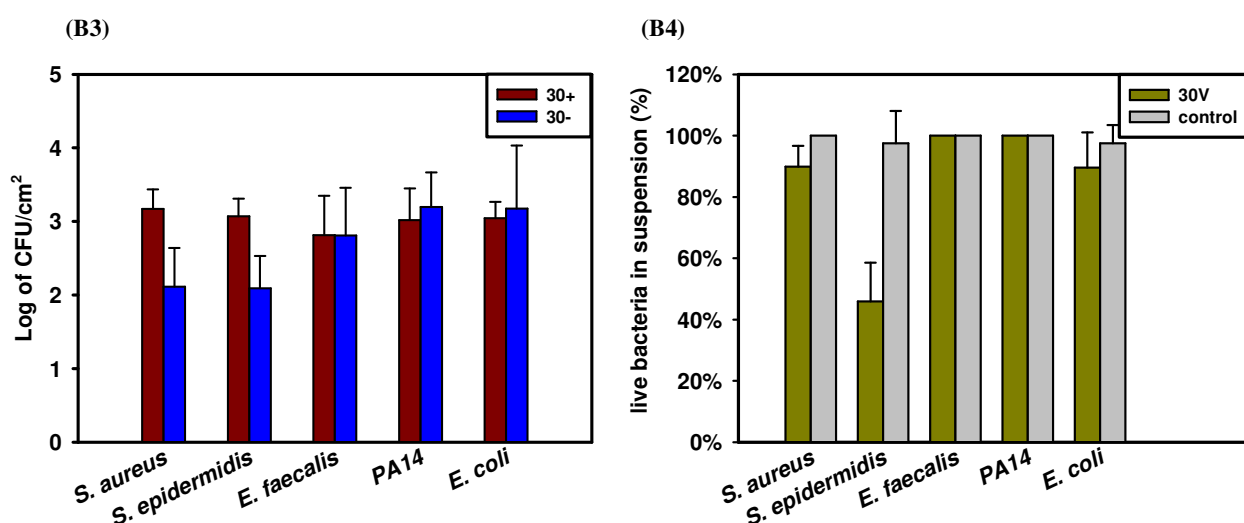


Figure 7. Adhesion of different bacterial species to the surface of PDMS coated copper (1mm) after 2 hours of contact at 30 V: (B3) live bacteria adhering to the surface; (B4) live bacteria in suspension; control: live bacteria in suspension without any electrode.

Table 1. Zeta potential of bacteria in sterile milli-Q water at a concentration of 10⁷-10⁸ CFU / ml.

Bacteria	Zeta potential (mV)	Percentage
<i>S. aureus</i> (ATCC 29213)	-39.3± 0.9	100%
<i>S. epidermidis</i> (ATCC 35984)	-38.5±1.7	51.80%±0.02
	-26.8±1.2	48.20%±0.02
<i>E. faecalis</i> (ATCC 29212)	-35.8±1.0	100%

<i>E. coli</i> (K12 MG1655)	-50.6±1.0	100%
<i>P. aeruginosa</i> (PA 14)	-41.6±0.9	100%

As expected, all bacterial membranes are negatively charged, but *E. coli* and *P. aeruginosa* bacteria have the lowest zeta potential and therefore the highest overall negative charge. Theoretically, with a higher negative charge, *E. coli* and *P. aeruginosa* should undertake stronger repulsive electrostatic interactions with the PDMS surface, resulting in lower adhesion to the anode surface, which is in contradiction with our experimental results (Figure 7). Therefore, these observations suggest that, in the presence of a PDMS coating, the electrostatic interactions are too weak to be the predominant factor governing bacterial adhesion. **There are two possible reasons why Staphylococcus species are more sensitive to the low surface polarization of PDMS: (1) they are Gram+ bacteria, which have only one external phospholipidic membrane, unlike Gram- bacteria, which have two; (2) they are spherical in shape with a lower contact surface, while the other bacteria are bacillus-shaped.**

4. Conclusion

In this work, we have studied the bacterial adhesion of Gram positive (*S. aureus*, *S. epidermidis* and *E. faecalis*) and Gram negative (*E. coli* and *P. aeruginosa*) bacteria to metal and PDMS electrode surfaces under an electric field. After 2h of contact with each of these bacteria, the Zn electrodes showed a difference of 1.5-2 log of UFC/cm² between cathode and anode at voltages of 0.2 and 0.4 V, without significant killing of bacteria in suspension. Under the same conditions, the Al electrodes were found to be inactive in limiting and directing bacterial adhesion, probably because of surface oxidation causing its passivation. However, at 1V, the Zn and Al electrodes became bactericidal by killing bacteria in suspension. On the other hand, the bactericidal effect of Cu electrodes was very high at 0 V and seems to be reinforced by the electrical field. Nevertheless, the bacterial adhesion on its surface was too weak to see a difference between the cathode and the anode. Once coated

with PDMS, the bactericidal effect of Cu disappeared and a difference of 1 log of UFC/cm², specific to staphylococcus species, was observed between the two electrodes above 10 V. Finally, this study demonstrates that the electrostatic force is the predominant factor governing the bacterial adhesion to Zn surfaces but not to those of Al and PDMS. For future works, high voltage should be used in order to increase the electrostatic bacterial repellent effect onto PDMS surfaces. Furthermore, metal electrodes could be used as physical disinfecting agents at 1V without current.

Acknowledgments

This work was funded by China Scholarship Council (CSC).

References

- [1] A. I. Doukeraki *et al.*, Methicillin-resistant food-related *Staphylococcus aureus*: a review of current knowledge and biofilm formation for future studies and applications, *Res. Microbiol.*, vol. 168 (2017) , pp. 1–15.
- [2] D. Romero, Bacterial determinants of the social behavior of *Bacillus subtilis*, *Res. Microbiol.*, vol. 164 (2013), pp. 788-798.
- [3] J. Winięcka-Krusnell and E. Linder, Bacterial infections of free-living amoebae, *Res. Microbiol.*, vol. 152 (2001), pp. 613–619.
- [4] M. Salwiczek *et al.*, Emerging rules for effective antimicrobial coatings, *Trends Biotechnol.*, vol. 32 (2014), no. 2, pp. 82–90.
- [5] B. Gottenbos, H. J. Busscher, H. C. Van Der Mei, and P. Nieuwenhuis, Pathogenesis and prevention of biomaterial centered infections, *Mater. Sci. Mater. Med.*, vol. 13 (2002), no. 8, pp. 717–722.
- [6] W. M. Jr. Dunne, Bacterial Adhesion : Seen Any Good Biofilms Lately ? Bacterial Adhesion : Seen Any Good Biofilms Lately ?, *Clin. Microbiol. Rev.*, vol. 15, no. 2 (2002), pp. 155–166.
- [7] M. Cloutier, D. Mantovani, and F. Rosei, Antibacterial Coatings: Challenges, Perspectives, and Opportunities, *Trends Biotechnol.*, vol. 33, no. 11 (2015), pp. 637–652.
- [8] D. Alves and M. Olívia Pereira, Mini-review: Antimicrobial peptides and enzymes as promising candidates to functionalize biomaterial surfaces, *Biofouling*, vol. 30 (2014), no. 4, pp. 483–499.
- [9] L. Liu, B. Ercan, L. Sun, K. S. Ziemer, and T. J. Webster, Understanding the Role of Polymer Surface Nanoscale Topography on Inhibiting Bacteria Adhesion and Growth, *ACS Biomater. Sci. Eng.*, vol. 2, no. 1 (2016), pp. 122–130.

- [10] C. Satriano, G. M. L. Messina, S. Carnazza, S. Guglielmino, and G. Marletta, Bacterial adhesion onto nanopatterned polymer surfaces, *Mater. Sci. Eng. C*, vol. 26, no. 5–7 (2006), pp. 942–946.
- [11] J. Hasan and K. Chatterjee, Recent advances in engineering topography mediated antibacterial surfaces, *Nanoscale*, vol. 7, no. 38 (2015), pp. 15568–15575.
- [12] Y. Ammar, D. Swailes, Ben Bridgens, J. Chen, Influence of surface roughness on the initial formation of biofilm, *Surface and Coatings Technology*, vol 284 (2015), pp. 410-416.
- [13] J. Foksowicz-Flaczyk *et al.*, Multifunctional durable properties of textile materials modified by biocidal agents in the sol-gel process, *Surface and Coatings Technology*, vol 304 (2016), pp. 160-166.
- [14] K. Lewis and A. M. Klibanov, Surpassing nature: Rational design of sterile-surface materials, *Trends Biotechnol.*, vol. 23, no. 7 (2005), pp. 343–348.
- [15] R. Kaur and S. Liu, Antibacterial surface design – Contact kill, *Prog. Surf. Sci.*, vol. 91, no. 3 (2016), pp. 136–153.
- [16] R. A. Procaccini, C. A. Studdert and S. A. Pellice, Silver doped silica-methyl hybrid coatings. Structural evolution and antibacterial properties, *Surface and Coatings Technology*, vol. 244 (2014), pp. 92-97.
- [17] H. Kao *et al.*, Metal ion-dependent tailored antibacterial activity and biological properties of polydopamine-coated titanium implants, *Surface and Coatings Technology*, vol 378 (2019), pp. 124998.
- [18] D. Campoccia, L. Montanaro, and C. R. Arciola, A review of the biomaterials technologies for infection-resistant surfaces, *Biomaterials*, vol. 34, no. 34 (2013), pp. 8533–8554.
- [19] A. C. Riosa, C. G. Moutinho, F. C. Pinto, F. S. Del Fiol, A. Jozala, M. V. Chaud, M. M.D.C. Vila, J. A. Teixeira, V. M. Balcão. Alternatives to overcoming bacterial resistances: State-of-the-art. *Microbiological Research*, vol. 191 (2016), pp. 51–80.
- [20] D. Freebairn, D. Linton, E. Harkin-Jones, D. S. Jones, B. F. Gilmore, and S. P. Gorman, Electrical methods of controlling bacterial adhesion and biofilm on device surfaces, *Expert Rev. Med. Devices*, vol. 10, no. 1 (2013), pp. 85–103.
- [21] J. L. Del Pozo, M. S. Rouse, J. N. Mandrekar, J. M. Steckelberg, and R. Patel, The electricidal effect: reduction of *Staphylococcus* and *Pseudomonas* biofilms by prolonged exposure to low-intensity electrical current, *Antimicrob. Agents Chemother.*, vol. 53, no. 1 (2009), pp. 41–45.
- [22] J. L. Del Pozo *et al.*, The electricidal effect is active in an experimental model of *Staphylococcus epidermidis* chronic foreign body osteomyelitis, *Antimicrob. Agents Chemother.*, vol. 53, no. 10 (2009), pp. 4064–4068.

- [23] Z. Hazan *et al.*, Effective prevention of microbial biofilm formation on medical devices by low-energy surface acoustic waves, *Antimicrob. Agents Chemother.*, vol. 50, no. 12 (2006), pp. 4144–4152.
- [24] R. Caubet *et al.*, A radio frequency electric current enhances antibiotic efficacy against bacterial biofilms, *Antimicrob. Agents Chemother.*, vol. 48, no. 12 (2004), pp. 4662–4664.
- [25] J. L. Del Pozo, M. S. Rouse, and R. Patel, Bioelectric effect and bacterial biofilms. A systematic review, *Int. J. Artif. Organs*, vol. 31, no. 9 (2008), pp. 786–795.
- [26] J. W. Costerton, B. Ellis, K. Lam, F. Johnson, and A. E. Khoury, Mechanism of electrical enhancement of efficacy of antibiotics in killing biofilm bacteria., *Antimicrob. Agents Chemother.*, vol. 38, no. 12 (1994), pp. 2803–2809.
- [27] J. L. Del Pozo, M. S. Rouse, J. N. Mandrekar, M. F. Sampedro, J. M. Steckelberg, and R. Patel, Effect of electrical current on the activities of antimicrobial agents against *Pseudomonas aeruginosa*, *Staphylococcus aureus*, and *Staphylococcus epidermidis* biofilms, *Antimicrob. Agents Chemother.*, vol. 53, no. 1 (2009), pp. 35–40.
- [28] S. A. Blenkinsopp, A. E. Khoury, and J. W. Costerton, Electrical enhancement of biocide efficacy against *Pseudomonas aeruginosa* biofilms., *Appl. Environ. Microbiol.*, vol. 58, no. 11 (1992), pp. 3770–3773.
- [29] J. Jass and H. M. Lappin-Scott, The efficacy of antibiotics enhanced by electrical currents against *Pseudomonas aeruginosa* biofilms, *Antimicrob. Chemother.*, vol. 38, no. 6 (1996), pp. 987–1000.
- [30] J. P. Busalmen and S. R. De Sanchez, Adhesion of *Pseudomonas fluorescens* (ATCC 17552) to nonpolarized and polarized thin films of gold, *Appl. Environ. Microbiol.*, vol. 67, no. 7 (2001), pp. 3188–3194.
- [31] J. P. Busalmen and S. R. de Sánchez, Electrochemical polarization-induced changes in the growth of individual cells and biofilms of *Pseudomonas fluorescens* (ATCC 17552), *Appl. Environ. Microbiol.*, vol. 71, no. 10 (2005), pp. 6235–6240.
- [32] I. Gall, M. Herzberg, and Y. Oren, The effect of electric fields on bacterial attachment to conductive surfaces, *Soft Matter*, vol. 9, no. 8 (2013), pp. 2443–2452.
- [33] G. Grass, C. Rensing, and M. Solioz, Metallic copper as an antimicrobial surface, *Appl. Environ. Microbiol.*, vol. 77, no. 5 (2011), pp. 1541–1547.
- [34] M. Vincent, R. E. Duval, P. Hartemann, and M. Engels-Deutsch, Contact killing and antimicrobial properties of copper, *Appl. Microbiol.*, vol. 124, no. 5 (2018), pp. 1032–1046.
- [35] F.S.da Silva *et al.*, Corrosion resistance and antibacterial properties of copper coating deposited by cold gas spray, *Surface and Coatings Technology*, vol.

- 361 (2019), pp. 292-301.
- [36] S. Pandit, S. Shanbhag, M. Mauter, Y. Oren, and M. Herzberg, Influence of Electric Fields on Biofouling of Carbonaceous Electrodes, *Environ. Sci. Technol.*, vol. 51, no. 17 (2017), pp. 10022–10030.
- [37] J. Y. H. Lee *et al.*, Global spread of three multidrug-resistant lineages of *Staphylococcus epidermidis*, *Nat. Microbiol.*, vol. 3, no. 10 (2018), pp. 1175–1185.
- [38] V. D. Wells, E. S. Wong, B. E. Murray, P. E. Coudron, D. S. Williams, and S. M. Markowitz, Infections due to beta-lactamase-producing, high-level gentamicin-resistant *Enterococcus faecalis*, *Ann. Intern. Med.*, vol. 116, no. 4 (1992), pp. 285–292.
- [39] A. Y. Peleg and D. C. Hooper, Hospital-Acquired Infections Due to Gram-Negative Bacteria, *New Engl. J. Med. Rev.*, vol. 362, no. 19 (2010), pp. 1804–1813.
- [40] S. Mamoudou, D. Lassina, and K. Fla, Les infections à *Pseudomonas aeruginosa* au service des maladies infectieuses du CHU YO, Burkina Faso: À propos deux cas, *Pan Afr. Med. J.*, vol. 21 (2015), pp. 183–186.
- [41] R. A. Welch, E. P. Dellinger, B. Minshew, and S. Falkow, Haemolysin contributes to virulence of extra-intestinal *E. coli* infections, *Nature*, vol. 294, no. 5842 (1981). pp. 665–667.