

New determination of the 3He mixing ratio in the Earth's lower atmosphere from an international tritium intercomparison exercise

P. Jean-Baptiste, E. Fourré, Philippe Cassette

► To cite this version:

P. Jean-Baptiste, E. Fourré, Philippe Cassette. New determination of the 3He mixing ratio in the Earth's lower atmosphere from an international tritium intercomparison exercise. Applied Geochemistry, 2018, 98, pp.17-21. 10.1016/j.apgeochem.2018.09.003 . hal-03107216

HAL Id: hal-03107216 https://hal.science/hal-03107216v1

Submitted on 22 Jan 2021

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers. L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

1	New determination of the ³ He mixing ratio in the Earth's lower atmosphere from				
2	an international tritium intercomparison exercise				
3					
4	P. Jean-Baptiste ¹ , E. Fourré ¹ , P. Cassette ²				
5	P. Jean-Baptiste, E. Fourre, P. Cassette				
6	1				
7	¹ Laboratoire des Sciences du Climat et de l'Environnement, CEA-CNRS-UVSQ, CEA-				
8	Saclay, 91191 Gif-sur-Yvette, France.				
9	² LNE-LNHB, CEA-Saclay, 91191 Gif-sur-Yvette, France				
10					
11	Corresponding author : Philippe Jean-Baptiste (pjb@lsce.ipsl.fr)				
12					
13	Abstract.				
14					
15	The light isotope of helium, ³ He, is essentially a primordial substance entrapped within				
16	the Earth's interior during the formation of the planet. It is released into the atmosphere by				
17	volcanic/magmatic activity, and eventually escapes to outer space. ³ He is also produced by				
18	the radioactive beta-decay of tritium. Hence, measurements of ³ He can be used to derive the				
19	concentration of tritium. The so-called " ³ He ingrowth" method uses a mass spectrometer to				
20	detect the amount of ³ He that accumulates in a sample during a given period of storage. The				
21	³ He measurements are classically calibrated against an air standard. The method thus relies				
22	on the accurate knowledge of the atmospheric mixing ratio of ³ He. This value is based on				
23	mass spectrometric measurements with gravimetrically or volumetrically prepared ³ He				
24	standard mixtures. Here, we apply the ³ He ingrowth method in reverse, using a solution of				
25	tritiated water prepared for an international comparison of tritium activity measurements to				
26	precisely determine the ³ He mixing ratio of our air standard. The measured atmospheric				
27	mixing ratio of ${}^{3}\text{He}$, based on a series of ten measurements, is [${}^{3}\text{He}$]=7.12 \pm 0.06 ppt. This				
28	value is between 1% and 2% lower than previous determinations reported in the literature.				
29	However, all results remain statistically consistent.				
30					
31	Keywords: Helium-3, tritium, mass spectrometry				

- 33 **1. Introduction.**
- 34

In the ³He ingrowth method, the activity of tritium is determined via the mass 35 spectrometric measurement of the helium-3 (³He) produced by the radioactive decay of 36 tritium (Clarke et al., 1976). Because the atmospheric residence time of helium (~10⁶ years) 37 is much longer than the mixing time of the atmosphere (~10 years only), the ³He content of 38 39 the atmosphere is the same over the whole globe (Glückhauf and Paneth, 1946; Jean-Baptiste and Fourré, 2012). Air is thus a convenient ³He standard, that is classically used by 40 the tritium laboratories applying the ³He ingrowth technique. The value of the ³He mixing ratio 41 42 in atmospheric air is therefore an important parameter because any uncertainty in this value 43 directly affects the measured tritium concentrations. This value appears to be reasonably 44 well known : One direct determination was by Davidson and Emerson, 1990. They used 45 mass spectrometry with gravimetrically prepared ³He standards and found a value of 46 7.27±0.20 ppt; other relevant publications (Table 1), which concern the ⁴He content of air 47 (Glückauf, 1944; Glückauf, 1946; Oliver et al., 1984; Holland and Emerson, 1987) and the 48 ³He/⁴He ratio of air (Mamyrin et al., 1970; Clarke et al., 1976; Sano et al., 1988; Hoffman and 49 Nier, 1993) lead to a mean value of 7.21 with a standard uncertainty of the mean equal to 50 ± 0.07 ppt (calculated by a bootstrap technique). However, all these determinations rely on 51 gravimetrically or volumetrically prepared ³He mixtures. Therefore, we thought that determining the atmospheric mixing ratio of ³He using a totally independent method would be 52 53 of some interest. Because we routinely use the ³He ingrowth method for tritium 54 measurements (Jean-Baptiste et al., 1992; 2010), we were able to apply the ³He ingrowth method in reverse, using a solution of tritiated water prepared for an international comparison 55 of tritium activity measurements to determine the ³He mixing ratio of our air standard. 56

57

58 **2. The CCIR(II) 2009 International Tritium Intercomparison**

59

60 An international comparison of activity measurements of a solution of tritiated water was organised by the Consultative Committee for Ionizing Radiation (CCIR) in 2009. The tritiated 61 62 water was prepared and dispatched to the participants by the Laboratoire National Henri 63 Becquerel (LNHB), the French National Metrology Institute for radioactivity standards. Fifteen laboratories took part in the exercise (Table 2) and reported a total of 22 independent results. 64 65 Most laboratories applied the triple-to-double coincidence ratio (TDCR) method in liquid 66 scintillation counting (LSC). The TDCR method is a primary standardization method of 67 measuring radioactivity, mainly used by metrology laboratories. It requires a special liquid 68 scintillation (LS) counter equipped with three photomultipliers (A, B and C) in coincidence.

Such instrumentation is generally designed and constructed by national metrology laboratories around the world. The TDCR system allows the observation of double AB, BC, and CA and triple ABC coincidences, making it possible to measure the absolute activity of the radioactive solution, independently of the detection efficiency (Broda et al., 1988; Broda and Pochwalski, 1992; Cassette and Vatin, 1992; Stanga et al., 2006).

74 The reference time and date used were 00:00 UTC, 31 May 2009 -. The Power-75 Moderated weighted Mean formalism – PMM (Pommé, 2012) was used to evaluate the Key 76 Comparison Reference Value (KCRV). The value given by the MKEH (Budapest, Hungary) 77 was identified as an outlier by the PMM procedure. In addition, the results of BARC, IRMM 78 obtained by methods using ³H external standards were not used to calculate the KCRV The 79 KCRV calculated using the PMM method is thus 37.10 ± 0.19 Bg/mg, corresponding to a 80 relative uncertainty of 0.51% (Ratel and Michotte, in prep.). A summary of the results is given 81 in Fig. 1 and Table 2.

82

83 **3. Method**

- 84
- 85 3.1 Dilution Procedure

86 Half a liter of a tritium solution was prepared from the tritiated water distributed for the 87 CCIR(II) 2009 International Tritium Intercomparison by two-step gravimetric dilution with 88 "tritium-free" groundwater (0.09 \pm 0.01 Bq/kg). First, in a glove box flushed with argon, a few 89 drops (113.05±0.01 mg) of the initial tritiated water were added with a syringe to 90 11.02±0.02 g of "tritium-free" water. Then, in the same way, 135.52±0.01 mg of this water 91 was in turn added to 473.20±0.02 g of "tritium-free" water, leading to a reduction factor of the 92 initial tritium concentration of $(3.435\pm0.007)\times10^5$ and a final solution of ~100 Bg/kg. The 93 weighing process consisted in weighing the empty and the filled containers and, in case of 94 the tritium standard, the transfer container (syringe) before and after the transfer. All dilutions 95 were performed using calibrated balances and calibrated weights traceable to the French 96 national mass standards, checking the zero reading and making test weights before and after 97 each weighing process. Buoyancy corrections were applied. The combined uncertainty of the 98 weighing procedure was calculated according to the Guide to the expression of uncertainty in 99 measurement (JCGM, 2008).

100

101 3.2 Sample preparation and ³He mass spectrometry

102 Ten 100 ml low-helium diffusivity Corning 1724 glass bulbs were filled with 103 approximately 40 g of the prepared standard solution. To minimize ³He blank, the bulbs were

pre-baked in a flow of argon at 600°C for 24 hours to remove the helium dissolved in the glass. The samples were degassed using a routine procedure (Jean-Baptiste et al., 1992). However, to avoid any bias due to isotope fractionation that might have occurred during pumping, a special water trap at 77K was inserted between the sample and the pumping unit to trap water vapor and to transfer it back into the sample at the end of the degassing.

109 The storage time was about 120 days. ³He which accumulated during this period of time 110 was measured with a MAP-215-50 mass spectrometer (Jean-Baptiste et al., 2010). Classically, along with the tritiugenic ³He signal, a small ⁴He signal (n^{4} He_{res}< 5×10⁻¹⁴ mol) can 111 112 be detected as well. This ⁴He corresponds to the small air residue left behind at the end of 113 the degassing step, but also, to a minor extent, to diffusion through the glass bulb (Jean-114 Baptiste et al., 1989) and leaking through adapter fittings. The corresponding ³He signal $(n^{3}He_{res} < 7 \times 10^{-20} \text{ mol}, \text{ i.e., representing about 0.08\% of the measured }^{3}He signal)$ can be 115 calculated by applying the ³He/⁴He ratio of this air residue, R_{res}. The statistics of 116 117 measurements on samples analysed immediately following degassing (i.e., with no tritiugenic ³He contribution) show that R_{res} is identical to the ³He/⁴He ratio of air, R_a , within ±10%. 118 119 Hence R_{res} can be written as follows: $R_{res} = \alpha R_a$, with $\alpha = 1.0 \pm 0.1$. The ³He blank of the inlet system, n^{3} He_{blank} is less than 5×10⁻²⁰ mol. Most of it is due to the O'ring which is used to 120 121 attach the glass bulb to the inlet system. The ³He/⁴He ratio of this line blank is not statistically 122 different from R_a , hence we assume that $R_{blank} = R_{res} = \alpha R_a$.

The measurements are calibrated against an air standard drawn from a 5 L tank filled 123 124 with clean air at known pressure, temperature and relative humidity conditions, through a precisely calibrated volume V=122.2 \pm 0.1 (1 σ) mm³ (Jean-Baptiste et al., 2014). The total 125 126 number of aliquots withdrawn from the 5 L tank is recorded in order to take into account the decreasing pressure in the tank. ⁴He⁺ is measured on a Faraday cup. The ³He⁺ ion beam 127 128 (~250 ions/sec for an air standard with about 3.7×10^{-17} ³He mole) passes through an 129 electrostatic filter before impinging the detector (a 16-stage electron multiplier connected to a pulse counting system). The ³He background is very low (< 0.05 count/sec) when employing 130 the electrostatic filter, which constitutes the ultimate limit for the ³He detection. The counting 131 132 procedure consists of five series of counting of the ³He⁺ signal interspaced by five 133 measurements of the ⁴He⁺ peak and baseline. Each series consists of ten 10-seconds 134 integrations on the ³He⁺ peak and on the baseline, corresponding to a total counting time of 135 500 sec on the peak and 500 sec on the baseline.

In routine operation, each sample measurement is followed by a standard air aliquot (Jean-Baptiste et al., 1992; 2010). A correction is routinely applied to take into account the pressure effect in the source due to the fact that the sample contains some 10^{-14} mol of gas only whereas the air aliquot contains about 10^{-10} mol of helium and neon (neon is not retained by the charcoal trap at 77K). For this special experiment however, to avoid any additional uncertainty arising from this correction, an aliquot of the air standard was introduced in the inlet line with each sample so as to keep the pressure in the source identical for the standard and for the sample.

With this special protocol, the amount of helium-3 (n³He_{meas}) and helium-4 (n⁴He_{meas}) corresponding to the (sample+standard) measurement obeys the following equations:

146

$$n^{3}He_{meas} = n^{3}He_{tri} + n^{3}He_{std} + n^{3}He_{res} + n^{3}He_{blank}$$
(1)

$$n^{4}He_{meas} = n^{4}He_{std} + n^{4}He_{res} + n^{4}He_{blank}$$
(2)

where $n^{3}He_{std}$ and $n^{4}He_{std}$ are the ³He and ⁴He amount in the air standard aliquot, respectively; $n^{3}He_{res}$ and $n^{4}He_{res}$ are the residual amounts of ³He and ⁴He, respectively, left behind at the end of the degassing step; and $n^{3}He_{blank}$, $n^{4}He_{blank}$ are the amount of ³He and ⁴He, respectively, of the blank of the inlet system. $n^{3}He_{tri}$ is the amount of tritiugenic ³He produced during the storage time

$$n^{3}He_{tri}$$
 (in mol) = T × [1-exp(- $\lambda\tau$)] (3)

where T (in mol) is the amount of tritium in the sample at the date of the bulb closure and λ is the decay constant for tritium (Lucas and Unterweger, 2000).

159 Using equation (2), equation (1) can be rewritten as follows:

160
$$n^{3}He_{meas} - n^{3}He_{std} - \alpha R_{a} (n^{4}He_{meas} - n^{4}He_{std}) = n^{3}He_{tri}$$
 (4)

161

or

162
$$n_{std}^{a} [^{3}He] [(N3_{meas}/N3_{std} - 1) - \alpha (N4_{meas}/N4_{std} - 1)] = n^{3}He_{tri}$$
 (5)

where n_{std}^{a} is the amount of dry air in the standard air aliquot, [³He] is the atmospheric mixing ratio of ³He, N3_{meas}, N4_{meas}, N3_{Std} and N4_{Std} are the ³He and ⁴He peaks height corresponding to n³He_{meas}, n⁴He_{meas}, n³He_{std} and n⁴He_{std}. Note than in equation (5), the correction term $\alpha(N4_{meas}/N4_{std} - 1)$ is less than 0.1% of the main term (N3_{meas}/N3_{std} - 1).

Finally, equations (3) and (5) give the atmospheric mixing ratio of ³He as a function of the amount T of tritium in the sample at the date of the bulb closure, where T is given by the intercomparison exercise and the dilution factor :

171
$$[{}^{3}\text{He}] = \text{T} \times [1 - \exp(-\lambda \tau)] / n^{a}_{std} / [(N3_{meas}/N3_{std} - 1) - \alpha(N4_{meas}/N4_{std} - 1)]$$

172

173 **4. Results and discussion**

175 The results of the ten measurements are displayed in Table 3 and Fig.2. The arithmetical 176 mean of the ten determinations of the air ³He mixing ratio is $[^{3}He] = 7.12$ ppt. The individual 177 uncertainty on each determination (± 0.09 ppt) takes into account all existing uncertainties 178 including random uncertainties (Category A uncertainties in JCGM, 2008), i.e. counting 179 statistics and sample weight (±0.01%) as well as systematic uncertainties (Category B 180 uncertainties in JCGM, 2008): uncertainty on the tritium value of the initial solution as 181 determined by the CCIR(II)-2009 intercomparison (±0.51%), on the dilution (±0.2%), on 182 meteorogical parameters (pressure, temperature, humidity) of the air standard (±0.25%), on 183 the volume of the standard air aliquot ($\pm 0.08\%$), on the value of α ($\pm 10\%$) and λ ($\pm 0.2\%$). The 184 propagation of uncertainties is calculated by combining all uncertainties using a Monte-Carlo 185 approach. The calculation shows that the systematic and random uncertainties are \pm 0.05 ppt 186 and \pm 0.07 ppt, respectively. This is fully consistent with the experimental standard deviation 187 of the ten measurements (± 0.07 ppt – see Table 3), which only takes into account random 188 fluctuations. With ten determinations, the standard uncertainty of the mean is equal to 189 0.055 ppt, corresponding to a relative standard uncertainty of 0.8% on the determination of 190 the ³He mixing ratio. Hence, our best estimate of the ³He mixing ratio is $[^{3}He]=7.12\pm0.06$ ppt. 191 This is between 1% and 2% lower than the previous determinations reported in the literature, 192 7.27±0.20 ppt and 7.21±0.07 ppt (see section 1) but all values are statistically consistent 193 within their standard uncertainties (see Fig. 2). With the abundance of ⁴He in the atmosphere 194 equal to 5.23±0.01 ppm (average of the four values in Table 1), this leads to an atmospheric ${}^{3}\text{He}/{}^{4}\text{He}$ ratio of $(1.36\pm0.01)\times10^{-6}$ instead of $(1.38\pm0.02)\times10^{-6}$ (average of the five values in 195 Table 1). Note that the present-day 3 He/ 4 He value may have decrease slightly compared with 196 197 this value because of the increasing injection of radiogenic ⁴He into the atmosphere by the 198 consumption of oil and natural gas. However, the magnitude of this decrease (between 0% 199 and 0.8% - see Lupton and Evans, 2004; Lupton and Evans, 2013; Brennwald et al., 2013; 200 Mabry et al., 2015) is still debated because of the difficulty to find well-preserved air archives 201 and to accurately measure such a tiny change.

202 A systematic 2% positive offset between the results based on the ³He ingrowth method 203 and the Miami Tritium Laboratory beta-particle counting results (relative to the US National 204 Bureau of Standards, former name of the National Institute of Standards and Technology 205 tritiated water standard) has already been noted in the paper by Clarke et al. (1976). At the 206 time, the authors attributed this discrepancy to a possible underestimation of tritium half-life. 207 However, a later review of tritium half-life (Lucas and Unterweger, 2000) shows that this 208 explanation is unlikely. With the value of the atmospheric mixing ratio of ³He determined in 209 the present study, this 2% discrepancy disappears, thus suggesting that it was indeed due to 210 an overestimation of the atmospheric mixing ratio of ³He. Although the implications for ³He or ³H measurements are limited, we think that this new value of the ³He mixing ratio in atmospheric air should be adopted by the tritium-helium community for consistency with tritium laboratories using beta-particle counting.

214

5. Summary and Conclusions

To re-determine the atmospheric mixing ratio of ³He, we applied the ³He ingrowth method 216 217 in reverse, using a solution of tritiated water prepared for the international comparison of 218 tritium activity measurements CCIR(II)-2009. This was done by preparing a tritium solution by 219 two-step gravimetric dilution of a small aliquot of this primary solution. Compared to our 220 routine protocol, we used special procedures both for sample preparation and mass 221 spectrometric measurements to further increase the precision: for sample preparation, 222 isotope fractionation due to water evaporation during degassing was suppressed by trapping 223 the evaporated water at liquid nitrogen temperature and transferring it back into the sample 224 at the end of the degassing step, thus avoiding any bias in the isotope fractionation 225 correction. In the mass spectrometer, we added an aliquot of the air standard on top of each 226 sample so as to keep the pressure in the source essentially identical for the standard and for 227 the sample thus avoiding any additional uncertainty arising from the usual pressure 228 correction. Our main conclusions are as follows:

Our estimated value of the atmospheric mixing ratio of ³He is [³He]=7.12±0.06 ppt,
 corresponding to a relative standard uncertainty of 0.8%.

- This value is between 1% and 2% lower than the previous, less precise determinations
 reported in the literature. Nevertheless, all values are statistically consistent within their
 standard uncertainties.

- The adoption of this new value removes the systematic 2% positive offset noted by Clarke
 et al. (1976) between their results based on the ³He ingrowth method and the Miami Tritium
 Laboratory beta-particle counting results.

237

238 Acknowledgments

239

Data supporting this study are available in Table 2 and Table 3 of the present manuscript.

- 242
- 243 **References**
- 244

- 245 Brennwald, M.S., Vogel, N., Figura, S., Vollmer, M.K., Langenfelds, R., Paul Steele, L.,
- 246 Maden, C., Kipfer, R., 2013. Concentrations and isotope ratios of helium and other noble
- gases in the Earth's atmosphere during 1978–2011. Earth Planet. Sci. Lett. 366, 27–37.
- 248 Broda, R., Pochwalski K., Radoszewski T., 1988. Calculation of liquid-scintillation detector
- 249 efficiency. Appl Radiat Isot, 1988, 39: 159–164
- 250 Broda, R., Pochwalski, K., 1992. The enhanced triple to double coincidence ratio (ETDCR)
- 251 method for standardization of radionuclides by liquid scintillation counting. Nucl Instrum252 Methods A 312, 85–89.
- 253 Cassette, P., Vatin, R., 1992. Experimental evaluation of TDCR models for the 3 PM liquid
- scintillation counter. Nucl. Instrum. Methods A 312, 95-99.
- 255 Clarke, W.B., Jenkins, W.J., Top, Z., 1976. Determination of tritium by mass spectrometric
- 256 measurement of 3He. Int. J. App. Radiat. Isot. 27, 515-522.
- Davidson, T.A., and Emerson, D.E., 1990. Direct determination of the Helium-3 content of atmospheric air by mass spectrometry. J. Geophys. Res. 95, 3565-3569.
- Glückauf, E., 1944. A simple analysis of the helium content of air. Trans. Faraday Soc. 40,436-438
- Glückauf, E., 1946. A micro-analysis of the helium and neon contents of air. Proc. Roy. Soc.
 London Ser A 185, 98-119.
- Glückauf, E., and Paneth, F.A., 1946. The helium content of atmospheric air. Proc. Roy. Soc.
 London Ser A 185, 89-98.
- Hoffman, J.H. and Nier, A.O., 1993. Atmospheric helium isotopic ratio. Geophys. Res. Lett.
 20, 121-123.
- Holland, P.W., and Emerson, D.E., 1987. A determination of the Helium-4 content of near
 surface atmospheric air within the continental United States. J. Geophys. Res. 92, 12,55712,566.
- Jean-Baptiste, P., Andrié, C., Lelu, M., 1989. Helium diffusion through glass. Glass Tech. 30,228-230.
- Jean-Baptiste, P., Mantisi, F., Dapoigny, A., Stievenard, M., 1992. Design and performance
- 273 of a mass spectrometric facility for measuring helium isotopes in natural waters and for low-
- level tritium determination by the ³He ingrowth method. Appl. Radiat. Isot. 43, 881-891.

- Jean-Baptiste, P., Fourré, E., Dapoigny, A., Baumier, D., Baglan, N., Alanic, G., 2010. ³He
- 276 mass spectrometry for very low-level measurement of organic tritium in environmental
- 277 samples. J. Environ. Rad., 101, 185-190.
- Jean-Baptiste, P., Fourré, E., 2012. Meridional distribution of the atmospheric ³He/⁴He ratio.
- 279 Goldschmidt 2012 Conference Abstracts, Montreal, at : <u>https://goldschmidtabstracts.info/</u>
- Jean-Baptiste, P., Cassette, P., Fourré, E., Tartès, I., Dapoigny, A., 2014. Measurement of
- the French national tritiated-water standard by helium-3 mass spectrometry. Applied
- 282 Radiation and Isotopes, 87, 157-161.
- 283 Joint Committee for Guides in Metrology JCGM, 2008. Evaluation of measurement data –
- guide to the expression of uncertainty in measurement. At https//www.bipm.org/utils/common
 /documents/jcgm/JCGM_100_2008_E.pdf
- Lucas, L.L., and Unterweger, M.P., 2000. Comprehensive review and critical evaluation of
- the half-life of tritium. Journal of Research of the National Institute of Standards andTechnology 105, 541-549.
- Lupton, J., and Evans, L., 2004. The atmospheric helium isotope ratio: Is it changing ? Geophys. Res. Lett. 31, L13101, doi: 10.1029/2004GL020041.
- Lupton, J., and Evans, L., 2013. Changes in the atmospheric helium ratio over the past 40years. Geophys. Res. Lett. 40, 6271-6275.
- Mabry, J., Lan, T., Boucher, C., Burnard, P., Brennwald, M., Langenfelds, R., Marty, B. (2015) No evidence for change of the atmospheric helium isotope composition since 1978 from re-analysis of the cape grim air archive. Earth and Planetary Science Letters 428, 134– 138.
- 297 Mamyrin, B., Anufriev, G.S., Kamenskiy, I.L., Tolstikhin, I.N., 1970. Determination of the 298 isotopic composition of atmospheric helium. Geochem. Int. 7, 498-505.
- 299 Oliver, B.M., Bradley, J.G., Farrar, H., 1984. Helium concentration in the Earth's lower 300 atmosphere. Geochim. Cosmochim. Acta 48, 1759-1767.
- 301 Sano, Y., Wakita, H., Sheng, X., 1988. Atmospheric helium isotope ratio. Geochemical
 302 Journal 22, 177-181.
- Pommé, S., 2012. Determination of a reference value, associated standard uncertainty and
 degrees of equivalence for CCIR(II) key comparison data. European Commission, Joint
 Research Centre, Institute for Reference Materials and Measurements, Retiesweg 111, 2440
 Geel, Belgium

- 307 Ratel, G., and Michotte, C., International comparison of activity measurements of a solution
- 308 of tritiated water CCIR(II)-2009 (in preparation).
- 309 Stanga, D., Moreau, I., Cassette, P., 2006. Standardization of tritiated water by two improved
- 310 methods. Appl. Radiat. Isot. 64, 1203-1206.

312 Figure captions

313

Fig. 1: Results of the CCIR(II)-2009 international intercomparison of activity measurements of tritiated water used in the present study. All error bars are 1-sigma standard uncertainties.

316

Fig. 2: Results of the ten mass spectrometric measurements of the atmospheric ³He mixing ratio carried out in this study (black open circles). The two red open squares are the atmospheric ³He mixing ratios reported in the literature by direct measurement (Davidson and Emerson, 1990) and by combining the determination of the atmospheric ⁴He mixing ratio (Glückauf, 1944; Glückauf, 1946; Oliver et al., 1984; Holland and Emerson, 1987) with the ³He/⁴He ratio of air (Mamyrin et al., 1970; Clarke et al., 1976; Sano et al., 1988; Hoffman and Nier, 1993). All error bars are at 1-sigma.

324

325 Table captions

326

327 Table 1: Atmospheric ⁴He mixing ratios and ${}^{3}\text{He}/{}^{4}\text{He}$ values from the literature.

328

329 Table 2 : Tritium concentrations measured by the participants of the CCIR(II)-2009

330 international intercomparison.

331

332 Table 3 : Results of the ten mass spectrometric measurements of the atmospheric ³He

333 mixing ratio carried out in this study.

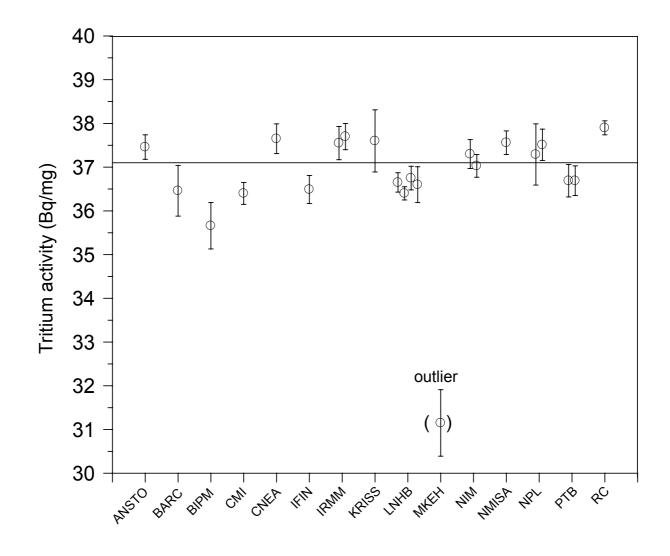


Figure 1

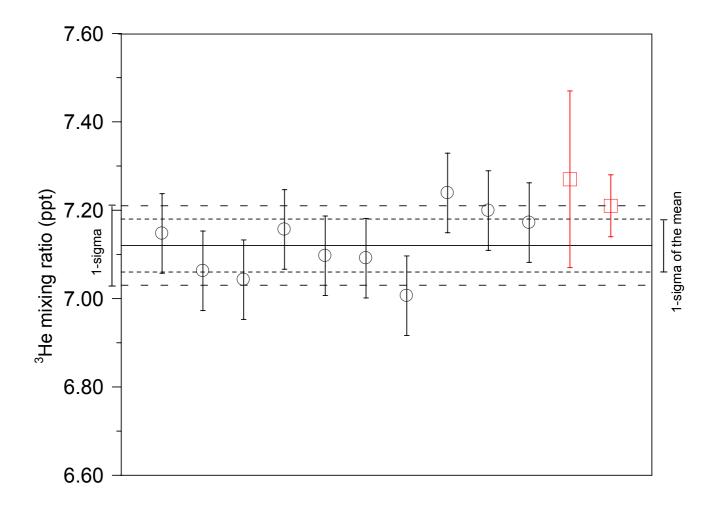


Figure 2

References	³ He/ ⁴ He (x10 ⁶)		
Mamyrin et al (1970)	1,399 ± 0,013		
Clarke et al. (1976)	1,384 ± 0,006		
Sano et al (1988)	1,343 ± 0,013		
Davidson et al.(1988)	1,393 ± 0,014		
Hoffman & Nier (1993)	1,371 ± 0,019		
References	⁴ He (ppm)		
Glückauf (1944)	5,24 ± 0,03		
Glückauf (1946)	5,239 ± 0,004		
Oliver et al (1984)	5,222 ± 0,002		
Holland & Emerson (1987)	5,220 ± 0,004		

Table 1

Organisation		Method	Tritium activity (Bq/mg)
ANSTO	Australian Nuclear Science and Technology Organisation, Lucas Heights, Australia	4p(LS)b TDCR	37,46 ± 0,28
BARC	Bhabha Atomic Research Centre, Trombay, Mumbai, India	4p(LS)b with 3H efficiency tracing	36,46 ± 0,58
BIPM	Bureau International des Poids et Mesures, Sèvres, France	4p(LS)b TDCR	35,66 ± 0,53
CMI	Czech Metrology Institute, Inspectorate for Ionizing Radiations, Prague	4p(LS)b TDCR	36,40 ± 0,25
CNEA	Comisión Nacional de Energía Atómica, Buenos Aires, Argentina	4p(LS)b TDCR	37,65 ± 0,34
IFIN	Institute of Research & Development for Physics and Nuclear Engineering, Bucharest	4p(LS)b TDCR	36,49 ± 0,32
IRMM	Institute for Reference Materials and Measurements, Geel, Belgium	4p(LS)b TDCR	37,55 ± 0,38
IRMM		4p(LS)b with 3H efficiency tracing	37,70 ± 0,30
KRISS	Korea Research Institute of Standards and Science, Yuseong, Daejon, Republic of Korea	4p(LS)b TDCR	37,60 ± 0,71
LNHB	Laboratoire National Henri Becquerel, CEA-Saclay, Gif-sur-Yvette, France	Differential proportional counting	36,65 ± 0,22
LNHB		4p(LS)b TDCR with CET	36,40 ± 0,15
LNHB		4p(LS)b TDCR	36,75 ± 0,27
LNHB		4p(LS)b TDCR with a digital MAC3	36,60 ± 0,41
MKEH	Magyar Kereskedelmi Engedélyezési Hivatal, Budapest, Hungary	4p(LS)b with 54Mn efficiency tracing	31,15 ± 0,76
NIM		4p(LS)b CIEMAT/NIST	37,30 ± 0,33
NIM	National Institute of Metrology, Beijing, Peoples Republic of China	4p(LS)b TDCR	37,03 ± 0,26
NMISA	National Metrology Institute of South Africa, Cape Town, South Africa	4p(LS)b TDCR	37,56 ± 0,27
NPL		Differential proportional counting	37,29 ± 0,70
NPL	National Physical Laboratory, Teddington, United Kingdom	4p(LS)b TDCR	37,51 ± 0,36
PTB		4p(LS)b CIEMAT/NIST	36,69 ± 0,37
PTB	Physikalisch-Technische Bundesanstalt, Braunschweig, Germany	4p(LS)b TDCR	36,69 ± 0,34
RC	Institute of Atomic Energy, Radioisotope Centre POLATOM, Otwock-Świerk, Poland	4p(LS)b TDCR	37,90 ± 0,16

Table 2

Sample N°	[³ He] ppt		
1	7,15	±	0,09
2	7,06	±	0,09
3	7,04	±	0,09
4	7,16	±	0,09
5	7,10	±	0,09
6	7,09	±	0,09
7	7,01	±	0,09
8	7,24	±	0,09
9	7,20	±	0,09
10	7,17	±	0,09
Mean	7,12		
1-Sigma	0,07		

Table 3