



HAL
open science

Ultrasound-guided delivery and sonoporation

Michiel Postema, Spiros Kotopoulos, Anthony Delalande, Odd Helge Gilja

► **To cite this version:**

Michiel Postema, Spiros Kotopoulos, Anthony Delalande, Odd Helge Gilja. Ultrasound-guided delivery and sonoporation. *Ultrasound in Gastroenterology: 10-years Anniversary of National Centre for Ultrasound in Gastroenterology. A Symposium in Honour of Professor Svein Ødegaard, 2011, Bergen, Norway.* pp.57-59. hal-03189353

HAL Id: hal-03189353

<https://hal.science/hal-03189353>

Submitted on 3 Apr 2021

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Ultrasound-guided delivery and sonoporation

Michiel Postema¹, Spiros Kotopoulos^{1,2}, Anthony Delalande^{1,3}, Odd Helge Gilja^{2,3}

1. *Department of Physics and Technology, University of Bergen, Bergen, Norway*
2. *National Center for Ultrasound in Gastroenterology, Department of Medicine, Haukeland University Hospital, Bergen, Norway*
3. *Institute of Medicine, University of Bergen, Bergen, Norway*

Ultrasound contrast agents are commonly added to the blood stream in ultrasonic imaging: contrast-enhanced ultrasound (CEUS). They consist of microscopically small bubbles (microbubbles) encapsulated by elastic shells. The most common shell materials are phospholipids. During an ultrasound cycle microbubbles oscillate, *i.e.*, they expand and subsequently contract. Depending on their elastic properties, on the local conditions, and on the acoustic settings, they move in the direction of the sound field, coalesce with other microbubbles, fragment, jet, cluster, release their contents, and dissolve in the surrounding liquid.¹ The diverse behaviour of encapsulated microbubbles in different acoustic regimes has triggered the idea to use them as ultrasound-controlled vehicles to facilitate the delivery of therapeutic agents to a site of interest. **Such a noninvasive, localised, side-effect-free method would revolutionise drug delivery as we know it.**

Cellular uptake of drugs and deoxyribonucleic acid (DNA) is increased when the region of interest is under sonication, and even more so when an ultrasound contrast agent is present.² This increased uptake has been attributed to the formation of transient porosities in the cell membrane that have diameters up to 0.1 μm , *i.e.*, big enough for the transport of drugs into the cell. The pores reseal themselves within one minute. The ultrasound-assisted transient permeabilisation of a cell membrane is called sonoporation. Understanding the physics underlying sonoporation is of uttermost importance for the development of ultrasound-activated therapeutic agents.

There are five non-exclusive hypotheses for explaining the sonoporation phenomenon from a physics point of view.³ These have been summarised in Figure 1. It is noted that fragmenting microbubbles cannot create pores in cells, since fragmentation costs energy. (a) **Push**: During its expansion phase, a microbubble might touch a cell membrane surface. The pushing motion would then cause the cell membrane to be locally disrupted. The pushing mechanism would occur within half an ultrasound cycle. However, under typical sonication conditions, microbubble excursion amplitudes are low. Also, typically, microbubbles are much more flexible than cells. Our current understanding of microbubble physics does not support the push mechanism if the microbubble is not attached. However, if the microbubble is already attached to the cell membrane whilst expanding, pushing under influence of radiation forces might cause the membrane to rupture. The latter mechanism might occur over multiple cycles. (b) **Pull**: During the contraction phase of an oscillating microbubble, the plasma filling the void left by the contracting bubble might pull the cell membrane towards the microbubble. This pulling motion would then cause the cell membrane to be locally disrupted. The pulling mechanism would occur within half an ultrasound cycle. However, under typical sonication conditions, microbubble contractions do not result in an inertial collapse. Moreover, the replaceive mass of a contracting microbubble is much lower than the fluid supposedly causing the pull. Therefore, this mechanism is less plausible than the push mechanism in non-attached conditions. However, if the microbubble is attached to the cell membrane, a similar mechanism

might occur as described under (a), where pulling under the influence of radiation forces might cause the membrane to rupture. (c) **Jetting**: Jetting is the asymmetric collapse of a bubble, creating a funnel-shaped protrusion through the bubble that is directed towards a boundary. This spectacular phenomenon has actually been optically observed on a microscopic scale through cells.⁴ The jetting phenomenon occurs within half an ultrasound cycle. However, jetting exclusively occurs when using high acoustic amplitudes, at the upper end of clinical settings. Also, there has not been any proof yet of cell survival after jetting. Based on empiric studies that relate jet length to pore size, we excluded the role of jetting as a dominant mechanism involved in sonoporation.⁵ (d) **Streaming**: If a microbubble is fixed to a membrane, the fluid streaming around the oscillating bubbles creates enough shear to rupture the membrane.⁶ Here, long pulse lengths are required to set the fluid in motion. However, low acoustic amplitudes should suffice to create the rupturing shear of a typical cell membrane. Existing research has proven the feasibility of the streaming mechanism in bound conditions, so this mechanism should work for targeted contrast agents that attach to cells. Further research will show whether streaming around weakly-attached microbubbles creates enough shear for cell membranes to rupture. (e) **Translation**: Owing to radiation forces, lipid-encapsulated microbubbles may translate through cell membranes or channels in the cell membrane. The microbubble may lose part of its shell whilst passing through the cell membrane. As a result, the gas will dissolve after entry. In case of therapeutic loading, the load would be delivered directly into the target cell. This mechanism requires long pulse lengths and low acoustic amplitudes. Very recently, fluorescence-coated ultrasound contrast agent microbubbles were observed to move into HeLa cells at a low mechanical index (MI) of 0.15, using high-speed video footage under confocal microscopy,⁷ an example of which is given in Figure 2. The microbubbles dissolved after entering the cells. The cells survived the sonoporation treatment, confirming the transient character of sonoporation.

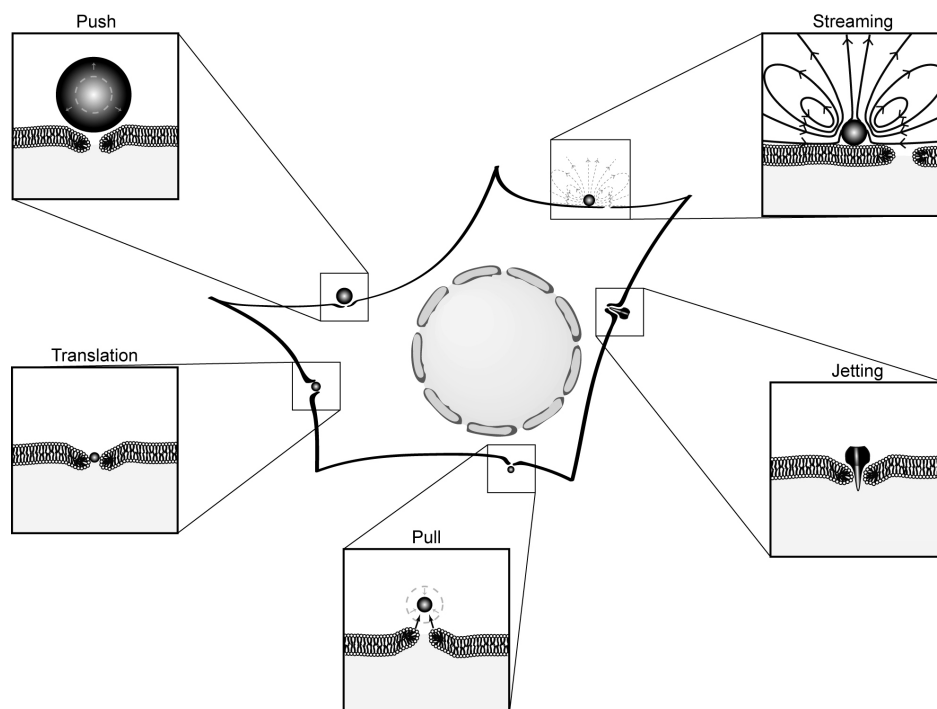


Figure 1: Schematic representation of the five physical mechanisms supposedly involved in sonoporation.

All five of these mechanisms require the presence of a microbubble in the vicinity of the cell. Yet, increased drug uptake has also been reported without the use of any ultrasound contrast agent, but merely an ultrasound field itself. Despite speculations about the role of inertial cavitation in the latter, clinical ultrasound scanners do not generate fields strong enough to create such spontaneous microbubbles in blood. Recently, it was found that (bilayer) cell membranes themselves act as cavitation nuclei.⁸ Even at modest acoustic pressures, cell membranes might rupture due to the building up of gas cavities inside the bilayer. This important finding would explain the sonoporation in the absence of ultrasound contrast agent microbubbles. Moreover, it explains why bubbles are attracted to cells that are not in the travel path of the ultrasound wave. However, given the low MI at which cells attract microbubbles, more study is required regarding the safe use of ultrasound contrast agents in long-pulse-length imaging.

In conclusion, in current clinical settings, four non-exclusive mechanisms are plausible for the physical explanation for sonoporation with the aid of ultrasound contrast agent microbubbles.

- ¹ Postema M, Gilja OH. Contrast-enhanced and targeted ultrasound. *World J Gastroenterol* **2011** 17:28–41.
- ² Postema M, Gilja OH. Ultrasound-directed drug delivery. *Curr Pharm Biotechnol* **2007** 8:355–361.
- ³ Postema M, Gilja OH, van Wamel A. CEUS and sonoporation. In: Postema M. *Fundamentals of Medical Ultrasonics*. London: Spon press **2011** 205–217.
- ⁴ Prentice P, Cuschieri A, Dholakia K, Prausnitz M, Campbell P. Membrane disruption by optically controlled microbubble cavitation. *Nature Phys* **2005** 1:107–110.
- ⁵ Postema M, Gilja OH. Jetting does not cause sonoporation. *Biomed Tech* **2010** 55(S1):19–20.
- ⁶ Marmottant P, Hilgenfeldt S. Controlled vesicle deformation and lysis by single oscillating bubbles. *Nature* **2003** 423:153–156.
- ⁷ Delalande A, Kotopoulis S, Rovers T, Pichon C, Postema M. Sonoporation at a low mechanical index. *Bub Sci Eng Technol* **2011** 3:3–11.
- ⁸ Krasovitski B, Frenkel V, Shoham S, Kimmel E. Intramembrane cavitation as a unifying mechanism for ultrasound-induced bioeffects. *Proc Nat Acad Sci* **2011** 108:3258–3263.

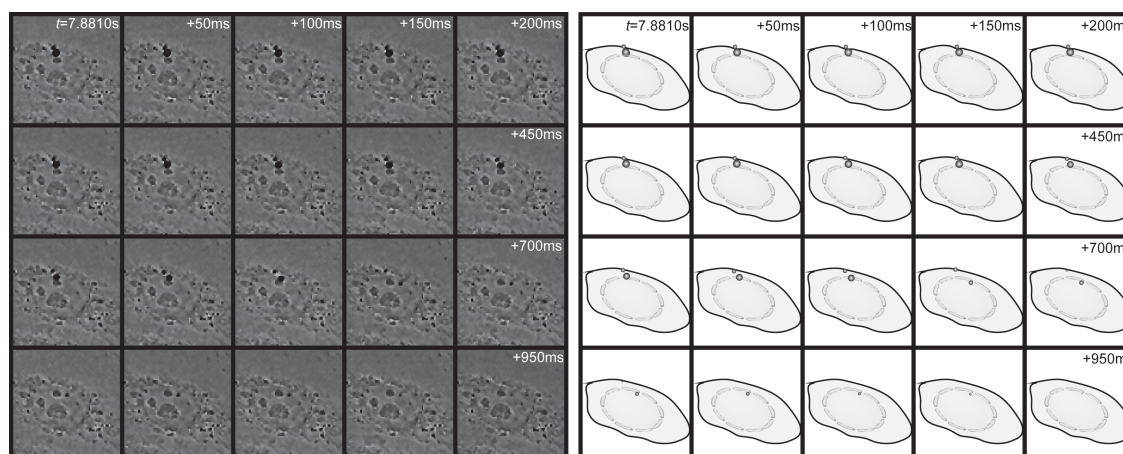


Figure 2: Translation of a microbubble into a HeLa cell. Each frame corresponds to a 37×37 - $(\mu\text{m})^2$ area.