



HAL
open science

JG-04 Low frequency Induction heating of a ferromagnetic catheter: feasibility

Y Liu, Z Xiang, J Garcia, B Newell, M Q Le, Benjamin Ducharne

► **To cite this version:**

Y Liu, Z Xiang, J Garcia, B Newell, M Q Le, et al.. JG-04 Low frequency Induction heating of a ferromagnetic catheter: feasibility. INTERMAG 2021, Apr 2021, Lyon (virtual conference), France. hal-03218900

HAL Id: hal-03218900

<https://hal.science/hal-03218900>

Submitted on 6 May 2021

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

JG-04 Low frequency Induction heating of a ferromagnetic catheter: feasibility.

Y. Liu^{1,3}, Z. Xiang¹, J. Garcia², B. Newell², M.Q. Le¹, B. Ducharne^{1,3}

¹Laboratoire de Génie Electrique et Ferroélectricité, INSA Lyon, FRANCE.

²School of Engineering Technology, Purdue University, IN USA.

³ELyTMaX UMI 3757, CNRS – Université de Lyon – Tohoku University, International Joint Unit, Tohoku University, Sendai, JAPAN.

Additive manufacturing of smart materials is a novel field in engineering. The ability to produce adaptable materials in varying geometries opens the door to the creation of a tremendous variety of new sensors, actuators and applications in domains including, transportation, energy production and medicine [1][2]. In this work, our objective is to build a ferromagnetic catheter by using additive manufacturing principles employed for the creation of smart materials. Induction heating phenomena takes place in the ferromagnetic catheter due to the influence of a varying magnetic excitation field. This contactless heat source can be used to heal locally and destroy damaged blood vessels. According to medical specialists, thermal ablation of varicose veins requires a temperature close to 120°C and time constants lower than a few seconds [3]. First investigation results showed great potential for success using the low frequency induction heating (LFIH) method but further surveys and validation steps are still needed before in vivo testing can commence.

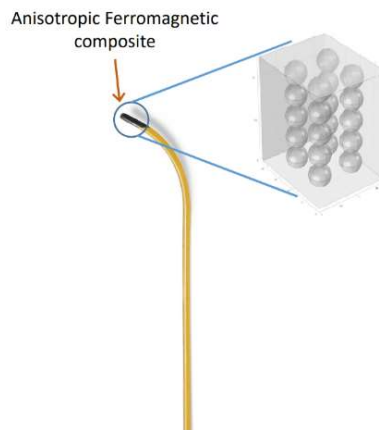


Fig. 1 – Illustration of the ferromagnetic catheter.

In this study, multi-physics simulation results, including ferromagnetic, thermal and fluid mechanics domains were compared to experimental data, then conclusions are proposed to establish the most adapted magnetic waveform (frequency) and its influence on the human tissues.

In our process, heat is transferred through a contactless method. The flexible 3D printed ferromagnetic catheter is subjected to an alternating magnetic excitation. Under the influence of the magnetic excitation, eddy currents are generated through the catheter creating heat. First

published results [4][5] describing this technique have experimentally demonstrated the feasibility of heat generation but the conditions tested and simulated were still far from the in vivo environment. In this study, we go deeper into the investigation process, we propose simulation results (magnetic, thermal ...) under much realistic experimental conditions. In [4], the authors limit the magnetic excitation signal to a few kHz. The purpose is to avoid undesired charge displacements in the surrounding tissue, but this restriction is strictly assumption based and further investigations must be under-taken to determine the optimal value for ablation while minimizing charge displacement. No further investigations have been proposed to establish a significant cutoff frequency.

In this new research, a ferromagnetic model for the simulation of the ferromagnetic composite magnetic behavior is developed first. This model is based on previous work on the same topic [6]-[9] and it investigates the frequency dependence of the composite hysteresis area, i.e. the heat generated through the LFIH influence. Next, comparisons between the model and experimental situations are investigated to set the ferromagnetic model parameters and to establish the most efficient LFIH frequency. Finally, multi-physics simulation results combined with experimental tests are reviewed to predict the ferromagnetic composite's behavior on living tissues under the influence of the optimized magnetic excitation.

Before validating the ferromagnetic catheter as a realistic treatment method for varicose veins, special attention must be given to the undesired charges or ionic displacements in the healthy surrounding tissues causing local temperature elevations and degradations. A compromise between treatment and negative effects on surrounding tissue must be made to establish the best working frequency. Numerical simulations are proposed to establish the optimized configuration of the magnetic source (frequency, amplitude) and of the ferromagnetic catheter behavior, these results constitute a huge step toward a first medical test.

References

- [1] Standard A. F2792, Pa, USA: ASTM International, 2012.
- [2] G.N. Levy, R. Schindel, J.P. Kruth, "Rapid manufacturing and rapid tooling with layer manufacturing (LM) technologies, state of the art and future perspectives", *CIRP Annals*, Vol. 52, Iss. 2, pp. 589 – 609, 2003.
- [3] S. Nehemiah, D. Carradice, T. Wallace, G.E. Smith, I.C. Chetter, "Endovenous thermal ablation for healing venous ulcers and preventing recurrence", *Cochrane Library*, Iss. 13, 2013.
- [4] Z. Xiang, K.I. Jakkpat, B. Ducharne, J.F. Capsal, N.D. Schiava, J.F. Mogniote, P.J. Cottinet, P. Lermusiaux, M.Q. Le, "Enhancing low-frequency induction heating effect of magnetic composites for medical applications", *polymers* 2020, 12(2), 386, 2020.
- [5] Z. Xiang, B. Ducharne, N.D. Schiava, J.F. Capsal, P.J. Cottinet, G. Coativy, P. Lermusiaux, M.Q. Le, "Induction Heating-based Low-Frequency Alternating Magnetic Field: High Potential of Ferromagnetic Composites for Medical Applications", *Mat. & Des.*, Vol. 174, 107804, 2019.
- [6] M. A. Raulet, B. Ducharne, J.P. Masson, and G. Bayada, "The magnetic field diffusion equation including dynamic hysteresis: a linear formulation of the problem", *IEEE Transactions on Magnetics*, Vol. 40, n° 2, pp. 872-875, 2004.
- [7] B. Ducharne, G. Sebald, D. Guyomar, G. Litak, "Fractional model of magnetic field penetration into a toroidal soft ferromagnetic sample", *Int. J. of Dyn. And Cont.*, pp. 1-8, 2017.
- [8] Z. Xiang, B. Gupta, M.Q. Le, P.J. Cottinet, B. Ducharne, "Hysteresis model of 3D printed magnetic particles based polymer composite materials", 2018 IEEE International Magnetics Conference (INTERMAG), pp. 1 – 5, 2018.
- [9] B. Gupta, B. Ducharne, G. Sebald and T. Uchimoto, "Magnetic lump model for the hysteresis frequency dependence of a polymer matrix", proceeding of the 21st international conference on the Computation of Electromagnetic Fields COMPUMAG, 2017.