



**HAL**  
open science

## Te<sub>2</sub> absorption spectrum from 19000 to 24000 cm<sup>-1</sup>

Amanda J. Ross, Joseph M Cardon

► **To cite this version:**

Amanda J. Ross, Joseph M Cardon. Te<sub>2</sub> absorption spectrum from 19000 to 24000 cm<sup>-1</sup>. Journal of Molecular Spectroscopy, 2022, 384, pp.111589. 10.1016/j.jms.2022.111589 . hal-03584038

**HAL Id: hal-03584038**

**<https://hal.science/hal-03584038>**

Submitted on 22 Feb 2022

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

## Te<sub>2</sub> absorption spectrum from 19000 to 24000 cm<sup>-1</sup>

Amanda J. Ross<sup>1</sup>, and Joseph M. Cardon<sup>2</sup>


<sup>1</sup>Institut Lumière Matière, Université Claude Bernard Lyon 1, CNRS, Université de Lyon, F-69622 Villeurbanne, France.

<sup>2</sup>Ideal Vacuum Products, 5910 Midway Park Blvd NE, Albuquerque, NM 87109, USA.

*Corresponding Author : Amanda J. Ross, e-mail amanda.ross@univ-lyon1.fr*

### Graphical Abstract

#### Te<sub>2</sub> atlas as an ASCII file

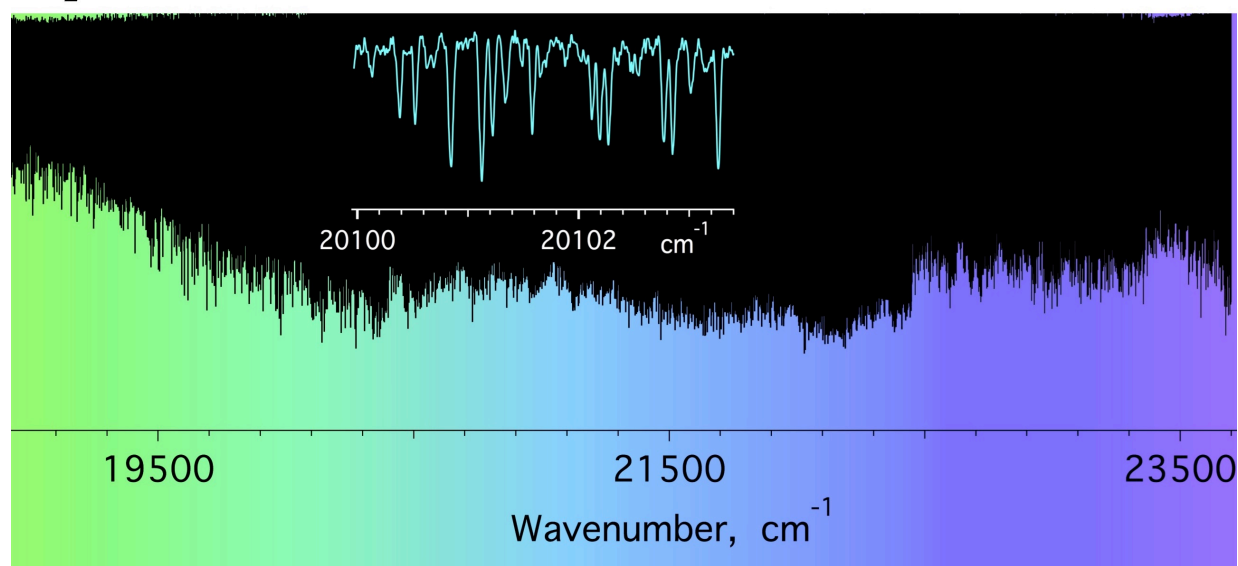

### Abstract

A Fourier-transform absorption spectrum of <sup>130</sup>Te<sub>2</sub> has been recorded from 19000 to 24000 cm<sup>-1</sup> at approximately 620 °C; a transmission spectrum is made available in ASCII format. The spectrum is intended to aid spectral calibration in the blue-violet region. It extends slightly beyond the paper version of the Tellurium atlas, published in 1980 (J. Cariou and P. Luc, 'Atlas du spectre d'absorption de la molécule de tellure', Laboratoire Aime-Cotton CNRS (1980)).

## Introduction

This work was motivated by interest in having a digital record of the absorption spectrum of tellurium vapour, as a supplement to the paper atlas of Cariou and Luc<sup>1</sup> in order to simplify comparison and scaling between laboratory reference signals and this spectral atlas. The strong and crowded  $A0_u^+ - X0_g^+$  bands of  $Te_2$  have been known for many years, and provide useful benchmarks for calibration beyond  $20000\text{ cm}^{-1}$ , where room-temperature B-X  $I_2$  absorption cuts off. Tellurium melts at around  $450\text{ }^\circ\text{C}$  and  $Te_2$  is the dominant form in the vapour phase, giving saturated vapour pressures of 2 Torr at  $550\text{ }^\circ\text{C}$  and 10.5 Torr at  $635\text{ }^\circ\text{C}$ <sup>2</sup>. Barrow and du Parcq noted that isotopically pure tellurium was critical to analysis of the A-X and B-X systems<sup>3</sup>, and this is equally important in obtaining a useable reference spectrum. There are 8 naturally occurring isotopes of tellurium, the most abundant of these are  $^{130}\text{Te}$  (34.1%),  $^{128}\text{Te}$  (31.7%),  $^{126}\text{Te}$  (18.8%) and  $^{125}\text{Te}$  (7.1%)<sup>4</sup>. The sample used in this work was a standard 10 cm sealed evacuated cell supplied by Ideal Vacuum Products, containing a small amount of  $^{130}\text{Te}$ .

## Experiment

The tellurium cell was placed in a purpose-built furnace, designed to maintain temperature to within  $\pm 7\text{ }^\circ\text{C}$ . The furnace is resistively heated with a single zone ceramic fiber heating element. It is fitted with fused silica windows to produce better temperature homogeneity across the cell than an open furnace would allow; this also minimizes deposition of tellurium on the window faces of the sealed reference cell. The temperature is monitored by a type K thermocouple and stabilized by a PID control loop<sup>5</sup>. We worked at temperatures between  $600$  and  $640\text{ }^\circ\text{C}$  to provide significant absorption without saturation. Emission from a quartz halogen bulb (Osram) operated at up to 11 Amp, 22 Volts dc passed through the cell, and was focused on the 'emission port' aperture of a Fourier transform spectrometer (Bomem DA3). Optical filters were selected so that the spectrum ( $417\text{-}510\text{ nm}$ ) could be recorded in overlapping  $\sim 2000\text{ cm}^{-1}$  pieces, to reduce problems related to detector saturation at zero optical path difference coupled with weak interference signals elsewhere – an issue associated with broadband input. This also allowed us to record spectra at instrumental resolution nominally better than Doppler width without exceeding the W2000 computer memory limit of  $10^6$  points in our interferograms. Between 200 and 600 interferograms

were averaged in each segment of the spectrum to improve the signal/noise ratio. The quartz 'visible' beamsplitter performed well for wavelengths above 425 nm. Below this cut-off, it was replaced by the 'UV' beamsplitter. The short-wavelength limit was imposed by low signal levels in the tail of emission from the white light source. Interferograms were collected on a silicon avalanche photodiode, at an instrumental resolution varying from  $0.02\text{ cm}^{-1}$  at the long wavelength end of the spectrum to  $0.035\text{ cm}^{-1}$  in the violet. Interferograms were zero-padded by a factor of 2. A small part of the spectrum is illustrated in Figure 1. We show a raw spectrum and a transmittance trace generated by dividing the experimental absorption spectrum by a baseline contour to create a dimensionless Y axis. The raw intensity scale is arbitrary and uncorrected for instrumental response. The baseline in the transmittance spectrum appears noisy, but is in fact reproducible, revealing many weak transitions not necessarily listed in ref. 1.

Although the Fourier transform spectrometer is in principle self-calibrated by reference to its internal stabilised HeNe laser, we further processed the wavenumber scales to match established reference data, including the Doppler-free measurements from Gillaspay and Sansonetti (using frequency modulation)<sup>6</sup>, from Scholl and co-workers (via saturated absorption)<sup>7</sup> and three unblended lines at 444 nm from Coker and co-workers<sup>8</sup>, in addition to some 500 reference peaks taken from the existing Doppler-limited atlas of ref. 1. The choice of Doppler-limited reference lines was initially random, but severe outliers (clearly the result of trying to match blended lines) were discarded. We minimized the differences between the selected reference values and those returned by a 'peaks above threshold' algorithm, looking for upwards zero-crossings in a boxcar-smoothed first derivative in our 'transmittance' spectrum, fitting to a  $\Delta\sigma = a + b\sigma$  linear expression. These corrections to the raw wavenumber scale were of the order of  $0.03\text{ cm}^{-1}$  at  $23000\text{ cm}^{-1}$ .

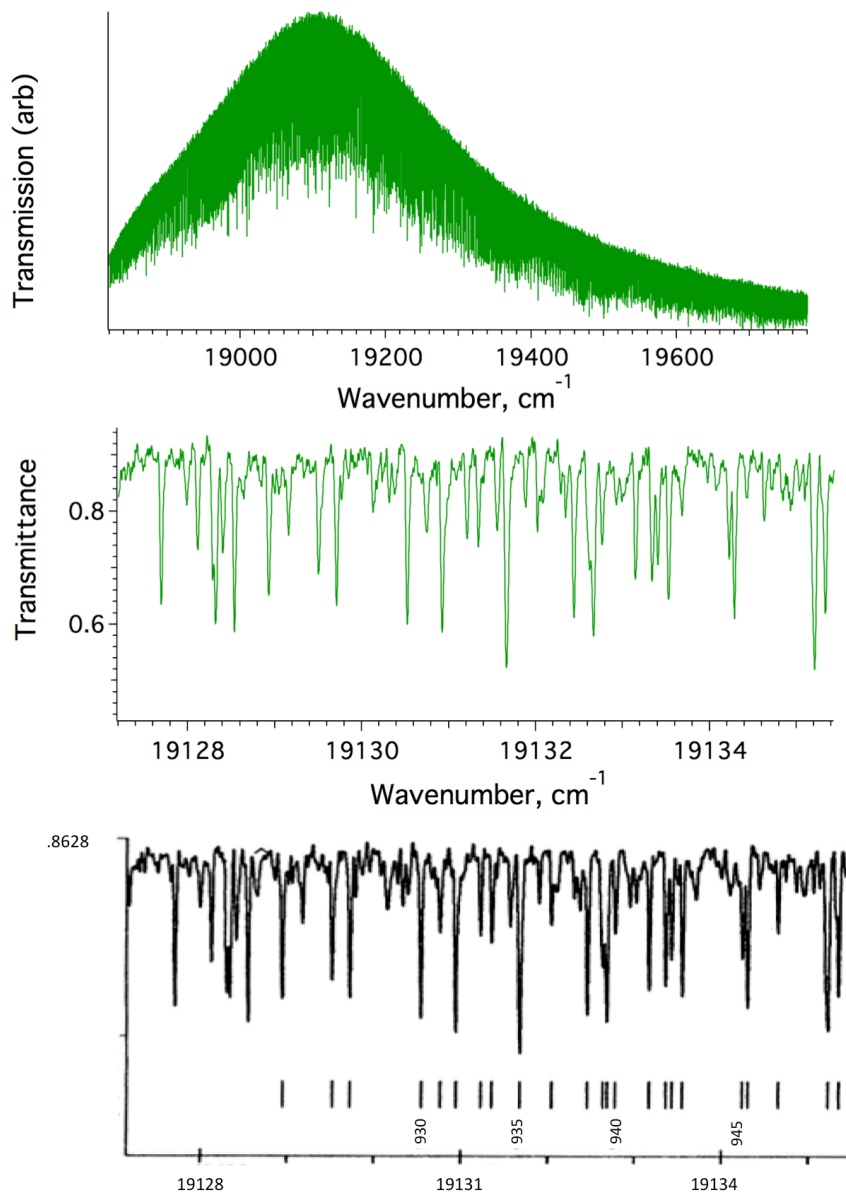


Figure 1. Illustration of the portion of the Tellurium absorption spectrum recorded through a combination of a blue-green filter (Corning glass 5-61) and a narrow-pass filter centred at 506 nm. The upper trace shows the raw absorption spectrum. The middle trace shows an  $8 \text{ cm}^{-1}$  window in the corresponding transmittance spectrum. The lower trace displays a scan of the same region from the paper atlas of ref. 1 for comparison, reproduced with permission from Laboratoire Aimé Cotton.

The measured FWHM linewidths of isolated peaks are between  $0.04$  and  $0.09 \text{ cm}^{-1}$ , and we would expect peak positions for resolved features to be determined with uncertainties about ten times smaller. Figure 2 illustrates the deviations of peak positions determined from our composite

spectrum with respect to our selection of transitions listed in the literature. The lines are wider than one would expect from considerations of Doppler broadening alone, and since  $^{130}\text{Te}$  has zero nuclear spin, we assume this results from a degraded performance of the Fourier transform spectrometer at short wavelengths.

Once the calibration controls were complete, we spliced and concatenated the pieces of spectrum using cubic spline interpolation to accommodate successive segments with interleaving wavenumber scales. This also allowed us to impose the intervals between data points as multiples of  $0.001\text{ cm}^{-1}$  in the Supplementary Data files.

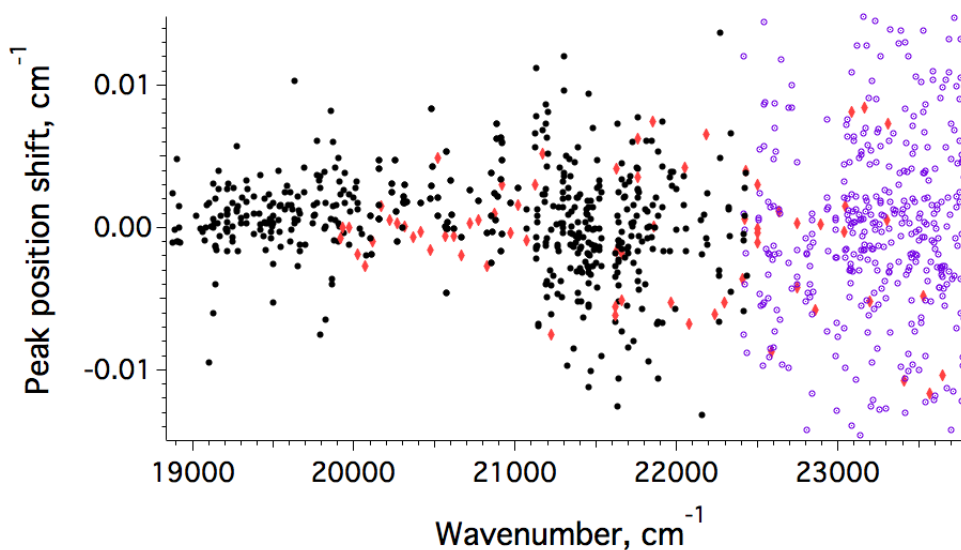


Figure 2. Scatter plot showing differences in  $\text{cm}^{-1}$  between peak positions determined as zero derivatives in our spectrum minus reference peak positions. Circles refer to the Doppler limited atlas<sup>1</sup>, diamonds (red) are shifts from the sub-Doppler values<sup>6-8</sup>. Open (violet) circles are from the lower-resolution spectra recorded with the UV beamsplitter.

The composite spectrum is available to download in ASCII format from <https://data.mendeley.com/datasets/kmkbwtjhd3/1>, or may be obtained from the authors on request. The combination of optics and sources available has restricted the spectral range we can record; the spectrum actually extends to higher wavenumbers. Our spectrum extends a short way beyond the tellurium atlas of Luc and Cariou, but the spectral resolution is clearly lower than theirs below 450 nm. Nevertheless, these data should still prove to be a convenient secondary standard for Doppler-limited applications. We became motivated to record this spectrum while investigating the blue

$^4\Sigma^- - ^4\Sigma^-$  bands of  $\text{AlC}^9$ , where the sparser density of optogalvanic lines of Ar and Ne made calibration somewhat difficult, and we note that tellurium dimer is being used for calibration in other laboratories<sup>10-13</sup>. Although the optogalvanic spectrum of uranium<sup>14,15</sup> is also useful as a spectral reference in this wavelength range, the greater density of useful lines in the  $^{130}\text{Te}_2$  absorption spectrum is advantageous for the calibration of smaller wavenumber intervals.

### Acknowledgements

The authors wish to acknowledge the support of Ideal Vacuum Products LLC for this work, and to thank Professor D. Clouthier and Dr T. Smith for their helpful remarks and suggestions.

### References

1. P. Luc and J. Cariou, 'Atlas du spectre d'absorption de la molécule de tellure', CNRS, Laboratoire Aimé Cotton (1980).
2. R. E. Machol and E. F. Westrum, *J. Am. Chem. Soc.* **80** (12), 2950-2952 (1958).
3. R. F. Barrow and R. P. D. Parcq, *Proc. R. Soc. Lon. Ser-A* **327** ( ), 279-287 (1972).
4. J. Meija, T. B. Coplen, M. Berglund, W. A. Brand, P. De Bièvre, M. Gröning, N. E. Holden, J. Irrgeher, R. D. Loss, T. Walczyk and T. Prohaska, *Pure Appl. Chem.* **88** (3), 293-306 (2016).
5. PID Plug and Play Heater Control System from Ideal Vacuum Products LLC  
<https://www.idealvac.com/Ideal-Vacuum-Heavy-Duty-20A/pp/P107361>.
6. J. D. Gillaspay and C. J. Sansonetti, *J. Opt. Soc. Am. B* **8** (12), 2414-2419 (1991).
7. T. J. Scholl, S. J. Rehse, R. A. Holt and S. D. Rosner, *J. Opt. Soc. Am. B* **22** (5), 1128-1133 (2005).
8. J. Coker, H. Q. Fan, C. P. McRaven, P. M. Rupasinghe, T. Z. Yang, N. E. Shafer-Ray and J. E. Furneaux, *J. Opt. Soc. Am. B* **28**, 2934-2939 (2011).
9. D. J. Clouthier and A. Kalume, *J. Chem. Phys.* **144**, 034305 (2016).
10. M. Fan, C. A. Holliman, A. L. Wang and A. M. Jayich, *Phys. Rev. Lett.* **122**, 223001 (2019).
11. D. J. Matthew, S. H. Oh, A. Sevy and M. D. Morse, *J. Chem. Phys.* **144**, 214306 (2016).
12. J. R. Schmitz and M. C. Heaven, *J. Mol. Spectrosc.* **377**, 111426 (2021).
13. Z. N. Vealey, L. Foguel and P. H. Vaccaro, *J. Phys. Chem. A* **123**, 6506-6526 (2019).
14. A. J. Ross, P. Crozet, A. G. Adam and D. W. Tokaryk, *J. Mol. Spectrosc.* **369**, 111270 (2020).
15. B. A. Palmer, R. A. Keller and R. Engleman Jr, Los Alamos informal report **LA 8251-MS** (1980).