



**HAL**  
open science

## An organic transistor for the selective detection of a tropane alkaloid utilizing a molecularly imprinted polymer

Qi Zhou, Yui Sasaki, Kohei Ohshiro, Haonan Fan, Valentina Montagna, Carlo Gonzato, Karsten Haupt, Tsuyoshi Minami

► **To cite this version:**

Qi Zhou, Yui Sasaki, Kohei Ohshiro, Haonan Fan, Valentina Montagna, et al.. An organic transistor for the selective detection of a tropane alkaloid utilizing a molecularly imprinted polymer. *Journal of materials chemistry B*, In press, 10.1039/D2TB01067D . hal-03709006

**HAL Id: hal-03709006**

**<https://hal.science/hal-03709006>**

Submitted on 29 Jun 2022

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

# An organic transistor for the selective detection of a tropane alkaloid utilizing a molecularly imprinted polymer

Received 00th January 20xx,  
Accepted 00th January 20xx

Qi Zhou,<sup>a</sup> Yui Sasaki,<sup>a</sup> Kohei Ohshiro,<sup>a</sup> Haonan Fan,<sup>a</sup> Valentina Montagna,<sup>b</sup> Carlo Gonzato,<sup>b</sup> Karsten Haupt<sup>b,\*</sup> and Tsuyoshi Minami<sup>a,\*</sup>

DOI: 10.1039/x0xx00000x


This study proposes a chemical sensing approach for the selective detection of a tropane alkaloid drug based on an extended-gate-type organic field-effect transistor (OFET) functionalized with a molecularly imprinted polymer (MIP). From the viewpoint of pharmaceutical chemistry, the development of versatile chemical sensors to determine the enantiomeric purity of over-the-counter (OTC) tropane drugs is important because of their side effects and different pharmacological activities depending on their chirality. To this end, we newly designed an OFET sensor with a MIP (MIP-OFET) as the recognition element for a tropane drug based on a high complementarity among a template (*i.e.*, (*S*)-hyoscyamine) and functional monomers such as *N*-isopropylacrylamide and 2,2-dimethyl-4-pentenoic acid. Indeed, the MIP optimized by density functional theory (DFT) has succeeded in the sensitive and selective detection of (*S*)-hyoscyamine (as low as 1  $\mu$ M) by the combination of the OFET, with highly selective recognition sites in the MIP. The MIP-OFET was further applied to determine the enantiomeric excess (*ee*) of commercially available (*S*)-hyoscyamine, and the linearity changes in the threshold voltages of the OFET corresponded to the % *ee* values of (*S*)-hyoscyamine. Overall, the validation with tropane alkaloids revealed the potential of the MIP combined with OFET as a chemical sensor chip for OTC drugs in real-world scenarios.

## 1. Introduction

Alkaloid drugs classified in natural products<sup>1</sup> such as narcotics and psychotropics possess strong pharmacological activity toward the nervous systems because positively charged nitrogen atoms in these drugs are capable of binding to protein receptors through electrostatic interactions.<sup>2</sup> Among them, tropane skeletons based on 8-azabicyclo[3.2.1]octane are employed as the main component of drugs including atropine, scopolamine, etc.,<sup>3</sup> while such muscarinic blocking drugs could potentially evoke side effects (hallucination, memory impairment, blurred vision, etc.).<sup>4</sup> In particular, atropine is one of the antidotes to treat intoxications by organophosphorus derivatives, whereas relationships between these neurobiological side effects and the tropane drugs are still unclear.<sup>5</sup> In addition, the pharmacological activity of tropane drugs significantly depends on their chirality. Indeed, atropine is racemic hyoscyamine, and only the (*S*)-hyoscyamine enantiomer shows pharmacological activity.<sup>4</sup> Taking into consideration the strict regulations concerning enantiomeric purity in the pharmaceutical industry, the accurate and easy

determination of enantiomeric excess (*ee*) of over-the-counter (OTC) drugs is required.<sup>6-9</sup>

To date, the detection of atropine has been performed by utilizing liquid chromatography equipped with tandem mass spectrometry, which achieved the % *ee* determination of atropine.<sup>10,11</sup> However, such conventional instrumental methods are complicated and time-consuming because of the pre-processing of samples. Therefore, we focused on an organic field-effect transistor (OFET) device<sup>12-18</sup> as a sensing platform for tropane alkaloid detection. The transistor characteristics rely on potential changes on a gate electrode.<sup>19</sup> Indeed, OFETs can quantify chemical information by an appropriate sensor

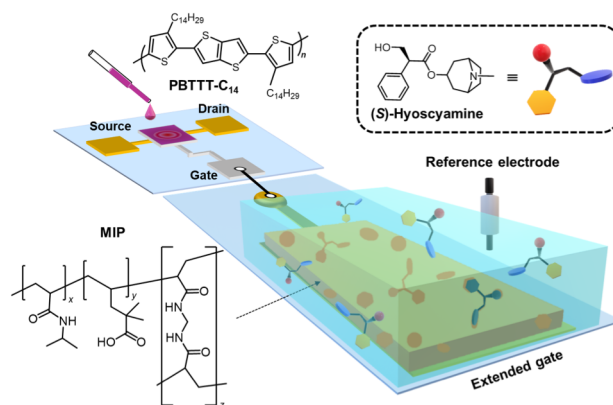

**Fig. 1** Schematic illustration of the tropane drug sensor based on the extended-gate type OFET functionalized with the MIP.

<sup>a</sup> Institute of Industrial Science, The University of Tokyo, 4-6-1 Komaba, Meguro-ku, Tokyo, 153-8505, Japan.

<sup>b</sup> CNRS Enzyme and Cell Engineering Laboratory, Université de Technologie de Compiègne, Rue du Docteur Schweitzer, CS 60319, 60203 Compiègne Cedex, France  
Electronic Supplementary Information (ESI) available: Characterization of the MIP and the extended-gate electrode, FT-IR, FM-AFM, fabrication details and basic characteristics of the OFET, DFT calculation results, selectivity test, HPLC charts of enantiomeric excess of (*S*)-hyoscyamine. See DOI: 10.1039/x0xx00000x

design utilizing the gate electrode. In an extended-gate-type OFET, a molecular recognition scaffold on the separated gate electrode (*i.e.*, extended-gate) as the sensing part is connected to the gate of the OFET, which allows chemical sensing in aqueous media.<sup>20-22</sup>

For the detection of tropane derivatives, elaborate receptor designs considering high steric hindrance are necessary.<sup>23</sup> Conventional alkaloid sensors based on cavity molecules and molecular clefts have been widely studied,<sup>23-28</sup> but the development of easy-to-use drug sensors is still challenging because of the difficulty of appropriate receptor designs. In this regard, molecular imprinting is capable of generating cavities for specific analyte recognitions by noncovalent interactions (hydrogen bonds,  $\pi$ - $\pi$  interactions, electrostatic interactions, etc.) in synthetic polymers (molecularly imprinted polymers, MIPs), achieving highly sensitive and selective detection.<sup>29-35</sup> With this three-dimensional recognition space, MIPs were shown to successfully detect tropane drugs.<sup>36-38</sup> However, previous works on the use of MIPs for the detection of atropine did not report on the selective discrimination of (*S*)-hyoscyamine.<sup>39-42</sup> Besides, previous reports have confirmed that MIPs can be formed as thin layers or membranes on substrates including electrodes,<sup>43-46</sup> interfacing MIPs with the extended-gate electrode should be possible. **Indeed, the detectability of extended-gate-type inorganic FETs functionalized with MIPs for various chemical species has been revealed.**<sup>47-49</sup> Hence, we propose herein an extended-gate-type OFET functionalized with a novel MIP (MIP-OFET) based on poly(*N*-isopropylacrylamide-*co*-2,2-dimethyl-4-pentenoic acid-*co*-*N,N'*-methylenebisacrylamide) (p(NIPAM-*co*-DMPA-*co*-MBAAM)) for the detection of (*S*)-hyoscyamine and its *ee* determination (Fig. 1).

## 2. Experimental

### 2.1. Materials

Reagents and solvents employed in this study were commercially available and used as supplied. *N*-Isopropylacrylamide (NIPAM),<sup>50</sup> 2,2-dimethyl-4-pentenoic acid (DMPA), *N,N'*-methylenebisacrylamide (MBAAM),<sup>43</sup> and ammonium persulfate for the synthesis of the MIP and a non-imprinted polymer (NIP), tetradecylphosphonic acid for the dielectric layer, and the analytes such as (*S*)-hyoscyamine, atropine, tropine, solifenacin succinate, tropicamide, and oxybutynin hydrochloride were purchased from Tokyo Chemical Industry Co., Ltd. The reagents purchased from FUJIFILM Wako Pure Chemical Industries, Ltd. were potassium chloride (KCl), hydrogen tetrachloroaurate(III) tetrahydrate (HAuCl<sub>4</sub>), *N*-ethylethanamine and tetramethylethylenediamine (TEMED). Poly{2,5-bis(3-tetradecylthiophen-2-yl)thieno[3,2-*b*]thiophene} (PBTTT-C<sub>14</sub>),<sup>51</sup> tropic acid, and 1,2-dichlorobenzene were purchased from Merck KGaA. The organic solvent and reagents obtained from Kanto Chemical Co., Inc. were 2-propanol, potassium hexacyanoferrate(III) (K<sub>3</sub>Fe(CN)<sub>6</sub>), sodium hydroxide, *n*-hexane, and disodium

hydrogenphosphate dodecahydrate (Na<sub>2</sub>H<sub>2</sub>PO<sub>4</sub>). For the device fabrication, a glass substrate (model Eagle XG, 2 cm×2.5 cm), gold (Au) particle, and aluminum (Al) wire (1 $\phi$ ) were purchased from Corning, Inc., Tanaka Kikinokogyo Co., Ltd, and Furuuchi Chemical Co., Ltd., respectively. A silver paste (Dotite, type: D-500) purchased from Fujikura Kasei Co., Ltd. was utilized for the OFET measurements. The electrochemical measurements were carried out using a Pt wire counter electrode and an Ag/AgCl reference electrode (model: RE-1B), which were purchased from BAS Inc. CYTOP™ (model CTL-809M) with perfluorotributylamine and a polyethylene naphthalate (PEN) were supplied from AGC Co., Ltd. and TOYOBO Co., Ltd., respectively. Aqueous solutions for all experiments were prepared by using Milli-Q water (18.2 M $\Omega$  cm). The enantiomeric purity of hyoscyamine was investigated by high-performance liquid chromatography (HPLC) with a chiral column (Daicel CHIRALCEL OZ-H). The enantiomeric purity of the commercially available (*S*)-hyoscyamine was determined to be 90.2% *ee* (Fig. S16, Electronic Supplementary Information (ESI)<sup>†</sup>).

### 2.2. Measurements

The complex of monomers with (*S*)-hyoscyamine was optimized by density functional theory (DFT) calculations in a package of Gaussian 16 REV. C. 011.<sup>52</sup> Chronoamperometry and differential pulse voltammetry (DPV) were carried out on an SP-300 potentiostat (Biologic). In the electrochemical measurement, the potential was scanned from 0 V to 0.45 V in K<sub>3</sub>Fe(CN)<sub>6</sub> (5 mM) with phosphate buffer (100 mM, pH 7.0) containing KCl (100 mM) at 25 °C. The synthesized MIP was evaluated by a Fourier transform infrared spectrophotometer (FT-IR) (Nicolet55, Thermo Fisher Scientific Inc.) with a KBr pellet and with a variable angle grazing angle ATR (Harrick Scientific), a field-emission scanning electron microscope (FE-SEM) (JSM6330F, JEOL), and a frequency modulation atomic force microscope (FM-AFM) (NanoWizard® 3 BioScience AFM, Bruker). The electrical characteristics of all OFET devices were measured using a source meter (Keithley 2602B).

### 2.3. Fabrication of the MIP and NIP electrodes

NIPAM (83 mg, 0.73 mmol), MBAAM (3 mg, 0.019 mmol), (*S*)-hyoscyamine (53 mg, 0.18 mmol), and DMPA (25  $\mu$ L, 0.18 mmol) were dissolved in Milli-Q water (2.5 mL), and then the mixture was stirred for 20 min at 25 °C under an inert atmosphere. After becoming a colorless and transparent solution, TEMED (2.7  $\mu$ L, 0.018 mmol) was added to the mixture solution and stirred for 2 min. Then, ammonium persulfate (3 mg, 0.013 mmol) was added to the mixture solution, followed by stirring for 2 min. After maintaining the aqueous solution for 8 h at 25 °C under an inert atmosphere, a colorless macro hydrogel was obtained. The hydrogel was washed with an HCl solution (10 mM) 3 times. For the characterization of the obtained polymer by FT-IR, the hydrogel was dried at 70 °C for 5 h by using a vacuum dry oven (AVO-200NB, ETTAS). The NIP was synthesized according to the abovementioned procedure without using (*S*)-hyoscyamine,

while NaOH (2 mg, 0.05 mmol) was added to improve the solubility of DMPA.

The extended-gate Au electrode with 15 mm<sup>2</sup> of the conductive area and 100 nm in thickness was fabricated on the PEN film by utilizing thermal evaporation equipment (SVC-700TMSG/SVC-7PS80, SANYU Electron). An Au nanostructure (AuNS) was modified on the surface of the extended-gate electrode in an HAuCl<sub>4</sub> solution (100 mM) by chronoamperometry based on a three-electrode system. The potential was fixed at -0.1 V for 60 s. The treated electrode was rinsed with ultrapure water 3 times, followed by drying with N<sub>2</sub> gas flow. The MIP layer was synthesized by drop-casting the aqueous solution containing monomers, (*S*)-hyoscyamine, and the initiator (*i.e.*, the combination of TEMED and ammonium persulfate) (8 μL) onto the extended-gate electrode. The treated electrode was kept at 25 °C for 8 h under ambient conditions to attach the MIP to the surface of the AuNS on the extended-gate electrode. The electrode was rinsed with the HCl solution (10 mM) 3 times and subsequently immersed in the phosphate buffer (100 mM, pH 7.0) containing KCl (100 mM) at 25 °C for 4 h for removing the residue of the template. The NIP attached electrode was fabricated according to the above-mentioned procedure without (*S*)-hyoscyamine. The MIP or NIP attached electrode for FE-SEM and FT-IR characterization was dried at 70 °C for 5 h in the vacuum dry oven.


#### 2.4. Fabrication and operation of the extended-gate-type OFET

Vacuum thermal evaporation equipment was applied to fabricate an aluminium gate electrode (30 nm in thickness) on the glass substrate. The aluminium oxide formed by a reactive ion etching (SAMCO RIE-10NR) was treated with tetradecylphosphonic acid to form a double dielectric layer. Next, source and drain Au electrodes (30 nm in thickness) were deposited using vacuum thermal evaporation equipment. Subsequently, a 1,2-dichlorobenzene solution containing PBTTT-C<sub>14</sub> was drop cast onto a channel region of the OFET. Finally, the surface of the polymer semiconductive layer was fully covered with CYTOP<sup>TM</sup>. The MIP or NIP modified extended-gate electrode was connected to the OFET through a copper conductive cable, and the gate voltage was applied through the Ag/AgCl reference electrode. The detectability of the extended-gate-type OFET was assessed under ambient conditions. The fabricated OFET device showed low-voltage operable transistor characteristics (< |3| V), which was suitable for chemical sensing applications. More details of the fabrication process and basic transistor characteristics were summarized in the ESI<sup>†</sup>.

### 3. Results and discussion


#### 3.1. Optimization and characterization of the MIP and its modification on the extended-gate electrode

NIPAM and DMPA were selected as main monomers, because these monomers possess amide and carboxy groups capable of forming hydrogen bonds with the target (*S*)-hyoscyamine. Moreover, DMPA was selected owing to the steric effect

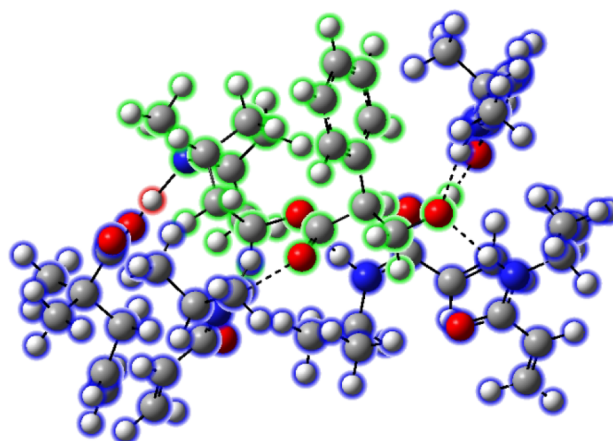

**Fig. 2** The molecular complex (NIPAM:DMPA:(*S*)-hyoscyamine = 4:1:1) optimized by DFT calculation at the B3LYP (D3BJ)/def2SVP level with IEFPCM solvent model (solvent set as water).

derived from its branch methyl groups for the detection of the bulky structural drug.<sup>53</sup> Besides, MBAAM was employed as the crosslinker,<sup>54</sup> resulting in a 3D MIP network for increasing the specific surface area (*vide infra*). To design the MIP for (*S*)-hyoscyamine, DFT calculation was performed by Gaussian 16 at B3LYP(D3BJ)/def2SVP level with IEFPCM solvent model (solvent set as water),<sup>55-58</sup> the result of which was visualized by GaussView 6.0.16.<sup>59</sup> Four types of complexes composed of NIPAM, DMPA, and (*S*)-hyoscyamine at different molar ratios were optimized by the DFT calculation. In this regard, the binding energies were precisely calculated with the IEFPCM solvent model and the counterpoise method, which could decrease the influence of the basis set superposition error (BSSE) (Table S1<sup>†</sup>). Among them, the complex with the molar ratio (NIPAM: DMPA: (*S*)-hyoscyamine = 4:1:1) showed the lowest binding energy (-107.74 kJ/mol), which revealed the high complementarity through six hydrogen bonds among (*S*)-hyoscyamine, NIPAM, and DMPA (Fig. 2). Therefore, the MIP was synthesized by radical polymerization according to the above molar ratio. The DPV measurement of the MIP was carried out to evaluate the changes in the peak current after the template extraction. Almost no changes in the peak current

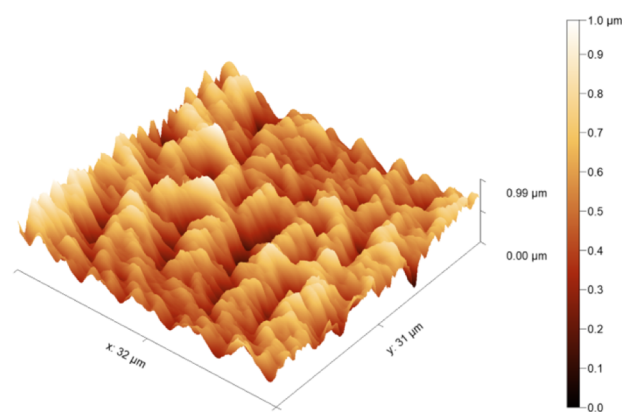

**Fig. 3** FM-AFM image of the MIP-gold nanostructure (AuNS) attached extended-gate electrode.

after third-time extraction implied the removal of the template completely (Fig. S5<sup>†</sup>). The obtained product was characterized by FT-IR, and the absorption peaks corresponding to C=O stretching (1727 cm<sup>-1</sup> for carboxylic acid, 1646 cm<sup>-1</sup> for amide), N-H stretching (3305 cm<sup>-1</sup>), C-C stretching of C-CO-O (1166 cm<sup>-1</sup>), C-N stretching (1369 cm<sup>-1</sup>), C-H stretching (2969 cm<sup>-1</sup>), N-H bending (1540 cm<sup>-1</sup>) and CH<sub>2</sub> bending (1454 cm<sup>-1</sup>) bands supported the successful preparation of the MIP [*i.e.*, p(NIPAM-co-DMPA-co-MBAAM)] (Fig. S1(A)<sup>†</sup>). Meanwhile, the FT-IR result of the NIP showed similar peaks (Fig. S1(B)<sup>†</sup>), which were derived from the same monomers of the NIP as the MIP.

Next, chronoamperometry was utilized to form the AuNS layer<sup>60</sup> on the thermally deposited Au extended-gate electrode, which could enhance the adhesion by physisorption between the MIP layer and the Au electrode. The surface morphology of the polymer-attached extended-gate electrodes was evaluated by FE-SEM and FM-AFM. The FE-SEM image of the MIP indicated that a porous xerogel was formed with some macropores, offering a large specific surface area. In addition, sharp architectures derived from gold needles were observed (Fig. S3(A)). Meanwhile, the NIP showed a rather plain surface with fewer macropores (Fig. S3(B)). Moreover, the FM-AFM image of the bare Au electrode showed low surface roughness with a root mean square deviation (*Rq*) of ~5 nm (Fig. S4(A)<sup>†</sup>), while the AuNS modified Au electrode displayed higher surface roughness with *Rq* of ~220 nm (Fig. S4(B)<sup>†</sup>). Furthermore, a decrease in the surface roughness was observed in the MIP-AuNS modified electrode (*Rq*: ~144 nm) (Fig. 3). The observed change in the *Rq* value after immobilization of the MIP suggested that the surface of the AuNS layer was fully covered by the MIP layer with ~200 nm in thickness. On the other hand, the NIP without the template showed a rather plain surface (*Rq*: ~120 nm) with fewer macropores (Fig. S4(C)<sup>†</sup>) as also observed in the FE-SEM. Such difference in the surface morphology was

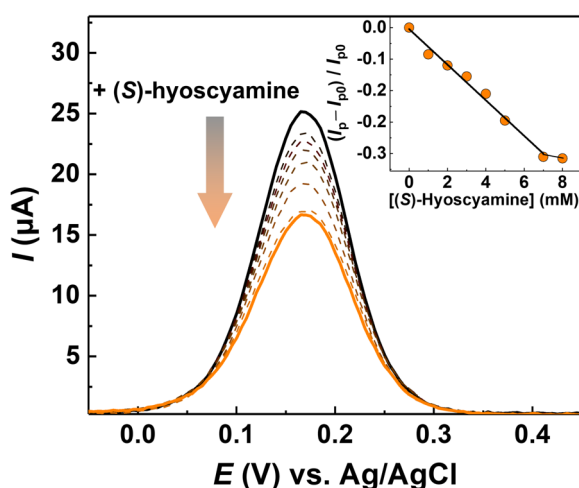


Fig. 4 DPV results of the MIP-AuNS electrode by adding (*S*)-hyoscyamine in a phosphate buffer (100 mM, pH 7.0) containing K<sub>3</sub>Fe(CN)<sub>6</sub> (5 mM) and KCl (100 mM) at 25 °C. Inset represents the ratio of the peak current (*I<sub>p</sub>*) changes of the MIP-AuNS electrode. The terms *I<sub>p0</sub>* and *I<sub>p</sub>* indicate the peak current before and after adding (*S*)-hyoscyamine, respectively. [(*S*)-Hyoscyamine] = 0.0–8.0 mM.

probably derived from the extraction of the template that was as much as 16.6 mol% of all components. The FT-IR (ATR) spectrum of the electrode further supported the attachment of the MIP on the electrode by the observed absorption peaks originating from p(NIPAM-co-DMPA-co-MBAAM) (Fig. S2<sup>†</sup>).

Subsequently, the detectability of the MIP-AuNS attached electrode for (*S*)-hyoscyamine was investigated by DPV (Fig. 4). Here, the MIP-AuNS attached electrode, the Ag/AgCl electrode, and the Pt wire played roles as the working electrode, the reference electrode, and the counter electrode, respectively. As a negative control experiment, the AuNS extended-gate electrode functionalized with the NIP (NIP-AuNS electrode) that did not contain (*S*)-hyoscyamine during polymerization was also assessed. The peak current (*I<sub>p</sub>*) of the MIP-AuNS modified Au electrode decreased with an increase of (*S*)-hyoscyamine concentration, indicating that the absorption of (*S*)-hyoscyamine prevented the electrochemical redox reaction of a ferricyanide anion.<sup>61</sup> On the other hand, the peak current of the NIP-AuNS electrode showed a weaker response compared with the MIP-AuNS electrode, implying that the specific binding sites in the MIP-AuNS electrode contributed to the response of (*S*)-hyoscyamine (Fig. S6<sup>†</sup>).

### 3.2. Detection of (*S*)-hyoscyamine by the extended-gate-type OFET

The electrical detection of (*S*)-hyoscyamine by using the MIP-OFET was performed in a phosphate buffer (100 mM, pH 7.0 at 25 °C) containing KCl (100 mM). In these conditions, almost all amino groups of the target are protonated, while almost all carboxy groups of the MIP are deprotonated.<sup>62</sup> Hence, strong electrostatic interactions and hydrogen bonds can contribute to the capture of the target. Fig. 5 shows transfer characteristics of the MIP-OFET upon the addition of (*S*)-hyoscyamine. The transfer curves were negatively shifted with the increase of the

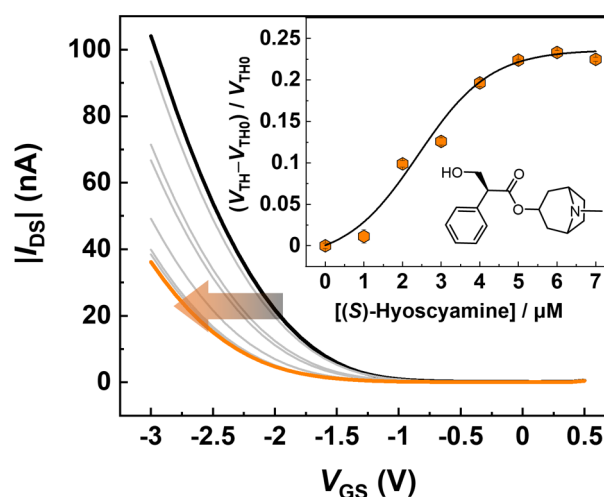


Fig. 5 Transfer characteristics of the MIP-OFET upon the addition of (*S*)-hyoscyamine in a phosphate buffer (100 mM, pH 7.0) containing KCl (100 mM) at 25 °C. Inset represents the titration isotherm corresponding to the (*S*)-hyoscyamine induced *V<sub>Th</sub>* shift. [(*S*)-Hyoscyamine] = 0.0–7.0 µM.

target alkaloid drug concentration, and the corresponding change of the threshold voltages ( $V_{TH}$ ) of the OFET provided a sigmoidal titration curve. The negative shift of the transfer curve was derived from the surface potential change on the extended-gate electrode induced by the accumulation of the positively charged molecules.<sup>19</sup> The sigmoidal response could be due to the hydration of the target.<sup>63</sup> Notably, the OFET-based chemical sensor could achieve highly sensitive detection in contrast to conventional electrochemical apparatuses (e.g., Faraday current response recorded by electrochemical stations)<sup>64</sup> owing to its inherent amplification properties. Indeed, the micromolar level detection implied higher sensitivity in comparison to the conventional electrochemical hyoscyamine sensor.<sup>65</sup>

### 3.3. Selectivity test

The selectivity of the MIP-OFET was investigated against muscarinic blocking drugs [*i.e.*, (*S*)-hyoscyamine, scopolamine, tropicamide, solifenacin, and oxybutynin],<sup>4</sup> major metabolites of atropine *i.e.*, tropic acid and tropine).<sup>66</sup> Fig. 6 represented the highest response to (*S*)-hyoscyamine stemmed from the high complementarity between the target alkaloid and the cavities of the MIP. The components of (*S*)-hyoscyamine, tropine and tropic acid were selected to clarify the contribution skeleton for molecular recognition based on the MIP. The observed moderate response to tropine suggested that the detectability of (*S*)-hyoscyamine by the MIP could rely on the skeleton of 8-azabicyclo[3.2.1]octane over that of 3-hydroxy-2-phenylpropanoate. Remarkably, the MIP succeeded in the discrimination of (*S*)-hyoscyamine from the drug possessing a similar structure (*i.e.*, scopolamine) because the epoxide moiety of scopolamine could form an intramolecular hydrogen bond with the protonated tertiary amino group ( $pK_a = 7.8$ )<sup>67</sup> of scopolamine at pH 7.0. Indeed, the DFT calculation result in Fig. S14<sup>†</sup> clearly showed the isosurface between the oxygen atom of the epoxide moiety and the protonated tertiary amino group, indicating that the electron density increased owing to the intramolecular hydrogen bond. Such interaction would cause the conformation change and weaken the interactions between the protonated tertiary amino group of scopolamine and the carboxylate group of the MIP, which lead to the weak response for scopolamine.

### 3.4. Determination of % ee of (*S*)-hyoscyamine

Finally, the % ee determination of (*S*)-hyoscyamine was performed by using the MIP-OFET. Toward the realization of the easy-to-use chemical sensor for OTC drugs,<sup>68</sup> the chiral discriminatory power of the OFET-based sensor<sup>69-71</sup> was evaluated from 0.2 to 90.2 % ee according to the enantiomeric purity of the commercially available (*S*)-hyoscyamine (Figs. S15 and S16<sup>†</sup>). As shown in Fig. S17<sup>†</sup>, the transistor characteristics shifted by increasing % ee values of (*S*)-hyoscyamine. In this regard, Fig. 7 shows the linear dependency of the  $V_{TH}$  on the % ee of (*S*)-hyoscyamine. Thus, the MIP-OFET seems to have the

potential as a chemical sensor for OTC drugs in real-world applications.

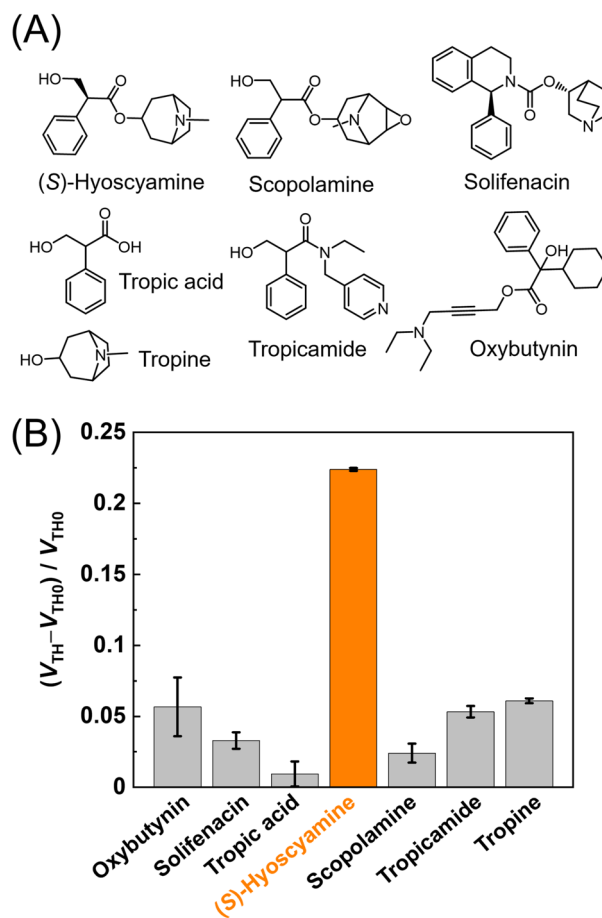


Fig. 6 (A) Chemical structures of muscarinic blocking drugs and metabolites of atropine. (B) Result of the selectivity test against 7 analytes. Three repetitions were carried out for each analyte in a phosphate buffer (100 mM, pH 7.0) containing KCl (100 mM) at 25 °C. [Analyte] = 5.0  $\mu$ M.

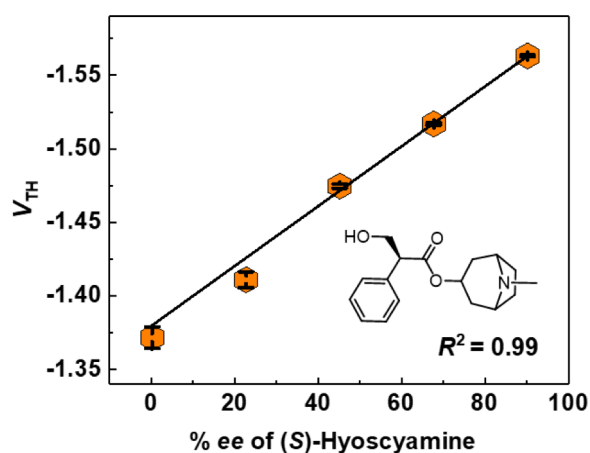


Fig. 7 Threshold voltage ( $V_{TH}$ ) corresponding to the % ee value of (*S*)-hyoscyamine in a phosphate buffer (100 mM, pH 7.0) containing KCl (100 mM) at 25 °C. The overall hyoscyamine concentration was set to 5.0  $\mu$ M.

## Conclusions

In summary, we designed and fabricated a chemical sensor based on the MIP-OFET for sensitive and selective discrimination of (S)-hyoscyamine. The DFT calculation was applied for optimizing the ratio design of the MIP components, resulting in the appropriate molar ratio to form the favorable complex of (S)-hyoscyamine with monomer units through hydrogen bonds. The MIP-AuNS attached extended-gate electrode was connected to the OFET and applied to the electrical detection of (S)-hyoscyamine. The OFET-based sensor device successfully detected (S)-hyoscyamine with high sensitivity. Furthermore, we applied the MIP-OFET to the % ee determination of commercially available (S)-hyoscyamine for the evaluation of the usability of the sensor device against OTC drugs in real-world scenarios. We believe that our strategy for the development of analytical devices based on organic electronics could broaden the horizon of the chemical sensing applications in drug analysis.

## Author Contributions

QZ synthesized and characterized the MIP and the NIP and performed electrochemical measurements. YS wrote the manuscript with QZ. KO measured FE-SEM of the MIP and NIP electrodes, and operated FT-IR measurements. HF and KO fabricated the OFET devices and characterized the transistor characteristics. VM and CG made a helpful discussion. KH and TM conceived the entire project.

## Conflicts of interest

The authors declare no competing financial interest.

## Acknowledgements

TM gratefully acknowledges the financial support from JSPS KAKENHI (Grant nos. JP21H01780, JP20K21204, JP20H05207, and JP22H04524), Core-to-Core Program, and JST CREST (Grant no. JPMJCR2011). K.H. acknowledges financial support from Institut Universitaire de France. QZ thanks the JSPS, Research Fellow for Young Scientists (DC1) (Grant no. JP22J23433). YS also thanks to the JSPS KAKENHI (Grant no. JP22K14706) and the Sasakawa Scientific Research Grant. TM also thanks Asahi Glass Co., Ltd. for supplying CYTOP, TOYOBO Co., Ltd. for supplying the PEN film, and Daicel Co., Ltd. for the measurement of high-performance liquid chromatography to determine the % ee value of (S)-hyoscyamine.

## References

1. P. Srinivasan and C. D. Smolke, *Nature*, 2020, **585**, 614-619.
2. J. Schmitz, D. van der Mey, M. Bermudez, J. Klockner, R. Schrage, E. Kostenis, C. Trankle, G. Wolber, K. Mohr and U. Holzgrabe, *J. Med. Chem.*, 2014, **57**, 6739-6750.
3. J. H. Xu, S. C. Zheng, J. W. Zhang, X. Y. Liu and B. Tan, *Angew. Chem. Int. Ed.*, 2016, **55**, 11834-11839.
4. A. M. Lakstygala, T. O. Kolesnikova, S. L. Khatsko, K. N. Zabegalov, A. D. Volgin, K. A. Demin, V. A. Shevyrin, E. A. Wappler-Guzzetta and A. V. Kalueff, *ACS Chem. Neurosci.*, 2019, **10**, 2144-2159.
5. D. J. Meagher, *BMJ.*, 2001, **322**, 144-149.
6. M. Hu, H. T. Feng, Y. X. Yuan, Y. S. Zheng and B. Z. Tang, *Coord. Chem. Rev.*, 2020, **416**, 213329.
7. X. L. Chen, Y. Kang and S. Zeng, *Chirality*, 2018, **30**, 609-618.
8. J. Clayden, W. J. Moran, P. J. Edwards and S. R. LaPlante, *Angew. Chem. Int. Ed.*, 2009, **48**, 6398-6401.
9. N. M. Maier, P. Franco and W. Lindner, *J. Chromatogr. A*, 2001, **906**, 3-33.
10. R. Soares, A. K. Singh, E. R. M. Kedor-Hackmann and M. Santoro, *J. AOAC Int.*, 2009, **92**, 1663-1672.
11. D. Castilla-Fernandez, D. Moreno-Gonzalez, J. F. Garcia-Reyes, E. Ballesteros and A. Molina-Diaz, *Food Chem.*, 2021, **347**, 129020.
12. S. Yuvaraja, A. Nawaz, Q. Liu, D. Dubal, S. G. Surya, K. N. Salama and P. Sonar, *Chem. Soc. Rev.*, 2020, **49**, 3423-3460.
13. H. Li, W. Shi, J. Song, H. J. Jang, J. Dailey, J. S. Yu and H. E. Katz, *Chem. Rev.*, 2019, **119**, 3-35.
14. C. C. Zhang, P. L. Chen and W. P. Hu, *Chem. Soc. Rev.*, 2015, **44**, 2087-2107.
15. L. Torsi, M. Magliulo, K. Manoli and G. Palazzo, *Chem. Soc. Rev.*, 2013, **42**, 8612-8628.
16. C. Z. Liao and F. Yan, *Polym. Rev.*, 2013, **53**, 352-406.
17. M. Y. Mulla, P. Seshadri, L. Torsi, K. Manoli, A. Mallardi, N. Ditaranto, M. V. Santacroce, C. Di Franco, G. Scamarcio and M. Magliulo, *J. Mater. Chem. B*, 2015, **3**, 5049-5057.
18. F. X. Werkmeister, T. Koide and B. A. Nickel, *J. Mater. Chem. B*, 2016, **4**, 162-168.
19. P. Bergveld, *Sens. Actuator B-Chem.*, 2003, **88**, 1-20.
20. R. Kubota, Y. Sasaki, T. Minamiki and T. Minami, *ACS Sens.*, 2019, **4**, 2571-2587.
21. Q. Zhou, M. Q. Wang, S. Yagi and T. Minami, *Nanoscale*, 2021, **13**, 100-107.
22. K. Asano, Y. Sasaki, Q. Zhou, R. Mitobe, W. Tang, X. Lyu, M. Kamiko, H. Tanaka, A. Yamagami, K. Hagiya and T. Minami, *J. Mater. Chem. C*, 2021, **9**, 11690-11697.
23. A. K. Yatsimirsky, *Nat. Prod. Commun.*, 2012, **7**, 369-380.
24. M. A. Beatty, A. J. Selinger, Y. Q. Li and F. Hof, *J. Am. Chem. Soc.*, 2019, **141**, 16763-16771.
25. M. Sapotta, A. Hofmann, D. Bialas and F. Wurthner, *Angew. Chem. Int. Ed.*, 2019, **58**, 3516-3520.
26. J. Y. Chen, L. M. Chen, Y. H. Zhang, L. Zhao, M. Dong, Z. Meng, Q. B. Meng and C. J. Li, *Chem. Commun.*, 2022, **58**, 3370-3373.
27. T. Minami, N. A. Esipenko, B. Zhang, L. Isaacs, R. Nishiyabu, Y. Kubo and P. Anzenbacher, *J. Am. Chem. Soc.*, 2012, **134**, 20021-20024.
28. E. G. Shcherbakova, B. Zhang, S. Gozem, T. Minami, P. Y. Zavalij, M. Pushina, L. D. Isaacs and P. Anzenbacher, *J. Am. Chem. Soc.*, 2017, **139**, 14954-14960.
29. T. Takeuchi and H. Sunayama, *Chem. Commun.*, 2018, **54**, 6243-6251.
30. L. X. Chen, X. Y. Wang, W. H. Lu, X. Q. Wu and J. H. Li, *Chem. Soc. Rev.*, 2016, **45**, 2137-2211.
31. L. X. Chen, S. F. Xu and J. H. Li, *Chem. Soc. Rev.*, 2011, **40**, 2922-2942.

32. M. J. Whitcombe, I. Chianella, L. Larcombe, S. A. Piletsky, J. Noble, R. Porter and A. Horgan, *Chem. Soc. Rev.*, 2011, **40**, 1547-1571.
33. A. Mier, I. Maffucci, F. Merlier, E. Prost, V. Montagna, G. U. Ruiz-Esparza, J. V. Bonventre, P. K. Dhal, B. T. S. Bui, P. Sakhaii and K. Haupt, *Angew. Chem. Int. Ed.*, 2021, **60**, 20849-20857.
34. E. Paruli, T. Griesser, F. Merlier, C. Gonzato and K. Haupt, *Polym. Chem.*, 2019, **10**, 4732-4739.
35. Y. H. Shim, E. Yilmaz, L. A. Solange and K. Haupt, *Analyst*, 2004, **129**, 1211-1215.
36. J. Zuo, X. Y. Zhang, X. Y. Li, Z. W. Li, Z. R. Li, H. H. Li and W. C. Zhang, *RSC Adv.*, 2019, **9**, 19712-19719.
37. M. P. Chantada-Vazquez, J. Sanchez-Gonzalez, E. Pena-Vazquez, M. J. Taberner, A. M. Bermejo, P. Bermejo-Barrera and A. Moreda-Pineiro, *Biosens. Bioelectron.*, 2016, **75**, 213-221.
38. P. Lenain, J. D. Di Mavungu, P. Dubruel, J. Robbens and S. De Saeger, *Anal. Chem.*, 2012, **84**, 10411-10418.
39. J. Y. Sun, L. J. Zhang, X. Liu, A. X. Zhao, C. Hu, T. Gan and Y. M. Liu, *J. Electroanal. Chem.*, 2021, **903**, 115843.
40. A. Khataee, J. Hassanzadeh and E. Kohan, *Spectrochim. Acta A Mol. Biomol. Spectrosc.*, 2018, **205**, 614-621.
41. J. Abbasifar and A. Samadi-Maybodi, *J. Fluoresc.*, 2016, **26**, 1645-1652.
42. M. Nakamura, M. Ono, T. Nakajima, Y. Ito, T. Aketo and J. Haginaka, *J. Pharm. Biomed. Anal.*, 2005, **37**, 231-237.
43. Y. B. Wei, Q. Zeng, J. Z. Huang, X. R. Guo, L. L. Wang and L. S. Wang, *ACS Appl. Mater. Interfaces*, 2020, **12**, 24363-24369.
44. A. Wojnarowicz, P. S. Sharma, M. Sosnowska, W. Lisowski, T. P. Huynh, M. Pszona, P. Borowicz, F. D'Souza and W. Kutner, *J. Mater. Chem. B*, 2016, **4**, 1156-1165.
45. H. da Silva, J. G. Pacheco, J. Magalhaes, S. Viswanathan and C. Delerue-Matos, *Biosens. Bioelectron.*, 2014, **52**, 56-61.
46. N. Leibl, L. Duma, C. Gonzato, K. Haupt, *Bioelectrochemistry*, 2020, **135**, 107541.
47. Z. Iskierko, A. Chęcinska, P. S. Sharma, K. Golebiewska, K. Noworyta, P. Borowicz, K. Fronc, V. Bandi, F. D'Souza and W. Kutner, *J. Mater. Chem. C*, 2017, **5**, 969-977.
48. T. Kajisa, W. Li, T. Michinobu and T. Sakata, *Biosens. Bioelectron.*, 2018, **117**, 810-817.
49. Z. Iskierko, P. S. Sharma, K. R. Noworyta, P. Borowicz, M. Cieplak, W. Kutner and A. M. Bossi, *Anal. Chem.*, 2019, **91**, 4537-4543.
50. S. Beyazit, B. T. S. Bui, K. Haupt and C. Gonzato, *Prog. Polym. Sci.*, 2016, **62**, 1-21.
51. I. McCulloch, M. Heeney, C. Bailey, K. Genevicius, I. Macdonald, M. Shkunov, D. Sparrowe, S. Tierney, R. Wagner, W. M. Zhang, M. L. Chabynyc, R. J. Kline, M. D. McGehee and M. F. Toney, *Nat. Mater.*, 2006, **5**, 328-333.
52. M. J. Frisch, G. W. Trucks, H. B. Schlegel, G. E. Scuseria, M. A. Robb, J. R. Cheeseman, G. Scalmani, V. Barone, G. A. Petersson, H. Nakatsuji, X. Li, M. Caricato, A. V. Marenich, J. Bloino, B. G. Janesko, R. Gomperts, B. Mennucci, H. P. Hratchian, J. V. Ortiz, A. F. Izmaylov, J. L. Sonnenberg, Williams, F. Ding, F. Lipparini, F. Egidi, J. Goings, B. Peng, A. Petrone, T. Henderson, D. Ranasinghe, V. G. Zakrzewski, J. Gao, N. Rega, G. Zheng, W. Liang, M. Hada, M. Ehara, K. Toyota, R. Fukuda, J. Hasegawa, M. Ishida, T. Nakajima, Y. Honda, O. Kitao, H. Nakai, T. Vreven, K. Throssell, J. A. Montgomery Jr., J. E. Peralta, F. Ogliaro, M. J. Bearpark, J. Heyd, E. N. Brothers, K. N. Kudin, V. N. Staroverov, T. A. Keith, R. Kobayashi, J. Normand, K. Raghavachari, A. P. Rendell, J. C. Burant, S. S. Iyengar, J. Tomasi, M. Cossi, J. M. Millam, M. Klene, C. Adamo, R. Cammi, J. W. Ochterski, R. L. Martin, K. Morokuma, O. Farkas, J. B. Foresman and D. J. Fox, Gaussian 16 (Revision C.01), Gaussian, Inc., Wallingford CT, 2016.
53. X. Feás, C. A. Fente, S. V. Hosseini, J. A. Seijas, B. I. Vázquez, C. M. Franco and A. Cepeda, *Mater. Sci. Eng. C*, 2009, **29**, 398-404.
54. G. Pan, Q. Guo, Y. Ma, H. Yang, B. Li, *Angew. Chem. Int. Ed.*, 2013, **125**, 7045-7049.
55. R. Krishnan, J. S. Binkley, R. Seeger and J. A. Pople, *J. Chem. Phys.*, 1980, **72**, 650-654.
56. G. W. Spitznagel, T. Clark, P. V. Schleyer and W. J. Hehre, *J. Comput. Chem.*, 1987, **8**, 1109-1116.
57. P. J. Stephens, F. J. Devlin, C. F. Chabalowski and M. J. Frisch, *J. Phys. Chem.*, 1994, **98**, 11623-11627.
58. S. Grimme, J. Antony, S. Ehrlich and H. Krieg, *J. Chem. Phys.*, 2010, **132**, 154104-1/19.
59. R. Dennington, T. A. Keith and J. M. Millam, Gaussview (version 6.0.16), Semichem Inc., Wallingford, CT, 2016.
60. Y. D. Liu, Z. C. Liu, F. Zhao and Y. Tian, *Angew. Chem. Int. Ed.*, 2021, **60**, 14429-14437.
61. S. Motia, B. Bouchikhi, E. Llobet and N. El Bari, *Talanta*, 2020, **116**, 120953-1/12.
62. U. Domanska, A. Pobudkowska, A. Pelczarska and P. Gierycz, *J. Phys. Chem. B*, 2009, **113**, 8941-8947.
63. Z. Mskolczy, M. Megyesi, O. Toke and L. Biczok, *Phys. Chem. Chem. Phys.*, 2019, **21**, 4912-4919.
64. F. Yan, M. Zhang and J. Li, *Adv. Healthcare Mater.*, 2014, **3**, 313-331.
65. S. S. Badawy, Y. M. Issa and A. A. Mutair, *J. Pharm. Biomed. Anal.*, 2005, **39**, 117-124.
66. M. J. Vandermeer, H. K. L. Hundt and F. O. Muller, *J. Pharm. Pharmacol.*, 1986, **38**, 781-784.
67. H. Weinstein, S. Srebrenik, S. Maayani and M. Sokolovsky, *J. Theor. Biol.*, 1977, **64**, 295-309.
68. Y. Sasaki, S. Kojima, V. Hamedpour, R. Kubota, S. Y. Takizawa, I. Yoshikawa, H. Houjou, Y. Kubo and T. Minami, *Chem. Sci.*, 2020, **11**, 3790-3796.
69. M. Y. Mulla, E. Tuccori, M. Magliulo, G. Lattanzi, G. Palazzo, K. Persaud and L. Torsi, *Nat. Commun.*, 2015, **6**, 6010.
70. Y. W. Sun, Y. Wang, Y. F. Wu, X. P. Wang, X. G. Li, S. R. Wang and Y. Xiao, *Anal. Chem.*, 2018, **90**, 9264-9271.
71. X. P. Wang, Y. Wang, Y. F. Wu and Y. Xiao, *Analyst*, 2019, **144**, 2611-2617.