



# Robot-assisted spine surgery guided by conductivity sensing: first preclinical experiments demonstrate X-ray free breach detection

Jimmy Da Silva, Thibault Chandanson, Guillaume Morel

## ► To cite this version:

Jimmy Da Silva, Thibault Chandanson, Guillaume Morel. Robot-assisted spine surgery guided by conductivity sensing: first preclinical experiments demonstrate X-ray free breach detection. The Hamlyn Symposium on Medical Robotics, Jun 2019, London, United Kingdom. 10.31256/HSMR2019.38 . hal-03768353

**HAL Id: hal-03768353**

**<https://hal.science/hal-03768353>**

Submitted on 3 Sep 2022

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

# Robot-assisted spine surgery guided by conductivity sensing: first preclinical experiments demonstrate X-ray free breach detection

Jimmy Da Silva<sup>1,2</sup>, Thibault Chandanson<sup>1</sup>, Guillaume Morel<sup>2</sup>

<sup>1</sup>SpineGuard, Vincennes

<sup>2</sup>Sorbonne Université, CNRS, INSERM, ISIR - Paris,  
jimmy.dasilva@spineguard.com

## INTRODUCTION

Inserting screws in vertebral pedicles is a major issue in spinal fusion surgery. Due to their proximity to critical anatomical regions (spinal cord, aorta), misplaced screws can induce complications [1]. Free-handed positioning results in high inaccuracy. To try to improve precision of this surgery, new medical robots and tools emerged from the research community and arrived in the market in the last few years [2], such as SpineAssist [3] from Mazor, ROSA [4] from Zimmer Biomet, iSYS 1 [5] from Interventional Systems.

Available systems rely on fluoroscopy or CT scans taken during the procedure for position checking. Notably, there is no real-time control of the gesture.

The current paper discloses a concept involving a robotic arm that holds a drill equipped with an electrical conductivity sensor. A control law couples the sensor to the robot control in such a way that vertebral breach can be avoided during vertebrae drilling. First *in vivo* experiments are shown.

## MATERIALS AND METHODS

The experimental setup is a combination of the DSG technology developed by SpineGuard, a 7 DOFs robot arm WAM sold by Barrett Technology, and a motor. See Fig. 1.

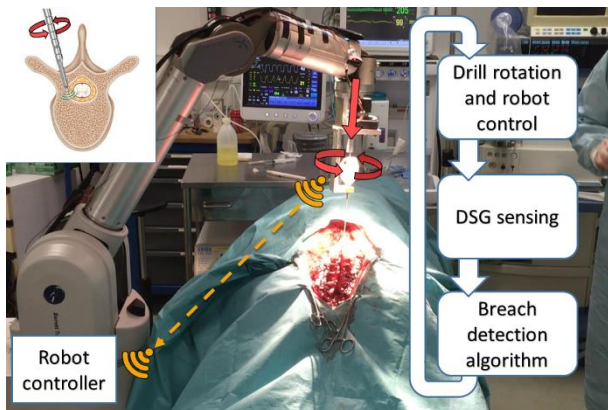


Fig. 1 Experimental setup

DSG technology [6,7,8] is a bipolar, local electrical conductivity sensor that pulses current flow at the tip of its probe. The current clinical setup is as follows: when manipulating a pedicle preparation tool equipped with DSG, a surgeon can distinguish between tissues and be alerted prior to an imminent cortical breach: this is

achieved by changes in the pitch and cadence of an audio signal and a flashing LED light.

In this work, the DSG signal  $s(t)$  is used to detect a breach as follows (see Fig. 2). It is assumed that the tool has initially been inserted in cancellous bone. The system then waits for the detection of an event: cortical bone penetration is detected when  $s(t)$  gets below a threshold  $s_1$ . A breach alert is then produced when  $s(t) > s_2$  with  $s_2 = s_{min} + \delta s$ , where  $s_{min} = \min_{0 \leq \tau \leq t} s(\tau)$  and  $\delta s$  is a given differential threshold.

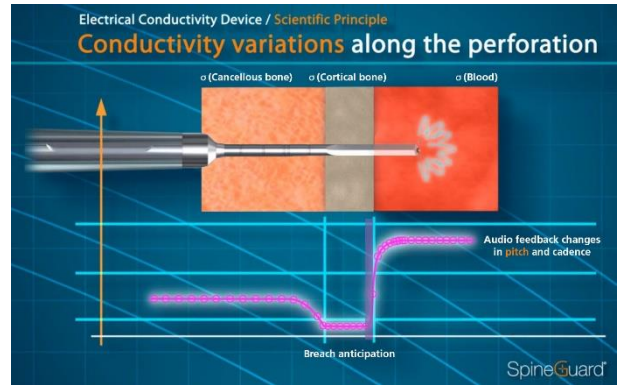


Fig. 2 DSG technology principle.

As for the robot control (see Fig. 3), at the beginning of the procedure, a transparent mode is provided to position the drill tip by comanipulation. A semi-transparent mode is then proposed allowing for orienting the drill around its tip. A simple click on a GUI starts the drilling algorithm at a constant speed  $v_{des}$ .

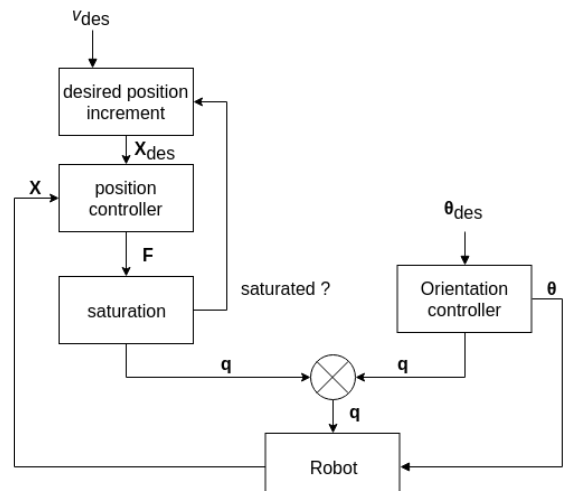


Fig. 3 Control scheme.

When the drilling starts, an operational space orientation and position controller starts running. The desired orientation  $\theta_{des}$  is servoed to its initial value  $\theta_{ini}$ . The desired position  $X_{des}$  is computed by:

$$X_{des}(t + dt) = X_{des}(t) + v_{des} dt z_{ini}, \quad (1)$$

where  $dt$  is the control period,  $z_{ini}$  is the drill axis direction and  $v_{des}$  is an adjustable penetration speed. As a security, when the resulting control force  $\|F_p\|$  reaches a given value  $F_{pmax}$ , then the position increment is nulled.


## RESULTS

*In vivo* experiments have been performed on pigs, under the control of veterinary surgeons and after approbation of an ethics comity.

Parameters of the experiments were as follows:

- Drilling motor rotation = 300 rpm,
- $s_1 = 150mV$ ,  $\delta s = 300mV$
- $dt = 2ms$
- $F_{pmax} = 10N$

The surgeon was asked to manipulate the robot arm in a transparent mode so that the drill bit could perforate the spinous process of the vertebra, then click on the GUI to start the drilling.

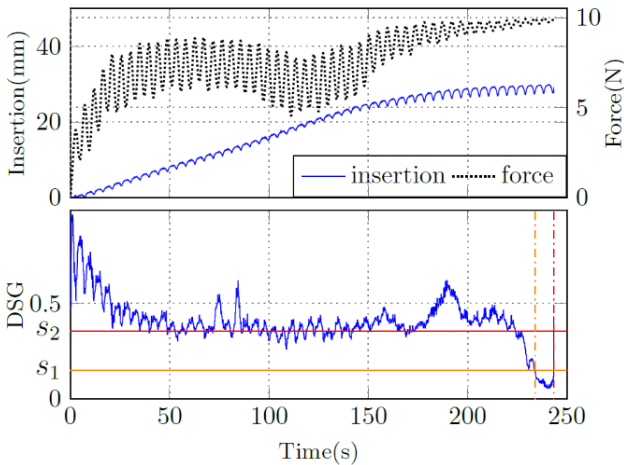

**Fig. 4** Robot and DSG signals during an experiment

The curve of the DSG signal (Fig. 4) shows the expected signature: high signal at the entrance, then stabilization in the spongy phase, decrease in the cortical bone around  $s_1$ , followed by a fast rise stopped to  $s_2$ .

The force and position curves exhibit oscillations. These correspond to the breathing of the animal. Notice that the position controller involves a simple PD compensator without integral action, leading to compliance observable through the oscillations of the insertion (or penetration depth) signal.

Further, due to the force limitation, the velocity decreases when the resistance is getting higher, offering an extra layer of safety.

## DISCUSSION

The current setup allows to stop the drilling right before breaching out.

An innovative system for radiation-free breach anticipation during spine surgery has been presented. It uses a measurement of the local conductivity to determine if a breach out of the bone is imminent.

The *in vivo* experiments were successfully performed but further improvements can be considered to increase robustness and accuracy.

For instance, the values of variables  $s_1$  and  $\delta s$  have been manually set. Further experiments have shown that these values need to be adjusted depending on the patient's anatomy and bone state. A more sophisticated signal-processing algorithm needs to be defined in order to eliminate the tuning of these parameters and allow the recognition of a conductivity change pattern.

Further, the DSG technology could be used in many bone surgeries as a safety sensor to reduce the use of x-rays.

## REFERENCES

- [1] J. E. Lonstein, F. Denis, J. H. Perra, M. R. Pinto, M. D. Smith, and R. B. Winter, "Complications associated with pedicle screws", *JBJS*, vol. 81, no. 11, pp. 1519-1528, 1999.
- [2] F. Shweikeh, J. P. Amadio, M. Arnell, Z. R. Barnard, T. T. Kim, J. P. Johnson, and D. Drazin, "Robotics and the spine: a review of current and ongoing applications", *Neurosurgical focus*, vol. 36, no. 3, p. E10, 2014.
- [3] A. Bertelsen, J. Melo, E. Sanchez, and D. Borro, "A review of surgical robots for spinal interventions", *The International Journal of Medical Robotics and Computer Assisted Surgery*, vol. 9, no. 4, pp. 407-422, 2013.
- [4] M. Lefranc and J. Peltier, "Evaluation of the rosa<sup>TM</sup> spine robot for minimally invasive surgical procedures", *Expert review of medical devices*, vol. 13, no. 10, pp. 899-906, 2016.
- [5] J. Kettenbach, L. Kara, G. Toporek, M. Fuerst, and G. Kronreif, "A robotic needle-positioning and guidance system for ct-guided puncture: Ex vivo results", *Minimally invasive therapy & allied technologies*, vol. 3, no. 5, pp. 271-278, 2014.
- [6] C. Bolger, M. O. Kelleher, L. McEvoy, M. Brayda-Bruno, A. Kaelin, J.-Y. Lazenec, J.-C. Le Huec, C. Logroscino, P. Mata, P. Moreta, *et al.*, "Electrical conductivity measurement: a new technique to detect iatrogenic initial pedicle perforation", *European Spine Journal*, vol. 16, no. 11, pp. 1919-1924, 2007.
- [7] O. Suess and M. Schomacher, "Control of Pedicle Screw Placement with an Electrical Conductivity Measurement Device: Initial Evaluation in the Thoracic and Lumbar Spine", *Advances in Medicine*, 2016.
- [8] C. Bolger and M. Bourlion, "Pedicle navigation in spondylolisthesis" in *Spondylolysis, Spondylolisthesis, and Degenerative Spondylolisthesis*, ch. 28, pp. 227-236, Lippincott Williams & Wilkins, 2006.