



HAL
open science

Sphere choice in Mirau interferometric microsphere assisted profilometry

Rayenne Boudoukha, Stéphane Perrin, Assia Guessoum, Nacer-Eddine Demagh, P. Montgomery, Sylvain Lecler

► **To cite this version:**

Rayenne Boudoukha, Stéphane Perrin, Assia Guessoum, Nacer-Eddine Demagh, P. Montgomery, et al.. Sphere choice in Mirau interferometric microsphere assisted profilometry. SPIE Photonics Europe, 2022, Strasbourg, France, SPIE, Apr 2022, Strasbourg, France. 10.1117/12.2631094 . hal-03838994

HAL Id: hal-03838994

<https://hal.science/hal-03838994v1>

Submitted on 18 Nov 2022

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Sphere choice in Mirau interferometric microsphere assisted profilometry

R. Boudoukha

J. Schiffler

S. Perrin

A. Guessoum

N. Demagh

P. Montgomery

S. Lecler

ICube Research Institute,
University of Strasbourg- CNRS-INSA
Applied Optics Laboratory,
University of Ferhat Abbas – Setif 1

SPIE Photonics Europe
Strasbourg, France - 4th April 2022



Contents


- 1. Microsphere-assisted microscopy**
- 2. Mirau interferometric configuration**
- 3. Linnik interferometric configuration**

Microsphere assisted microscopy

Classical microscopy : limited by diffraction (~ 200 nm, visible)



In 1873, Ernst Abbe :




How to enhancement the resolution ?

Label free technique ?

Full-field imaging ?

Microsphere assisted microscopy

A glass μ -sphere
on a Si grating




The microsphere behaves
as a lens

Resolution :

100 nm in air

50 nm in immersion




[Perrin, Label-Free Super-Resol. Micro., Springer, 2019]

Microsphere assisted microscopy


A meso-scale phenomenon

Evanescent waves
conversion in far field



[Boudoukha, MDPI Photonics, 2021]



2 pt sources virtual image simulation
in-phase sources Out-of-phase sources



[Kassamakov, Lecler *et al.*, Sci. Rep.7, 3683, 2017]

Interferometric configuration

Mirau versus Linnik configuration



To measure phase and deduce profile

Mirau configuration

Sodalime glass sphere



$\varnothing = 6 \mu\text{m}$ ($n = 1.5$)

$\lambda_0 = 600 \text{ nm}$, x50 (ON = 0.55), in air

Melamine formaldehyde sphere


$\varnothing = 11 \mu\text{m}$ ($n = 1.68$)

$\lambda_0 = 600 \text{ nm}$, x50 (ON = 0.55), in air

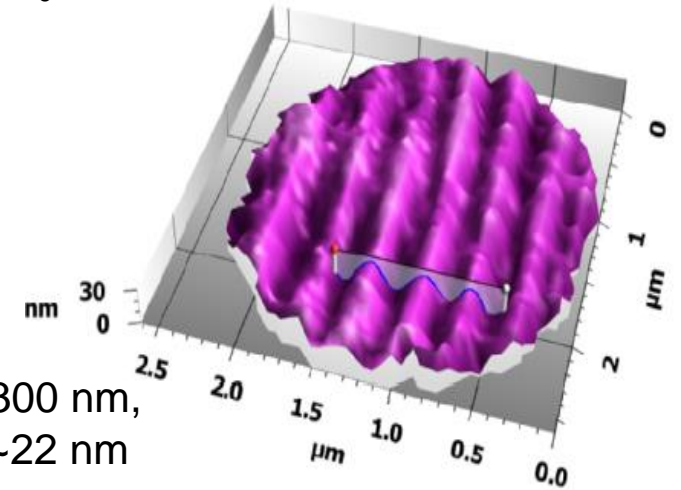

Blu-Ray :
period of 300 nm,
height of ~22 nm

~~$\varnothing = 20 \mu\text{m}$ ($n = 1.5$)~~




Currently only for small sphere

($R < 15 \mu\text{m}$)

[Kassamakov et al., Sci. Rep.7, 3683, 2017]

Mirau configuration



.....
Coherence plane

Image plane


Coherence length

μ -sphere depth of field

Linear displacement


Exponential displacement

μ -sphere depth of field




Virtual image simulation


Linnik configuration




Linnik without fringes



Linnik with fringes



Resolution standard:
Si gratings
Period = 3 μm




Linnik configuration in white light
with 50x objectives (ON = 0.85)

[S. Perrin et al., Applied Optics 56 (2017)]

Linnik with sphere compensation in the ref. arm

24 μm glass sphere

Si Grating period: 600 nm





AFM

Microsphere – Non Compensated

Microsphere - Compensated

Si Grating period: 400 nm



[Perrin, Physical Review Applied, 2020]

Conclusion

- **Optical, label free, full field 2D super-resolution ($\lambda/5 \sim 100$ nm)**
 - A **meso-scale** phenomenon
- **Measuring phase for profile reconstruction**
 - In **Mirau** configuration for **sphere < 15 μm**
 - In **Linnik** configuration to **compensate sphere aberrations**

Thank you for your attention!

rayenne.boudoukha@etu.unistra.fr

