



**HAL**  
open science

## The detection of spectral signatures with IRS/SuperCam, Perseverance rover: instrument performance

C. Royer, T. Fouchet, Franck Montmessin, F. Poulet, O. Forni, J. R. Johnson,  
Olivier Gasnault, L. Mandon, C. Quantin- Nataf, R. C. Wiens, et al.

### ► To cite this version:

C. Royer, T. Fouchet, Franck Montmessin, F. Poulet, O. Forni, et al.. The detection of spectral signatures with IRS/SuperCam, Perseverance rover: instrument performance. 53rd Lunar and Planetary Science Conference, Lunar and Planetary Institute, Mar 2022, The Woodlands, TX, United States. pp.LPI Contribution No. 2678, 2022, id.1840. hal-03847223

**HAL Id: hal-03847223**

**<https://hal.science/hal-03847223v1>**

Submitted on 10 Nov 2022

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

### The detection of spectral signatures with IRS/SuperCam, Perseverance rover: instrument performance.

C. Royer<sup>1,\*</sup>, T. Fouchet<sup>1</sup>, F. Montmessin<sup>2</sup>, F. Poulet<sup>3</sup>, O. Forni<sup>4</sup>, J. R. Johnson<sup>5</sup>, O. Gasnault<sup>4</sup>, L. Mandon<sup>1</sup>, C. Quantin-Nataf<sup>6</sup>, P. Beck<sup>7</sup>, A. M. Ollila<sup>8</sup>, C. Pilorget<sup>2</sup>, P. Bernardi<sup>1</sup>, J.-M. Reess<sup>1</sup>, R. T. Newell<sup>8</sup>, S. Maurice<sup>2</sup>, R. C. Wiens<sup>8</sup> and the SuperCam team, <sup>1</sup>LESIA, Observatoire de Paris, Université PSL, CNRS, Sorbonne Université, Université de Paris, Meudon, France; <sup>2</sup>LATMOS/IPSL, UVSQ Université Paris-Saclay, Sorbonne Université, CNRS, Guyancourt, France; <sup>3</sup>Institut d'Astrophysique Spatiale, CNRS/Paris-Saclay University, France; <sup>4</sup>IRAP, CNRS, Université de Toulouse, UPS-OMP, Toulouse, France; <sup>5</sup>Applied Physics Laboratory, Johns Hopkins University, Laurel, Maryland, USA; <sup>6</sup>Université de Lyon, UCBL, ENSL, CNRS, LGL-TPE, Lyon, France; <sup>7</sup>Université Grenoble-Alpes, CNRS, IPAG, UMR 5274, Grenoble, France; <sup>8</sup>Los Alamos National Laboratory, Los Alamos, NM, USA; \*[clement.royer@obspm.fr](mailto:clement.royer@obspm.fr)

**Introduction:** The Perseverance rover (Mars 2020 mission, NASA) landed in Jerezo, the host crater of a paleolake, on February 18<sup>th</sup> 2021. Its main objective is the search for evidence of past habitability and the presence of potential biosignatures [1]. Amongst its science payload, the SuperCam instrument (LANL, JPL, and a consortium of French and Spanish laboratories) plays a central role in the geochemistry investigation by providing rapid, synergistic, fine-scale mineralogy, chemistry, and color imaging [2, 3]. In particular, it carries the first near-infrared spectrometer, IRS, to be operated on the Martian surface. IRS is a miniaturized point spectrometer (~1.15 mrad field of view) located in the SuperCam's mast unit. Its spectral range (1.3 – 2.6  $\mu\text{m}$  range) covers major silicate and hydrated mineral absorption

features. It extends the 0.4 – 0.85  $\mu\text{m}$  range of other SuperCam spectrometers to the near IR. IRS is an AOTF (Acousto-Optic Tunable Filter) based spectrometer, meaning that the light filtering is performed by a crystal excited by an acoustic wave, itself generated from a radiofrequency (RF) signal [4].

**Instrument calibration:** The AOTF technology allows unprecedented compactness and robustness, with excellent performance (SNR, spectra resolution, sensitivity). However, this type of monochromator is sensitive to internal thermal effects. These effects have been calibrated during the dedicated ground calibration [5]. This calibration shall be extended with new inputs from use of the instrument in real conditions, about sensitivity (I/F) to the instrument temperature. A dedicated flight calibration is currently

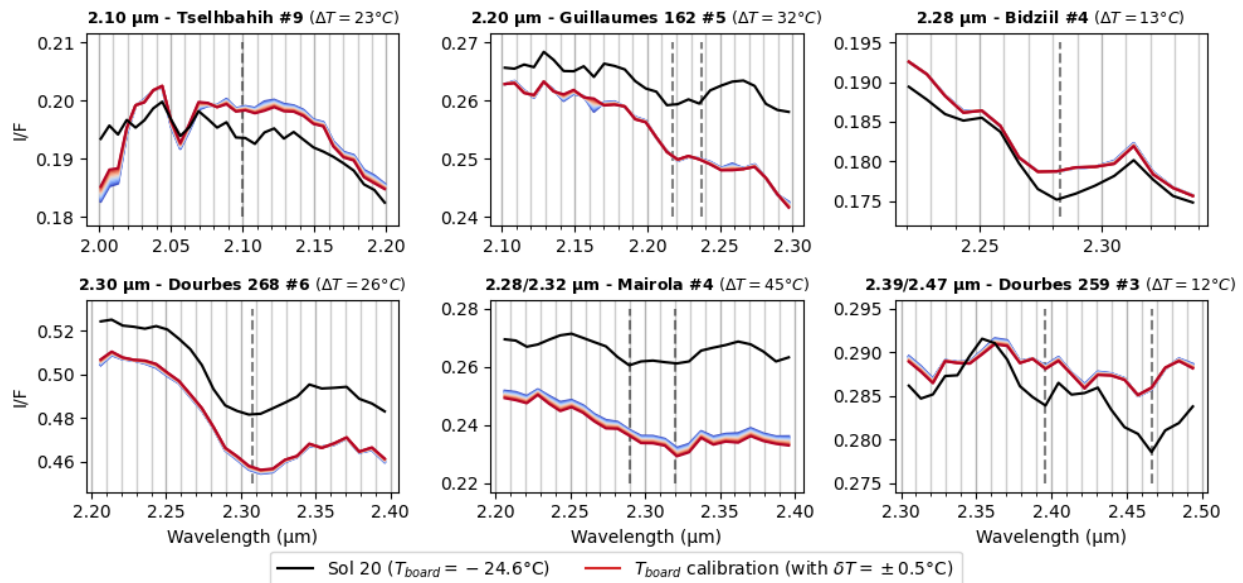


Figure 1: Sensitivity of various spectral signatures in the 2.0 – 2.5  $\mu\text{m}$  range, the most sensitive to thermal effects, illustrated on the most representative observations. In each panel, the black line is the current flight calibration based on Sol 20 White SCCT observation, the color lines are the IR board temperature ( $T_{\text{board}}$ ) calibration and the color gradient indicates its sensitivity at  $\pm 0.5^\circ\text{C}$ , corresponding to the  $T_{\text{board}}$  measurement precision. Dashed vertical lines highlight the detected absorption features. The temperature shift in parenthesis is the  $T_{\text{board}}$  difference between Sol 20 and the observation.

in progress to characterize these effects and provide unbiased reflectance spectra.

The actual state of the calibration, released in the NASA's Planetary Data System (Nov. 2021), relies on the observation of the IR White SuperCam Calibration Target (SCCT) [6] as a reflectance reference, and various algorithms to remove anomalous spectral points, atmospheric spectral signatures and increase the global signal to noise ratio (SNR). Finally, data are converted into reflectance using a local illumination model. The thermal behavior of IRS is still under study to derive a correction vector to the instrument transfer function (ITF) beyond what was done on the ground, and mostly above  $2.0 \mu\text{m}$ . The main thermal effect is the sensitivity of the RF power generator to the temperature of its electronic board (called  $T_{\text{board}}$ ). The data acquired so far allow to estimate potential biases and the detection limits of diagnostic spectral features, induced by this thermal effect (Fig. 1). The thermal calibration is thus derived from the interpolation of every IR White SCCT measurements over their value of  $T_{\text{board}}$  (Fig. 2).

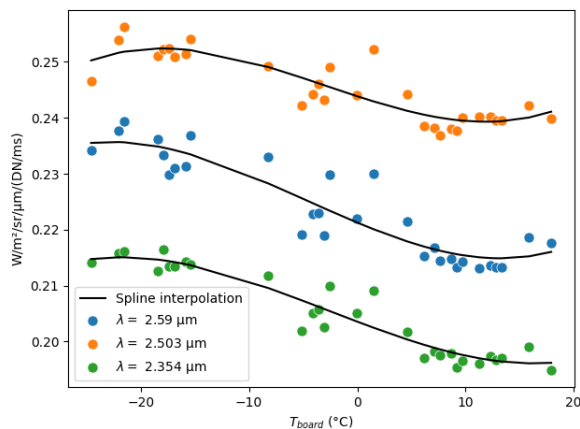


Figure 2: variation of the instrument response (ITF) with  $T_{\text{board}}$  for three sensitive wavelengths and their spline interpolation

**Updated sensitivity from flight calibration:** After about 300 Sols of exploration of the two geologic units Cf-fr and Seitah (up to Dec. 2021), many spectral features have been identified in the near-IR range and attributed to various primary and altered minerals, and salts [7]. The detection of these features is sensitive to the instrument calibration through several effects, illustrated in Fig. 1, mainly in the  $2.0 - 2.6 \mu\text{m}$  range. The first effect of the thermal calibration is the absolute reflectance shift, which is stronger for important temperature differences between the reference (Sol 20) and the actual measurements. More locally, the  $2.28$  and  $2.30 \mu\text{m}$  spectral signatures are often shifted by  $\sim 10 \text{ nm}$  and some other signatures are less deep or even disappear. The calibration's intrinsic sensitivity to  $T_{\text{board}}$  is also assessed within the precision of the IR board thermal probe ( $\pm 0.5^\circ\text{C}$ ). It corresponds to an additional error on the evaluation of the absolute level of the reflectance and is very faint ( $< 1 \%$ ) and stronger for high  $T_{\text{board}}$ . The  $2.5 - 2.6 \mu\text{m}$  range is particularly affected by temperature shifts due to a strong sensitivity of the instrument response.

**Discussion:** The effects of the IR board dependence with temperature are still under investigation. Lab measurements on IRS flight spare are ongoing to better constrain the behavior of the ITF than using only White SCCT observations – which are sensitive to photometric effects, aging – and then calibrate flight data. Notwithstanding the difference between Sol 20 and  $T_{\text{board}}$ -dependent calibrations, and photometric effects, the IRS' thermal behavior and SNR allow high confidence into the absolute reflectance, with a precision of a few percent (compliant with the required absolute precision of 20 %).

**References:** [1] Farley et al. (2020) Space Sci. Rev. 216.8, [2] Wiens et al. (2020), Space Sci. Rev. 217.1, [3] Maurice et al. (2021) Space Sci. Rev. 217.3, [4] Fouchet et al. (2022) Icarus 373, [5] Royer et al. (2020), RScI, [6] Manrique et al. (2020), Space Sci. Rev., [7] Mandon et al (2022), this conf.