



**HAL**  
open science

# Tissue internal strains computed by a Finite Element model of the human heel and measured from MR images

Alessio Trebbi, Mathieu Bailet, Antoine Perrier, Yohan Payan

## ► To cite this version:

Alessio Trebbi, Mathieu Bailet, Antoine Perrier, Yohan Payan. Tissue internal strains computed by a Finite Element model of the human heel and measured from MR images. 2022, Proceedings of the 27th Congress of the European Society of Biomechanics (ESB'2022). hal-03855309

**HAL Id: hal-03855309**

**<https://hal.science/hal-03855309>**

Submitted on 16 Nov 2022

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

# TISSUE INTERNAL STRAINS COMPUTED BY A FINITE ELEMENT MODEL OF THE HUMAN HEEL AND MEASURED FROM MR IMAGES

Alessio Trebbi <sup>1</sup>, Mathieu Bailet <sup>2</sup>, Antoine Perrier <sup>1,2,3</sup>, Yohan Payan <sup>1</sup>

1. Univ. Grenoble Alpes, CNRS, UMR 5525, VetAgro Sup, Grenoble INP, TIMC, 38000 Grenoble, France; 2. TwInSight, France; 3. Groupe hospitalier Diaconesses Croix Saint-Simon, France

## Introduction

Pressure ulcers are a severe disease mostly prevalent in patients that are bedridden or on wheelchair bound. These wounds can start developing in the deep layers of the skin of specific parts of the body, mostly on heels or sacrum, making them hard to detect in their early stages. It is recognized that prevention could be possible with the implementation of patient-specific Finite Element (FE) models to calculate dangerous levels of strains in the deep tissues that could trigger a pressure ulcer [1]. Validation of such FE models is a complex task. The current implemented techniques are limited as they consider only external displacements and pressures, or cadaveric samples [2]. In this work, we propose an *in vivo* technique for evaluating the simulations provided by an FE model of the human heel. This solution is based on the 3D non-rigid registration between two Magnetic Resonance (MR) images (one with heel at rest and the other one after applying a surface load below the heel) that is used to estimate tissue *in vivo* internal strains.

## Methods

A Magnetic Resonance-compatible device has been designed to apply external loads on the heel while acquiring 3D MR images [3] (Figure 1). Using non-rigid registration techniques, the deformation field between the undeformed and deformed configuration is computed. From the obtained deformation map the Green-Lagrange strain field is subsequently calculated. On the other hand, the segmentation from the unloaded MR image allowed to generate an ANSYS FE model of the heel. The MR load experiment was then simulated to compare the shear strain results between the FE method and the image registration (Figure 2).

## Results

The MR-compatible device permitted to obtain good quality images allowing for a reliable image registration. The strain distribution, calculated respectively with 3D image registration and FE, resemble the expected results showing the highest strains around the bony prominence of the calcaneus (Figure 2).

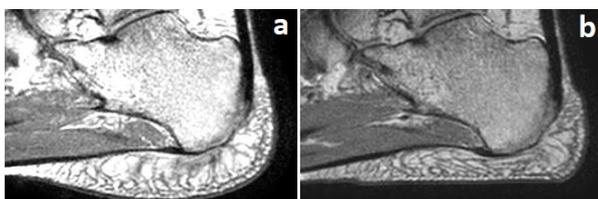


Figure 1: (a) MR image of the heel at rest. (b) MR image of the loaded heel.

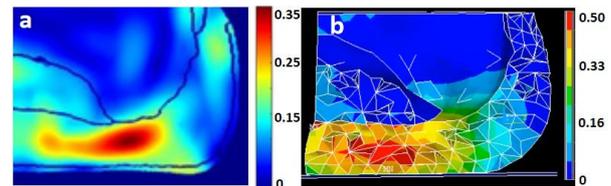


Figure 2: Comparison of tissue shear strains. (a) Green Lagrange strains map estimated from the displacement field computed in the image registration [2]. (b) Hencky shear strains computed by ANSYS.

## Discussion

The implemented technique adds a useful tool for better understanding the propagation of strains in heel deep tissues that could generate pressure ulcers. Strain estimations through 3D image registration offers a promising technique for evaluating FE models for biomechanical applications. Further investigation is required towards identifying optimal material parameters to be implemented in the FE model. This would allow to find a stronger match in terms of magnitude and location of computed strains with both techniques.

## References

- [1] K. K. Ceelen, A. Stekelenburg, S. Loerakker, G.J. Strijkers, D.L. Bader, K. Nicolay, F.P.T. Baaijens & C.W.J. Oomens (2008). Compression-induced damage and internal tissue strains are related, *J. Biomech.*, vol. 41, no. 16, pp. 3399–3404.
- [2] B. E. Keenan, S. L. Evans, and C. W. J. Oomens, “A review of foot finite element modelling for pressure ulcer prevention in bedrest: Current perspectives and future recommendations,” *J. Tissue Viability*, Jun. 2021, doi: 10.1016/J.JTV.2021.06.004.
- [3] A. Trebbi, A. Perrier, M. Bailet, and Y. Payan, “MR-compatible loading device for assessment of heel pad internal tissue displacements under shearing load,” *Med. Eng. Phys.*, vol. 98, pp. 125–132, Dec. 2021, doi: 10.1016/J.MEDENGPY.2021.11.006.

## Acknowledgements

This research has received funding from the European Union's Horizon 2020 research and innovation program under the Marie Skłodowska-Curie Grant Agreement No. 811965; project STINTS (*Skin Tissue Integrity under Shear*).