



HAL
open science

An optimized technique for red blood cells velocity measurement in microvessels

Sophie Roman, Sylvie Lorthois, Paul Duru, Frederic Risso

► To cite this version:

Sophie Roman, Sylvie Lorthois, Paul Duru, Frederic Risso. An optimized technique for red blood cells velocity measurement in microvessels. 18th Congress of the European Society of Biomechanics, Jul 2012, Lisbon, Portugal. pp.0, 2012. hal-04023100

HAL Id: hal-04023100

<https://hal.science/hal-04023100v1>

Submitted on 10 Mar 2023

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Open Archive TOULOUSE Archive Ouverte (OATAO)

OATAO is an open access repository that collects the work of Toulouse researchers and makes it freely available over the web where possible.

This is an author-deposited version published in : <http://oatao.univ-toulouse.fr/>
Eprints ID : 10183

To cite this version : Roman, Sophie and Lorthois, Sylvie and Duru, Paul and Risso, Frederic *An optimized technique for red blood cells velocity measurement in microvessels*. In: 18th Congress of the European Society of Biomechanics, 01 July 2012 - 04 July 2012 (Lisbon, Portugal).

Any correspondence concerning this service should be sent to the repository administrator: staff-oatao@listes-diff.inp-toulouse.fr

AN OPTIMIZED TECHNIQUE FOR RED BLOOD CELLS VELOCITY MEASUREMENT IN MICROVESSELS

Sophie Roman (1), Sylvie Lorthois (1), Paul Duru (1), Frédéric Risso (1)

1. Institut de Mécanique des Fluides de Toulouse, UMR CNRS 5502, France

Introduction

Oxygen and nutrient delivery to living tissues, as well as metabolic waste removal, are essentially determined by the dynamics of blood flow in microvascular networks. In these vessels, measuring the velocity distribution of red blood cells (RBCs) is still challenging. One of the most popular techniques used for that purpose is the *Dual-Slit* (DS), a temporal correlation technique, first introduced by Wayland and Johnson (1967): the vessel under study is trans-illuminated and two photo-sensors (slits) are positioned, separated by a known distance, L_s , along the vessel axis. The time modulation of light is recorded at both positions. A cross-correlation velocity, $V_{ds}=L_s/T_d$, is obtained, where T_d is the time delay for which the cross-correlation between the two signals is maximum. However, RBCs are positioned at different depths within the channel and thus move at different velocities. Baker and Wayland (1974) suggested that V_{ds} is related to a dynamic averaged velocity, but this has never been proved.

The aim of this work is to determine the relationship between the measured velocity V_{ds} and the actual velocity scales of the flow. For that purpose, the DS technique is first optimized using sequences of synthetic images representing RBCs flow. By this way, all the parameters characterizing the RBCs flow, including the shape of their velocity profile in the direction parallel to the incident light beam, which is inaccessible to the observer in real experiments, are controlled. The DS is then applied to *in vitro* RBCs flows in microchannels.

Methods

Synthetic image sequences are computer generated by simulating the flow of elliptical particles representing RBCs for various flow parameters: channel depth D , velocity V_{max} at the centre of the channel, shape of the velocity profile (from flat to parabolic) and RBCs volume fraction H . The parameters characterizing the technique are: spatial resolution (δ), frame rate (F), number of images in the sequence (M), slits width (w) and height (h), and distance between the slits (L_s).

***In vitro* RBCs flows** image sequences are recorded using square and rectangular PDMS micro-channels and human RBCs washed suspensions.

Results

The parametric study performed on synthetic images shows that, when L_s increases, the measured velocity V_{ds} approaches V_{max} , whatever the flow parameters. Thus, in optimal conditions (see Tab. 1), the measured velocity corresponds to V_{max} . The DS is then applied on *in vitro* image sequences for every position in the width of the channel, which leads to velocity profiles where each point represents the maximal velocity in the depth of the channel, see Fig. 1.

V_{im} (pixels/frame)	M	w and h (pixels)	L_s (RBCs size)
$V_{im} = \frac{V_{max} \delta}{F} < 0.15$	$V_{im} M > 9000$	$w=h=1$	5 to 10

Table 1: Operational parameters for an optimal use of the DS. V_{im} represents the maximal displacement of RBCs from one image to the other.

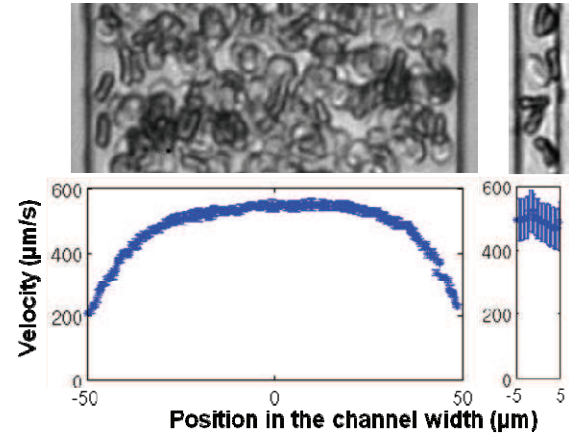


Figure 1: Typical images (bottom) and transverse velocity profiles (top) obtained for RBCs flow in a $20 \times 100 \mu\text{m}^2$ (left) and a $10 \times 10 \mu\text{m}^2$ (right) channel.

Discussion

We showed that, contrarily to previous thinking, the velocity measured by the *Dual-Slit* technique is the maximal velocity in the depth of the channel, provided that suitable conditions (Tab. 1) are applied. Therefore, many previous experimental results obtained by this technique might need to be revisited, with potential consequences on the phenomenology of microvascular flows.