



Delayed closed-loop neurostimulation for the treatment of pathological brain rhythms in mental disorders

Thomas Wahl, Joséphine Riedinger, Michel Duprez, Axel Hutt

► To cite this version:

Thomas Wahl, Joséphine Riedinger, Michel Duprez, Axel Hutt. Delayed closed-loop neurostimulation for the treatment of pathological brain rhythms in mental disorders. 2023. hal-04037276v2

HAL Id: hal-04037276

<https://hal.science/hal-04037276v2>

Preprint submitted on 20 Mar 2023 (v2), last revised 5 Jul 2023 (v4)

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Delayed closed-loop neurostimulation for the treatment of pathological brain rhythms in mental disorders

Thomas Wahl*, Joséphine Riedinger*[△], Michel Duprez*, Axel Hutt*

* ICube, MLMS, University of Strasbourg; MIMESIS Team, Inria Nancy - Grand Est, Strasbourg, France

[△] INSERM U1114, Neuropsychologie cognitive et physiopathologie de la schizophrénie, Strasbourg, France

Correspondence*:

Thomas Wahl

thomas.wahl@etu.unistra.fr

2 ABSTRACT

Mental disorders (MD) are among the top most demanding challenges in world-wide health. According to the World Health Organization, the burden of MDs continues to grow with significant impact on health and major social and human rights. A large number of MDs exhibit pathological rhythms, which serve as the disorders characteristic biomarkers. These rhythms are the targets for neurostimulation techniques. Open-loop neurostimulation employs stimulation protocols, which are rather independent of the patients health and brain state in the moment of treatment. Most alternative closed-loop stimulation protocols consider real-time brain activity observations but appear as adaptive open-loop protocols, where e.g. pre-defined stimulation sets in if observations fulfil pre-defined criteria. The present theoretical work proposes a fully-adaptive closed-loop neurostimulation setup, that tunes the brain activities power spectral density (PSD) according to a user-defined PSD. The utilized brain model is non-parametric and estimated from the observations via magnitude fitting in a pre-stimulus setup phase. Moreover, the algorithm takes into account possible conduction delays in the feedback connection between observation and stimulation electrode. All involved features are illustrated on pathological α - and γ -rhythms known from psychosis. To this end, we simulate numerically a linear neural population brain model and a non-linear cortico-thalamic feedback loop model recently derived to explain brain activity in psychosis.

20 **Keywords:** neurostimulation, closed-loop, control, real-time, delay, EEG

1 INTRODUCTION

Electrical neurostimulation is an old human idea, and has been a well-established therapy for mental disorders for few decades. Caius Plinius during Antiquity and Scribonius Largus, who lived in the first century AD, proposed respectively contacts with the Electric ray (Torpedo Fish) for the treatment of post-partum pain and severe headaches. In the 19th century, electrical stimulation was commonly prescribed by neurologists for nervous disease (Edel and Caroli, 1987). Today, various electrical stimulation techniques exist to modulate neuronal systems and novel techniques for an optimal clinical treatment of a specific

pathology gain more and more attention. They could be used as an additional therapeutic lever or as an alternative to pharmacological medication, thus representing a hope for pharmaco-resistant forms of disease.

Brain oscillations result from coordinated electrical neuronal tissues activity within and between structures and networks. Implicated in various neural processes, such as perception, attention and cognition, their disruption yields pathological rhythms, which reflect abnormal activity of the implicated brain network, notably at the cellular and molecular level (Basar, 2013). These pathological rhythms serve as good biomarkers for neuropathologies. For instance, neurophysiological studies have revealed that a large number of mental disorders exhibit pathological rhythms, which do not occur in healthy patients Schulman et al. (2011). Neurostimulation techniques have identified such pathological rhythms as good stimulation targets for the treatment of brain oscillatory disorders. Neurostimulation induces electric currents in neuronal tissue. Depending on the stimulation protocol, i.e. the temporal stimulation current shape, its duration and pause and the number of repetitions, neurostimulation can lead to neural plasticity effects or to pacemaker-like brain stimulation, respectively.

For example, Deep Brain Stimulation (DBS) is an invasive technique and proposed for patients suffering from severe pharmaco-resistant Parkinson's disease (PD) or obsessive-compulsive disorders. In PD patients aberrant hypersynchronicity and hyperactivity in the β -frequency band (12-30 Hz) of the basal ganglia-thalamocortical network can be addressed by the pharmacological medication (e.g. Levodopa) or DBS. The conventional DBS protocols focus on the subthalamic nucleus or globus pallidus stimulation

continuously at a temporally constant frequency about 130 Hz. The suppression of the pathological beta oscillations was correlated with improving motor symptoms (Kühn et al., 2008). Recent techniques (Fleming et al., 2020; Hosain et al., 2014) propose to apply an adaptive closed-loop stimulation protocol based on observed intracranial brain activity. In addition to this intracranial neurostimulation technique, transcranial electrical stimulation (TES) and transcranial magnetic stimulation (TMS) are non-invasive neuromodulation approaches in which, respectively, a low electrical current and a magnetic field are applied to the cortical tissues. The TES current modalities include direct currents (tDCS), i.e. constant currents, alternating current (tACS), i.e. typically oscillatory currents, and random noise-shape currents (tRNS), which typically includes frequencies above the β -frequency band. It was shown that tDCS can improve cognitive performance in healthy subjects (Brunelin et al., 2012) and patients (Stagg et al., 2018) and it is applied as a therapeutic means to target brain network dysfunctions, such as Attention-Deficit/Hyperactivity Disorder (Nejati et al., 2020) and major depressive disorder (Bennabi and Haffen, 2018).

Although the neurostimulation techniques mentioned above may permit to alleviate mental disorder patients from symptoms, the success rate of these treatments is still limited (Nasr et al., 2022). This underperformance results from non-optimal choices of the stimulation protocol originating from the lack of understanding of the underlying neural response to stimulations and the non-patient specific stimulation protocol. In other words, typically the stimulation protocol (including size, duration, repetition cycle of the stimulation signal) is open-loop, i.e. pre-defined without taking into account the current brain/health state of the patient (Paulus, 2011). This non-optimal approach is inferior to so-called closed-loop techniques, which adapt to the patients current brain/health state. Such an adaptive, or closed-loop, approach has been introduced for intracranial (Prosky et al., 2021; Stanslaski et al., 2022; Hartshorn and Jobst, 2018) and transcranial stimulation (Tervo et al., 2022). Recently proposed closed-loop methods are adaptive in the sense that a pre-defined stimulation signal is applied when observed brain activity fulfills certain

70 criteria, such as passing an amplitude or power threshold. While this adaptive approach improves existing
71 open-loop methods, the pre-defined stimulation signal may still be non-optimally chosen.

72 We propose to estimate a stimulation signal on the basis of observed brain activity. The target stimulation
73 signal is not pre-defined as in the open-loop setting but computed according to a pre-defined target spectral
74 power distribution of the brain activity. To our best knowledge, this focus on a target brain activity spectral
75 distribution has not been proposed before in a closed-loop neurostimulation setup. We argue that it is
76 the natural choice for a closed-loop optimization in the presence of pathological rhythms: typically the
77 pathology is identified by an abnormal power in a certain frequency band and the closed-loop control aims
78 to modify this power value in such a way that the final brain activity power spectral distribution resembles
79 the distribution of a healthy subject. This approach implies the hypothesis that modifying the observed
80 pathological brain rhythms of a patient to resemble brain rhythms of a healthy subject renders the patients
81 brain state and improves the patients health situation. This assumption was motivated by the impressive
82 improving impact of DBS in psychiatric disorders (Holtzheimer and Mayberg, 2011).

83 Technically, the proposed method aims to reshape the spectral distribution of observed data, such as
84 electroencephalographic data (EEG). For illustration, we consider pathological brain rhythms observed
85 in psychosis in the α - (Howells et al., 2018) and γ -band (Leicht et al., 2015). Our method relies on
86 the extraction and the filtering in real-time of the brain resting state activity signal, using the EEG and
87 an estimated brain response model. The underlying brain model is fully non-parametric and estimated
88 from observed resting state EEG. Moreover, we consider the fact that the closed-loop feedback exhibits
89 a certain conduction delay between measurement and stimulation. This conduction delay results from the
90 transmission delay in the hardware and the numerical computation time of the stimulation signal. Very
91 first estimates of this delay time are in the range of few tens of milliseconds (Private communication,
92 Isope, 2020), i.e. in the range of EEG signal time scales. Consequently, the present feedback delay in
93 real-world systems may affect the methods performance. To our best knowledge, the present study is the
94 first considering delays in closed-loop neurostimulation systems.

95 The remaining article is organized as follows : Section 2 presents the neurostimulation setup and the
96 closed-loop circuit studied in the rest of this paper. Then, we propose a model-based controller design to
97 apply desired modifications to the observed activity signal. Subsequently, we propose a model estimation
98 method to extract the brain input response model needed for the controller design. Later, we address
99 the problem of the closed-loop delay by designing an additional system to approximate the future values
100 of the observations. Finally, we present two brain models, which illustrate and validate the proposed
101 method. Then, Section 3 presents the simulation results of our circuits, including the accuracy of the
102 model estimation step and the delay compensation. Lastly, in section 4, we discuss the results of the
103 method presented in the paper compared to the state of the art, mention limitations and pinpoint some
104 perspectives and possible experimental tests.

2 MATERIAL AND METHODS

105 2.1 Neurostimulation setup

106 We build a theoretical plant as a circuit containing a stimulation element and an observation element,
107 both connected to the model brain system under study. In real practice, the stimulation element
108 corresponds to the neurostimulation device, such as a TES system or a TMS coil. In contrast, the
109 observation element may represent electro-/magneto-encephalographic electrodes (in the following called

110 EEG) or electrodes observing Local Field Potential. We define the time-dependent functions $u : \mathbb{R} \rightarrow \mathbb{R}$
 111 and $y : \mathbb{R} \rightarrow \mathbb{R}$ as the input stimulation current and the output EEG signal, respectively.

112 If no input current is applied, the output is a non-zero stochastic signal y_0 corresponding to the measured
 113 resting state EEG activity and a non-zero neurostimulation current alters the output signal as a linear
 114 response. This alteration is caused by a change in the brain activity in response to the neurostimulation
 115 input and a direct measurement of the input current. The latter is undesirable as it is not correlated with
 116 brain dynamics but only with neurostimulation and measurement devices. In the following, we assume
 117 that observations include brain dynamics correlated output only while direct current measurements are
 118 filtered out. A method to remove the direct current measurement from the EEG signal is discussed in
 119 Section 4.

120 Then, we define the plant \mathcal{P} as the system that takes u as its input and generates an output y which is
 121 equal to y_0 when no input is applied. By modeling the dynamics of \mathcal{P} , our goal is a neurostimulation
 122 signal u that causes predetermined changes in the spectral power amplitude of the output signal y . In our
 123 case, the goal is to increase the activity in the alpha band (8 – 12Hz) and decrease the activity in the
 124 gamma band (25 – 55Hz).

125 2.2 Linear time invariant model

126 We assume that the observed output response to a small neurostimulation input u is linear and time-
 127 invariant (LTI). This assumption is supported by multiple results across literature (Liu et al., 2010;
 128 Popivanov et al., 1996; Kim and Ching, 2016). Thus, there is an underlying LTI system \mathcal{G} that produces an
 129 output y_u for any given input u . For this system, we can define a function $g : \mathbb{R} \rightarrow \mathbb{R}$, which is the output
 130 produced by the plant input response system \mathcal{G} in response to a unit impulse signal $\delta(t)$. This function g
 131 is also called the unit impulse response of \mathcal{G} and we have

$$y_u(t) = g(t) * u(t) := \int_{-\infty}^{+\infty} g(t')u(t - t')dt'.$$

132 with time t and $*$ denotes the convolution over time. It leads to the total plant output

$$y(t) = y_0(t) + y_u(t) = y_0(t) + g(t) * u(t). \quad (1)$$

133 With this choice of model, the contribution of the neurostimulation response to the total output is purely
 134 additive, allowing us to focus the analysis on \mathcal{G} , which represents the neurostimulation response part of
 135 the plant system. We also see that y_0 , the resting state activity, contains the stochastic part of the output,
 136 while y_u can be predicted for any known input signal u if we have a model for the system \mathcal{G} . A method to
 137 estimate the plant input response model \mathcal{G} is presented in section 2.4.

138 2.3 Closed-loop control

139 In this section, we suppose that the function g is known. The estimation of g will be the aim of section
 140 2.4.

To close the loop, we generate the plant input signal u as the output of a linear controller \mathcal{K} in response
 to the plant output y

$$u(t) = k(t) * y(t),$$

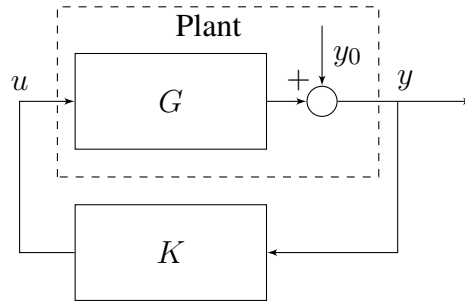


Figure 1. Closed-loop neurostimulation circuit

141 where $k : \mathbb{R} \rightarrow \mathbb{R}$ is the unit impulse response of the controller \mathcal{K} . We can now rewrite Eq. (1) as

$$y(t) = y_0(t) + g(t) * k(t) * y(t). \quad (2)$$

142 Here, we assume that no delay between observation and stimulation application is present. We will relax
 143 this condition in section 2.5. To solve Eq. (2), we apply the Laplace transform defined for each time-
 144 dependent function $x : \mathbb{R} \rightarrow \mathbb{R}$ by

$$X(s) = \mathcal{L}\{x(t)\}(s) := \int_{0-}^{+\infty} x(t)e^{-st} dt, \quad (3)$$

Thus, we define $Y : \mathbb{C} \rightarrow \mathbb{C}$, $Y_0 : \mathbb{C} \rightarrow \mathbb{C}$, $G : \mathbb{C} \rightarrow \mathbb{C}$ and $K : \mathbb{C} \rightarrow \mathbb{C}$ as the Laplace transforms of respectively y , y_0 , g and k , allowing us to write Eq. (2) as

$$Y(s) = Y_0(s) + G(s)K(s)Y(s).$$

145 Hence

$$Y(s) = \frac{1}{1 - G(s)K(s)} Y_0(s). \quad (4)$$

146 We now have an equation for the closed-loop output in function of the resting state activity. A block
 147 diagram of the closed-loop circuit is shown in Fig. 1. Hence to design the frequency distribution of y we
 148 tune the frequency distribution of the transfer function K of the controller \mathcal{K}

149 Controller synthesis

150 Our closed-loop setup aims to tune the observation power spectrum, or equivalently, the choice of
 151 $Y(s)$ subjected to the resting state $Y_0(s)$. To this end, we define a linear filter \mathcal{H} with transfer function
 152 $H : \mathbb{C} \rightarrow \mathbb{C}$ and

$$Y(s) = Y_0(s) + H(s)Y_0(s). \quad (5)$$

153 Specifically, we intend to restore the physiological state of the brain, e.g. of a schizophrenic patient as
 154 our motivation, with an observed EEG presenting low alpha activity and high gamma activity. The chosen
 155 filter \mathcal{H} is a weighted double bandpass filter with positive weight in the α -frequency band to increase α -
 156 power and negative weights in the γ -band to decrease the systems γ -activity. The filter's transfer function
 157 is defined as

parameter	description	value
f_1	α -band natural frequency	10ms
B_1	α -band width	4Hz
c_1	α -band weight	1.0
f_2	γ -band natural frequency	40ms
B_2	γ -band width	30Hz
c_2	γ -band weight	-0.5

Table 1. Parameter set of the filter \mathcal{H} . The frequency parameters are chosen based on the alpha frequency range (8-12Hz) and the gamma frequency range (25-55Hz) in an EEG. The weighting parameters c_1 and c_2 , respectively positive and negative, corresponding to the choice to increase the alpha activity and decrease the gamma activity.

$$H(s) = c_1 \frac{2\pi B_1 s}{s^2 + 2\pi B_1 s + (2\pi f_1)^2} + c_2 \frac{2\pi B_2 s}{s^2 + 2\pi B_2 s + (2\pi f_2)^2}.$$

158 The exact parameters of \mathcal{H} are shown in table 1.

159 We can synthesize the closed-loop controller \mathcal{K} , by combining equations (4) and (5) and solving for K
160 as

$$\begin{aligned} \frac{1}{1 - G(s)K(s)} Y_0(s) &= Y_0(s) + H(s)Y_0(s) \\ K(s) &= \frac{H(s)}{(1 + H(s))G(s)}. \end{aligned} \quad (6)$$

161 Therefore, if we know the plant input response transfer function G , we can find that desired controller
162 transfer function K by Eq. (6). Once the transfer function is obtained, we can use it to find a corresponding
163 state-space representation (Hespanha, 2018) for time domain simulations.

164 2.4 Model estimation

165 The design of our closed-loop controller requires estimating the plant input response system \mathcal{G} , which
166 in practice includes the brain dynamics, the neurostimulation device and the observation device. Our
167 approach includes the estimation of \mathcal{G} directly from observed brain activity, such as EEG of the patient.
168 This ensure that the estimated plant model will be as close as possible to the real brain dynamics in the
169 corresponding experimental conditions. To this end, we first need to find a way to measure the plant input
170 response without also measuring the plant resting state activity. This is not trivial since the observed signal
171 is the sum of the resting state activity and the stimulation response.

172 Signal extraction

173 Let us consider an open-loop setup with an arbitrary input u applied to the plant, which generates the
174 output described by Eq. (1). In this equation, we only know u and y , and want to estimate the impulse
175 response g . The problem is that we cannot observe y_0 only during the stimulation. Hence, based on
176 previous data recordings, we need to find a way to predict the dynamics of y_0 during the stimulation.

First, we provide the following standard definitions that are important in the subsequent discussion. For any time domain signal $x : \mathbb{R} \rightarrow \mathbb{R}$, we denote the Fourier transform by

$$\hat{x}(f) = \mathcal{F}\{x(t)\}(f) := \int_{-\infty}^{\infty} x(t)e^{-2\pi i f t} dt. \quad (7)$$

We define $\alpha_0 : \mathbb{R} \rightarrow \mathbb{R}$ and $\alpha_u : \mathbb{R} \rightarrow \mathbb{R}$ such as $\alpha_0(t) = y_0(t) - \bar{y}_0$ and $\alpha_u(t) = y_u(t) - \bar{y}_u$ where \bar{y} , \bar{y}_0 and \bar{y}_u are respectively the ensemble means of y , y_0 and y_u .

We assume that y_0 is a wide-sense-stationary (WSS) random process, i.e. its mean and variance do not depend on time. According to the Wiener-Khinchin theorem (Khinchine, 1934; Gardiner, 2004), the autocorrelation function of a wide-sense-stationary random process has a spectral decomposition given by the power spectrum of that process

$$S_{yy}(f) = |\hat{\alpha}(f)|^2,$$

where $\hat{\alpha} : \mathbb{R} \rightarrow \mathbb{C}$ is the Fourier transform of $\alpha(t) = y(t) - \bar{y} \in \mathbb{R}$ and $S_{yy} : \mathbb{R} \rightarrow \mathbb{R}^+$ is the spectral density of y .

Then, we can write Eq. (1) as

$$\bar{y} + \alpha(t) = \bar{y}_0 + \alpha_0(t) + \bar{y}_u + \alpha_u(t),$$

where $\bar{y} = \bar{y}_0 + \bar{y}_u$. The equation then simplifies to

$$\alpha(t) = \alpha_0(t) + \alpha_u(t).$$

By application of the Fourier transform, we obtain

$$\hat{\alpha}(f) = \hat{\alpha}_0(f) + \hat{\alpha}_u(f)$$

and

$$|\hat{\alpha}(f)|^2 = |\hat{\alpha}_0(f)|^2 + |\hat{\alpha}_u(f)|^2 + 2\text{Re}[\hat{\alpha}_0(f)\hat{\alpha}_u(f)^*].$$

In the following, we compute the ensemble average of each term of this equation. Since α and α_u are two independent processes sampled at different times and $\langle \hat{\alpha}_0 \rangle = \langle \hat{\alpha}_u \rangle = 0$.

Hence

$$\langle 2\text{Re}(\hat{\alpha}_0(f)\hat{\alpha}_u(f)^*) \rangle = 2\text{Re}[\langle \hat{\alpha}_0(f)\hat{\alpha}_u(f)^* \rangle] = 0.$$

Here and in the following, $\langle \cdot \rangle$ denotes the ensemble average. We point out that although Eq. (8) does hold when considering the ensemble average of the signals, fluctuations around 0 still remain in Eq. (8) for finite ensemble number of finite time signals.

Nevertheless, this yields

$$\langle |\hat{\alpha}_u(f)|^2 \rangle = \langle |\hat{\alpha}(f)|^2 \rangle - \langle |\hat{\alpha}_0(f)|^2 \rangle. \quad (8)$$

Using Eq. (1), we can express $\hat{\alpha}_u$ in terms of the input impulse response g and the input u

$$\begin{aligned}\hat{\alpha}_u(f) &= \mathcal{F}\{y_u(t) - \bar{y}_u\}(f) \\ &= \mathcal{F}\{g(t) * [u(t) - \bar{u}]\}(f) \\ &= \hat{g}(f)\mathcal{F}\{u(t) - \bar{u}\}(f).\end{aligned}\quad (9)$$

This equation permits to estimate the transfer function \hat{g} , see Section 3.

To express the transfer function \hat{g} in Laplace space, we use the fact that a unit impulse response function is non-zero only for positive time values t . Hence, based on equations (3) and (7), for $s = 2\pi if$, we can write the Laplace transform G as

$$G(2\pi if) = \int_{0-}^{+\infty} g(t)e^{-2\pi ift}dt = \int_{-\infty}^{+\infty} g(t)e^{-2\pi ift}dt = \hat{g}(f).$$

We now need a method to generate a LTI system with a transfer function that matches the magnitude data computed with the formula. This is achieved by the magnitude vector fitting algorithm.

Magnitude vector fitting

Our goal is now to find a transfer function G corresponding the magnitude data $|\hat{g}(f)|^2$. For this purpose, we use a variant of the vector fitting algorithm design to work even with only the magnitude data. This method is called magnitude vector fitting (De Tommasi et al., 2010).

It allows to fit a passive LTI system to data by fitting the model transfer function. The system is synthesized such that the mean square error between the magnitude data sample and the transfer function evaluated at the same frequency points is minimized. De Tommasi et al. (2010) show that the transfer function of the fitted model reproduces both the magnitude and the phase shift of the original transfer function, although the fitting has been performed using sampled magnitude data only.

By minimizing the mean square error, the algorithm ensures that the transfer function of the fitted model accurately matches the original model as represented by the reconstructed gain data. Furthermore, to assess the accuracy of the reconstruction, we also compare the fitted model to the transfer function of the linearized brain model used for the simulation. This allows to double-check the validity of the reconstructed magnitude and also to verify if the reconstructed phase fits the phase of the original model as closely as possible cf. Fig 3C,D.

2.5 Delay compensation

Realistic feedback loops exhibit conduction delays between the moment of observation and feedback stimulation. Reasons for such delays are finite conduction speeds in cables, electronic switches, interfaces and delays caused by the controller device to compute numerically adapted stimuli. In systems with large time scales, such as controlled mechanical devices on the centimeter or larger scale, such delays may be negligible. Conversely biological systems such as the brain evolve on a millisecond scale and conduction delays may play an important role. Preliminary estimation of input and output devices of desktop computers have revealed an approximate delay of ~ 10 ms. By virtue of such delays, it is important to take them into account in the closed-loop between the moment of observation and stimulation.

The different sources of delay can be represented as plant input and output delays. Since the controller \mathcal{K} is LTI, the input and output delays can be concatenated into one single plant input delay. Hence, in our setup, we model the delay as an input delay τ in the system \mathcal{G} , modifying $y(t) = g(t) * u(t)$ in Eq. (1) to $y(t) = g(t) * u(t - \tau)$. The Smith predictor (Smith, 1959) (Morari and Zafiriou, 1989) is a known method to compensate such delay times. However, in the present problem, this approach allows controlling a limited frequency band only (see Fig. 7A)). Consequently, it was necessary to invent another method. Since the plant input u is generated by the controller \mathcal{K} , we modify the controller to compensate the delay. To this end, the new controller \mathcal{K} is chosen to estimate the future value of u instead of the present value. A method to apply this controller modification is presented in Section 3.2.

2.6 Brain models

Our closed-loop control method works for any LTI brain model. Furthermore, we want to show that it also produces good results on non-linear brain models, for which the neurostimulation input response behaves closely to an LTI system, when the input is sufficiently small. To this end, we present two models used to test our method. The first one is a linear neural population model of cortical activity, and the second one is a non-linear cortico-thalamic neural population model with cortico-thalamic delay.

2.6.1 Linear brain model

We describe neural population activity with a noise-driven linear model Hutt (2013). The model is composed of two pairs of interacting excitatory and inhibitory populations. Here we have $V_{e,i}^{(1,2)} : \mathbb{R} \rightarrow \mathbb{R}$, representing the mean activity of the associated population, where $V_e^{(1,2)}$ and $V_i^{(1,2)}$ correspond respectively to excitatory and inhibitory populations. Each population is driven by noise $\xi_{1,2} : \mathbb{R} \rightarrow \mathbb{R}$ and the external input $u : \mathbb{R} \rightarrow \mathbb{R}$, according to the following differential equations:

$$\begin{cases} \tau_{e,1} \frac{dV_e^{(1)}(t)}{dt} = (-1 + N_{11})V_e^{(1)}(t) - N_{11}V_i^{(1)}(t) + b_1u(t) + \xi_1(t), \\ \tau_{i,1} \frac{dV_i^{(1)}(t)}{dt} = N_{21}V_e^{(1)}(t) + (-1 - N_{21})V_i^{(1)}(t) + b_2u(t), \\ \tau_{e,2} \frac{dV_e^{(2)}(t)}{dt} = (-1 + N_{12})V_e^{(2)}(t) - N_{12}V_i^{(2)}(t) + b_3u(t) + \xi_2(t), \\ \tau_{i,2} \frac{dV_i^{(2)}(t)}{dt} = N_{22}V_e^{(2)}(t) + (-1 - N_{22})V_i^{(2)}(t) + b_4u(t), \end{cases} \quad (10)$$

where the noise $\xi_{1,2}$ is uncorrelated Gaussian distributed with zero mean and variance $\kappa_{1,2}^2 = 10^{-7}$, and the stimulation u is weighted by the coupling constants $b_i > 0$ of the corresponding population. In addition, $\tau_{(e,i),(1,2)}$ are the synaptic time constants of the populations, and constants $N_{ij} > 0$ are interaction gains of the respective population. Table 2 provides the parameters employed in subsequent simulations.

The observed output

$$y(t) = V_e^{(1)}(t) - V_i^{(1)}(t) + V_e^{(2)}(t) - V_i^{(2)}(t)$$

is a sum of the effective field potential $V_e^{(j)} - V_i^{(j)}$ of both populations $j = 1, 2$, cf. Fig. 7 (top panels).

The simulation of the linear brain model in time domain is done using the library `control` of `python`. The numerical integration is computed thanks to matrix exponential (Van Loan, 1978), with a simulation sampling time of 1ms.

parameter	description	value
$\tau_{e,1,2}$	exc. synaptic time constant	5ms
$\tau_{i,1,2}$	inhib. synaptic time constant	20ms
N_{11}	first exc. linear coefficient	1.15
N_{21}	first inhib. linear coefficient	0.63
N_{12}	second exc. linear coefficient	2.52
N_{22}	second inhib. linear coefficient	6.6
N	number of neurons	1000
$\kappa_{1,2}^2$	noises variances	$10^{-4}/N$
$b_{1,2}$	input coupling constants	0.18
$b_{3,4}$	input coupling constants	0.14

Table 2. Parameter set of model (10). The choice of parameter is partially based on the paper in which it was developed (see Hutt (2013)).

2.6.2 Cortico-thalamic brain model

A different model considers the cortico-thalamic feedback circuit (Riedinger and Hutt, 2022). It describes the cortex layers I-III and the cortico-thalamic loop between cortical layers IV-VI, the thalamic relay cell population and the reticular structure. The cortical layer I-III exhibits mean activity of excitatory cells v and inhibitory cells w . Similarly, layer IV-VI exhibits the mean activity V_e and V_i and thalamic relay cell populations the mean activity $V_{th,e}$ and $V_{th,i}$. Moreover, the reticular structure has the mean activity V_{ret} . The fibers between the cortex and thalamus and the cortex and reticular structure exhibit a finite conduction delay τ (Riedinger and Hutt, 2022; Hashemi et al., 2015). The 7-dimensional dynamical system of the brain state $\mathbf{x} = (v, w, V_e, V_i, V_{th,e}, V_{th,i}, V_{ret}) \in \mathbb{R}^7$ obeys

$$\begin{cases} \dot{\mathbf{x}}(t) &= \mathbf{F}(\mathbf{x}(t), \mathbf{x}(t - \tau)) + \boldsymbol{\xi}(t) + \mathbf{B}u(t), \\ y(t) &= \mathbf{C}\mathbf{x}(t), \end{cases} \tag{11}$$

where the superscript t denotes transposition, $\mathbf{F} \in \mathbb{R}^7$ is a nonlinear vector function, $\mathbf{B} \in \mathbb{R}^{7 \times 1}$ is the input coupling matrix and $\mathbf{C} \in \mathbb{R}^{1 \times 7}$ is the observation matrix. We mention that $\mathbf{B} = (b_1, b_2, b_3, b_4, 0, 0, 0)^t$, $b_i > 0$, i.e. only the cortical layers are stimulated with weights b_i . The observation y captures the activity of the cortical excitatory populations (Riedinger and Hutt, 2022; Nunez and Srinivasan, 2006) with $\mathbf{C} = (c_1, 0, c_3, 0, 0, 0, 0)$, $c_i > 0$. For more details, please see the Appendix.

The time domain simulations of the cortico-thalamic model is done by numerical integration using the fourth-order Runge-Kutta method implemented by the `scipy` library in `python` with a maximum simulation time step of 1 ms. The signal produced by this cortico-thalamic brain model is shown in Fig. 2.

3 RESULTS

The present work addresses two major problems in closed-loop control: the correct model choice of the systems dynamics and the present conduction delay. The subsequent sections propose solutions for both problems and illustrate them in some detail by applying them to the linear brain activity model from section 2.6.1. The final section demonstrates the closed feedback loop for the cortico-thalamic brain model from Section 2.6.2.

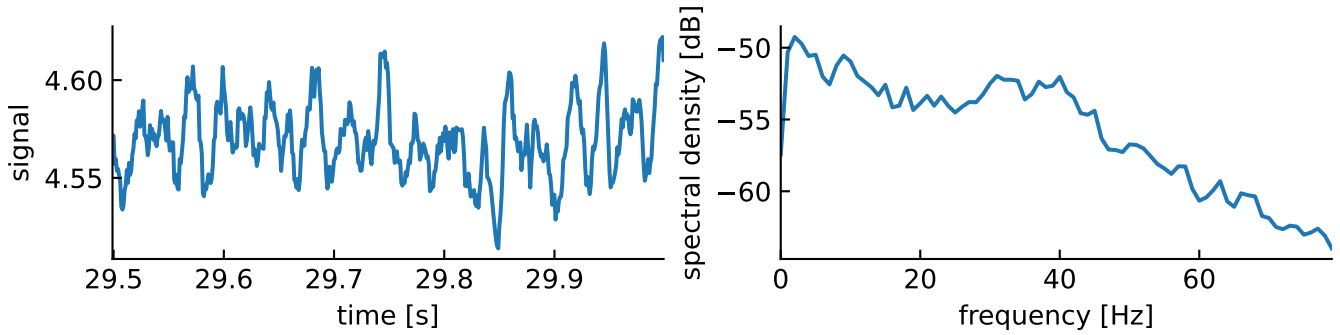


Figure 2. Resting state activity computed from the cortico-thalamic brain model. Left: Observation time series in a certain time window. Right: Power spectral density of the observation time series.

3.1 Model estimation

Equations (8) and 9 permit to express the magnitude of $\hat{g}(f)$ in terms of the spectral densities of observable signals

$$\begin{aligned} |\hat{g}(f)|^2 |\mathcal{F}\{u(t) - \bar{u}\}(f)|^2 &= |\hat{\alpha}(f)|^2 - |\hat{\alpha}_0(f)|^2 \\ |\hat{g}(f)|^2 S_{uu}(f) &= S_{yy}(f) - S_{y_0y_0}(f) \\ |\hat{g}(f)|^2 &= \frac{S_{yy}(f) - S_{y_0y_0}(f)}{S_{uu}(f)}. \end{aligned} \quad (12)$$

The spectral density functions $S_{y_0y_0}$ and S_{yy} may be estimated numerically from output data before and during a stimulation with a known chosen stimulation function u . The estimation may be performed by applying conventional methods, such as the Welch method (Welch, 1967). These estimations provide the magnitude of the transfer function $|\hat{g}|$ by utilizing Eq. (12). In detail, at first, we considered the linear model (10) and injected a white noise current into the plant gaining the system's response signal together with the resting state activity, cf. Fig. 3A. The subsequent estimation of $S_{yy}(f)$, $S_{y_0y_0}(f)$ and $S_{uu}(f)$ (see Fig. 3B) from the data permitted to compute the brain input response model $\hat{g}(f)$ by Eq. (12). We observe a very good accordance of the original model response function and its estimation in magnitude (see Fig. 3C) and phase (see Fig. 3D).

The remaining error in the estimated model compared to the original model depends on the amplitude of the driving noise ξ , cf. Fig. 4. High driving noise can also cause the magnitude vector fitting algorithm not to converge, leading to a non-minimal mean-square error between the fitted and the original models when evaluated at the frequency sample points used for the algorithm.

This problem can be solved by increasing the amplitude of the input current u that we inject in the plant, which decreases the contribution of the rest state driving noise ξ to the output signal relative to the input current. Although the remaining dominant input current is also noisy, its value at any time or frequency is known, meaning that it is canceled out in the ratio $\frac{S_{yy}}{S_{uu}}$ in Eq. (12). This effectively leads to lower noise in the transfer function magnitude data extracted with Eq. (12). The limitation is then set by the maximum amplitude of the current we are allowed to inject into the brain in a given neurostimulation setup. Indeed, the amplitude of the current is limited both for safety reasons that are beyond the scope of this paper and because of the assumption of linearity on which our method is based and which requires small currents.

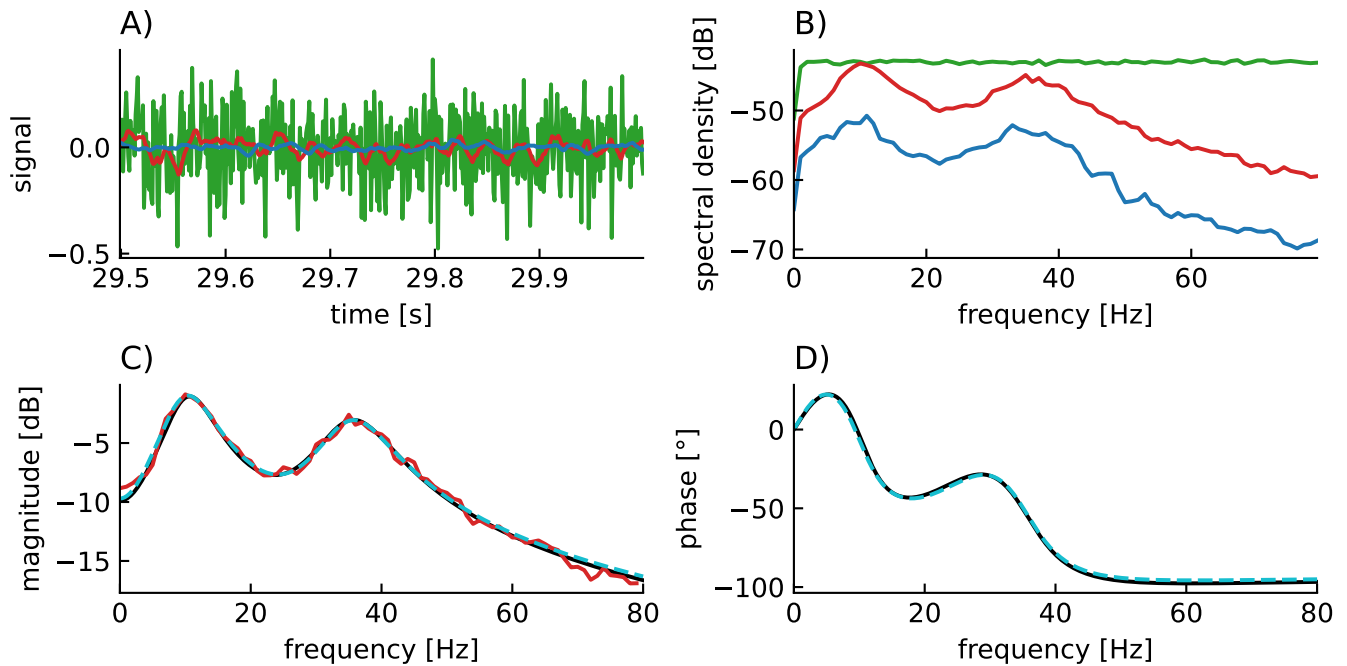


Figure 3. The magnitude vector fitting algorithm successfully reconstructs the transfer function G from magnitude-only data. **A)** Time series of the resting state activity (blue), the input signal (green) and the stimulation response (red). **B)** Spectral densities of the simulated input signal (green), the resting state activity (blue) and the stimulation response (red). The input signal is a white noise with chosen standard deviation 0.005. **C)** Reconstructed gain $|\hat{g}|$ of the plant input response. The fitted model (dashed cyan) accurately matches the original model (black). The red curve is the raw data used for fitting, computed from the spectral density data in panel A) using Eq. (12). **D)** Reconstructed phase of the plant input response \hat{g} .

3.2 Delay compensation

Delay compensation is achieved by adding another LTI system at the output of the controller \mathcal{K} cf. Fig. 5, whose purpose is to reproduce the transfer function of a negative delay. We call this system the predictor ϕ .

However, perfectly reproducing the transfer function of a negative delay would be impossible since the associated time-domain system would then be a perfect predictor, which is a non-causal, i.e. un-physical, system. Nonetheless, we can build a causal and stable system that behaves almost like a perfect predictor, however only in the frequency ranges of interest.

The numerical implementation of the controller necessitates discretization in time. Consequently, it is reasonable to choose the predictor design as a discrete-time system, meaning that for any input signal at $x_t : \mathbb{R} \rightarrow \mathbb{R}$ at an instant $t \in \mathbb{R}$, it approximately predicts the future signal $x_{t+\Delta t}$ where $\Delta t \in \mathbb{R}$ is the sampling time chosen when building the predictor. Since x is a discrete sequence, its transfer function is obtained using the Z-transform, defined as

$$X(z) = \mathcal{Z}\{x_{n\Delta t}\}(z) := \sum_{n=0}^{\infty} x_{n\Delta t} z^{-n},$$

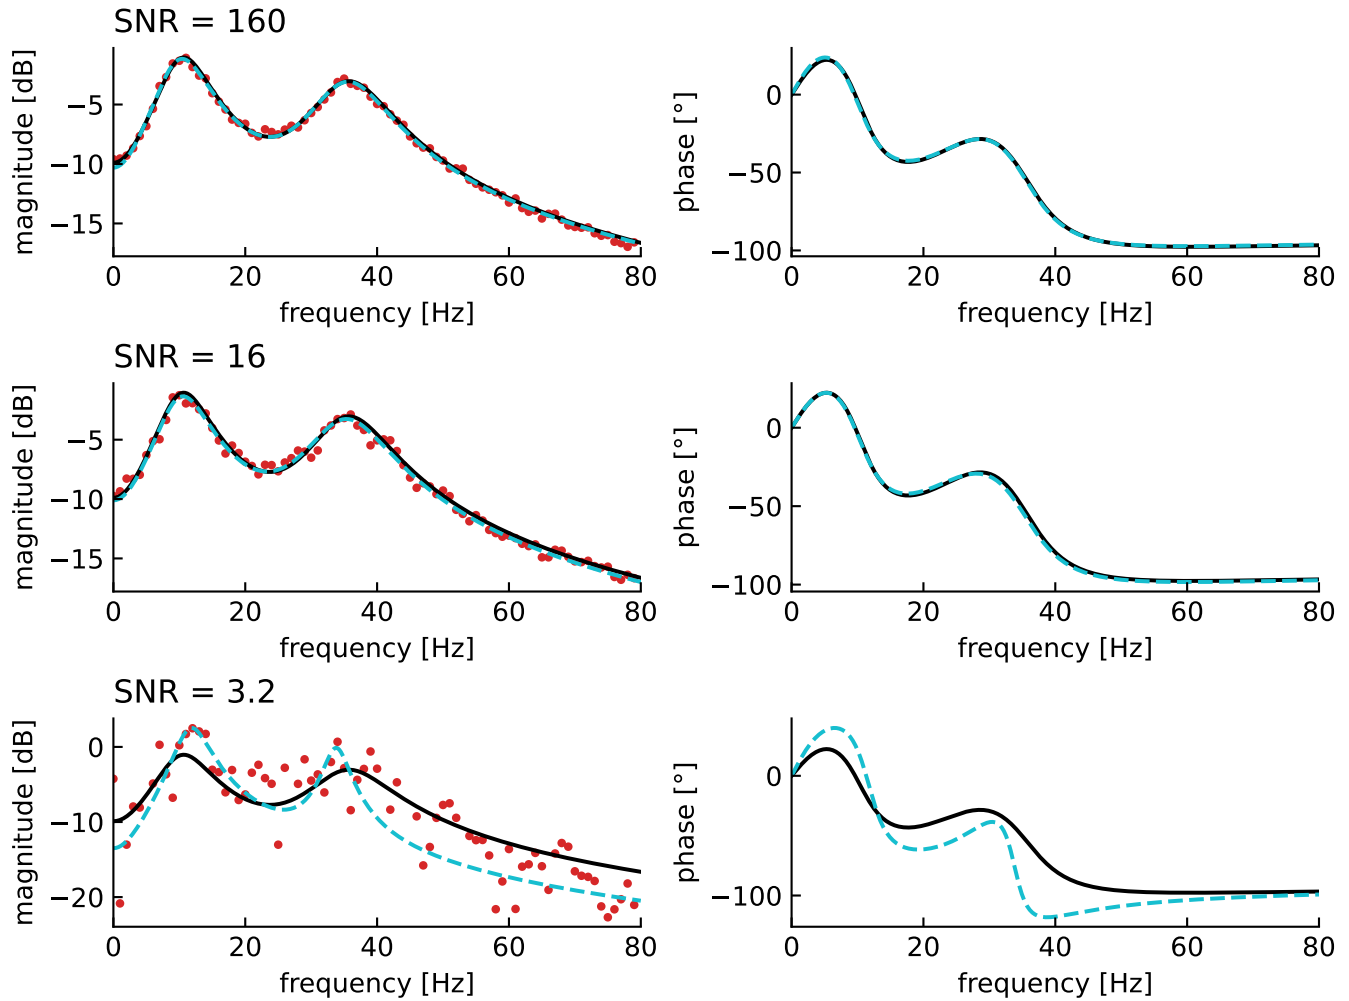


Figure 4. The magnitude vector fitting algorithm's performances depend on the amplitude ratio of the stimulation current and the driving noise. Each row correspond to a different signal-to-noise ratios (SNR), computed as the ratio between the mean input coupling strength and the mean noise standard deviation. The transfer function magnitude data (red dots) are then used to synthesize a plant model via the magnitude vector fitting algorithm. The left (right) column corresponds to the transfer function magnitude (transfer function phase). We see that the noise levels in the transfer function magnitudes are higher for stronger brain-driving noise. The fitted model is coded in dashed cyan and deviates more from the original model for higher noise levels.

with $z \in \mathbb{C}$ and $X : \mathbb{C} \rightarrow \mathbb{C}$. Then the transfer function $\Phi : \mathbb{C} \rightarrow \mathbb{C}$ of a negative delay of one step Δt applied to x would simply be $\Phi(z) = z$, the Z-transform of a one-step delay. However, this choice would be non-causal, which is not implementable numerically in time. Nevertheless, to obtain a stable and implementable system with a transfer function as close as possible to z , we chose the ansatz

$$\Phi(z_0) = \frac{b_0 z_0 + b_1}{z_0 - a} = z_0, \quad (13)$$

for a fixed value $z = z_0$ and where $a \in \mathbb{R}$ is the pole of the system and $b_0 \in \mathbb{R}$ and $b_1 \in \mathbb{R}$ are the polynomial coefficients of the numerator of Φ . This equation corresponds to the transfer function of a discrete LTI system with exactly one pole and one zero, which is the closest form of a proper rational function to the identity function of z in the sense that it has only one more pole. We add the additional

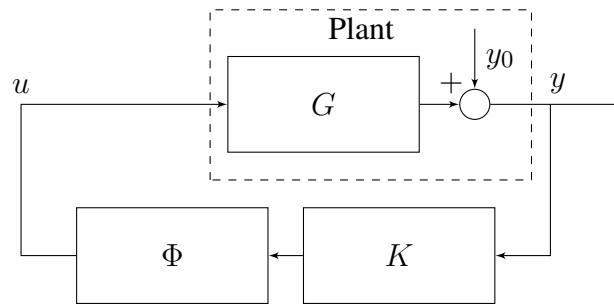


Figure 5. Closed-loop neurostimulation circuit with predictor

constraints that $|a| < 1$, since this is the necessary and sufficient condition for the discrete predictor ϕ to be stable.

We choose to reformulate this problem by setting a as a free parameter. This way, we can select any a between -1 and 1 , and the remaining parameters are found by solving the linear equation $b_0 z_0 + b_1 = z_0(z_0 - a)$, where $z \in \mathbb{C}$ is a chosen complex frequency point at which we want this equation to hold. Since there are two unknowns, we can write a second equation in which we want the derivative of each side of the equation also to be equal, yielding $b_0 = 2z_0 - a$. By replacing b_0 in the first equation, we obtain

$$\begin{aligned} z_0(2z_0 - a) + b_1 &= z_0(z_0 - a) \\ b_1 &= -z_0^2. \end{aligned}$$

In the z -domain, the zero frequency corresponds to $z_0 = 1$. We choose to solve this equation for this point, hence we can replace a , b_0 and b_1 in Eq. (13) which yields

$$\Phi(z) = \frac{(2 - a)z - 1}{z - a}. \quad (14)$$

This transfer function can then be converted to an associated state-space representation and used for time domain simulations with a sampling time Δt . The output of this system will then be $y_t \approx u_{t+\Delta t}$ for any input signal u_t . Simulating delays greater than the system sampling time is simply achieved by concatenating multiple times this predictor system. Here the delay has to be a multiple of the sampling time. This predictor can then be appended to the output of the digital controller \mathcal{K} .

To avoid closed-loop instability, we must limit the amplitude of the feedback signal computed from the controller input signal. This amplitude is determined by the three systems \mathcal{G} , \mathcal{H} and \mathcal{K} . Since \mathcal{G} is defined by the system under study and \mathcal{H} is the chosen filter defining the desired modifications in the frequency distribution of the observed signal, ϕ (or equivalently parameter a) is the only degree of freedom. Figure 6 shows the region of closed-loop stability as a function of the predictor pole a and the delay.

Because the predictor has a gain that is still slightly greater than one in the frequency ranges of interest, we reduce the weights of the filter \mathcal{H} to compensate for the excess gain at the α and γ -peaks. To do this, we simply divide the weight of each band by the magnitude of the predictor system evaluated at the band's natural frequency. This reduces the errors in the closed-loop transfer function in the α and γ -ranges.

Figure 7(B) shows results combining the model estimation by vector fitting and the delay compensation. The proposed closed-loop control yields an increase in α -power and a decrease in γ -power according to the employed target filter \mathcal{H} . The application of a conventional reference signal control and Smith

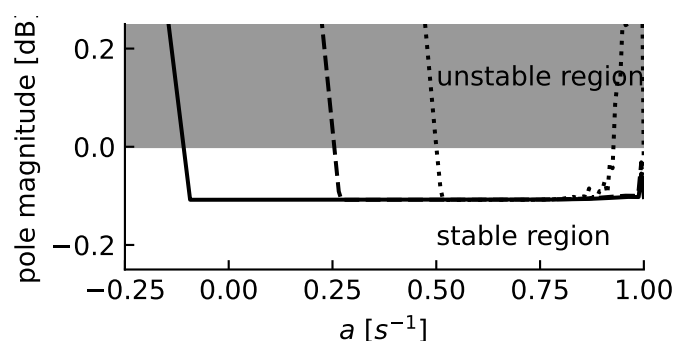


Figure 6. The predictor pole location affects the closed-loop stability. The magnitude of the pole with the highest magnitude in the closed-loop transfer function parameterizes the stability of the closed-loop. Indeed, if this value is less than 0 dB, then all the poles of the closed-loop transfer function have a magnitude less than 0 dB, meaning that the system is stable. The system is unstable otherwise. Here the full curve, the dashed curve and the dotted curve correspond to predictors for delays of 3 ms, 5 ms and 10 ms, respectively. The higher the delay is, the lower is the size of the region of closed-loop stability for a .

341 predictor for delay compensation (Fig. 7(A)) does not yield a reduction of higher γ -frequency activity.
 342 This can also be seen in Fig. 7(bottom panel), showing that the proposed scheme adapts much better to
 343 the target gain function than the reference signal control scheme. Generally, both methods fail to adapt
 344 well to very high-frequencies (details not shown).

345 3.2.1 Accuracy

346 3.2.2 Stability

347 As discussed earlier, delay compensation can destabilize the closed-loop system depending on the
 348 parameters of its components. However, if the correct predictor pole is chosen based on Fig. 6, the
 349 closed-loop will remain stable. These values are computed under the assumption that there are no model
 350 estimation errors. If we take into account the inaccuracies in the fitted brain model compared to the original
 351 brain model, extra gain can add up in the feedback signal, introducing again the risk of destabilizing the
 352 closed-loop. This is trickier to solve, as we assume here that in a real experimental setup that, it is very
 353 difficult to reduce these remaining errors further by the method proposed. Hence the solution is either to
 354 simply reduce the amplitude of the spectral density modification that we want to apply by reducing the
 355 amplitude of the transfer function of filter \mathcal{H} , or to reduce the amplitude of the predictor \oplus reducing its
 356 accuracy and possibly increasing delay errors. In any case, the inaccuracies in the estimated brain model
 357 create errors in the closed-loop transfer function regardless of the delay.

358 3.3 Application to cortico-thalamic circuit model

359 To extend the analysis to a biologically more realistic model, we employed a nonlinear cortico-
 360 thalamic brain model (cf. section 2.6.2). Fitting a linear transfer function to the brain model activity as
 361 described above, we found a good accordance of fitted and original model as can be seen in Fig. 9(A),B).
 362 Small deviations in the gain and the phase resulted from the internal delay in the brain model and its
 363 non-linearity. Indeed, the magnitude vector fitting algorithm does not reproduce this delay but instead
 364 synthesizes a linear system that has no delay but still approximates well the transfer function of the original
 365 model. Nonetheless, the non-linearity of this model can also decrease the accuracy of the fitting, as we
 366 are trying to represent a non-linear input response model by a linear one. However, this effect is only seen
 367 when the current is large enough for the non-linear part of the response to be significant.

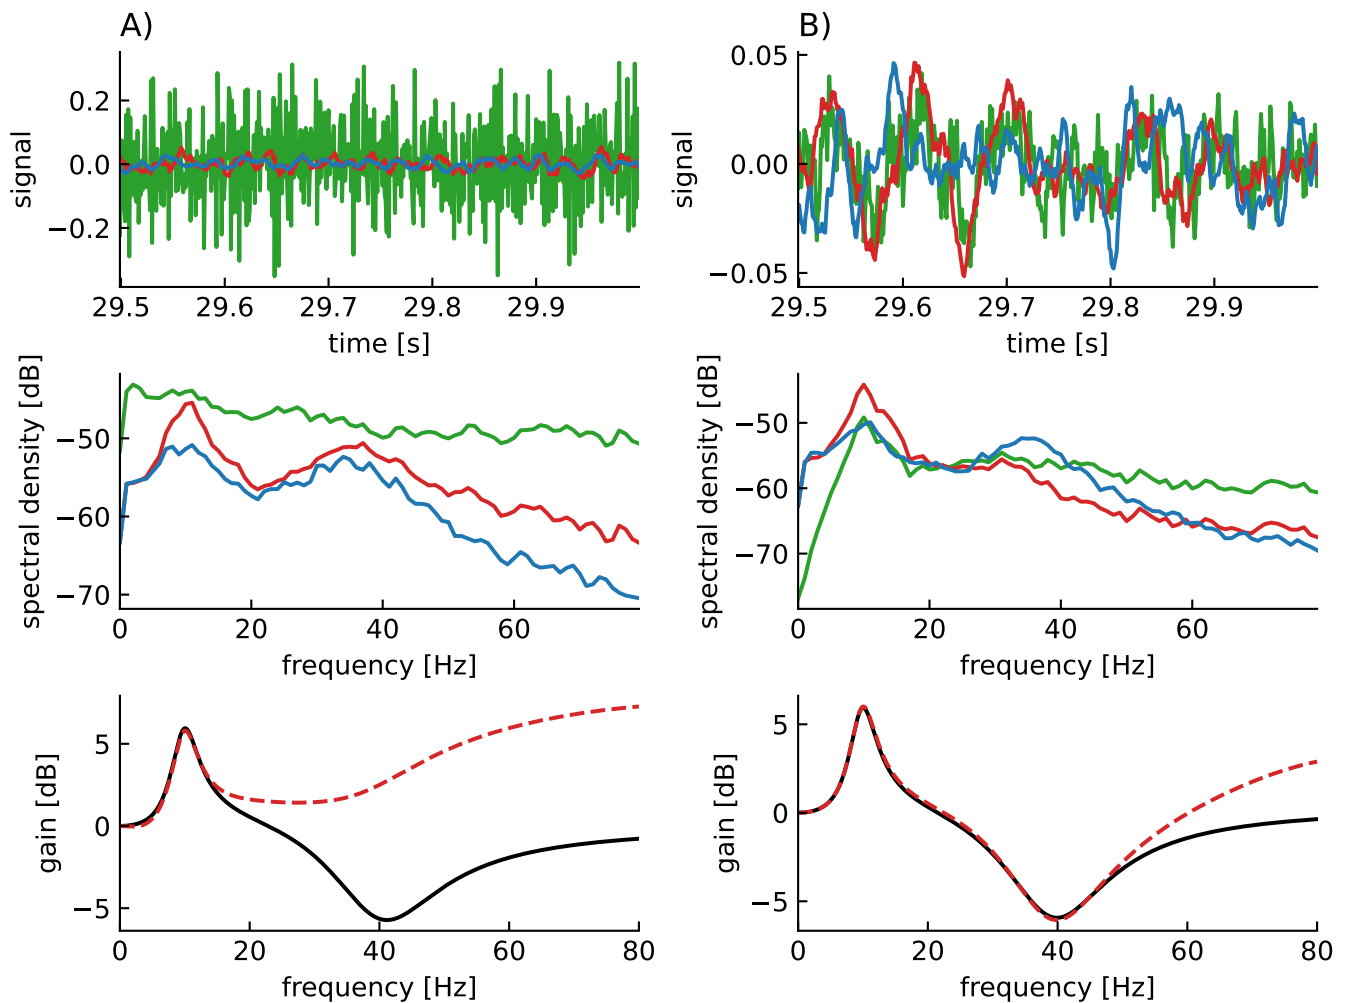


Figure 7. Model-based closed-loop neurostimulation with delay compensation successfully decreases gamma activity while reference signal-based control with Smith predictor fails. **A)** Simulation data of the reference signal-based control design with Smith predictor. **B)** Simulation data of the model-based control design with delay compensation. The upper panels show the time series of the resting state activity signal y_0 (blue) and the closed-loop output signal y (red) and the input current u (green). The amplitude of the stimulation current is much larger for reference signal-based control than for model-based control. The center panels show spectral densities of the resting state activity signal y_0 (blue), the closed-loop output signal y (red) and the input current u (green). The activity is increased in the alpha range and decreased in the gamma range for model-based control, however, is increased everywhere for reference signal-based control. The spectral density of the input current is again much larger for reference signal-based control than for model-based control. The lower panels show the spectral density gain from y_0 to y of the closed-loop systems. The dashed red curve is computed from the closed-loop transfer function and the black curve is the target curve computed from the transfer function $1 + H(s)$. We see that the implemented closed-loop applies the correct modifications in alpha and gamma ranges for model-based control but not for reference signal-based control where the error is large for frequencies above the alpha range. The conduction delay is 5ms and the value of the parameter a in the delay compensation scheme is chosen to $a = 0.55$

368 In fact, the model-based control enhances α -activity and diminishes γ -activity in good accordance to
 369 the imposed filter \mathcal{H} (see Fig. 9C)). This can also be seen in the closed-loop transfer function, which
 370 corresponds well to the target transfer function (see Fig. 9D)) for small and medium frequencies. The

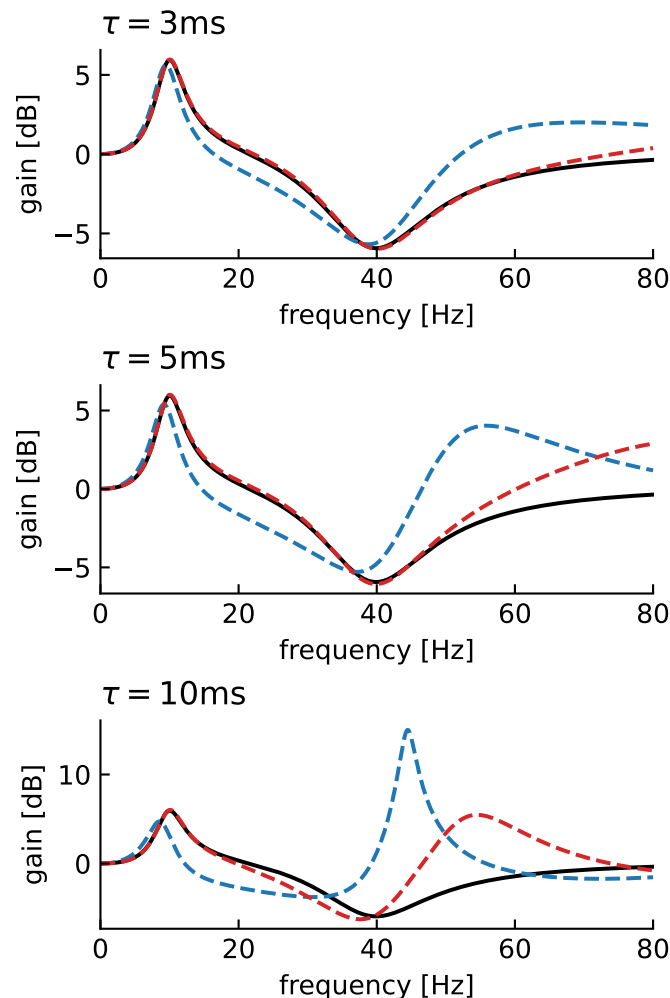


Figure 8. Delay decreases the accuracy of the closed-loop transfer function For uncompensated delay (dashed blue curve), the closed-loop transfer function significantly deviates from the target transfer function defined as $1 + H(s)$ (black curve). Delay compensation (dashed red curve) reduces the deviation from the target transfer function in the α - and γ -frequency range for delays of 3ms and 5ms. However, the error is still large in the γ -range for a delay of 10ms.

371 closed-loop transfer function deviates from the target transfer function for large frequencies beyond the
 372 γ -frequency range. This results from the employed conduction delay.

373 To elucidate better the functions of the different elements of the proposed method, we applied a second
 374 closed-loop setup, where the neurostimulation input was applied to the first three layers of the cortex
 375 modeled by u and v and to the reticulum modeled by V_{ret} (Fig. 10). In this setting, the response in the
 376 high-frequency ranges are mainly produced by the cortex, while the response in low-frequency ranges
 377 originates mainly from the reticulum and the thalamic relay structure, with a gap approximately between
 378 10Hz and 20Hz. The weak response between 10 Hz and 20 Hz observable cf. Fig. 10A is compensated
 379 by the controller, which produces a high magnitude stimulation in the closed-loop for these frequencies
 380 cf. Fig. 10C. The second consequence is the inaccuracy of the closed-loop output in the low-frequency
 381 ranges, this is caused by the rather long cortico-thalamic internal delay. This delay yields a larger phase
 382 shift at low-frequencies and originates from the fact that we observe signals in the cortex, but stimulate in
 383 the reticulum.

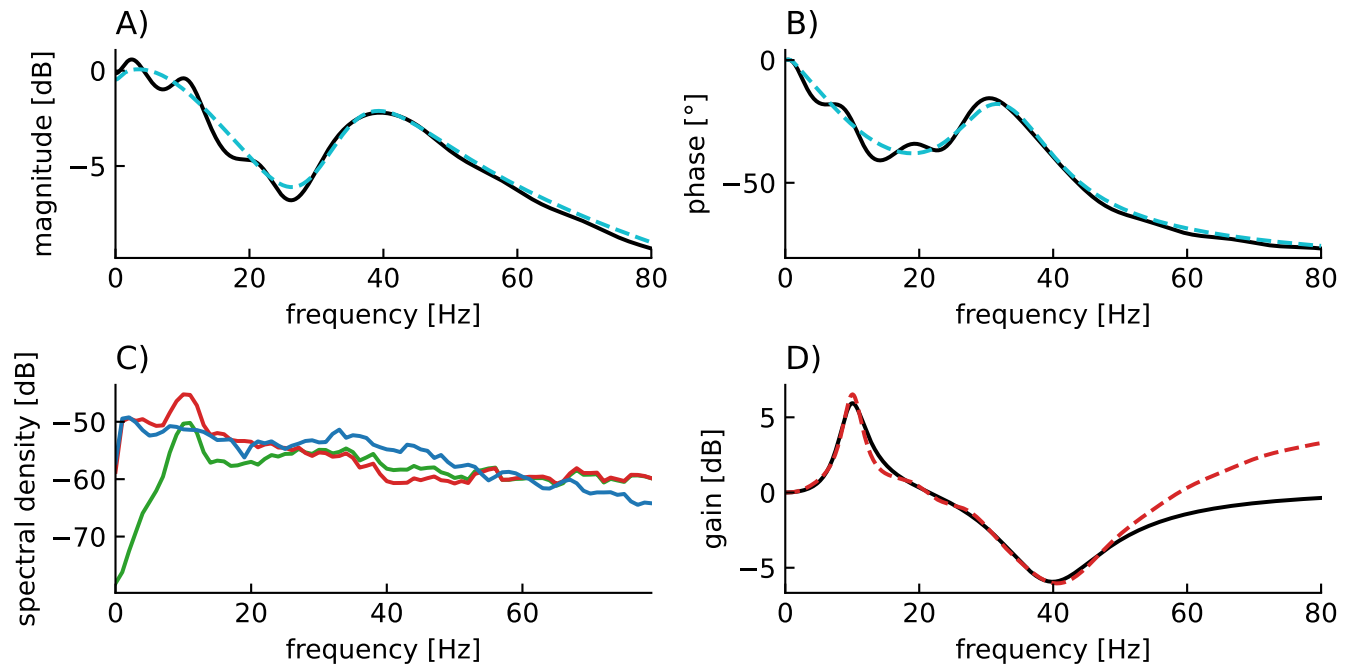


Figure 9. Fitted model-based control using the cortico-thalamic brain model successfully reproduces the target transfer function in the frequency domains of interest. A) Magnitude of the fitted brain model transfer function (dashed cyan) compared to the magnitude of the original cortico-thalamic brain model transfer function (black). **B)** Phase shift of the fitted transfer function (dashed cyan) compared to the magnitude of the original transfer function (black). **C)** Spectral densities of the rest state activity signal (blue), the stimulated brain output (red) and the stimulation signal (green). **D)** Closed-loop transfer function (dashed red), compared to the target transfer function $1 + \hat{H}(s)$ (black).

4 DISCUSSION

The goal of the proposed method was to design a delayed closed-loop control method to apply defined modifications to the spectral distribution of an observed signal, such as EEG or LFP. The presented work explicitly describes all the steps needed to build a delayed closed-loop neurostimulation setup to restore the physiological brain state of a patient Hebb et al. (2014). Since the controller is modeled as a linear time-invariant system, its implementation is lightweight, straightforward, and easily applicable in most embedded systems. Applications to a simple neural populations model (Fig. 7) and to a biologically plausible cortico-thalamic feedback system (Fig. 9 and 10) demonstrate its elements and their impact on the control performance.

392 Main contributions

393 Model estimation

We assume resting state activity signal driven by noise, when no neurostimulation is applied. Injecting a stimulation creates an additional response that adds to the resting state. Consequently, both the resting state signal and response signal can be observed separately in experimental practice and they serve to estimate a linear state-space model as outlined in section 3.1. This approach is successful for both simplified linear models (cf. Figs. 3,4) and neurophysiological realistic nonlinear models (cf. Fig. 9). This approximation is suitable for nonlinear systems whose dynamics evolve close to a stationary state. Several studies have already exposed evidence confirming that the measured brain dynamics behave mostly linearly

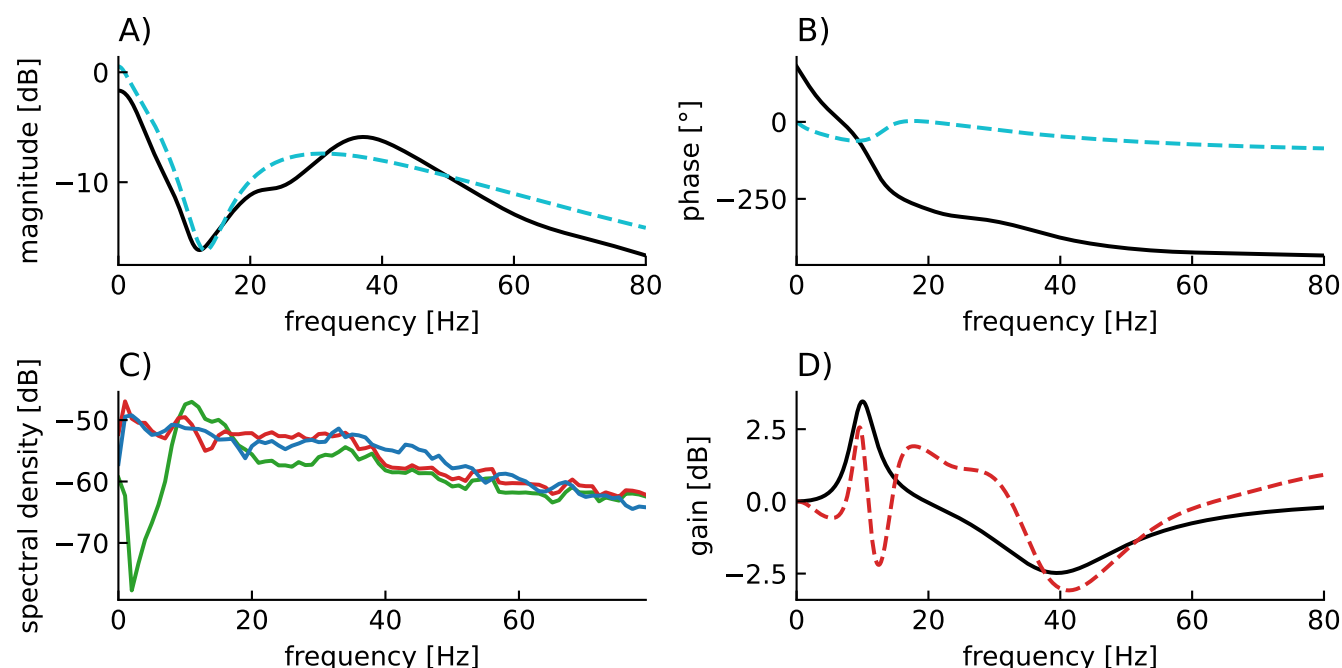


Figure 10. Reticulum stimulation yields incorrect closed-loop gain in low-frequency ranges. **A)** Magnitude of the fitted brain model transfer function (dashed cyan) compared to the magnitude of the original cortico-thalamic brain model transfer function (black). **B)** Phase shift of the fitted transfer function (dashed cyan) compared to the magnitude of the original transfer function (black). **C)** Spectral densities of the rest state activity signal (blue), the stimulated brain output (red) and the stimulation signal (green). **D)** Closed-loop transfer function (dashed red), compared to the target transfer function $1 + \hat{H}(s)$ (black).

at macroscopic scales (Liu et al., 2010), (Popivanov et al., 1996). Moreover, in the case of the brain response to small neurostimulation input, our assumption of the linear brain response is supported by results of (Kim and Ching, 2016). The authors of this study measured the controllability Gramian of their brain model with nonlinear sigmoid transfer function, similar to the cortico-thalamic brain model (Riedinger and Hutt, 2022) used in this paper. If the system exhibits nonlinear dynamics far from any linear approximation, such as bistable dynamics and chaotic evolution, the proposed vector fitting technique may yield a too large model error and thus instability of the closed-loop feedback. The hypothesis of macroscopically linear dynamics has also recently been tested against various nonlinear models (Nozari et al., 2020). While that work included fitting methods for both linear and nonlinear brain models, our work chose the paradigm of purely frequency domain model fitting with the magnitude vector fitting algorithm (De Tommasi et al., 2010) and applied it to the brain input response system, which we could isolate thanks to a simple open-loop neurostimulation setup. While models have already been studied in application to neurostimulation (Modolo et al., 2011), (Wagner et al., 2014), we propose a straightforward black box modeling approach that is directly usable for adaptive closed-loop neurostimulation, and is technically applicable easily for each individual patients before any closed-loop neurostimulation sessions.

Delay compensation

Conduction delays of a few milliseconds in the transmission between observation and stimulation may be negligible in systems evolving on time scales of seconds or longer, but may play an important role in neural systems. Our study demonstrates that such feedback delays may introduce control errors

and we show how these errors can be avoided by a novel delay compensation method (section 3.2). Application to the linear model (7) demonstrated its superior performance compared to a conventional delay compensation method. Delay compensating systems have already been described in other work (Hosseini et al., 2019), (Guo et al., 2004). However, we used a design primarily focused on the correction of a gain error in the closed-loop transfer function, whereas the majority of the current research is based on time domain criterion and stability enforcement (Ledva et al., 2017), (Sönmez and Ayasun, 2015). The methods performance, i.e. how well the total gain function fits to the pre-defined transfer function, is good for low-frequencies but weakens for frequencies exceeding a limit frequency. Note that frequency domain compensation has also already been achieved, notably via delay equalizers (Podilchak et al., 2009). However, this would restrict the frequency range in which the delay is compensated, and create additional errors in the surrounding frequencies. Other designs include filters with negative group delays, however their applications are limited to band limited input signals (Bukhman and Bukhman, 2004), (Voss, 2017). The predictor design we presented also relies on negative group delay, enabling delay compensation in a large frequency band, while still being applicable to the brain EEG, which is inherently not band limited, because of the noise. Nonetheless, while our predictor design allows to significantly decrease the delay errors in the closed-loop transfer function, the delay still imposes a limit on the controllable frequency range. The larger the delay, the smaller is this limit frequency. Low performance may induce instability in the feedback loop (Mirkin and Palmor, 2005) and thus should be avoided. A corresponding stability criteria has been proposed, cf. Fig. 6. Better predictor designs could allow better performance of the closed-loop system for larger delays. The improvement of the accuracy of our closed-loop neurostimulation setup by building more efficient predictor designs is in progress and we refer the reader to future work.

Limits of our methodology

Experimental stimulation parameters and safety

Experimental stimulation protocols have to ensure the subjects safety (Ko, 2021) and thus avoid stimulus-induced health risks and complications. For instance, tDCS may be administered for a duration of 60 minutes and a maximum current of 4 mA without yielding health risks. However, parameters beyond these limits may yield adverse effects in subjects, such as skin lesions similar to burns and mania or hypomania in patients with depression (Matsumoto and Ugawa, 2017). The proposed method does not limit the stimulation duration *per se*, but of course the duration can be chosen accordingly without constraining the method. The method adapts the systems brain rhythms to the target rhythms very rapidly on a time scale of less than a second and hence permits rather short stimulation duration longer than a second.

Moreover, the proposed method does not specify absolute stimulation current magnitude applied. The impact of stimulation at certain magnitudes depends heavily on the stimulation type. In tDCS, anodal stimulation with positive currents have a different impact as cathodal stimulation with negative currents. In addition, currents are thought to have to pass a certain threshold to yield a measurable effect. In tACS (Moliadze et al., 2012), stimulating in the α -frequency range large and small magnitudes yield excitation and inhibition, respectively, while intermediate magnitudes yield weak effects. Stimulating with a range of frequencies, as in tRNS (Potok et al., 2022), a 1mA peak-to-peak amplitude for 10 minutes stimulation duration does not yield adverse effects. We conclude that it is not straight-forward to decide which stimulation magnitude applied in the presented method would be safe for human subjects, since the stimulation signal is neither constant, single frequency oscillation nor random noise. In sum, we argue that

a maximum peak-to-peak amplitude of 1mA for few tens of minutes may not yield adverse effects, but still may evoke a measurable impact on observations and the brain state. Of course, future experimental studies will gain deeper insights.

Model internal delay

The internal delay in the brain is not reproducible by the magnitude vector fitting algorithm, which relies on the time invariance of the signals. Hence, this will cause errors in the transfer function of the fitted model (cf. Fig. 9) that are larger for higher contribution of the delay in the output, cf. Fig. 10. To limit this effect, we must minimize the delay between the application of the neurostimulation input and the measurement of the response to this input as much as possible by taking into account the delay between the different brain regions.

Estimating the closed-loop delay

For delay compensation, in this paper, we assumed that we know the conduction delay in the closed-loop. However, although it is a single constant parameter, we would need a method to measure it for a real closed-loop neurostimulation setup. A straightforward way to do this would be to inject any current into the plant and measure the time lag between the moment at which we inject the input current and the moment at which we measure the output signal. This estimated delay would then correspond to the total closed-loop delay except for the computation delay of the digital controller \mathcal{K} . This computation delay can be easily measured with the same software used for computation, as it corresponds to the delay needed to perform constant-size matrix multiplications. Moreover, several methods have already been developed to estimate the conduction delays in linear systems (Schier, 1997), (Dudarenko et al., 2014).

Direct input current measurements

One of the main challenges to solve for closed-loop neurostimulation is the elimination of direct transmission artifacts from the measured EEG signal (Iturrate et al., 2018). Indeed, when measuring the plant output signal, a portion of the measured signal might be a direct measurement of the input current without any influence from the brain dynamics. In the ideal case, one intends to minimize the contribution of the stimulation input to the observed signal since it would mean that the measured EEG signal does not fully correspond to the brain activity. Hence, reading the EEG of the patient would be more difficult for the user of our closed-loop setup, and the contribution of the brain dynamics to the closed-loop would be smaller. A simple solution to this problem is discussed further below.

Perspectives

The control proposed allows to perform accurate frequency shaping of the systems' activity spectral distribution. However, this approach is limited to linear models of the brain stimulation response. This may be disadvantageous if the systems dynamics exhibit nonlinear behavior (see e.g. (Hutt and beim Graben, 2017)) as we want to represent the brain dynamics realistically. Furthermore, in real-case scenarios, we would also have to take into account the noise in the acquisition of the signal by the sensor and in the application of the input signal by the actuator.

Filtering out direct input current measurements

Filtering out the direct input current measurements is achievable with our setup removing the strictly proper system requirement while using the magnitude vector fitting algorithm to measure the brain input response. In other words, while fitting the brain input response system, we want the fitted model to be able

to contain a direct transmission term corresponding to the direct current measurement. Hence, if the real plant input response contains a significant direct transmission term, it will be identified by the magnitude vector fitting algorithm when synthesizing the estimated plant input response. The second step is then simply to subtract the feedthrough term multiplied by the input current to the plant output signal. Thus, the remaining part of the signal would only correspond to the brain dynamics.

Application to multiple inputs multiple outputs plants

For now, we only focused on plant with a signal input signal and a single output signal. However, in a real setup, the EEG measurement is typically composed of multiple channels corresponding to different electrodes. This can also be true for the neurostimulation device. For example, with electric current stimulation, we can inject multiple signals using multiple electrodes. This can be simply solved by feeding a single input to each input channel and summing each output to a single output channel. However, when we separate the different channels, we can have more control over each individual's output channels. When we have multiple inputs and output, the plant is then a Multiple-Inputs Multiple-Outputs (MIMO) system. Everything developed in this paper is generalizable to MIMO systems, with one caveat: when solving Eq. (6), a unique solution only exists if the system has as more outputs than it has inputs. The user can always ensure this, by using as many neurostimulation input channels than there are EEG output channels. In this generalized setup, we can also define the filter \mathcal{H} to apply different modifications to each output channel.

Neurostimulation effects on larger time scales

Our method relies only on the short term dynamics of the brain, using signal feedback and delay compensation to produce an adaptive stimulation current and obtain the desired EEG frequency distribution. However, more traditional neurostimulation techniques rely on the long term dynamics of neural plasticity, which is not modeled in the brain models we use in this paper. Long term brain adaptation to neurostimulation could cause the EEG frequency distribution to diverge from the desired frequency distribution after several minutes of stimulation. This effect could be compensated either by reiterating the model identification step and performing neurostimulation again, or by adjusting the weight of the filter \mathcal{H} according to the observed changes in real-time. Incorporating the effect of neural plasticity in the brain models would allow our method to produce predictable and durable modification to the EEG frequency distribution, even after we stop the stimulation.

CONFLICT OF INTEREST STATEMENT

The authors declare that the research was conducted in the absence of any commercial or financial relationships that could be construed as a potential conflict of interest.

AUTHOR CONTRIBUTIONS

TW, AH and MD contributed to the development of the methods presented in this study. TW produced the source code used for the simulations. JR and AH wrote the introduction section. TW and AH wrote the other sections of the manuscript. All the authors read and approved the submitted version.

FUNDING

This research was funded by Inria in the "Action Exploratoire" project *A/D Drugs*.

DATA AVAILABILITY STATEMENT

539 The source code used for the simulation results can be freely accessed here: [https://github.com/](https://github.com/Thomas-Wahl/neuroclodec)
 540 Thomas-Wahl/neuroclodec

REFERENCES

- 541 Basar, E. (2013). Brain oscillations in neuropsychiatric disease. *Dialogues Clin Neurosci.* 15, 291–300.
 542 doi:10.31887/DCNS.2013.15.3/ebasar
- 543 Bennabi, D. and Haffen, E. (2018). Transcranial direct current stimulation (tdcs): A promising treatment
 544 for major depressive disorder? *Brain Sci.* 8, 81. doi:10.3390/brainsci8050081
- 545 Brunelin, J., Mondino, M., Gassab, L., Haesebaert, F., Gaha, L., Suaud-Chagny, M., et al.
 546 (2012). Examining transcranial direct-current stimulation (tDCS) as a treatment for hallucinations
 547 in schizophrenia. *Am J Psychiatry.* 169, 719–724. doi:10.1176/appi.ajp.2012.11071091
- 548 Bukhman, N. and Bukhman, S. (2004). On the negative delay time of a narrow-band signal as it passes
 549 through the resonant filter of absorption. *Radiophysics and Quantum Electronics* 47, 68–76. doi:https:
 550 //doi.org/10.1023/B:RAQE.0000031672.70934.3a
- 551 De Tommasi, L., Gustavsen, B., and Dhaene, T. (2010). Robust transfer function identification via
 552 an enhanced magnitude vector fitting algorithm. *IET control theory & applications* 4, 1169–1178.
 553 doi:http://dx.doi.org/10.1049/iet-cta.2009.0025
- 554 Dudarenko, N., Polinova, N., and Ushakov, A. (2014). Fundamental matrix of linear continuous system
 555 in the problem of estimating its transport delay. *Nauchno-Tekhnicheskii Vestnik Informatsionnykh*
 556 *Tekhnologii, Mekhaniki i Optiki* 14
- 557 Edel, Y. and Caroli, F. (1987). Histoire de l'électrochoc : des traitements électriques à la
 558 convulsivothérapie en psychiatrie. *Bulletin d'histoire de l'électricité* 9, 87–114. doi:http://dx.doi.
 559 org/10.3406/helec.1987.1012
- 560 Fleming, J., Dunn, E., and Lowery, M. (2020). Simulation of closed-loop deep brain stimulation control
 561 schemes for suppression of pathological beta oscillations in parkinson's disease. *Front. Neurosci.* 14,
 562 166. doi:10.3389/fnins.2020.00166
- 563 Gardiner, C. (2004). *Handbook of Stochastic Methods* (Springer, Berlin). doi:http://dx.doi.org/10.1007/
 564 978-3-662-05389-8
- 565 Guo, L., Cardullo, F., Houck, J., Kelley, L., and Wolters, T. (2004). New predictive filters for
 566 compensating the transport delay on a flight simulator. In *AIAA Modeling and Simulation Technologies*
 567 *Conference and Exhibit.* 5441. doi:https://doi.org/10.2514/6.2004-5441
- 568 Hartshorn, A. and Jobst, B. (2018). Responsive brain stimulation in epilepsy. *Ther Adv Chronic Dis.* 9,
 569 135–142. doi:10.1177/2040622318774173
- 570 Hashemi, M., Hutt, A., and Sleight, J. (2015). How the cortico-thalamic feedback affects the EEG power
 571 spectrum over frontal and occipital regions during propofol-induced anaesthetic sedation. *J. Comput.*
 572 *Neurosci.* 39, 155. doi:0.1007/s10827-015-0569-1.
- 573 Hebb, A. O., Zhang, J. J., Mahoor, M. H., Tsiokos, C., Matlack, C., Chizeck, H. J., et al. (2014). Creating
 574 the feedback loop: closed-loop neurostimulation. *Neurosurgery Clinics* 25, 187–204. doi:https://doi.
 575 org/10.1016/j.nec.2013.08.006
- 576 Hespanha, J. P. (2018). *Linear systems theory* (Princeton university press). doi:http://dx.doi.org/10.2307/
 577 j.ctvc772kp
- 578 Holtzheimer, P. and Mayberg, H. (2011). Deep brain stimulation for psychiatric disorders. *Annu Rev*
 579 *Neurosci.* 34, 2890307. doi:10.1146/annurev-neuro-061010-113638

- Hosain, M., Kouzani, A., and Tye, S. (2014). Closed loop deep brain stimulation: an evolving technology. *Australas Phys Eng Sci Med.* 37, 619–634. doi:10.1007/s13246-014-0297-2
- Hosseini, S. A., Toulabi, M., Dobakhshari, A. S., Ashouri-Zadeh, A., and Ranjbar, A. M. (2019). Delay compensation of demand response and adaptive disturbance rejection applied to power system frequency control. *IEEE Transactions on Power Systems* 35, 2037–2046. doi:10.1109/TPWRS.2019.2957125
- Howells, F. M., Temmingh, H. S., Hsieh, J. H., van Dijen, A. V., Baldwin, D. S., and Stein, D. J. (2018). Electroencephalographic delta/alpha frequency activity differentiates psychotic disorders: a study of schizophrenia, bipolar disorder and methamphetamine-induced psychotic disorder. *Translational psychiatry* 8, 1–11. doi:http://dx.doi.org/10.1038/s41398-018-0105-y
- Hutt, A. (2013). The anesthetic propofol shifts the frequency of maximum spectral power in eeg during general anesthesia: analytical insights from a linear model. *Frontiers in Computational Neuroscience* 7, 2. doi:10.3389/fncom.2013.00002
- Hutt, A. and beim Graben, P. (2017). Sequences by metastable attractors: interweaving dynamical systems and experimental data. *Front. Appl. Dyn. Syst. Stat.* 3, 11. doi:https://doi.org/10.3389/fams.2017.00011
- Iturrate, I., Pereira, M., and Millán, J. d. R. (2018). Closed-loop electrical neurostimulation: challenges and opportunities. *Current Opinion in Biomedical Engineering* 8, 28–37. doi:http://dx.doi.org/10.1016/j.cobme.2018.09.007
- Khintchine, A. (1934). Korrelationstheorie der stationären stochastischen prozesse. *Mathematische Annalen* 109, 604–615. doi:10.1007/BF01449156
- Kim, S. A. and Ching, S. (2016). Quasilinearization-based controllability analysis of neuronal rate networks. In *2016 American Control Conference (ACC)* (IEEE), 7371–7376. doi:10.1109/ACC.2016.7526836
- Ko, M. (2021). Safety of transcranial direct current stimulation in neurorehabilitation. *Brain Neurorehabil.* 14, e9. doi:10.12786/bn.2021.14.e9
- Kühn, A. A., Kempf, F., Brücke, C., Gaynor Doyle, L., Martinez-Torres, I., Pogosyan, A., et al. (2008). High-frequency stimulation of the subthalamic nucleus suppresses oscillatory β activity in patients with parkinson's disease in parallel with improvement in motor performance. *Journal of Neuroscience* 28, 6165–6173. doi:10.1523/JNEUROSCI.0282-08.2008
- Ledva, G. S., Vrettos, E., Mastellone, S., Andersson, G., and Mathieu, J. L. (2017). Managing communication delays and model error in demand response for frequency regulation. *IEEE Transactions on Power Systems* 33, 1299–1308. doi:10.1109/TPWRS.2017.2725834
- Leicht, G., Vauth, S., Polomac, N., Andreou, C., Rauh, J., Mußmann, M., et al. (2015). EEG-Informed fMRI Reveals a Disturbed Gamma-Band-Specific Network in Subjects at High Risk for Psychosis. *Schizophrenia Bulletin* 42, 239–249. doi:10.1093/schbul/sbv092
- Liu, Z., Rios, C., Zhang, N., Yang, L., Chen, W., and He, B. (2010). Linear and nonlinear relationships between visual stimuli, eeg and bold fmri signals. *Neuroimage* 50, 1054–1066. doi:https://doi.org/10.1016/j.neuroimage.2010.01.017
- Matsumoto, H. and Ugawa, Y. (2017). Adverse events of tdcS and tacs: A review. *Clinical Neurophysiology Practice* 2, 19–25. doi:https://doi.org/10.1016/j.cnp.2016.12.003
- Mirkin, L. and Palmor, Z. J. (2005). *Control Issues in Systems with Loop Delays* (Boston, MA: Birkhäuser Boston). 627–648. doi:10.1007/0-8176-4404-0_27

- Modolo, J., Legros, A., Thomas, A. W., and Beuter, A. (2011). Model-driven therapeutic treatment of neurological disorders: reshaping brain rhythms with neuromodulation. *Interface focus* 1, 61–74. doi:https://doi.org/10.1098/rsfs.2010.0509
- Moliadze, V., Atalay, D., Antal, A., and Paulus, W. (2012). Close to threshold transcranial electrical stimulation preferentially activates inhibitory networks before switching to excitation with higher intensities. *Brain Stimul.* 5, 505–511. doi:10.1016/j.brs.2011.11.004
- Morari, M. and Zafiriou, E. (1989). *Robust process control* (Morari)
- Nasr, K., Haslacher, D., Dayan, E., Censor, N., Cohen, L. G., and Soekadar, S. R. (2022). Breaking the boundaries of interacting with the human brain using adaptive closed-loop stimulation. *Progress in Neurobiology* 216, 102311. doi:https://doi.org/10.1016/j.pneurobio.2022.102311
- Nejati, V., Salehinejad, M., Nitsche, M., Najian, A., and Javadi, A. (2020). Transcranial direct current stimulation improves executive dysfunctions in adhd: Implications for inhibitory control, interference control, working memory, and cognitive flexibility. *J. Atten. Disord.* 24, 1928–1943. doi:10.1177/1087054717730611
- Nozari, E., Bertolero, M. A., Stiso, J., Caciagli, L., Cornblath, E. J., He, X., et al. (2020). Is the brain macroscopically linear? a system identification of resting state dynamics. *arXiv preprint arXiv:2012.12351* doi:https://doi.org/10.48550/arXiv.2012.12351
- Nunez, P. and Srinivasan, R. (2006). *Electric Fields of the Brain: The Neurophysics of EEG* (Oxford University Press, New York - Oxford). doi:http://dx.doi.org/10.1093/acprof:oso/9780195050387.001.0001
- Paulus, W. (2011). Transcranial electrical stimulation (tes – tdc; trns, tacs) methods. *Neuropsychological Rehabilitation* 21, 602–617. doi:10.1080/09602011.2011.557292. PMID: 21819181
- Podilchak, S. K., Frank, B. M., Freundorfer, A. P., and Antar, Y. M. (2009). High speed metamaterial-inspired negative group delay circuits in cmos for delay equalization. In *2009 2nd Microsystems and Nanoelectronics Research Conference (IEEE)*, 9–12. doi:10.1109/MNRC15848.2009.5338974
- Popivanov, D., Dushanova, J., Mineva, A., and Krekule, I. (1996). Detection of successive changes in dynamics of eeg time series: linear and nonlinear approach. In *Proceedings of 18th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (IEEE)*, vol. 4, 1590–1591. doi:10.1109/IEMBS.1996.647565
- Potok, W., van der Groen, O., Bächinger, M., Edwards, D., and Wenderoth, N. (2022). Transcranial random noise stimulation modulates neural processing of sensory and motor circuits, from potential cellular mechanisms to behavior: A scoping review. *eNeuro* 9, ENEURO.0248–21.2021. doi:10.1523/ENEURO.0248-21.2021
- Prosky, J., Cagle, J., Sellers, K., Gilron, R., de Hemptinne, C., Schmitgen, A., et al. (2021). Practical closed-loop strategies for deep brain stimulation: Lessons from chronic pain. *Front. Neurosci.* 15, 762097. doi:10.3389/fnins.2021.762097
- Riedinger, J. and Hutt, A. (2022). Mathematical model insights into eeg origin under transcranial direct current stimulation (tdcs) in the context of psychosis. *Journal of Clinical Medicine* 11, 1845. doi:http://dx.doi.org/10.3390/jcm11071845
- Schier, J. (1997). Estimation of transport delay using parallel recursive modified gram–schmidt algorithm. *International journal of adaptive control and signal processing* 11, 431–442. doi:https://doi.org/10.1002/(SICI)1099-1115(199708)11:5<3C431::AID-ACS417>3E3.0.CO;2-Q
- Schulman, J. J., Cancro, R., Lowe, S., Lu, F., Walton, K. D., and Llinás, R. R. (2011). Imaging of thalamocortical dysrhythmia in neuropsychiatry. *Front. Hum. Neurosci.* 5, 69. doi:10.3389/fnhum.2011.00069

- Smith, O. J. (1959). A controller to overcome dead time. *ISA J.* 6, 28–33
- Sönmez, S. and Ayasun, S. (2015). Stability region in the parameter space of pi controller for a single-area load frequency control system with time delay. *IEEE Transactions on Power Systems* 31, 829–830. doi:10.1109/TPWRS.2015.2412678
- Stagg, C., Antal, A., and Nitsche, M. (2018). Physiology of transcranial direct current stimulation. *J ECT* 34, 144–152. doi:10.1097/YCT.0000000000000510
- Stanslaski, S., Farooqi, H., Sanabria, D., and Netoff, T. (2022). Fully closed loop test environment for adaptive implantable neural stimulators using computational models. *J. Med. Device* 16, 034501. doi:10.1115/1.4054083
- Tervo, A. E., Nieminen, J. O., Lioumis, P., Metsomaa, J., Souza, V. H., Sinisalo, H., et al. (2022). Closed-loop optimization of transcranial magnetic stimulation with electroencephalography feedback. *Brain Stimulation* 15, 523–531. doi:https://doi.org/10.1016/j.brs.2022.01.016
- Van Loan, C. (1978). Computing integrals involving the matrix exponential. *IEEE transactions on automatic control* 23, 395–404. doi:http://dx.doi.org/10.1109/TAC.1978.1101743
- Voss, H. U. (2017). A universal negative group delay filter for the prediction of band-limited signals. *arXiv preprint arXiv:1706.07326* doi:https://doi.org/10.48550/arXiv.1706.07326
- Wagner, T., Eden, U., Rushmore, J., Russo, C. J., Dipietro, L., Fregni, F., et al. (2014). Impact of brain tissue filtering on neurostimulation fields: a modeling study. *Neuroimage* 85, 1048–1057. doi:https://doi.org/10.1016/j.neuroimage.2013.06.079
- Welch, P. (1967). The use of fast fourier transform for the estimation of power spectra: A method based on time averaging over short, modified periodogram. *Trans. Audio Electroacoustics* AU-15, 70–73. doi:10.1109/TAU.1967.1161901

CORTICO-THALAMIC BRAIN MODEL DETAILS

690 The differential equation system (11) develops as

$$\begin{aligned}
 \tau_e \frac{dV_e(t)}{dt} &= -V_e(t) + F_e T_c(V_e(t) - V_i(t)) + F_{ct} T_{th}(V_{th,e}(t) - V_{th,i}(t)) + F_{ccx} S_e(v(t)) + \mu_e + I_e + \xi_e(t) + b_1 u(t) \\
 \tau_i \frac{dV_i(t)}{dt} &= -V_i(t) + F_i T_c(V_e(t) - V_i(t)) + \mu_i + I_i + \xi_i(t) + b_2 u(t) \\
 \tau_{th,e} \frac{dV_{th,e}(t)}{dt} &= -V_{th,e}(t) + F_{tc} T_c(V_e(t - \tau) - V_i(t - \tau)) + \mu_{th,e} + \xi_{th,e}(t) \\
 \tau_{th,i} \frac{dV_{th,i}(t)}{dt} &= -V_{th,i}(t) + F_{tr} T_{ret}(V_{ret}(t)) + \mu_{th,i} + \xi_{th,i}(t) \\
 \tau_{ret} \frac{dV_{ret}(t)}{dt} &= -V_{ret}(t) + F_{rt} T_{th}(V_{th,e}(t) - V_{th,i}(t)) + F_{rc} T_c(V_e(t - \tau) - V_i(t - \tau)) + \mu_{ret} + \xi_{ret}(t) \\
 \tau_{ce} \frac{dv(t)}{dt} &= -v(t) + F_{cx} S_e(v(t)) - M_{cx} S_i(w(t)) + M_{cx,th} T_{th}(V_{th,e}(t - \tau) - V_{th,i}(t - \tau)) + \mu_{ce} + I_{ce} + \xi_{ce}(t) + b_3 u(t) \\
 \tau_{ci} \frac{dw(t)}{dt} &= -w(t) - F_{cx} S_i(w(t)) + M_{cx} S_e(v(t)) + \mu_{ci} + I_{ci} + \xi_{ci}(t) + b_4 u(t)
 \end{aligned} \tag{15}$$

691 where the transfer functions are defined as

$$\begin{aligned}
 T_m(x) &= \frac{1}{2} \left(1 - \operatorname{erf} \left(-\frac{x}{\sqrt{2}\sigma_m} \right) \right) \\
 S_m(x) &= \frac{1}{2} \left(1 - \operatorname{erf} \left(-\frac{x}{\sqrt{2}\sigma_{cm}} \right) \right).
 \end{aligned} \tag{16}$$

The ξ_x terms represent the driving noises, which are uncorrelated Gaussian noise defined as

$$\langle \xi_x(t) \rangle = 0 \quad , \quad \langle \xi_x(t) \xi_y(t') \rangle = \frac{Q_x}{N} \delta_{xy} \delta(t - t'),$$

692 with $x = e, i, (th, e), (th, i), ret, ce, ci$. The variances in Eq. (16) are defined as

$$\begin{aligned}
 \sigma_c^2 &= \frac{Q_e}{\tau_e} + \frac{Q_i}{\tau_i}, & \sigma_{th}^2 &= \frac{Q_{th,e}}{\tau_{th,e}} + \frac{Q_{th,i}}{\tau_{th,i}}, & \sigma_{ret}^2 &= \frac{Q_{ret}}{\tau_{ret}} \\
 \sigma_{ce}^2 &= \frac{Q_{ce}}{\tau_{ce}}, & \sigma_{ci}^2 &= \frac{Q_{ci}}{\tau_{ci}}
 \end{aligned}$$

693 All the parameters are given in Table 3.

parameter	description	value
τ_e	exc. decay time (infragranular)	10 ms
τ_i	inh. decay time (infragranular)	50 ms
$\tau_{th,e}$	exc. decay time (relay)	5 ms
$\tau_{th,i}$	inh. decay time (relay)	30 ms
τ_{ret}	exc. decay time (reticular)	8 ms
τ_{ce}	exc. decay time (supragranular)	5 ms
τ_{ci}	inh. decay time (supragranular)	20 ms
τ	cortico-thalamic propagation delay	40 ms
F_e	exc. synaptic strength	1.0
F_i	inh. synaptic strength	2.0
F_{ct}	synaptic strength (relay \rightarrow cortex)	1.2
F_{tc}	synaptic strength (cortex \rightarrow relay)	1.0
F_{tr}	synaptic strength (reticular \rightarrow relay)	1.0
F_{rt}	synaptic strength (relay \rightarrow reticular)	0.3
F_{rc}	synaptic strength (cortex \rightarrow reticular)	0.6
F_{cx}	synaptic strength (exc. \rightarrow exc.)	2.18
M_{cx}	synaptic strength (inh. \rightarrow exc.)	3.88
F_{ccx}	synaptic strength (supragranular \rightarrow infragranular)	0.05
$F_{cx,th}$	synaptic strength (thalamic relay \rightarrow supragranular)	0.1
μ_e	exc. noise input (infragranular)	0.1
μ_i	inh. noise input (infragranular)	0.0
$\mu_{th,e}$	exc. noise input (relay)	1.3
$\mu_{th,i}$	inh. noise input (relay)	1.0
μ_{ret}	exc. noise input (reticular)	0.0
μ_{ce}	exc. noise input (supragranular)	0.05
μ_{ci}	inh. noise input (supragranular)	0.05
I_e	exc. resting input (infragranular)	2.7
I_i	inh. resting input (infragranular)	1.7
I_{ce}	exc. resting input (supragranular)	1.1
I_{ci}	inh. resting input (supragranular)	0.4
Q_e	exc. input noise variance (infragranular)	3×10^{-5}
Q_i	inh. input noise variance (infragranular)	0.001
$Q_{th,e}$	exc. input noise variance (relay)	2.5×10^{-6}
$Q_{th,i}$	inh. input noise variance (relay)	12.6×10^{-6}
Q_{ret}	exc. input noise variance (reticular)	10.9×10^{-6}
Q_{ce}	exc. input noise (supragranular)	2×10^{-5}
Q_{ci}	inh. input noise (supragranular)	8×10^{-5}
N	number of neurons	1000
$b_{1,2,3,4}$	input coupling constants	1
c_1	observation coefficient (supragranular)	0.3
c_3	observation coefficient (infragranular)	1

Table 3. Parameter set of model (15). The choice of parameters is for the most part based on the paper in which it was developed Riedinger and Hutt (2022).