



**HAL**  
open science

## Compact permanent magnet FTICR mass spectrometer

Joël Lemaire, Michel Heninger, Gérard Bellec, Gérard Mauclaire, Hélène Mestdagh, Pierre Boissel

► **To cite this version:**

Joël Lemaire, Michel Heninger, Gérard Bellec, Gérard Mauclaire, Hélène Mestdagh, et al.. Compact permanent magnet FTICR mass spectrometer. European Fourier Transform Mass Spectrometry conference (7th EFTMS), Mar 2004, Konstanz, Germany. hal-04216395

**HAL Id: hal-04216395**

**<https://hal.science/hal-04216395>**

Submitted on 24 Sep 2023

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

## Compact permanent magnet FTICR mass spectrometer


M. Heninger, J. Lemaire, G. Bellec, G. Mauclaire, H. Mestdagh, P. Boissel.

The range of applications and analytical power of Fourier Transform Ion Cyclotron Resonance Mass Spectrometry rest on ion trapping and selection capabilities : this allows MS<sup>n</sup> type experiments, often avoiding wet chemistry pre-separation steps. Simultaneous detection of a wide mass range is possible with very high resolution and unsurpassed accuracy of mass determination.



Existing FTICR mass spectrometers are very powerful analytical tools but heavy non transportable machines. Our goal in developing a compact and easy to move and operate FTICR machine is to bring the unique advantages of this technique to on-line or *in-situ* applications and, while maintaining performances and adaptability to various problem, to lower the cost of the spectrometer which constitutes an obstacle to a more frequent use of FTICR.


(CNRS patent : FR2835964)

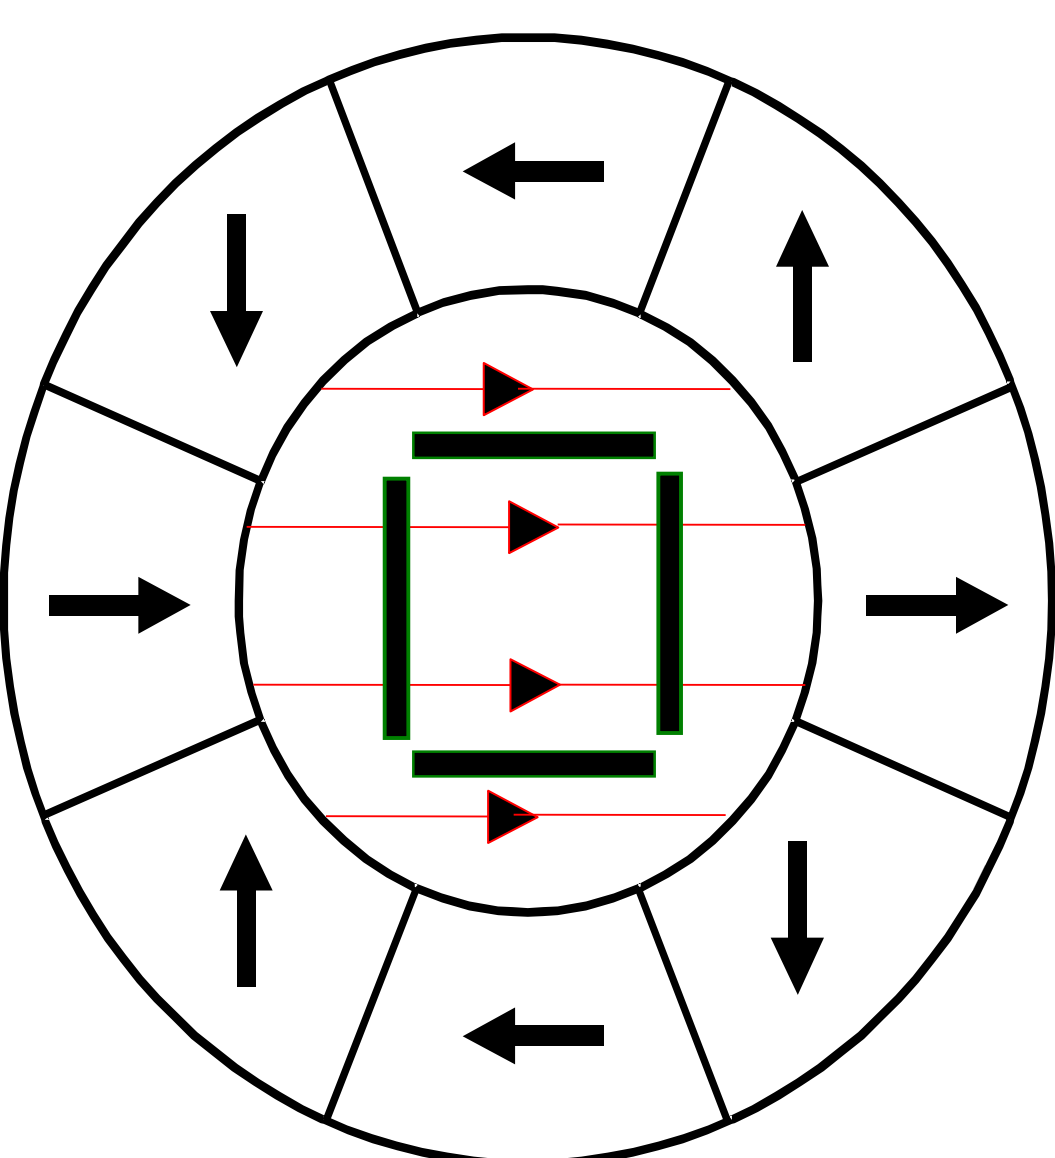

### MICRA

MICRA is based on a 1.25 Tesla structured permanent magnet of FeNdB weighing 40kg with a 5 cm internal bore. The ICR cell implemented in MICRA is cubic, with internal dimensions 2x2x2 cm. The cell has an open structure, in order to provide a wide optical access to the center. The main vacuum chamber is pumped by a 70L/s turbomolecular pump, backed by a three stages diaphragm pump, giving a nominal base pressure better than 3x10<sup>-9</sup> mbar. The mass spectrometer is controlled by a custom detection based on a standard PC computer fitted with commercial PCI cards for excitation/detection of the ions.


Mass range : 10-1000 Daltons  
 Weight : ~200 kg  
 Dimensions : 0.6x1.2x0.8 m  
 Détection limit : few ppm for VOC's traces  
 No fluids  
 Power : 1 kW

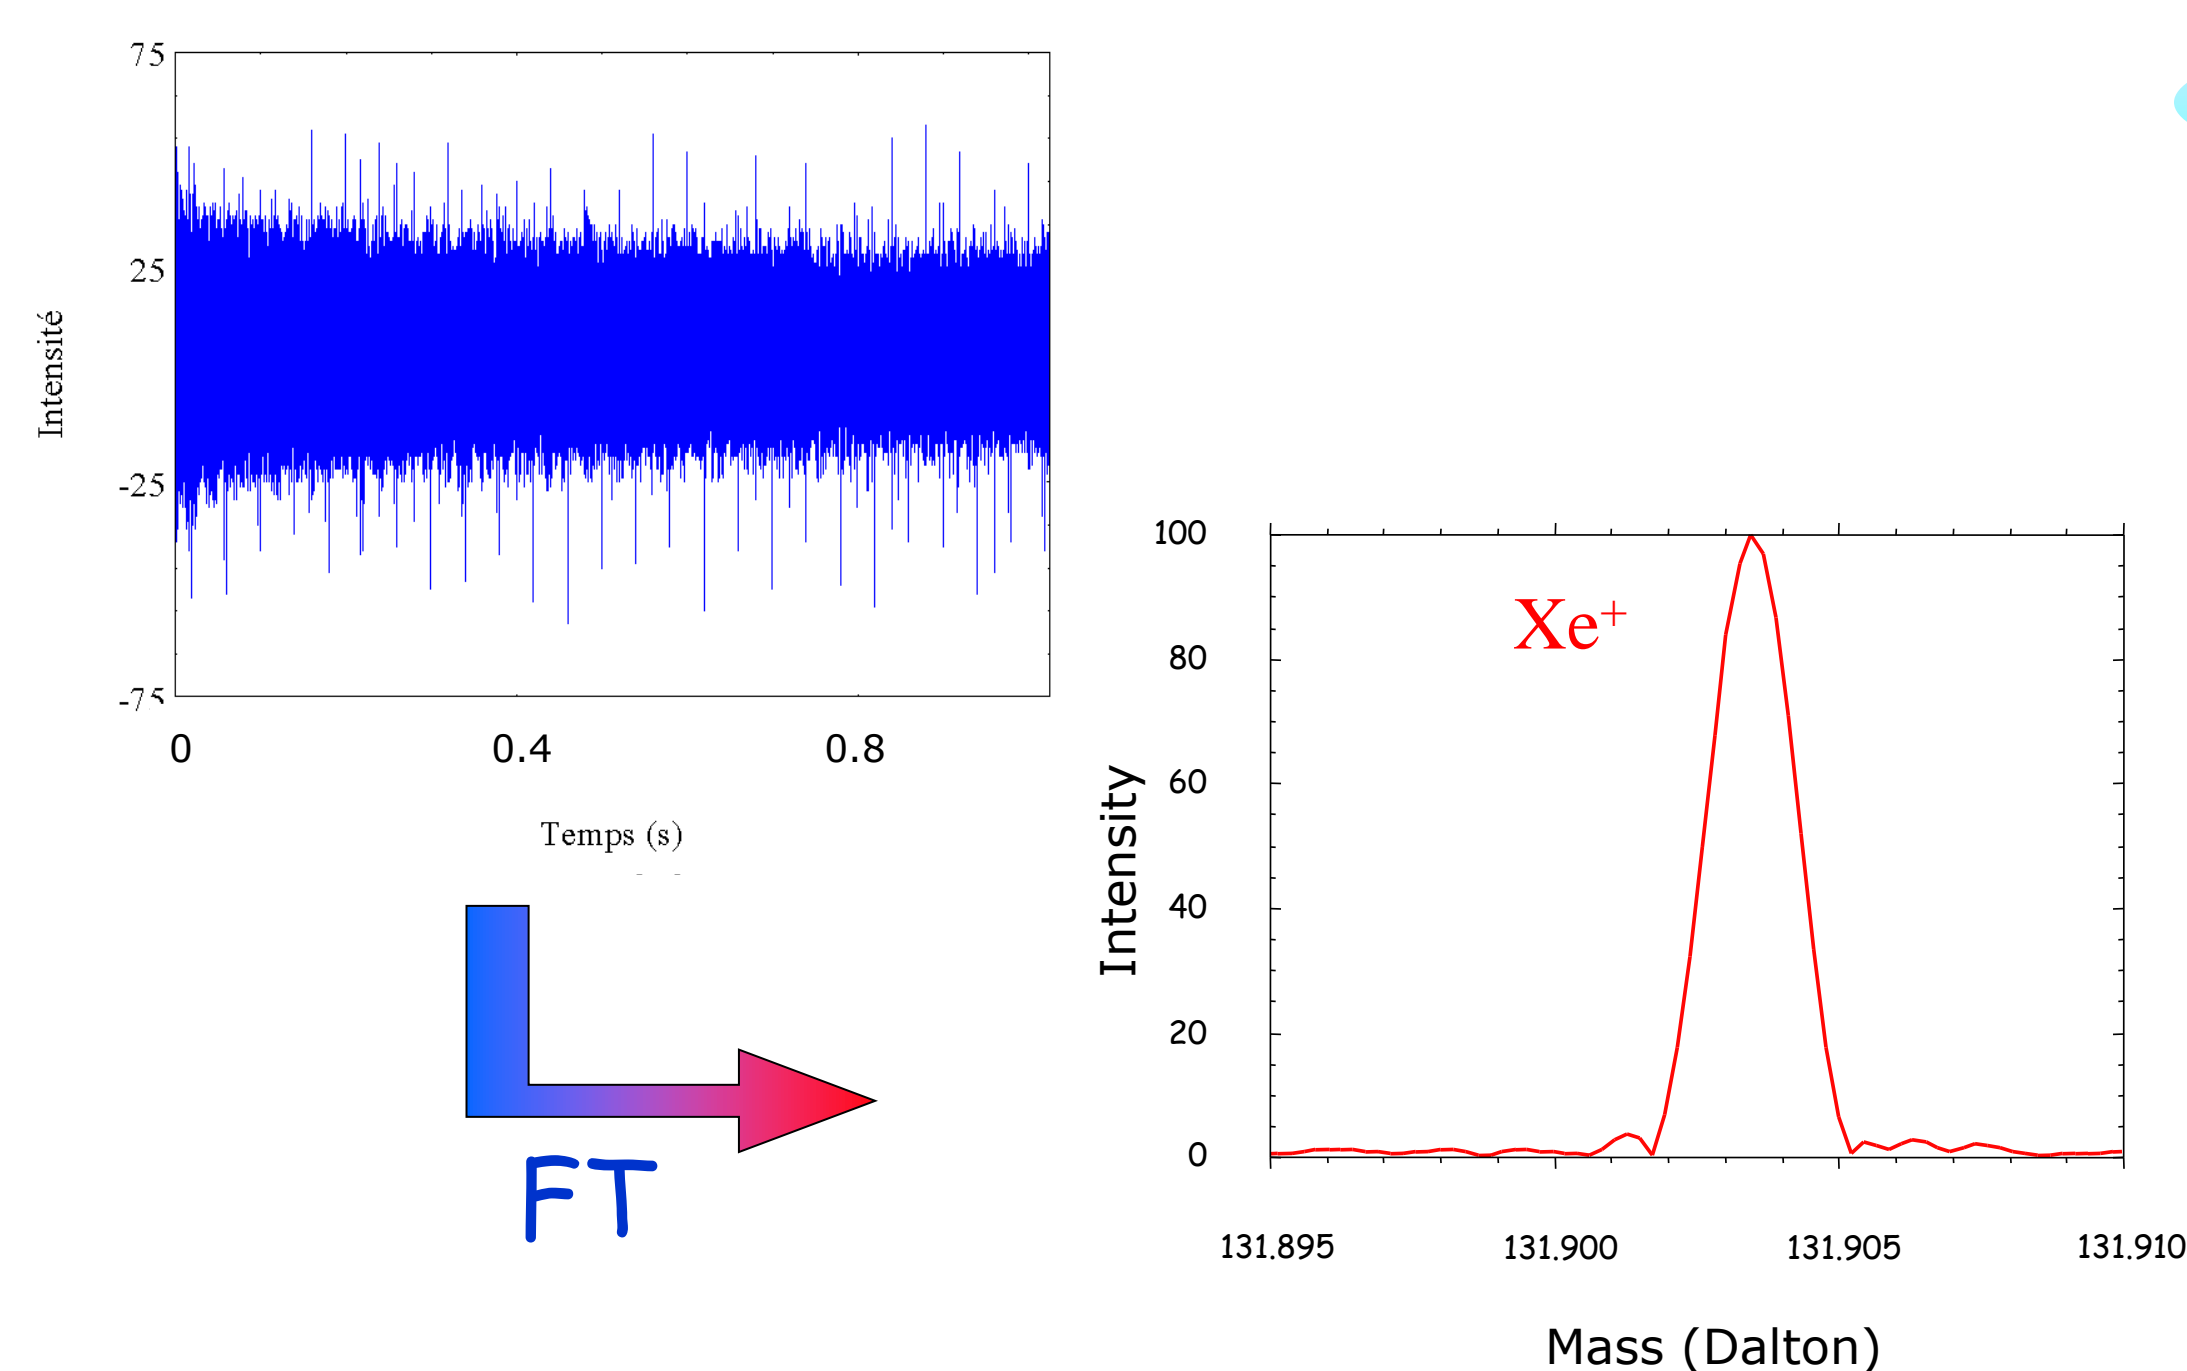

### Mass resolving power : high resolution


The mass resolving power for <sup>132</sup>Xe<sup>+</sup> is 73000

The ions CO<sub>2</sub><sup>+</sup> and N<sub>2</sub>O<sup>+</sup> with the same nominal mass m/z 44 and differing by 0.01 mass unit, are completely separated.

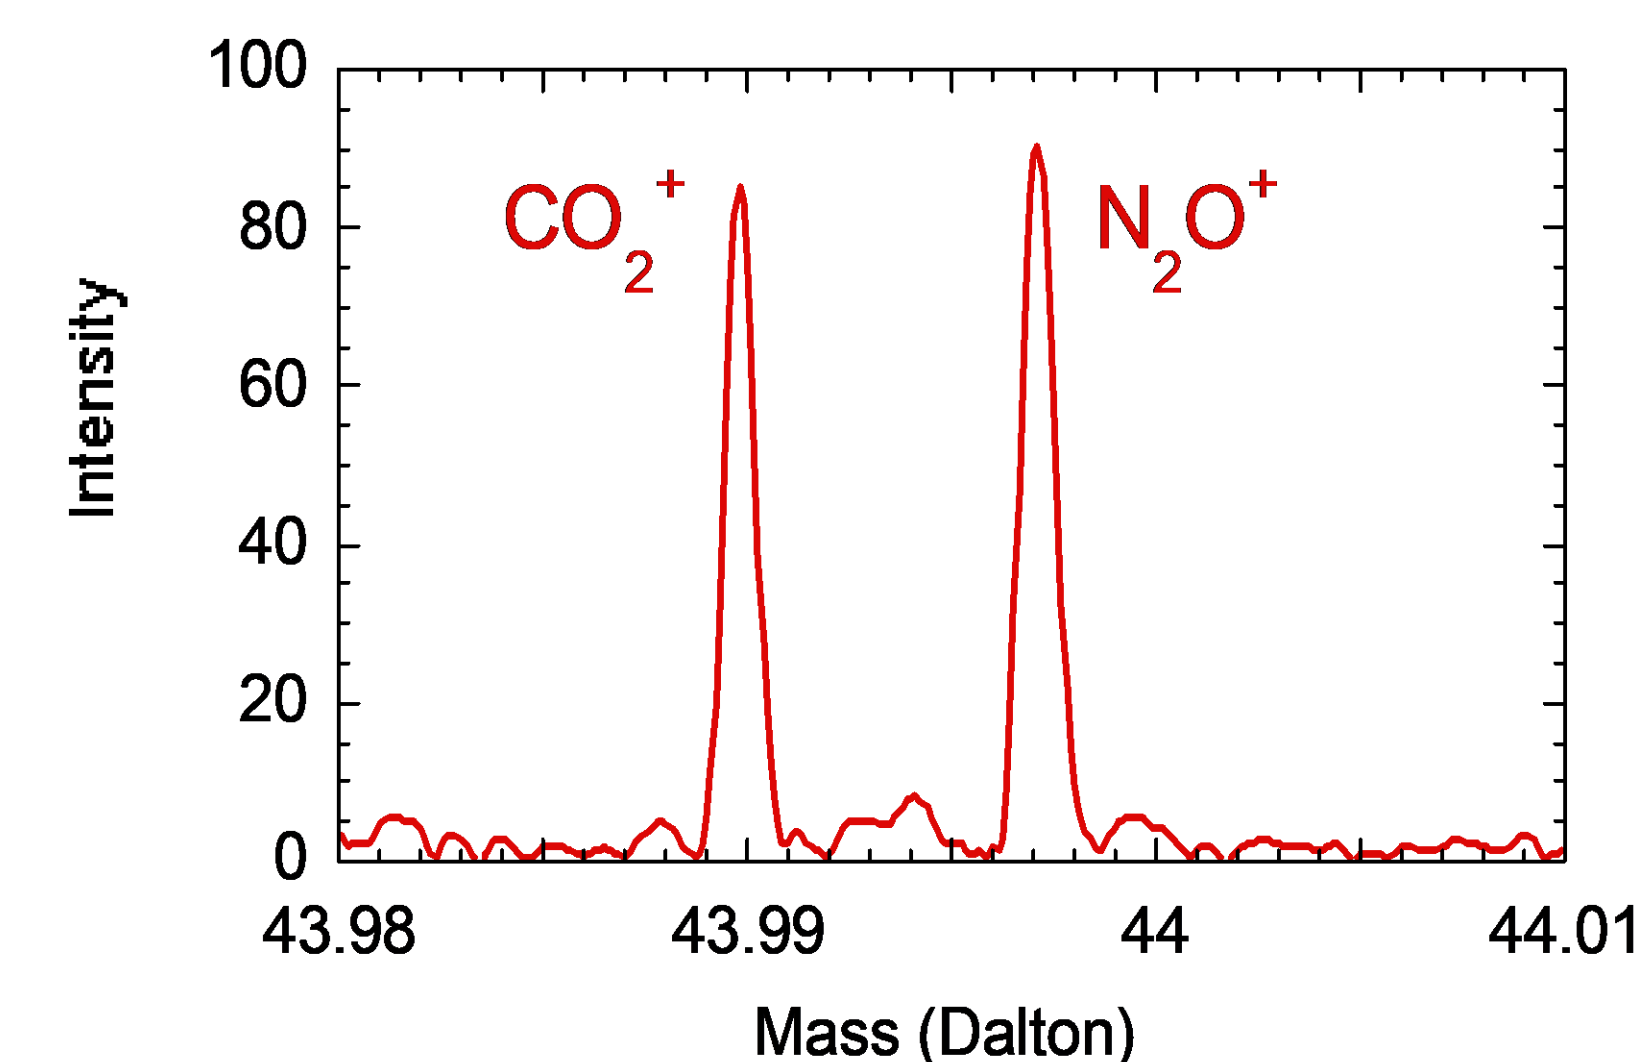


### Applications

#### Kinetic study

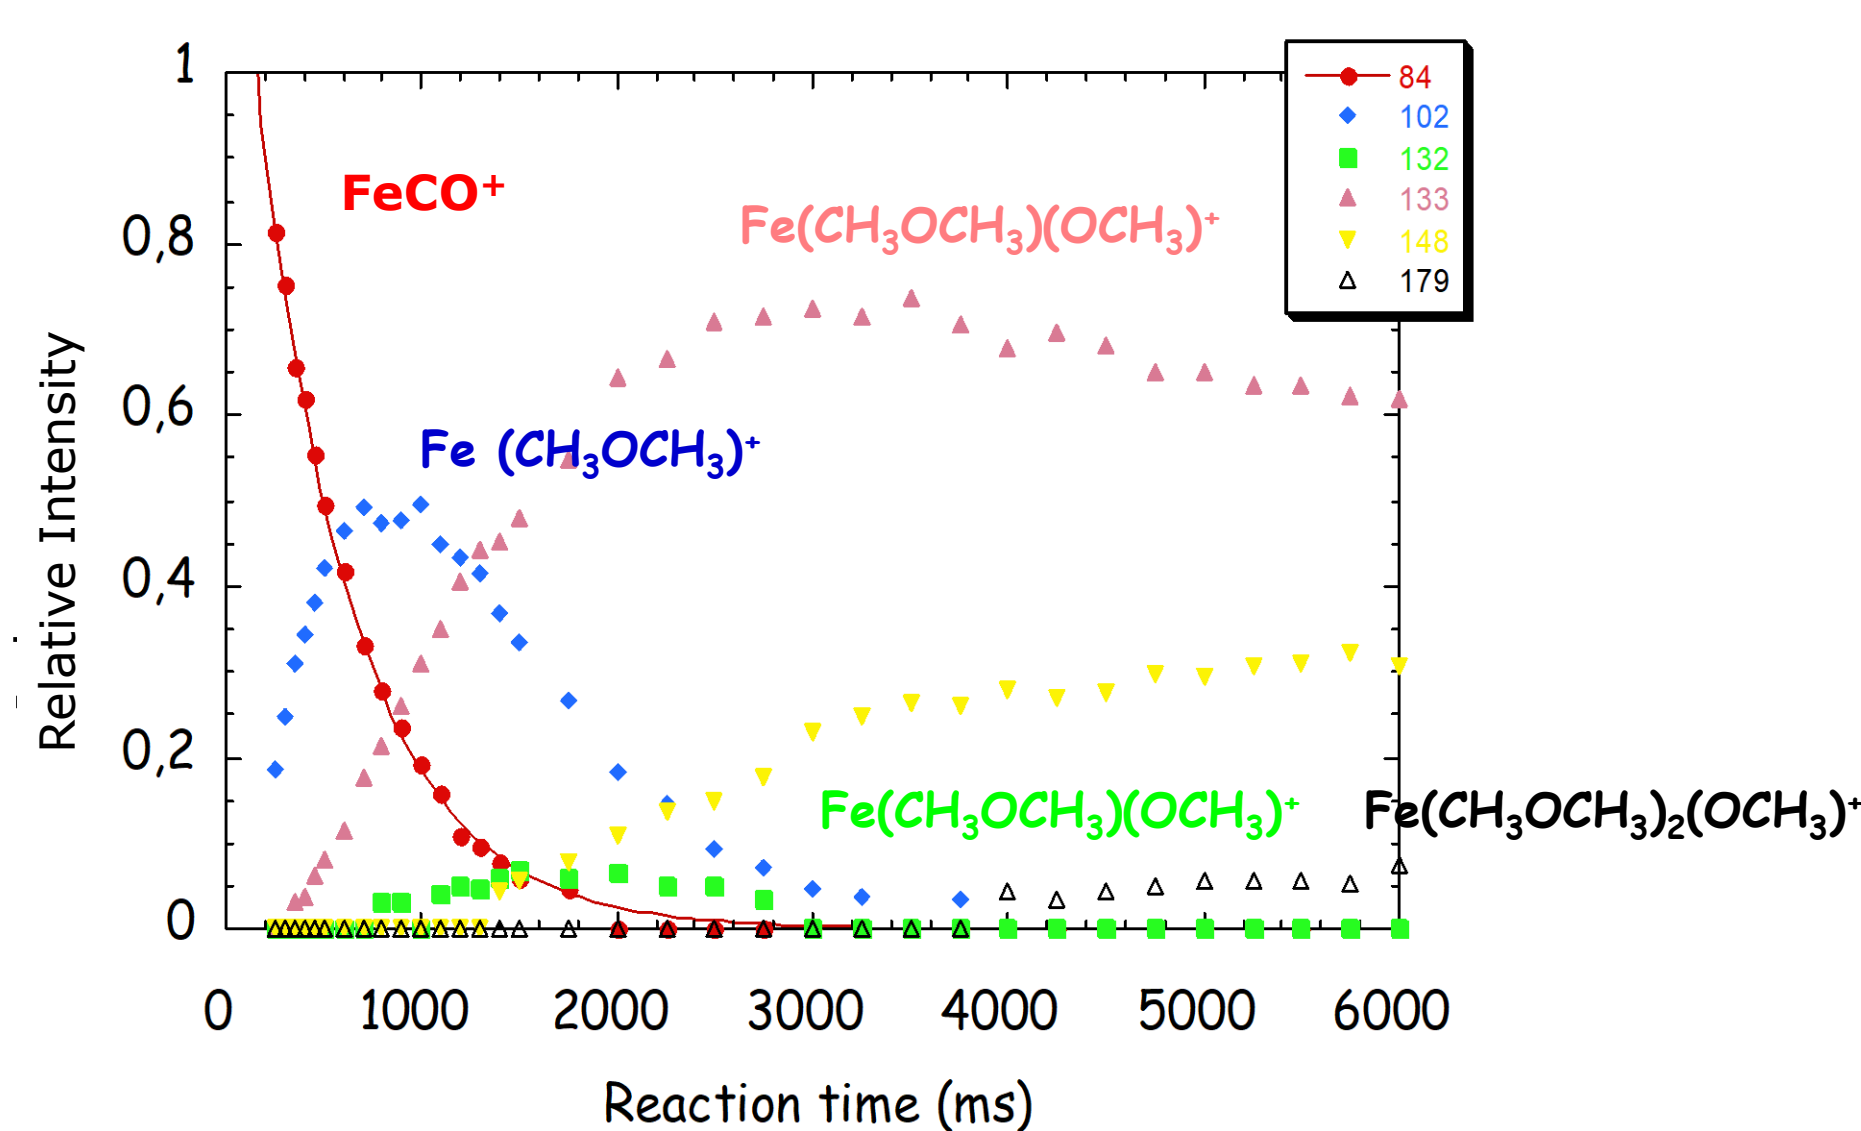


Successive ion-molecule reactions with FeCO<sup>+</sup> + Dimethyl ether system  
 $FeCO^+ + CH_3OCH_3 \rightarrow Fe(CH_3OCH_3)^+ + CO$   
 $Fe(CH_3OCH_3)^+ + CH_3OCH_3 \rightarrow \dots$

#### High resolution detection of Volatile Organic Compounds traces

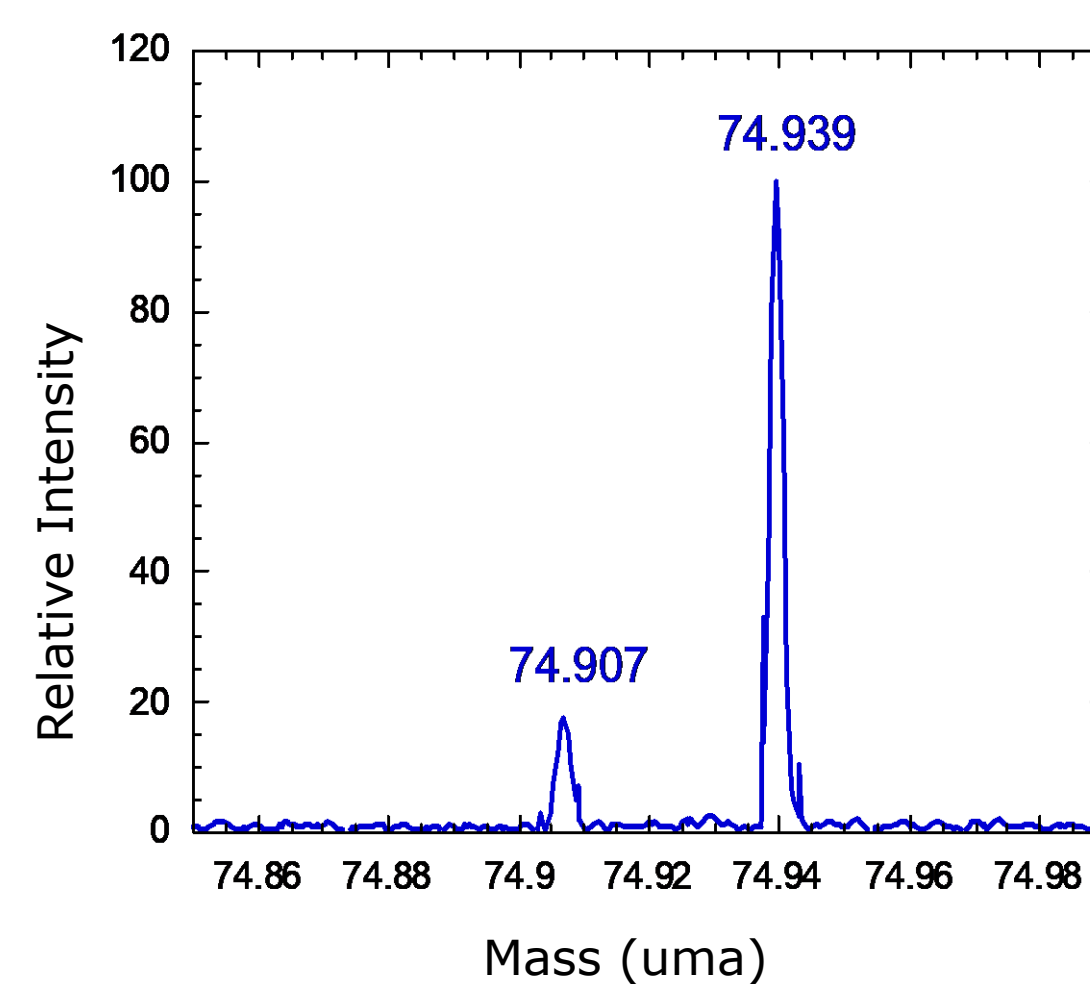

Proton transfer mass spectrometry on a mixture of C<sub>2</sub>H<sub>5</sub>OC<sub>2</sub>H<sub>5</sub> (Ethoxy ethane) and CH<sub>3</sub>COOCH<sub>3</sub> (Acetic acid) at ppm level in water using a membrane introduction system

#### InfraRed Multiphoton Dissociation (IRMPD) spectroscopy : Ion structure determination

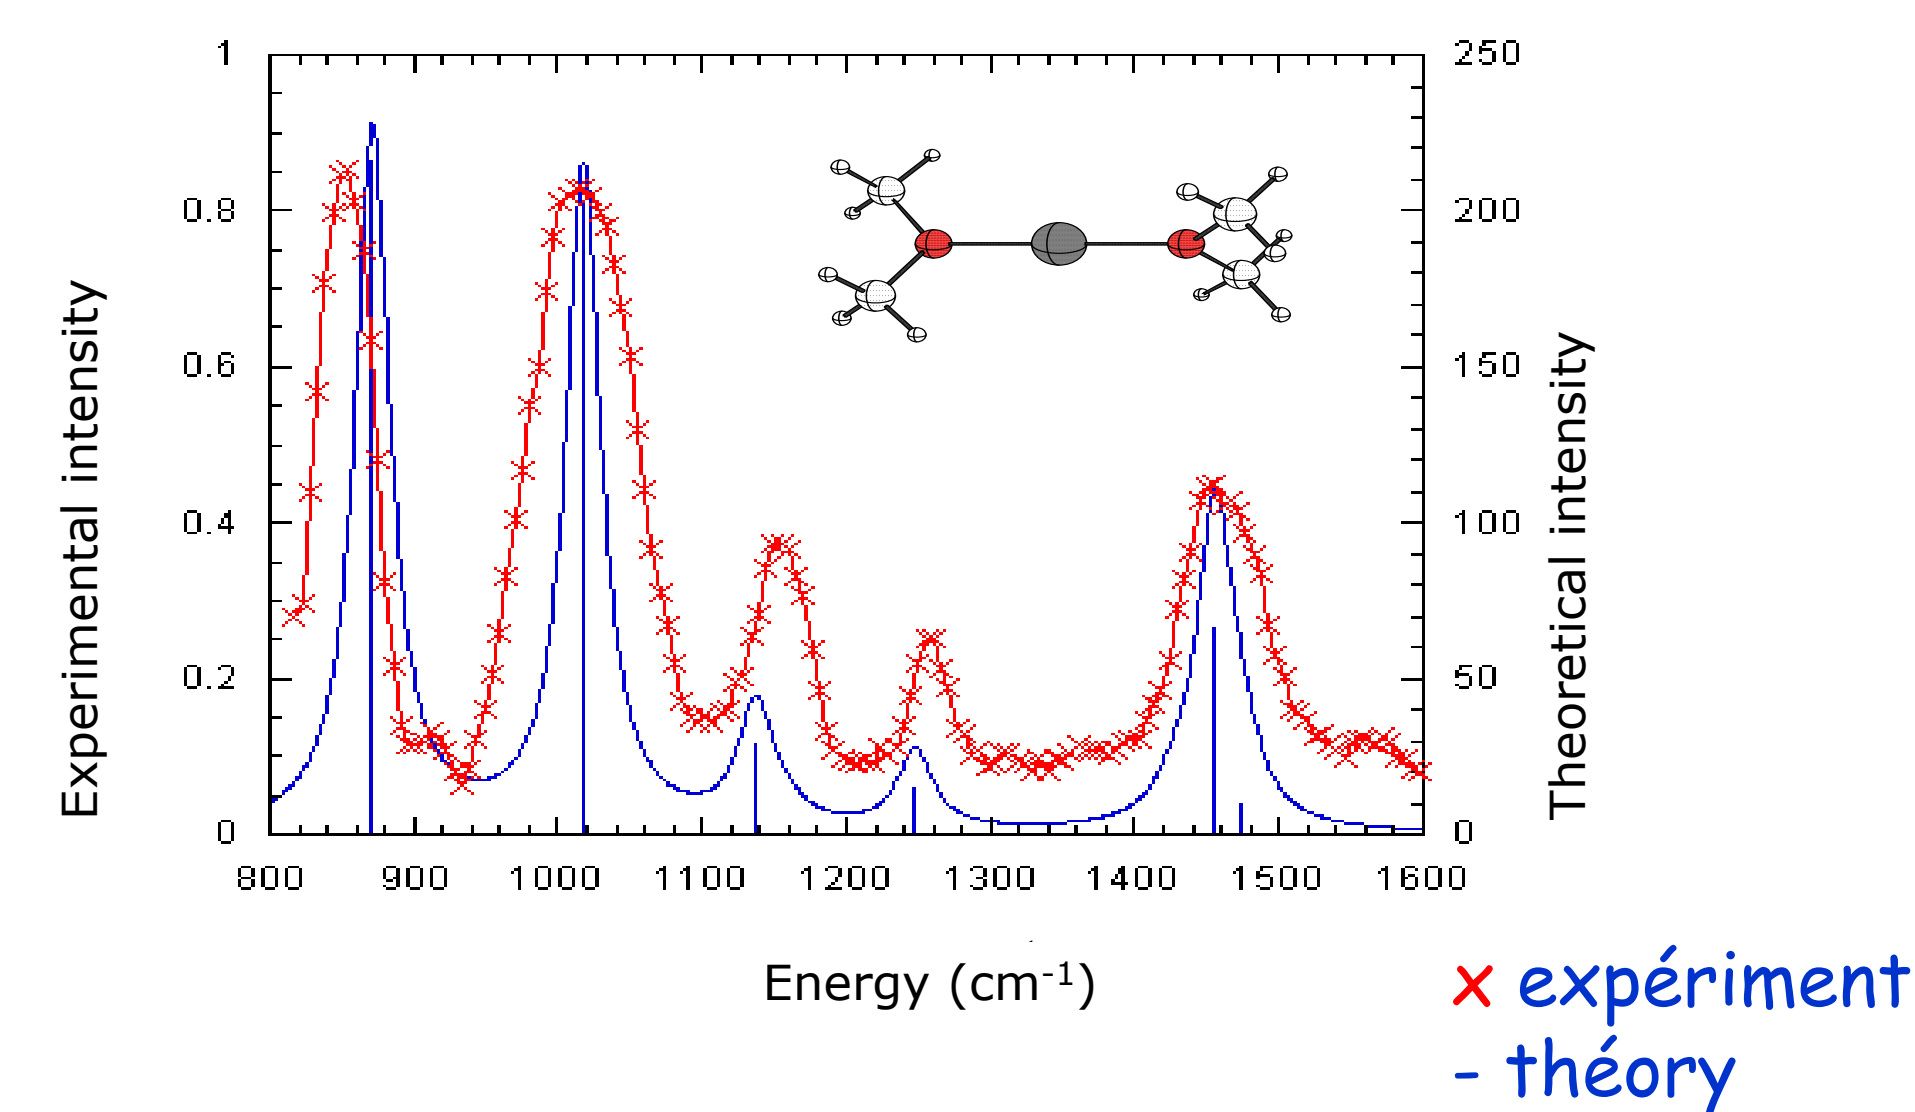

Infrared spectra of Fe(CH<sub>3</sub>OCH<sub>3</sub>)<sub>2</sub><sup>+</sup> ions.  
 Dissociation efficiency as a function of wavelength