

Recent methodological developments in data-dependent analysis and data-independent analysis workflows for exhaustive lipidome coverage

Marie Valmori, Vincent Marie, François Fenaille, Benoit Colsch, David

Touboul

▶ To cite this version:

Marie Valmori, Vincent Marie, François Fenaille, Benoit Colsch, David Touboul. Recent methodological developments in data-dependent analysis and data-independent analysis workflows for exhaustive lipidome coverage. Frontiers in Analytical Science, 2023, 3, 10.3389/frans.2023.1118742. hal-04279997

HAL Id: hal-04279997 https://hal.science/hal-04279997

Submitted on 10 Nov 2023

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers. L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Recent methodological developments in Data-Dependent Analysis and Data-Independent Analysis workflows for exhaustive lipidome coverage

- 1 Marie Valmori,^{1,2,\$} Vincent Marie,^{2,\$} François Fenaille,² Benoit Colsch,^{2,*} David Touboul^{1,3*}
- 2 ¹ Université Paris-Saclay, CNRS, Institut de Chimie Des Substances Naturelles, UPR 2301, 91198,
- 3 Gif-Sur-Yvette, France.
- ² Université Paris-Saclay, CEA, INRAE, Département Médicaments et Technologies pour La Santé
 (DMTS), MetaboHUB, F-91191, Gif sur Yvette, France.
- ³ Laboratoire de Chimie Moléculaire (LCM), CNRS UMR 9168, École Polytechnique, Institut
 Polytechnique de Paris, 91128, Palaiseau, France.
- 8 \$ Both authors equally contributed to the work
- 9 *** Correspondence:**
- 10 Co-corresponding Authors
- 11 benoit.colsch@cea.fr
- 12 david.touboul@cnrs.fr

Keywords: Lipidomics, Data-Dependent Acquisition, Data-Independent Acquisition, High Resolution Mass Spectrometry, Lipid annotation

15 Abstract

16 Untargeted lipidomics applied to biological samples typically involves the coupling of separation 17 methods to high-resolution mass spectrometry (HRMS). Getting an exhaustive coverage of the 18 lipidome with a high confidence in structure identification is still highly challenging due to the wide 19 concentration range of lipids in complex matrices and the presence of numerous isobaric and isomeric 20 species. The development of innovative separation methods and HRMS(/MS) acquisition workflows

- 21 helped improving the situation but issues still remain regarding confident structure characterization.
- To overcome these issues, thoroughly optimized MS/MS acquisition methods are needed. For this purpose, different methodologies have been developed to enable MS and MS/MS acquisition in parallel. Those methodologies, derived from the proteomics, are referred to Data Dependent Acquisition (DDA) and Data Independent Acquisition (DIA).
- In this context, this perspective paper presents the latest developments of DDA- and DIA-based
 workflows for lipidomics and lists available bioinformatic tools for the analysis of resulting spectral
 data.
- 29

30 **1** Introduction

31 Lipids represent a large class of primary metabolites playing vital biological functions to maintain homeostasis in living organisms, serving as energy storage and cell signaling processes (Züllig et al., 32 33 2020). They are also involved in a large number of heterogeneous diseases including cancer, neurodegenerative and metabolic disorders. Lipids are classified in 8 categories according to the Lipid 34 35 Maps classification system (Fahy et al., 2005, 2009; Liebisch et al., 2020) available online through the curated Lipid MAPS Structure Database (LMSD) gathering almost 48,000 unique lipid species in 2022 36 (https://www.lipidmaps.org/). Those categories can be further separated into classes, in which lipids 37 share some building blocks but also differ by the length of alkyl chains and number of unsaturations 38 39 creating a high diversity of closely related lipid species making their distinction highly challenging 40 (Quehenberger et al., 2010; Harayama and Riezman, 2018).

Lipidomics can be defined as a system-level analysis of lipids and their interacting factors (Wenk, 2005). Lipidomics is a subset of metabolomics requiring dedicated sample preparation, as lipids are mostly soluble in organic solvents (*e.g.* methyl tert-butyl ether, chloroform and methanol for Bligh-Dyer and Folch extractions), as well as specific analytical tools to qualitatively and quantitatively characterize complex samples.

One of the major challenges in lipidomics is to distinguish isobaric and isomeric lipid species by implementing either optimized hyphenated mass spectrometry (MS)-based methods and/or tandem mass spectrometry approaches. The fine structure elucidation of complex lipids, such as glycerophospholipids, requires the identification of the polar head group, the chain lengths and the position of the fatty acids together with the number and position of unsaturations or other chemical modifications of the lipid backbone. The precise characterization of lipid species is mandatory to interpret their biological or chemical roles in a defined context (Wenk, 2010).

Among the technical developments performed in the last 70 years, gas chromatography coupled to electron ionization - mass spectrometry (GC-EI-MS) can be considered as the first major tools towards lipidomics. Even if the techniques required complex sample preparation including subclasses separation and chemical derivatization, GC-MS allowed efficient profiling of the fatty acids composing complex lipids (Chiu and Kuo, 2020).

58 The multiple ionization sources and particularly soft ionization such as Electrospray Ionization (ESI),

59 Matrix-Assisted Laser Desorption/Ionization (MALDI) and Atmospheric Pressure Chemical/Photo-

60 Ionization (APCI/APPI), have made mass spectrometry as the technique of preference to perform

61 lipidome characterization and quantification. Also, Atmospheric Pressure ionization sources are mostly 62 employed for compounds difficult to ionize in ESI, mostly represented by neutral lipids such as

62 employed for compounds difficult to follize in ESI, mostly represented by neutral lipids such as

63 triacylglycerols or carotenoids (Byrdwell, 2001; Imbert et al., 2012).

64 The advent of liquid chromatography coupled to mass spectrometry (LC-MS) in the 80's offered new 65 perspectives as intact complex lipids can be directly separated, detected and isolated for tandem mass 66 spectrometry (MS/MS) experiments. Nevertheless, the low mass resolution instruments available at that time did not offer sufficient high mass measurement accuracy and led to difficulty in distinguishing 67 isobaric species. The commercialization of fast and robust high-resolution (HR)/high-mass accuracy 68 69 tandem mass spectrometers paved the route to the analysis of high-mass lipids thanks to extended mass 70 capacities and dynamic ranges (up to 4 decades on modern instruments), high ionization rate for increased sensitivity in both polarities and for all lipid sub-classes. Time-of-flight (TOF) mass 71 72 analyzers show the highest repetition rate. In terms of mass accuracy and resolving power, Fourier

This is a provisional file, not the final typeset article

73 Transform mass spectrometers, such as Orbitrap and Fourier-transform ion cyclotron resonance 74 (FTICR) instruments, are overpassing the TOF performances in spite of their slower acquisition rates limiting the number of data points per chromatographic peak. The Orbitrap-based instruments, since 75 their first commercialization with the LTQ-Orbitrap in 2006, have witnessed innovations in sensitivity, 76 77 resolution and scan speed (Eliuk and Makarov, 2015). The lipidome investigation can be now achieved at high throughput by either a shotgun approach (direct introduction into the mass spectrometer) or 78 79 using hyphenated MS-based techniques such as normal or reverse liquid phase or supercritical fluid 80 chromatography (Rustam and Reid, 2018). The common analysis workflow for those methods is based 81 on the acquisition at the MS level of robust data for biological and technical replicates together with 82 quality control (QC) injections to correct any deviation of the analytical chain. Then the identification 83 of relevant markers or compounds differentiating sample groups is further accomplished by tandem mass spectrometry (MS/MS) following multiple injections into the LC-MS/MS system using targeted 84 85 MS/MS workflows. MS/MS spectral data are necessary for the elucidation structure of lipids. The major part of the existing lipid databases mostly includes tandem mass spectra acquired under low-86 energy non-resonant collision-induced dissociation (CID) or higher energy collision dissociation 87 88 (HCD) conditions on hybrid TOF and Orbitrap-based instruments. But, multiple types of ion activation 89 modes (i.e. resonant and non-resonant activation modes) exist and can be employed in MS/MS and are 90 currently used to a lesser extent for high throughput lipidomics workflows.

As for classical proteomics approaches, the parallel acquisition of HRMS and MS/MS data can be achieved using either a Data-Dependent Analysis (DDA) or a Data-Independent Analysis (DIA) approach. In the following Perspective article, technical and practical considerations on DDA and DIA for lipidomics will be discussed to offer an overview of the latest developments and future trends in the field of lipidomics

95 the field of lipidomics.

96 2 DDA-based acquisition workflows

97 The DDA fragmentation method allows successive acquisitions of MS and MS/MS data. The most 98 widely used DDA acquisition method is often designated as the "DDA Top N". It consists of a cycle 99 of a single HRMS scan followed by the automatic selection and further fragmentation of the N most 100 intense signals in a defined m/z range (Figure 1). The first HRMS scan offers the unique possibility of getting high mass accuracy measurements, typically below 1-2 ppm. Unambiguous chemical formula 101 102 can be easily determined for small lipids, below m/z 300-400 but much higher mass accuracy (< 0.1 ppm) would be required to determine the elemental composition of complex lipids. 103 104 Then automatic MS/MS scans are programmed based on rules such as peak intensity and mass range 105 on HRMS data. This method enables fragmenting a high number of ions and leads to high-quality and 106 high-purity MS/MS spectra since the selection window is restricted to monoisotopic ions. 107 Nevertheless, precursor ions selection is a (semi-)stochastic event suffering from low analytical 108 reproducibility and favoring selection of the most abundant (but sometimes biologically irrelevant) 109 precursor ions to the detriment of other co-eluting relevant ones (Fenaille et al., 2017). These issues 110 can be partially overcome through the implementation of exclusion rules, typical after one or several 111 consecutive MS/MS experiments, . The number of selected ions must be thoroughly optimized 112 considering the MS/MS overall duty cycle (usually few tens to hundreds of milliseconds per MS/MS spectrum) and the LC peak width. A too high number of precursor ions will limit the number of 113 114 complete DDA cycles recorded per chromatographic peak, thus downgrading the quality of peak 115 integration and quantification at the MS level due to insufficient number of data points. This clearly advantages fast MS/MS scanning instruments such as hybrid TOF, with MS acquisition rate up to 100 116 117 Hz in both the MS and MS/MS modes (at 50K resolution) for the TripleTOF 6600 and timsTOF

- 118 instruments, compared to the latest generation of quadrupole-Orbitrap instruments (Orbitrap Exploris
- 119 series) working at 40 Hz at 7.5K resolution at m/z 200 (Perez de Souza et al., 2021).

120 Neumann et al. proposed a protocol to realize a better sampling in MS/MS mode by focusing on 121 biologically relevant and meaningful features (Neumann et al., 2013). First, a LC run at the MS level is performed, with the direct analysis of the data by preprocessing software XCMS for automated 122 123 annotation and statistical analysis to select significant features. Then methods with inclusion lists are created and performed on pooled samples using targeted MS/MS (tMS²) acquisition mode in order to 124 125 confirm previous annotations while also limiting the number of LC-MS/MS experiments. This method enables a better coverage of the sample by selecting lower abundance relevant features, while losing 126 127 the unbiased nature of DDA.

- Koelmel *et al.* developed an Iterative Exclusion IE-Omics approach whose goal is to create several non-redundant inclusion lists (Koelmel et al., 2017). First, a classic DDA acquisition is performed, and all the fragmented ions are added to an exclusion list. The workflow is repeated up to 5 times until the intensity of the precursor ions becomes too low for getting exploitable MS/MS data for automated annotation. When compared to 5 independent DDA scans performed on the same sample, the IE-Omics
- 133 method shows an increase of 30% in the coverage of the lipidome for a plasma sample.

134 A strategy based on an automated DDA inclusion list workflow, called Data-Set-Dependent Acquisition (DsDA), was developed by Broeckling et al. (Broeckling et al., 2018). This method reports 135 the specific combination of MS-data processing and target prioritization to enable a more 136 137 comprehensive MS/MS coverage of the metabolome. The workflow consists of Top4 DDA scan, then 138 data is automatically treated and a score is attributed to each MS/MS spectra to determine its 139 importance to be fragmented. A module, written in R programming language, forces the workflow to 140 fragment precursor ions not previously fragmented in order to improve the metabolome coverage. This novel method offered 45% more MS/MS features. In the recently introduced BoxCar method, the MS 141 142 spectrum is segmented in several windows to improve detection sensitivity and the dynamic range of 143 the MS acquisition (Meier et al., 2018). Under these conditions, less abundant ions can be isolated 144 during DDA, thus providing unprecedented structural information.

- Another recently introduced gas phase fractionation approach is the so-called Parallel Accumulation
 Serial Fragmentation (PASEF, available on timsTOF Pro instruments) that synchronizes Trapped Ion
 Mobility Spectrometry (TIMS) with MS/MS precursor selection and fragmentation. This acquisition
- 148 mode drastically multiplies the fragmentation speed and detection sensitivity thereby approaching
- 149 almost 100% duty cycle, thus annotating up to 1,100 unique lipids in 1 μ L of human plasma
- 150 (Vasilopoulou et al., 2020).

All the presented methods of DDA are suffering from the same issue. As the sample often needs to be injected several times (up to 5 in both positive and negative ionization modes), its volume needs to be sufficient and the global analysis time is significantly extended making it impossible to apply these strategies for large cohort analysis in the field of medicine or biology.

155 **3 DIA-based acquisition workflows**

156 DIA performance was first described in the proteomic field 18 years ago (Venable et al., 2004) and

- have been implemented for lipidomics (Schwudke et al., 2006). The application of DIA is essentially motivated by the wider accessible dynamic range (4 orders of magnitude) (Gillet et al., 2012), higher
- sensitivity and reproducibility and, more importantly, the unbiased characterization of complex
- 160 biological matrices (Venable et al., 2004).

This is a provisional file, not the final typeset article

- 161 Analyzing the lipidome by direct injection into the mass spectrometer without prior chromatographic
- 162 separation steps (shotgun approach) is highly attractive owing to the short acquisition time, the low
- 163 solvent consumption, and its ease of implementation even if ion suppression effects are usually
- reported (Schwudke et al., 2011; Yang and Han, 2016). Shotgun DIA mode is mainly based on MS^{ALL}
- 165 workflow (Simons et al., 2012) and aims at monitoring MS/MS spectral information with 1 Da mass
- isolation on a large mass range for a run time lasting less than 6 minutes (Simons et al., 2012). MS^{ALL}
 mode was efficient to identify and quantify lipids belonging to different classes in various biological
- 168 matrices (Simons et al., 2012; Gao et al., 2016, 2018, 2021).
 - 169 MS^E for Q-TOF or All Ion Fragmentation (AIF) for Orbitrap-based instruments consist in acquiring
 - alternating scans of all ions without mass filtering at two or three collision energies (Plumb et al., 2006)
 - 171 (Figure 1). Precursor information are retrieved at low collision energy whereas specific product ions
 - are given by higher collision energy, facilitating the annotation step by combining all the MS/MS data
- 173 into consensus MS/MS spectra (Plumb et al., 2006; Diedrich et al., 2013).
- 174 One of the first approaches of DIA-AIF method was implemented on a LC coupled to a single-stage 175 Orbitrap mass analyzer using polarity switching in a single analytical run and using either in source CID or HCD fragmentation (Gallart-Ayala et al., 2013). Annotation of both phospholipids and 176 177 triacylglycerols from serum samples for diagnosis of canine mammary cancer thanks to known retention times and typical diagnostic product ions was performed. Similarly, Castro-Perez et al. 178 179 reported the advantages of applying alternated low and high collision energies in positive and negative 180 ionization modes to identify lipids from human plasma (Castro-Perez et al., 2010). More recently, lipids 181 from human plasma and dermal fibroblasts extracts were annotated using DIA-AIF and HCD in both 182 polarities (Ventura et al., 2020a, 2020b).
- In order to improve the association of precursor ions with their corresponding fragments, SWATH (Sequential Window Acquisition of All THeoretical) has been developed (Gillet et al., 2012). The principle is to define sequential MS/MS experiments in reduced m/z windows, typically 10-20 Da to cover the whole mass range, all ions within these windows are then fragmented simultaneously
- 187 (Figure 1). It has been initially developed on hybrid TOF instruments since a high-speed acquisition is 188 mandatory, but can be now implemented on Orbitrap-based instruments (Fenaille et al., 2017). 189 SWATH experiments were performed to characterize 214 and 140 lipids from immortalized 190 keratinocytes in both positive and negative ionization modes, respectively. As statistical treatment of 191 the data is mainly based on retention times, authors strongly advise to add internal standards to correct 192 any deviation (Calderón et al., 2020; Cebo et al., 2021). Interestingly, SWATH can be employed for 193 compound annotation using MS/MS library search but also quantification at the MS/MS level because, 194 unlike classic DDA, it offers continuous MS/MS spectra acquisition for particular fragment ions.
- 195 One of the main drawbacks of DIA workflows is related to the obtained (highly) convoluted tandem 196 mass spectra. Indeed, isobaric or isomeric lipid species from different classes can produce overlapping 197 isotopic clusters that will be co-isolated and fragmented MS/MS thus yielding highly convoluted and 198 thereby difficult-to-match MS/MS spectra. For instance, protonated phosphatidylcholine (PC 33:1) and 199 phosphatidylethanolamine (PE 36:1) share the same elemental composition (Züllig and Köfeler, 200 2021b). The frequent presence of sodium adducts can bring additional spectral complexity with lipid 201 sodiated species isobaric to protonated unsaturated ones differing only by ~2mDa in some extreme 202 cases (Höring et al., 2020; Züllig and Köfeler, 2021b).

In DIA workflows, such as SWATH, the direct link between a given precursor ion and its corresponding fragments is often lost, which renders MS/MS data interpretation of unknown lipid species much more difficult than that of MS/MS data resulting from DDA protocols. Data treatment step, i.e. the concatenation and alignment of precursor and fragment ions, is indeed often considered as the critical point. This can be performed according to retention times (Castro-Perez et al., 2010) or by specific data filtering through mass defect calculation (Stagliano et al., 2010). A correlation-based deconvolution (CorrDec) method that uses correlation of ion abundances between precursor and

- 210 product ions has been developed to improve the metabolite annotation rate (Tada et al., 2020).
- 211

While SWATH techniques provide a better coverage of the lipidome, it comes at the cost of lower 212 213 quality spectra. Therefore, DIA SWATH method has been implemented together with DDA leading to 214 the hybrid DaDIA mode (Guo et al., 2021). The sequence is composed of blanks and samples analyzed in DIA SWATH mode and quality controls (QCs) in DDA mode. DDA MS/MS data provided high 215 quality spectra for the highest intensity features and are used to improve the deconvolution of SWATH 216 data for better quality. This hybrid method enables a better lipidome coverage while improving the 217 quality of deconvoluted SWATH spectra to a level similar to DDA spectra. Combination of 2D-LC, 218 DIA MS^E and DDA Top3, called HDDIDDA, outperforms DDA with a slightly higher annotation rate 219

and MS^E with a slightly higher coverage at the cost of a complex data treatment (Wang et al., 2022).

221 Even if DIA approach looks appealing in terms of numbers of annotated lipid species, the annotation 222 steps required the most exhaustive and reliable MS/MS databases including normalized retention times 223 if available. Acquiring MS/MS spectra from pure authentic standards is the best way to generate 224 spectral databases, but this is clearly unrealistic due to the cost and viability of pure compounds. The 225 most feasible strategy is to generate *in-silico* low-energy fragmentation spectra thanks to the welldocumented mechanisms of lipid fragmentation (Murphy, 2015) as defined in LipidBlast database. As 226 already documented in the literature, MS/MS data are strongly dependent on the type of tandem mass 227 228 spectrometer and the collision energy used that is challenging to normalize especially in the case of 229 small molecule analysis (Murphy, 2015). Thus, the information related to the relative intensities of the fragments cannot be easily employed to refine structure annotation making the match scoring process 230 231 less robust.

232 Several software solutions (Kitata et al., 2021) include modules capable of achieving the complete 233 pipeline from the conversion of vendor raw files to statistical analysis and through the identification 234 from integrated and/or implementable lipid libraries as exemplified in Table 1. While attributing ion products to the precursor ion is unproblematic in DDA mode, to reconstruct MS/MS data in DIA mode 235 236 remains highly challenging. To the best of our knowledge, only two robust software tools, *i.e.* MS-DIAL and DecoMetDIA, offer a deconvolution step for untargeted analysis in the DIA mode (Tsugawa 237 238 et al., 2019; Yin et al., 2019; Tada et al., 2020). Multiple processing strategies for DIA deconvolution 239 emerge in proteomics (Kitata et al., 2021) and are expected to be applied to small compounds in the 240 near future.

241 **4 Discussion and Conclusions**

Considering the rapid development of mass spectrometers in terms of scan speed, resolving power and mass accuracy, the analytical strategies for lipidomics have widely expanded during the last two decades. Beyond the use of high mass accuracy at MS level to suggest molecular formulas, MS/MS experiments are fully integrated in lipidomics workflows to provide successful semi-quantification and structural characterization. Both DDA and DIA methodologies require high acquisition rate tandem mass spectrometers to access deep lipidome. The quality of MS/MS data is needed for facilitating annotation but the total number of MS/MS scans on a unique feature is limited. Iterative DDA allows to exceed this limitation but significantly increases the sample consumption and the overall experimental time making this approach not compatible with the analysis of large cohorts. On the contrary, DIA significantly increases the number of annotated lipid species but is still far limited by the available software solutions (notably regarding spectra deconvolution).

Free software tools are reviewed in the Table 1 and three of them, namely MS-DIAL (Tsugawa et al., 254 2015), DecoMetDIA (Yin et al., 2019) and DecoID (Stancliffe et al., 2021) propose efficient 255 bioinformatic tools for the deconvolution of mixed tandem mass spectra obtained from SWATH 256 workflows.

257 Also, as exposed by Barbier Saint Hilaire et al., well-designing SWATH isolation windows can impact significantly the detection rate of targeted compounds (Barbier Saint Hilaire et al., 2020). The free 258 259 software tool SwathTUNER (Table 1) permits the automatized design of the variable isolations windows according either the Total Ion Current (TIC) or precursors density (Zhang et al., 2015) to 260 significantly lower the complexity of tandem mass spectra obtained in the DIA-SWATH mode. Also, 261 262 the commercial vendor Sciex proposes the SWATH® Acquisition module available on their TripleTOF® systems for the automatically designing of variable isolation windows, permitting the all-263 264 in-one acquisition workflow (https://sciex.com/technology/swath-acquisition).

265 Since a decade, ion mobility (IM) offers the unique possibility to separate ions not only on their m/z266 values but also on their shape in the gas phase, thus enabling the measure of collision cross-sections (CCSs). The IM time is fully compatible with the chromatographic time and the fast acquisition time 267 of modern mass spectrometers. Several groups demonstrated that lipid isomers bearing different fatty 268 chains but the same total number of carbons, including Z/E isomers, can be efficiently separated by 269 IM-MS (Paglia et al., 2015). MS^E experiments by coupling LC to IM-QTOF were performed for the 270 characterization of non-purified glycolipids extracts from Caenorhabditis elegans (Witting et al., 271 272 2021). The multidimensional information collected from chromatographic separation (Retention Time), ion mobility (CCS) and MS^E acquisition permits extended lipid annotation. Ion mobility 273 274 coupled to DIA or DDA approaches paves the way for a rather complete structural annotation and 275 (semi-)quantification of deep lipidome including all minor species, while also significantly improving 276 the quality of both DDA and DIA tandem mass spectra by separating isobaric/isomeric lipid ion species 277 prior to their isolation and fragmentation. The file sizes, from several hundreds of Mo to several Go 278 per injection, the limited software availability for efficiently handling resulting datasets and the 279 difficulty to generate absolute collision cross-sections for highly flexible molecules, such as lipids in 280 the gas phase, strongly restrict the full exploitation of the data acquired by DIA- or DDA- ion mobility.

281 A last issue in MS/MS is the efficient location of double bonds on lipid structures as dissociations at low-energy are not efficient (Ma et al., 2016). Prior chemical derivatization of carbon-carbon double 282 283 bonds either directly by a chemical agent (e.g. ozonolysis, epoxidation, hydroxylation) or facilitated by UV irradiation (e.g. Paternò - Büchi reaction) can lead to reaction products that can be further 284 fragmented under low-energy dissociation conditions to pinpoint the location of double bonds (Cao et 285 286 al., 2018; Harris et al., 2018). Nonetheless, the routine and broad application of these methods remain 287 limited due to the required long reaction time and the inadequate utilization with online LC-MS/MS workflows (Poad et al., 2017). Other fragmentation techniques can be also implemented. Electron-288 289 capture Dissociation (ECD) on a divalent metal complex of glycerophospholipids was proposed for 290 double bond location (James et al., 2011). Other electron-activated dissociation (EAD) types have been

- devised such as Electron-induced dissociation (EID) and Electron-Impact Excitation of Ions from Organics (EIEIO) compatible with singly-charged precursor ions (Baba et al., 2021). Ultraviolet photodissociation (UVPD) activation mode has recently been used to distinguish sn-positional isomers and to determine carbon-carbon double bonds location (Williams et al., 2017). Only few commercial instruments are now equipped with EAD, EID, EIEO or UVPD while relatively low yields of fragmentation are usually reported for those methods restricting their applications to abundant species even if the fragmentation process is fully compatible with LC peak width.
- Even if major progresses in lipidomics have been reported in the last years, improvements of each step of the workflow, from the sample preparation, the chromatography, the MS and MS/MS acquisition to the automated data treatment, are needed to expand lipidome coverage.

301 5 Author Contributions

302 VM and MV equally contributed to the work. All authors completed and approved the manuscript.

303 6 Acknowledgements

304 This study was supported by the MetaboHUB infrastructure (ANR-11-INBS-0010 grant).

The authors declare that the research was conducted in the absence of any commercial or financial relationships that could be construed as a potential conflict of interest.

307 7 References

- Alcoriza-Balaguer, M. I., Garcia-Cañaveras, J. C., López, A., Conde, I., Juan, O., Carretero, J., et al.
 (2019). LipidMS: An R Package for Lipid Annotation in Untargeted Liquid ChromatographyData Independent Acquisition-Mass Spectrometry Lipidomics. *Anal. Chem.* 91(1), 836–845.
 doi: 10.1021/acs.analchem.8b03409.
- 312 Baba, T., Ryumin, P., Duchoslav, E., Chen, K., Chelur, A., Loyd, B., et al. (2021). Dissociation of Biomolecules by an Intense Low-Energy Electron Beam in a High Sensitivity Time-of-Flight 313 314 Mass Spectrometer. J. Am. Soc. Mass Spectrom. 32(8), 1964–1975. doi: 315 10.1021/jasms.0c00425.
- Barbier Saint Hilaire, P., Rousseau, K., Seyer, A., Dechaumet, S., Damont, A., Junot, C., et al. (2020).
 Comparative Evaluation of Data Dependent and Data Independent Acquisition Workflows
 Implemented on an Orbitrap Fusion for Untargeted Metabolomics. *Metabolites* 10, 158. doi:
 10.3390/metabo10040158.
- Broeckling, C. D., Hoyes, E., Richardson, K., Brown, J. M., and Prenni, J. E. (2018). Comprehensive
 Tandem-Mass-Spectrometry Coverage of Complex Samples Enabled by Data-Set-Dependent
 Acquisition. *Anal. Chem.* 90, 8020–8027. doi: 10.1021/acs.analchem.8b00929.
- Byrdwell, W. C. (2001). Atmospheric pressure chemical ionization mass spectrometry for analysis of
 lipids. *Lipids* 36(4), 327–346. doi: 10.1007/s11745-001-0725-5.

Calderón, C., Rubarth, L., Cebo, M., Merfort, I., and Lämmerhofer, M. (2020). Lipid Atlas of
 Keratinocytes and Betulin Effects on its Lipidome Profiled by Comprehensive UHPLC–

- MS/MS with Data Independent Acquisition Using Targeted Data Processing. *PROTEOMICS* 20(11):e1900113. doi: 10.1002/pmic.201900113.
- Cao, W., Ma, X., Li, Z., Zhou, X., and Ouyang, Z. (2018). Locating Carbon–Carbon Double Bonds in
 Unsaturated Phospholipids by Epoxidation Reaction and Tandem Mass Spectrometry. *Anal. Chem.* 90(17), 10286–10292. doi: 10.1021/acs.analchem.8b02021.
- Castro-Perez, J. M., Kamphorst, J., DeGroot, J., Lafeber, F., Goshawk, J., Yu, K., et al. (2010).
 Comprehensive LC–MSE Lipidomic Analysis using a Shotgun Approach and Its Application to Biomarker Detection and Identification in Osteoarthritis Patients. *J. Proteome Res.* 9(5), 2377–2389. doi: 10.1021/pr901094j.
- Cebo, M., Calderón Castro, C., Schlotterbeck, J., Gawaz, M., Chatterjee, M., and Lämmerhofer, M.
 (2021). Untargeted UHPLC-ESI-QTOF-MS/MS analysis with targeted feature extraction at
 precursor and fragment level for profiling of the platelet lipidome with ex vivo thrombinactivation. J. Pharm. Biomed. Anal. 205:114301. doi: 10.1016/j.jpba.2021.114301.
- Chiu, H.-H., and Kuo, C.-H. (2020). Gas chromatography-mass spectrometry-based analytical
 strategies for fatty acid analysis in biological samples. *Journal of Food and Drug Analysis* 28,
 60–73. doi: 10.1016/j.jfda.2019.10.003.
- Diedrich, J. K., Pinto, A. F. M., and Yates, J. R. (2013). Energy dependence of HCD on peptide
 fragmentation: Stepped collisional energy finds the sweet spot. *J. Am. Soc. Mass Spectrom.*24(11), 1690–1699. doi: 10.1007/s13361-013-0709-7.
- Eliuk, S., and Makarov, A. (2015). Evolution of Orbitrap Mass Spectrometry Instrumentation. *Annu. Rev. Anal. Chem.* 8(1), 61–80. doi: 10.1146/annurev-anchem-071114-040325.
- Fahy, E., Subramaniam, S., Brown, H. A., Glass, C. K., Merrill, A. H., Murphy, R. C., et al. (2005). A
 comprehensive classification system for lipids. *J Lipid Res* 46, 839–861. doi: 10.1194/jlr.E400004-JLR200.
- Fahy, E., Subramaniam, S., Murphy, R. C., Nishijima, M., Raetz, C. R. H., Shimizu, T., et al. (2009).
 Update of the LIPID MAPS comprehensive classification system for lipids. *J Lipid Res* 50, S9–
 S14. doi: 10.1194/jlr.R800095-JLR200.
- Fenaille, F., Barbier Saint-Hilaire, P., Rousseau, K., and Junot, C. (2017). Data acquisition workflows
 in liquid chromatography coupled to high resolution mass spectrometry-based metabolomics:
 Where do we stand? *J. Chromatogr. A* 1526, 1–12. doi: 10.1016/j.chroma.2017.10.043.
- 357 Gallart-Ayala, H., Courant, F., Severe, S., Antignac, J.-P., Morio, F., Abadie, J., et al. (2013). Versatile 358 lipid profiling by liquid chromatography-high resolution mass spectrometry using all ion fragmentation and polarity switching. Preliminary application for serum samples phenotyping 359 canine 360 related mammary Acta doi: to cancer. Anal. Chim. 796. 75-83. 10.1016/j.aca.2013.08.006. 361
- Gao, F., McDaniel, J., Chen, E. Y., Rockwell, H. E., Nguyen, C., Lynes, M. D., et al. (2018). Adapted
 MS/MSALL Shotgun Lipidomics Approach for Analysis of Cardiolipin Molecular Species.
 Lipids 53(1), 133–142. doi: 10.1002/lipd.12004.

- Gao, F., McDaniel, J., Chen, E. Y., Rockwell, H., Lynes, M. D., Tseng, Y.-H., et al. (2016).
 Monoacylglycerol Analysis Using MS/MSALL Quadruple Time of Flight Mass Spectrometry.
 Metabolites 6(3):25. doi: 10.3390/metabo6030025.
- Gao, Y., Qi, Y., Huang, Y., Li, X., Zhou, L., and Zhao, S. (2021). Lipidomics Analysis of the Tears in
 the Patients Receiving LASIK, FS-LASIK, or SBK Surgery. *Front. Med.* 8:731462. doi:
 10.3389/fmed.2021.731462.
- Gillet, L. C., Navarro, P., Tate, S., Röst, H., Selevsek, N., Reiter, L., et al. (2012). Targeted Data
 Extraction of the MS/MS Spectra Generated by Data-independent Acquisition: A New Concept
 for Consistent and Accurate Proteome Analysis*. *Mol. Cell. Proteomics* 11(6), O111.016717.
 doi: 10.1074/mcp.O111.016717.
- Goracci, L., Tortorella, S., Tiberi, P., Pellegrino, R. M., Di Veroli, A., Valeri, A., et al. (2017). Lipostar,
 a Comprehensive Platform-Neutral Cheminformatics Tool for Lipidomics. *Anal. Chem.* 89(11),
 6257–6264. doi: 10.1021/acs.analchem.7b01259.
- Guo, J., Shen, S., Xing, S., and Huan, T. (2021). DaDIA: Hybridizing Data-Dependent and DataIndependent Acquisition Modes for Generating High-Quality Metabolomic Data. *Anal. Chem.*93, 2669–2677. doi: 10.1021/acs.analchem.0c05022.
- Harayama, T., and Riezman, H. (2018). Understanding the diversity of membrane lipid composition.
 Nat Rev Mol Cell Biol 19, 281–296. doi: 10.1038/nrm.2017.138.
- Harris, R. A., May, J. C., Stinson, C. A., Xia, Y., and McLean, J. A. (2018). Determining Double Bond
 Position in Lipids Using Online Ozonolysis Coupled to Liquid Chromatography and Ion
 Mobility-Mass Spectrometry. *Anal. Chem.* 90(3), 1915–1924. doi:
 10.1021/acs.analchem.7b04007.
- Hartler, J., Triebl, A., Ziegl, A., Trötzmüller, M., Rechberger, G. N., Zeleznik, O. A., et al. (2017).
 Deciphering lipid structures based on platform-independent decision rules. *Nat Methods* 14(12), 1171–1174. doi: 10.1038/nmeth.4470.
- Hartler, J., Trötzmüller, M., Chitraju, C., Spener, F., Köfeler, H. C., and Thallinger, G. G. (2011). Lipid
 Data Analyzer: unattended identification and quantitation of lipids in LC-MS data.
 Bioinformatics 27(4), 572–577. doi: 10.1093/bioinformatics/btq699.
- Höring, M., Ekroos, K., Baker, P. R. S., Connell, L., Stadler, S. C., Burkhardt, R., et al. (2020).
 Correction of Isobaric Overlap Resulting from Sodiated Ions in Lipidomics. *Anal. Chem.* 92, 10966–10970. doi: 10.1021/acs.analchem.0c02408.
- Hutchins, P. D., Russell, J. D., and Coon, J. J. (2018). LipiDex: An Integrated Software Package for
 High-Confidence Lipid Identification. *cels* 6(5), 621-625.e5. doi: 10.1016/j.cels.2018.03.011.
- Imbert, L., Gaudin, M., Libong, D., Touboul, D., Abreu, S., Loiseau, P. M., et al. (2012). Comparison
 of electrospray ionization, atmospheric pressure chemical ionization and atmospheric pressure
 photoionization for a lipidomic analysis of Leishmania donovani. *J. Chromatogr. A* 1242, 75–
 83. doi: 10.1016/j.chroma.2012.04.035.


- James, P. F., Perugini, M. A., and O'Hair, R. A. J. (2011). Electron capture dissociation of complexes
 of diacylglycerophosphocholine and divalent metal ions: Competition between charge
 reduction and radical induced phospholipid fragmentation. *J. Am. Soc. Mass Spectrom.* 19,
 978–986. doi: 10.1016/j.jasms.2008.03.006.
- Kirkwood, K. I., Pratt, B. S., Shulman, N., Tamura, K., MacCoss, M. J., MacLean, B. X., et al. (2022).
 Utilizing Skyline to analyze lipidomics data containing liquid chromatography, ion mobility
 spectrometry and mass spectrometry dimensions. *Nat Protoc*, 1–16. doi: 10.1038/s41596-02200714-6.
- Kitata, R. B., Yang, J.-C., and Chen, Y.-J. (2021). Advances in data-independent acquisition mass
 spectrometry towards comprehensive digital proteome landscape. *Mass Spectrom. Rev.*,
 e21781. doi: 10.1002/mas.21781.
- Kochen, M. A., Chambers, M. C., Holman, J. D., Nesvizhskii, A. I., Weintraub, S. T., Belisle, J. T., et
 al. (2016). Greazy: Open-Source Software for Automated Phospholipid Tandem Mass
 Spectrometry Identification. *Anal. Chem.* 88, 5733–5741. doi: 10.1021/acs.analchem.6b00021.
- Koelmel, J. P., Kroeger, N. M., Gill, E. L., Ulmer, C. Z., Bowden, J. A., Patterson, R. E., et al. (2017).
 Expanding lipidome coverage using LC-MS/MS data-dependent acquisition with automated
 exclusion list generation. *J Am Soc Mass Spectrom* 28, 908–917. doi: 10.1007/s13361-0171608-0.
- Li, H., Cai, Y., Guo, Y., Chen, F., and Zhu, Z.-J. (2016). MetDIA: Targeted Metabolite Extraction of Multiplexed MS/MS Spectra Generated by Data-Independent Acquisition. *Anal. Chem.* 88, 8757–8764. doi: 10.1021/acs.analchem.6b02122.
- Liebisch, G., Fahy, E., Aoki, J., Dennis, E. A., Durand, T., Ejsing, C. S., et al. (2020). Update on LIPID
 MAPS classification, nomenclature, and shorthand notation for MS-derived lipid structures. J.
 Lipid Res. 61(12), 1539–1555. doi: 10.1194/jlr.S120001025.
- Ma, X., Chong, L., Tian, R., Shi, R., Hu, T. Y., Ouyang, Z., et al. (2016). Identification and quantitation
 of lipid C=C location isomers: A shotgun lipidomics approach enabled by photochemical
 reaction. *Proc. Natl. Acad. Sci.* 113(10), 2573–2578. doi: 10.1073/pnas.1523356113.
- Meier, F., Geyer, P. E., Virreira Winter, S., Cox, J., and Mann, M. (2018). BoxCar acquisition method
 enables single-shot proteomics at a depth of 10,000 proteins in 100 minutes. *Nat Methods* 15, 431
 440–448. doi: 10.1038/s41592-018-0003-5.
- 432 Murphy, R. C. (2015). *Tandem mass spectrometry of lipids: molecular analysis of complex lipids*.
 433 Cambridge: Royal Society of Chemistry.
- Neumann, S., Thum, A., and Böttcher, C. (2013). Nearline acquisition and processing of liquid
 chromatography-tandem mass spectrometry data. *Metabolomics* 9, 84–91. doi:
 10.1007/s11306-012-0401-0.
- Paglia, G., Angel, P., Williams, J. P., Richardson, K., Olivos, H. J., Thompson, J. W., et al. (2015). Ion
 Mobility-Derived Collision Cross Section As an Additional Measure for Lipid Fingerprinting
 and Identification. *Anal Chem* 87, 1137–1144. doi: 10.1021/ac503715v.


- Perez de Souza, L., Alseekh, S., Scossa, F., and Fernie, A. R. (2021). Ultra-high-performance liquid
 chromatography high-resolution mass spectrometry variants for metabolomics research. *Nat Methods* 18(7), 733–746. doi: 10.1038/s41592-021-01116-4.
- Plumb, R. S., Johnson, K. A., Rainville, P., Smith, B. W., Wilson, I. D., Castro-Perez, J. M., et al.
 (2006). UPLC/MSE; a new approach for generating molecular fragment information for
 biomarker structure elucidation. *Rapid Communications in Mass Spectrometry* 20(13), 1989–
 1994. doi: 10.1002/rcm.2550.
- Poad, B. L. J., Green, M. R., Kirk, J. M., Tomczyk, N., Mitchell, T. W., and Blanksby, S. J. (2017).
 High-Pressure Ozone-Induced Dissociation for Lipid Structure Elucidation on Fast
 Chromatographic Timescales. *Anal. Chem.* 89(7), 4223–4229. doi: 10.1021/acs.analchem.7b00268.
- 451 Quehenberger, O., Armando, A. M., Brown, A. H., Milne, S. B., Myers, D. S., Merrill, A. H., et al.
 452 (2010). Lipidomics reveals a remarkable diversity of lipids in human plasma. *Journal of Lipid*453 *Research* 51, 3299–3305. doi: 10.1194/jlr.M009449.
- 454 Rustam, Y. H., and Reid, G. E. (2018). Analytical Challenges and Recent Advances in Mass
 455 Spectrometry Based Lipidomics. *Anal. Chem.* 90(1), 374–397. doi: 456 10.1021/acs.analchem.7b04836.
- Schwudke, D., Oegema, J., Burton, L., Entchev, E., Hannich, J. T., Ejsing, C. S., et al. (2006). Lipid
 Profiling by Multiple Precursor and Neutral Loss Scanning Driven by the Data-Dependent
 Acquisition. *Anal. Chem.* 78(2), 585–595. doi: 10.1021/ac051605m.
- Schwudke, D., Schuhmann, K., Herzog, R., Bornstein, S. R., and Shevchenko, A. (2011). Shotgun
 lipidomics on high resolution mass spectrometers. *Cold Spring Harb Perspect Biol* 3, a004614.
 doi: 10.1101/cshperspect.a004614.
- Simons, B., Kauhanen, D., Sylvänne, T., Tarasov, K., Duchoslav, E., and Ekroos, K. (2012). Shotgun
 Lipidomics by Sequential Precursor Ion Fragmentation on a Hybrid Quadrupole Time-of-Flight
 Mass Spectrometer. *Metabolites* 2(1), 195–213. doi: 10.3390/metabo2010195.
- 466 Stagliano, M. C., DeKeyser, J. G., Omiecinski, C. J., and Jones, A. D. (2010). Bioassay-directed
 467 fractionation for discovery of bioactive neutral lipids guided by relative mass defect filtering
 468 and multiplexed collision-induced dissociation. *Rapid Commun. Mass Spectrom.* 24(24), 3578–
 469 3584. doi: 10.1002/rcm.4796.
- 470 Stancliffe, E., Schwaiger-Haber, M., Sindelar, M., and Patti, G. J. (2021). DecoID Improves
 471 Identification Rates in Metabolomics through Database-Assisted MS/MS Deconvolution. *Nat*472 *Methods* 18, 779–787. doi: 10.1038/s41592-021-01195-3.
- Tada, I., Chaleckis, R., Tsugawa, H., Meister, I., Zhang, P., Lazarinis, N., et al. (2020). CorrelationBased Deconvolution (CorrDec) To Generate High-Quality MS2 Spectra from DataIndependent Acquisition in Multisample Studies. *Anal. Chem.* 92(16), 11310–11317. doi:
 10.1021/acs.analchem.0c01980.

- Tsugawa, H., Cajka, T., Kind, T., Ma, Y., Higgins, B., Ikeda, K., et al. (2015). MS-DIAL: dataindependent MS/MS deconvolution for comprehensive metabolome analysis. *Nat. Methods*12(6), 523–526. doi: 10.1038/nmeth.3393.
- Tsugawa, H., Satoh, A., Uchino, H., Cajka, T., Arita, M., and Arita, M. (2019). Mass Spectrometry
 Data Repository Enhances Novel Metabolite Discoveries with Advances in Computational
 Metabolomics. *Metabolites* 9, 119. doi: 10.3390/metabo9060119.
- Vasilopoulou, C. G., Sulek, K., Brunner, A.-D., Meitei, N. S., Schweiger-Hufnagel, U., Meyer, S. W.,
 et al. (2020). Trapped ion mobility spectrometry and PASEF enable in-depth lipidomics from
 minimal sample amounts. *Nat Commun* 11(1), 331. doi: 10.1038/s41467-019-14044-x.
- Venable, J. D., Dong, M.-Q., Wohlschlegel, J., Dillin, A., and Yates, J. R. (2004). Automated approach
 for quantitative analysis of complex peptide mixtures from tandem mass spectra. *Nat. Methods*1(1), 39–45. doi: 10.1038/nmeth705.
- Ventura, G., Bianco, M., Calvano, C. D., Losito, I., and Cataldi, T. R. I. (2020a). HILIC-ESI-FTMS
 with All Ion Fragmentation (AIF) Scans as a Tool for Fast Lipidome Investigations. *Molecules* 25(10):2310. doi: 10.3390/molecules25102310.
- Ventura, G., Calvano, C. D., Porcelli, V., Palmieri, L., De Giacomo, A., Xu, Y., et al. (2020b).
 Phospholipidomics of peripheral blood mononuclear cells (PBMCs): the tricky case of children with autism spectrum disorder (ASD) and their healthy siblings. *Anal. Bioanal. Chem.* 412(25), 6859–6874. doi: 10.1007/s00216-020-02817-z.
- Wang, H., Wang, H., Wang, X., Xu, X., Hu, Y., Li, X., et al. (2022). A novel hybrid scan approach
 enabling the ion-mobility separation and the alternate data-dependent and data-independent
 acquisitions (HDDIDDA): Its combination with off-line two-dimensional liquid
 chromatography for comprehensively characterizing the multicomponents from Compound
 Danshen Dripping Pill. *Analytica Chimica Acta* 1193, 339320. doi: 10.1016/j.aca.2021.339320.
- Wenk, M. R. (2005). The emerging field of lipidomics. *Nat Rev Drug Discov* 4(7), 594–610. doi: 10.1038/nrd1776.
- Wenk, M. R. (2010). Lipidomics: New Tools and Applications. *Cell* 143(6), 888–895. doi:
 10.1016/j.cell.2010.11.033.
- Williams, P. E., Klein, D. R., Greer, S. M., and Brodbelt, J. S. (2017). Pinpointing Double Bond and
 sn-Positions in Glycerophospholipids via Hybrid 193 nm Ultraviolet Photodissociation
 (UVPD) Mass Spectrometry. J. Am. Chem. Soc. 139(44), 15681–15690. doi:
 10.1021/jacs.7b06416.
- Witting, M., Schmidt, U., and Knoelker, H.-J. (2021). UHPLC-IM-Q-ToFMS analysis of maradolipids,
 found exclusively in Caenorhabditis elegans dauer larvae. *Anal. Bioanal. Chem.* 413(8), 2091–
 2102. doi: 10.1007/s00216-021-03172-3.
- Yang, K., and Han, X. (2016). Lipidomics: Techniques, applications, and outcomes related to
 biomedical sciences. *Trends Biochem Sci* 41, 954–969. doi: 10.1016/j.tibs.2016.08.010.

- Yin, Y., Wang, R., Cai, Y., Wang, Z., and Zhu, Z.-J. (2019). DecoMetDIA: Deconvolution of
 Multiplexed MS/MS Spectra for Metabolite Identification in SWATH-MS-Based Untargeted
 Metabolomics. *Anal. Chem.* 91(18), 11897–11904. doi: 10.1021/acs.analchem.9b02655.
- Zha, H., Cai, Y., Yin, Y., Wang, Z., Li, K., and Zhu, Z.-J. (2018). SWATHtoMRM: Development of
 High-Coverage Targeted Metabolomics Method Using SWATH Technology for Biomarker
 Discovery. *Anal. Chem.* 90, 4062–4070. doi: 10.1021/acs.analchem.7b05318.
- Zhang, Y., Bilbao, A., Bruderer, T., Luban, J., Strambio-De-Castillia, C., Lisacek, F., et al. (2015). The
 Use of Variable Q1 Isolation Windows Improves Selectivity in LC–SWATH–MS Acquisition.
 J. Proteome Res. 14(10), 4359–4371. doi: 10.1021/acs.jproteome.5b00543.
- Zhou, Z., Shen, X., Chen, X., Tu, J., Xiong, X., and Zhu, Z.-J. (2019). LipidIMMS Analyzer:
 integrating multi-dimensional information to support lipid identification in ion mobility—mass
 spectrometry based lipidomics. *Bioinformatics* 35(4), 698–700. doi:
 10.1093/bioinformatics/bty661.
- 527 Züllig, T., and Köfeler, H. C. (2021a). High Resolution Mass Spectrometry in Lipidomics. *Mass Spectrom. Rev.* 40(3), 162–176. doi: 10.1002/mas.21627.
- Züllig, T., and Köfeler, H. C. (2021b). HIGH RESOLUTION MASS SPECTROMETRY IN
 LIPIDOMICS. *Mass Spectrom Rev* 40, 162–176. doi: 10.1002/mas.21627.
- Züllig, T., Trötzmüller, M., and Köfeler, H. C. (2020). Lipidomics from sample preparation to data
 analysis: a primer. *Anal. Bioanal. Chem.* 412(10), 2191–2209. doi: 10.1007/s00216-01902241-y.

534

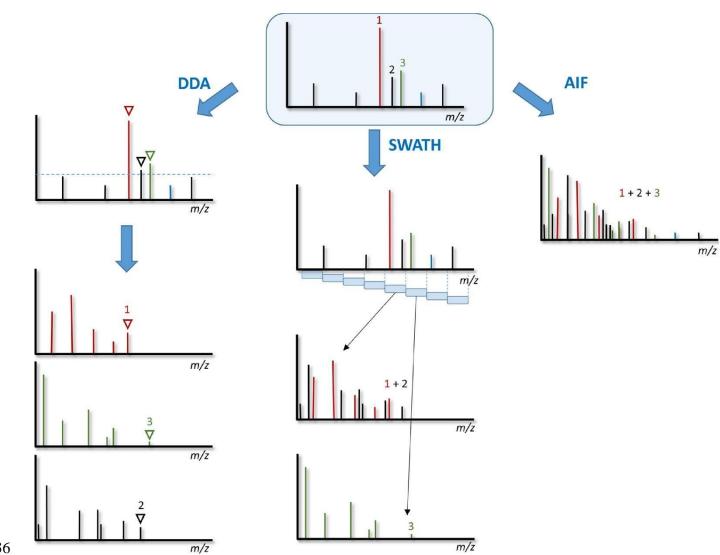



9 Table

Figure



Table 1 - Overview of software and tools for the processing of lipid identification step from spectral data acquired by tandem mass spectrometry in DDA and DIA. Remark: Software specified by * are commercial.

	Data processing			Lipid annotation		Station 1	
Software Tools	Peak detection	Peak alignment	Peak grouping	Precursor match	MS/MS match	tools	Application and descriptions
Lipid Search*	Х	Х	Х	Х	Х	Х	DDA: ESI-(LC)-MS/MS, identification from integrated lipid library, univariate statistics and MS/MS scoring. By Thermo Scientific TM .
LipidView [*] , Lipidyzer [*]	Х	Х	Х	Х	Х	Х	DDA: ESI-(LC)-MS/MS, identification from integrated lipid library, univariate statistics and MS/MS scoring. By SCIEX.
SimLipid*	Х	Х	Х	Х	Х	Х	DDA, DIA: ESI-(LC)-MS/MS identification from integrated lipid library, univariate statistical analysis and MS/MS scoring (MS ^E for DIA mode acquisition). By PREMIER Biosoft.
Lipostar*	Х	Х	Х	Х	Х	Х	DDA, DIA: ESI-LC-MS/MS identification from implementable lipid library, multivariate unsupervised and supervised statistical analyses (e.g. Principal Component Analysis (PCA), Partial Least-Squares (PLS)) (Goracci et al., 2017). By Molecular Discovery.
SwathTuner							DIA: Tool to tune method and optimize width windows for SWATH acquisitions (Zhang et al., 2015).
MS-DIAL	Х	Х	Х	X	х	Х	DDA, DIA: Deconvolution of MS/MS spectra of SWATH acquisition (two available algorithms) and identification from implementable lipid libraries with MS/MS scoring. Univariate and non-supervised statistics (<i>e.g.</i> T-test, PCA) (Tsugawa et al., 2015; Tada et al., 2020).
MetDIA	Х	Х	Х	Х	Х	Х	DIA: Targeted peak detection from SWATH acquisition according to implementable lipid libraries with MS/MS scoring, univariate statistics on precursors ion area (Li et al., 2016).
LipiDex	Х	Х	Х	Х	Х		DDA: Peak detection and identification from implementable lipid libraries (Hutchins et al., 2018).
LipidMS 3.0	Х	Х	Х	Х	Х		DDA, DIA: Targeted peak detection from the integrated lipid libraries (Alcoriza-Balaguer et al., 2019).
Skyline	Х	Х	Х	Х	Х		DDA, DIA: Targeted approach for identification according indexed Retention Time and Collision-Cross Section, MS and MS/MS spectra from implementable lipid libraries (Kirkwood et al., 2022).
DecoMetDIA	Х	Х	Х				DIA: Deconvolution of MS/MS spectra from SWATH acquisitions and identification according to implementable lipid libraries (Yin et al., 2019).
Greazy/ LipidLama	Х		Х	Х	Х		DDA: Peak detection and identification from set of theoretical phospholipids and fragments (Kochen et al., 2016).
DecoID				x	х		DDA, DIA: Peak detection, deconvolution of MS/MS spectra (LASSO regression algorithm) and identification according implementable lipid libraries (Stancliffe et al., 2021).
SWATHtoMRM				Х	Х		DIA: Targeted peak detection from SWATH acquisitions from implementable lipid libraries (Zha et al., 2018).
Lipid Data Analyzer2 (LDA2)				Х	Х		DDA, DIA: Semi-targeted approach for identification according to decision rules from various mass spectrometers (Hartler et al., 2011, 2017).
LipidMatch				Х	Х		DDA, DIA: Untargeted approach for identification according <i>in-silico</i> lipid libraries. For DIA, AIF uniquely (Koelmel et al., 2017).
LipidIMMS				X	Х		DDA, DIA: Targeted approach for identification according Retention Time and Collision- Cross Section predictions, MS and MS/MS spectra from integrated lipid libraries (Zhou et al., 2019).

PAGE * Arabic *