



HAL
open science

Microscopic fractures shown inside tablets after impact

Craig Stuart Carlson, Michiel Postema, Nicole Anderton, Markus Hannula,
Joonas Sorjonen, Hu Xinyue, Naoyuki Otake, Nobuki Kudo, Jari Hyttinen,
Jarkko Ketolainen

► **To cite this version:**

Craig Stuart Carlson, Michiel Postema, Nicole Anderton, Markus Hannula, Joonas Sorjonen, et al.. Microscopic fractures shown inside tablets after impact. *Japanese Journal of Applied Physics*, 2024, Special Issue on Ultrasonic Electronics 2023 (USE2023), 63 (2), pp.028005. 10.35848/1347-4065/ad21be . hal-04411113

HAL Id: hal-04411113

<https://hal.science/hal-04411113v1>

Submitted on 24 Jan 2024

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Distributed under a Creative Commons Attribution - NonCommercial - NoDerivatives 4.0
International License

ACCEPTED MANUSCRIPT

Microscopic fractures shown inside tablets after impact

To cite this article before publication: Craig S Carlson *et al* 2024 *Jpn. J. Appl. Phys.* in press <https://doi.org/10.35848/1347-4065/ad21be>

Manuscript version: Accepted Manuscript

Accepted Manuscript is “the version of the article accepted for publication including all changes made as a result of the peer review process, and which may also include the addition to the article by IOP Publishing of a header, an article ID, a cover sheet and/or an ‘Accepted Manuscript’ watermark, but excluding any other editing, typesetting or other changes made by IOP Publishing and/or its licensors”

This Accepted Manuscript is © 2024 The Japan Society of Applied Physics.



During the embargo period (the 12 month period from the publication of the Version of Record of this article), the Accepted Manuscript is fully protected by copyright and cannot be reused or reposted elsewhere.

As the Version of Record of this article is going to be / has been published on a subscription basis, this Accepted Manuscript will be available for reuse under a CC BY-NC-ND 3.0 licence after the 12 month embargo period.

After the embargo period, everyone is permitted to use copy and redistribute this article for non-commercial purposes only, provided that they adhere to all the terms of the licence <https://creativecommons.org/licenses/by-nc-nd/3.0>

Although reasonable endeavours have been taken to obtain all necessary permissions from third parties to include their copyrighted content within this article, their full citation and copyright line may not be present in this Accepted Manuscript version. Before using any content from this article, please refer to the Version of Record on IOPscience once published for full citation and copyright details, as permissions may be required. All third party content is fully copyright protected, unless specifically stated otherwise in the figure caption in the Version of Record.

View the [article online](#) for updates and enhancements.

Microscopic fractures shown inside tablets after impact

Craig S. Carlson^{1,2*}, Michiel Postema^{1,2}, Nicole Anderton¹, Markus Hannula¹,
Joonas Sorjonen³, Hu Xinyue⁴, Naoyuki Otake⁴, Nobuki Kudo⁴, Jari Hyttinen¹, and
Jarkko Ketolainen³

¹*BioMediTech, Faculty of Medicine and Health Technology, Tampere University, Korkeakoulunkatu 3, 33720 Tampere, Finland*

²*School of Electrical and Information Engineering, University of the Witwatersrand, Johannesburg, 1 Jan Smuts Laan, 2001 Braamfontein, South Africa*

³*School of Pharmacy, PromisLab, University of Eastern Finland, Yliopistoranta 8, 70210 Kuopio, Finland*

⁴*Faculty of Information Science and Technology, Hokkaido University, Kita 14 Jo, Nishi 9 Chome, Kita-ku, Sapporo, Hokkaido 060-0814, Japan*

In prior work, rough handling of oral tablets had been observed to drastically speed up their disintegration in water. The purpose of this study was to confirm or refute that the formation of internal microscopic fractures during rough handling is the underlying mechanism. Impacted and control tablets were subjected to micro-computed tomography and to brightness-mode ultrasound. The former revealed fracturing with a maximum crack width of 14 μm . The latter revealed strong acoustic response from the internal structure of the impacted tablets. These results confirm the hypothesis. Disintegration speed is used as a quality control mechanism after tablet manufacturing and transportation.

Oral pharmaceutical tablets comprise compressed powders.¹⁾ After the pois compaction process,²⁾ the presence of microscopic gas pockets has been observed inside tablets³⁾ that are released during disintegration in water.⁴⁾ The pulsation behaviour of tablet gas micropockets in an ultrasound field has been associated with rapid ultrasound-assisted tablet disintegration.^{5,6)} Disintegration time has been of interest for quality checks during the manufacturing process.⁷⁾ The acoustic amplitudes during tablet monitoring must be less than the inertial cavitation threshold,⁸⁻¹²⁾ to prevent the formation of free radicals¹³⁾ and the deposition of heat.^{14,15)}

In a prior study, it was reported that tablet disintegration is accelerated after rough handling of tablets.¹⁶⁾ In this study, we investigated if rough handling visibly alters the internal structure of the tablets. Microtomography is a common methodology to study internal structures of materials.¹⁷⁻²⁰⁾

*E-mail: craig.carlson@tuni.fi

Throughout this study, microcrystalline cellulose was used, as this is a commonly used tablet matrix material.²¹⁾

Avicel PH102 microcrystalline cellulose powder (Agro Ireland Limited, Cork, Ireland) underwent controlled compaction as previously described.¹⁶⁾ The resulting tablets each had a mass of 0.4 g, a diameter of 10 mm, and a height of 4.4 mm. Rough handling was ensured by using a *tool of hard knocks*, subjecting seventy tablets to a nut drop in a controlled procedure.¹⁶⁾ Nut drops were recorded with a FASTCAM MC1 high-speed camera (Photron (Europe) Limited, West Wycombe, Bucks, United Kingdom) with an 8–50-mm zoom lens (Waveshare Electronics, Shenzhen, China). A typical example of a nut drop is shown in Figure 1.

A representative tablet that had been subjected to impact and a control tablet were prepared for micro-computed tomography, by fixating them in a customised scaffold of acrylonitrile butadiene styrene cuboids. The scaffold was positioned in the centre of a rotating plate inside a MICROXCT-400 device (Carl Zeiss AG, Oberkochen, Germany). The tomographic imaging procedure was similar to those previously described.^{22,23)}

The X-ray source was operating at a power of 10 W and at a peak voltage of 60 kV. An exposure time of 1 s was set per image, whilst a detection scintillator with a 4× objective was being used. A total number of 1601 projections were acquired, evenly distributed over 360°. The resulting voxel size corresponded to $2.8 \times 2.8 \times 2.8 \mu\text{m}^3$. Three-dimensional images were reconstructed from the raw data by making use of XMRe-creator 8.1.6599 software (Zeiss). These images were converted to Tag Image File Format for further processing and measurement with ImageJ 1.53t (National Institutes of Health, Bethesda, MD, USA) software.

A number of ten impacted tablets and ten control tablets were subjected to brightness-mode ultrasonography by operating a similar setup as used in prior experiments.^{6,16)} An HFL38x 13–6-MHz linear probe of a SonoSite® M-Turbo® sonography device (FUJIFILM SonoSite, Inc., Bothell, WA, USA) was clamped vertically such that its face directed towards a 1-SHP coin reflector that had been fixed on the bottom of a 1220 Arctic box container (Plast 1 A/S, Hørsholm, Denmark) of $115 \times 115 \times 55\text{-mm}^3$ outer dimensions.

The vertical distance between the probe face and the reflector was 14 mm. Before each experiment, the container was filled with degassed purified water whose temperature was measured to be 18°C. During sonication, a tablet was manually placed on top of the reflector. Sonication in two-dimensional musculoskeletal pulsed brightness mode with an estimated machine-indicated mechanical index of 0.8 and a machine-indicated thermal index of 0.1 continued for 60 seconds. During this time, no temperature change was measured *in situ*. The

mechanical index and thermal index are machine-indicated values that may not be related to the *in-situ* indices in our 250-ml volume. They have been stated for repeatability purposes. The broadband acoustic pulse was measured to have a peak-negative pressure amplitude of 3 MPa. The machine-indicated mechanical indices were confirmed by measurements in free-field conditions. Adding reflective surfaces was not observed to change the amplitudes of the short individual pulses measured.

Each experiment generated an output of 450 brightness-mode frames. These frames were processed using MATLAB[®] (The MathWorks, Inc., Natick, MA, USA). Our prior work showed an average swelling rate of $0.23 \pm 0.04 \text{ mm s}^{-1}$ for impacted and a swelling rate of $0.18 \pm 0.01 \text{ mm s}^{-1}$ for control tablets.¹⁶⁾ In the present study we concentrated on scattering data from within the tablets under sonication.

Figure 2 shows two representative tomographic slices of a impacted tablet. It should be noted that the cross-sections do not cover the whole tablet but only a limited region. Thin but visible fractures can be observed to run within the tablet. The maximum width of a crack was measured to be $14 \mu\text{m}$. In the control slices, such fractures were not visible. The fractures observed had highly irregular shapes. Therefore, measuring the crack volume of tablet fractures and the associated linear acoustic resonance frequency may prove to be challenging.

Figure 3 shows a representative brightness-mode ultrasonic imaging sequence of an impacted tablet and a control tablet positioned on a 1-SHP coin reflector during swelling and disintegration. The perceived distance measured from the frames has been superimposed on the dataset presented in our prior study.¹⁶⁾ The internal structure shows a strong acoustic response of the impacted tablet compared to the control. Its disintegration was observed to commence from the location of strongest acoustic response. We interpret this internal region of strongest acoustic response to coincide with the region of internal fracturing from the impact the tablet had been subjected to. It should be noted that ultrasound has been used in this study to speed up tablet disintegration and the measurements thereof. It has not been intended to represent actual *in-vivo* situations.

As for the mechanism behind the accelerated disintegration of fractured tablets, there is room for speculation. A straightforward explanation is that the fracture connects microscopic air pockets, speeding up the water absorption of the tablet after initial water ingress. The influence of electromagnetic fields on the hydrophobicity of the compacted powder has not been taken into account.

In conclusion, micro-computed tomography and brightness-mode ultrasound revealed mi-

croscopic fractures inside impacted tablets. Additionally, brightness-mode ultrasound images revealed a strong acoustic response from the internal structure of the impacted tablets. These results confirm the hypothesis that the formation of internal microscopic fractures during rough handling is the underlying reason for their accelerated disintegration in water. Disintegration time is used as a quality control test after tablet manufacturing and transportation.

Acknowledgements

This work was supported by JSPS KAKENHI, Grant Numbers JP17H00864 and JP20H04542, by the National Research Foundation of South Africa, Grant Number 127102, and by the Academy of Finland, Grant Number 340026.

References

- 1) J. T. T. Leskinen, S.-P. Simonaho, M. Hakulinen, and J. Ketolainen, *Int. J. Pharm.* **442**, 27 (2013).
- 2) M. Sim, M. Kim, K. Ha, and J. Kim, *Jpn. J. Appl. Phys.* **58**, SGGB02 (2019).
- 3) C. S. Carlson, M. Hannula, and M. Postema, *Curr. Dir. Biomed. Eng.* **8**, 41 (2022).
- 4) N. Anderton et al., *Curr. Dir. Biomed. Eng.* **9**, 25 (2023).
- 5) Y. Zhou, N. Gu, and F. Yang, *Int. J. Pharm.* **586**, 119615 (2020).
- 6) C. S. Carlson, N. Anderton, A. Pohl, A. J. Smith, N. Kudo, and M. Postema, *Jpn. J. Appl. Phys.* **61**, SG1030 (2022).
- 7) D. Markl and J. A. Zeitler, *Pharm. Res.* **34**, 890 (2017).
- 8) T. Uchida, H. Sato, S. Takeuchi, and T. Kikuchi, *Jpn. J. Appl. Phys.* **49**, 07HE03 (2010).
- 9) T. Uchida, S. Takeuchi, and T. Kikuchi, *Jpn. J. Appl. Phys.* **50**, 07HE01 (2011).
- 10) R. Takagi, S. Yoshizawa, and S. Umemura, *Jpn. J. Appl. Phys.* **50**, 07HF14 (2011).
- 11) G. Kang, J. S. Huh, and M. J. Choi, *Jpn. J. Appl. Phys.* **56**, 07JC08 (2017).
- 12) T. Uchida, *Jpn. J. Appl. Phys.* **60**, SDDD04 (2021).
- 13) T. Aikawa and N. Kudo, *Jpn. J. Appl. Phys.* **60**, SDDD13 (2021).
- 14) T. Moriyama, S. Yoshizawa, and S. Umemura, *Jpn. J. Appl. Phys.* **51**, 07GF27 (2012).
- 15) N. Obara, S. Umemura, and S. Yoshizawa, *Jpn. J. Appl. Phys.* **60**, SDDE04 (2021).
- 16) C. S. Carlson et al., *Proc. 44th UltraSonic Electronics Symp.*, 2023, 2P2-4.
- 17) K. Mizuno, K. Yamashita, Y. Nagatani, and M. Matsukawa, *Jpn. J. Appl. Phys.* **50**, 07HF19 (2011).
- 18) S. Koike et al., *Jpn. J. Appl. Phys.* **52**, 096602 (2013).
- 19) L. N. Q. Huy, C.-Y. Lin, and C.-C. A. Chen, *Jpn. J. Appl. Phys.* **61**, 071005 (2022).
- 20) L. N. Q. Huy and L. N. Q. Hoa, *Jpn. J. Appl. Phys.* **62**, 056502 (2023).
- 21) G. Thoorens, F. Krier, N. Leclercq, B. Carlin, and B. Evrard, *Int. J. Pharm.* **473**, 64 (2014).
- 22) J. Virta et al., *Sci. Rep.* **10**, 13164 (2020).
- 23) E. Nurkkala, M. Hannula, C. S. Carlson, A. Hopia, J. Hyttinen, and M. Postema, *Curr. Dir. Biomed. Eng.* **9**, 5 (2023).

List of Figures

Fig. 1. High-speed video of the impact of a nut, dropped from 82-cm height, on a tablet sandwiched between two 1-SHP coins. The line density of the mesh corresponds to 1 mm^{-1} . Timestamps have been added to the lower right corners.

Fig. 2. Micro-computed tomography images of two x - y cross-sections of an impacted tablet at heights of $z=1.3 \text{ mm}$ (a), and $z=1.8 \text{ mm}$ (c). The fractures visible in the original frames (a,c) have been highlighted in blue (b,d).

Fig. 3. Brightness-mode imaging sequences of an impacted (a) and a control (c) tablet positioned on a 1-SHP coin reflector during swelling and disintegration. The distances r' perceived between transducer and tablet were measured from these frames and superimposed on the dataset presented in our prior study (b),¹⁶⁾ where impacted and control tablets are indicated by $+$ and \circ , respectively. The linear swelling rate was $0.23 \pm 0.04 \text{ mm s}^{-1}$ for impacted tablets ($-$), and $0.18 \pm 0.01 \text{ mm s}^{-1}$ for control tablets ($-$). The centre of the red circle indicates a strong acoustic response within the impacted tablet. Timestamps relative to the graph time axis have been added to the lower right corners. 1-cm scale bars have been added to the lower left corners.

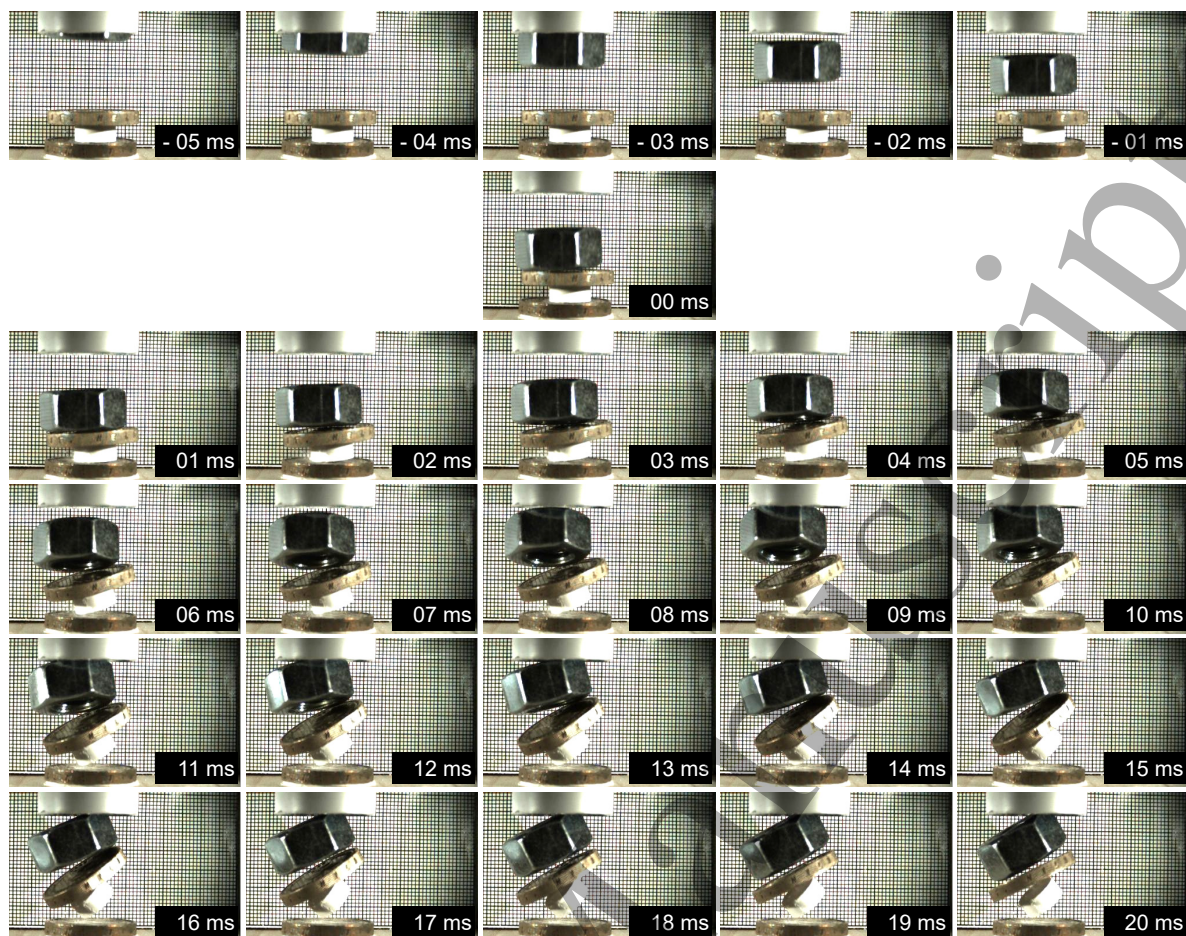


Fig. 1. High-speed video of the impact of a nut, dropped from 82-cm height, on a tablet sandwiched between two 1-SHP coins. The line density of the mesh corresponds to 1 mm⁻¹. Timestamps have been added to the lower right corners.

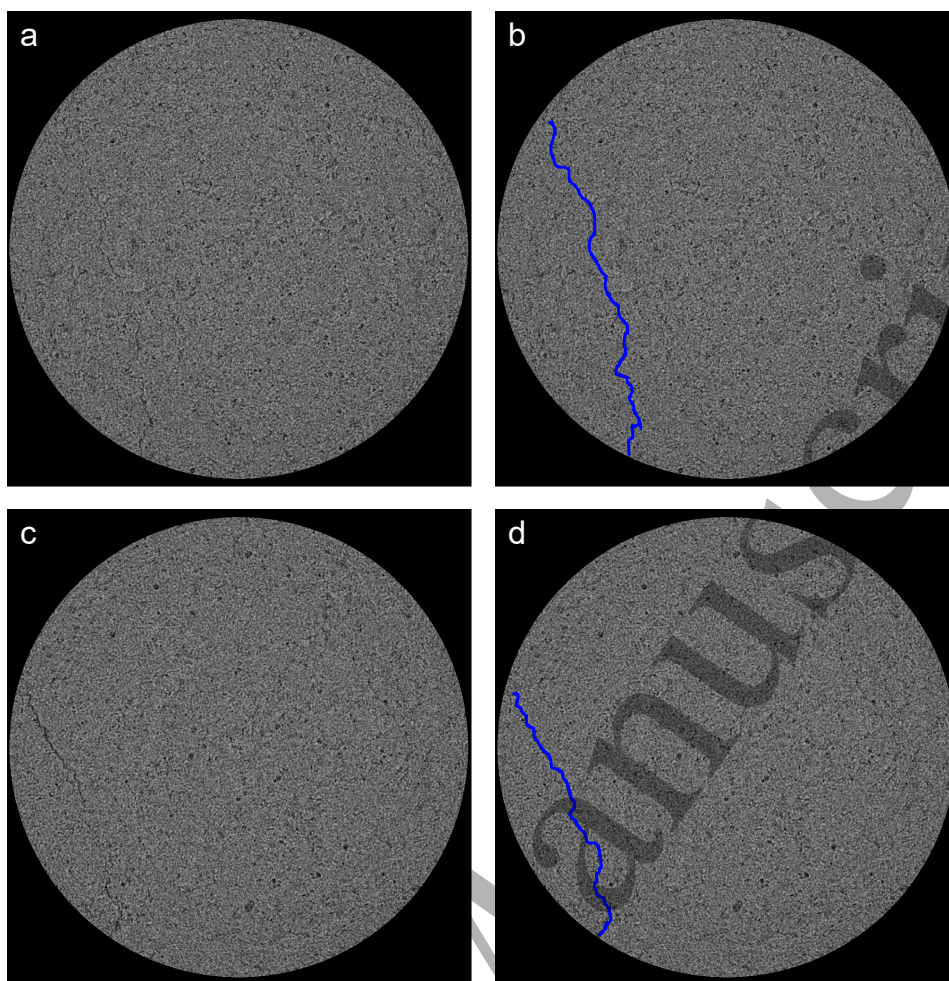


Fig. 2. Micro-computed tomography images of two x - y cross-sections of an impacted tablet at heights of $z=1.3$ mm (a), and $z=1.8$ mm (c). The fractures visible in the original frames (a,c) have been highlighted in blue (b,d).

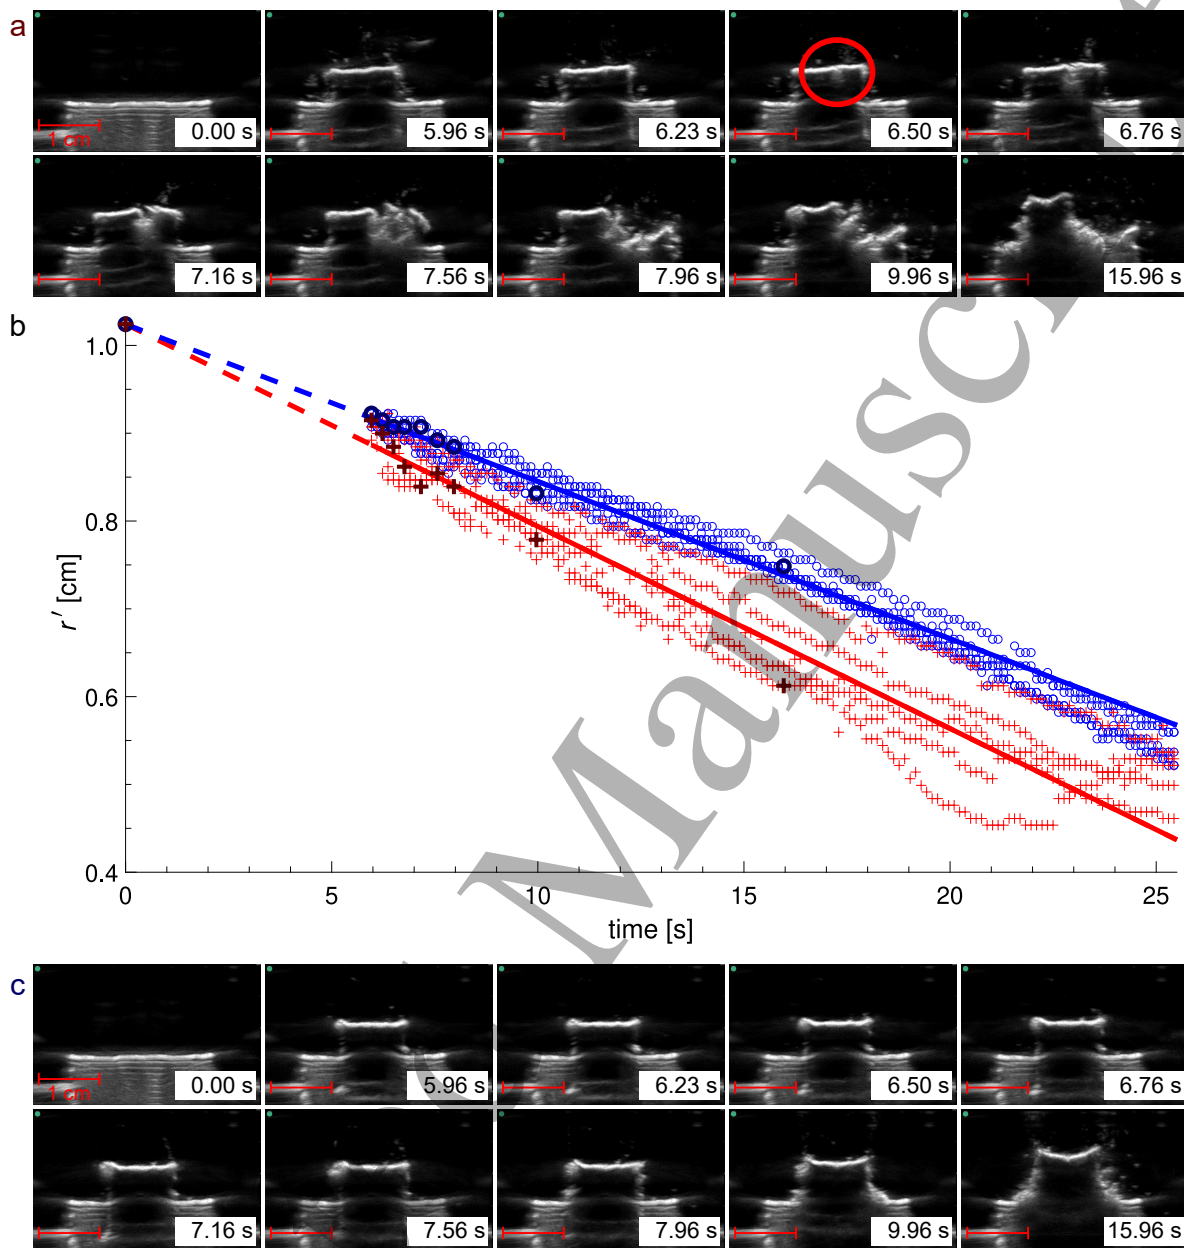


Fig. 3. Brightness-mode imaging sequences of an impacted (a) and a control (c) tablet positioned on a 1-SHP coin reflector during swelling and disintegration. The distances r' perceived between transducer and tablet were measured from these frames and superimposed on the dataset presented in our prior study (b),¹⁶⁾ where impacted and control tablets are indicated by $+$ and \circ , respectively. The linear swelling rate was $0.23 \pm 0.04 \text{ mm s}^{-1}$ for impacted tablets (---), and $0.18 \pm 0.01 \text{ mm s}^{-1}$ for control tablets (---). The centre of the red circle indicates a strong acoustic response within the impacted tablet. Timestamps relative to the graph time axis have been added to the lower right corners. 1-cm scale bars have been added to the lower left corners.