



**HAL**  
open science

## The effect of heat treatment on the mechanical behavior of an ASTM-F2063 nitinol stent intended for venous application

Achref Sallami, Pierrick Malecot, Fabrice Richard, Michaël Fontaine, Arnaud Lejeune, Sebastien David, Paul Vescovo, Christophe Moureaux, Philippe Stempfélé

### ► To cite this version:

Achref Sallami, Pierrick Malecot, Fabrice Richard, Michaël Fontaine, Arnaud Lejeune, et al.. The effect of heat treatment on the mechanical behavior of an ASTM-F2063 nitinol stent intended for venous application. E-MRS 2023 Spring Meeting, May 2023, Strasbourg, France. hal-04576558

**HAL Id: hal-04576558**

**<https://hal.science/hal-04576558>**

Submitted on 15 May 2024

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



# The effect of heat treatment on the mechanical behavior of an ASTM-F2063 nitinol stent intended for venous application

Achref Sallami<sup>1,2</sup>, Pierrick Malecot<sup>3,4</sup>, Fabrice Richard<sup>1</sup>, Michaël Fontaine<sup>3</sup>, Arnaud Lejeune<sup>1</sup>, Sébastien David<sup>2</sup>, Paul Vescovo<sup>2</sup>, Christophe Moureaux<sup>2</sup>, and Philippe Stempflié<sup>3</sup>

<sup>1</sup>Université de Franche-Comté, CNRS, institut FEMTO-ST, F-25000 Besançon, France  
<sup>2</sup>Cisteo MEDICAL, 1 rue Anne de Pardieu, F-25000 Besançon, France  
<sup>3</sup>SUPMICROTECH, CNRS, institut FEMTO-ST, F-25000 Besançon, France  
<sup>4</sup>Université de Bretagne Sud, CNRS, IRDL, F-56100 Lorient, France


## Objectives

1. Discuss the effect of heat treatment on the behavior of an ASTM-F2063 biomedical nitinol.
2. Maximizing the superelastic capacity of the stent in order to avoid irreversible plastic slippage and minimize the stiffness of the stent to limit the pressure on the diseased venous system.
3. Identifying the parameters of the material's constitutive law in order to simulate the behavior of the stent under mechanical loading.

## Abstract

Super elastic nitinol is an adaptive material belonging to the shape memory alloys (SMA) family. This material can reach a higher level of deformation and has the ability to return to its initial configuration by a simple discharge. This specific behavior and its biocompatibility favor the use of this material in the medical field with numerous applications. Among the best known medical applications of superelastic nitinol are self-expanding stents. In this work, the effect of heat treatment on the behavior of an ASTM-F2063 biomedical nitinol is studied. The main objectives of this work are, on the one hand, to maximize the superelastic capacity of the stent in order to avoid irreversible plastic slippage and to minimize the stiffness of the stent in order to limit the pressure on the diseased venous system and, on the other hand, to identify the parameters of the material's constitutive law in order to simulate the behavior of the stent under mechanical loading.

## Methodology

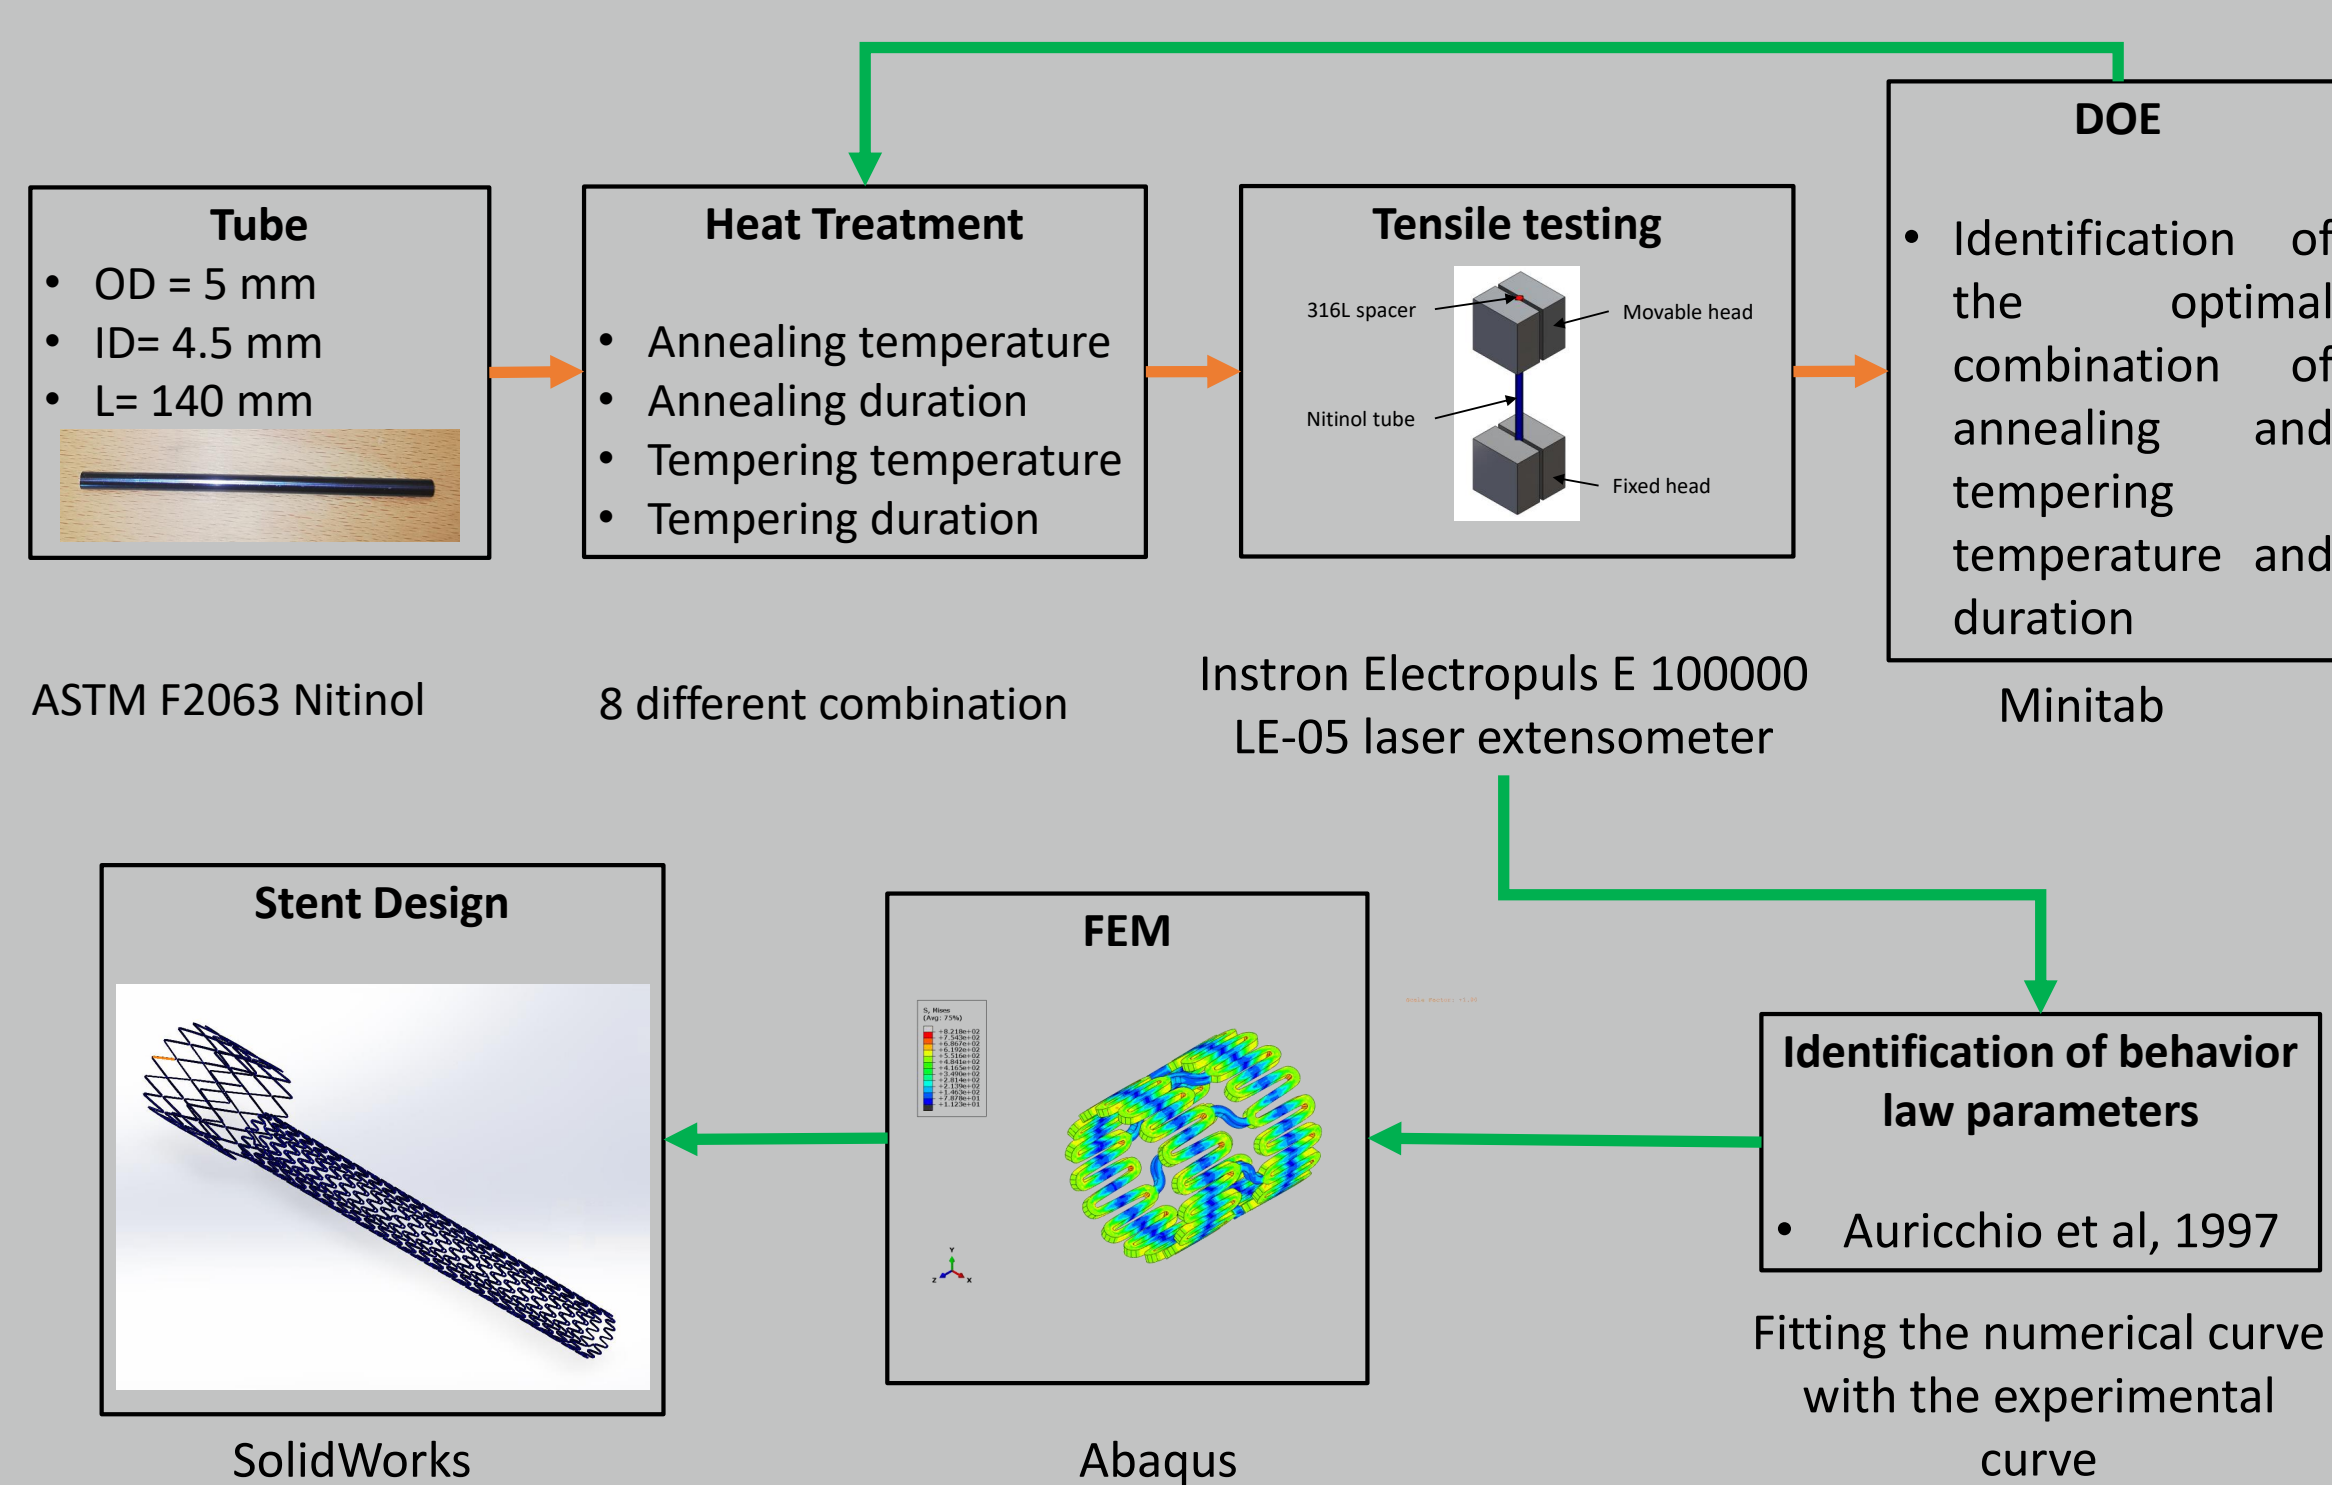

## DOE results

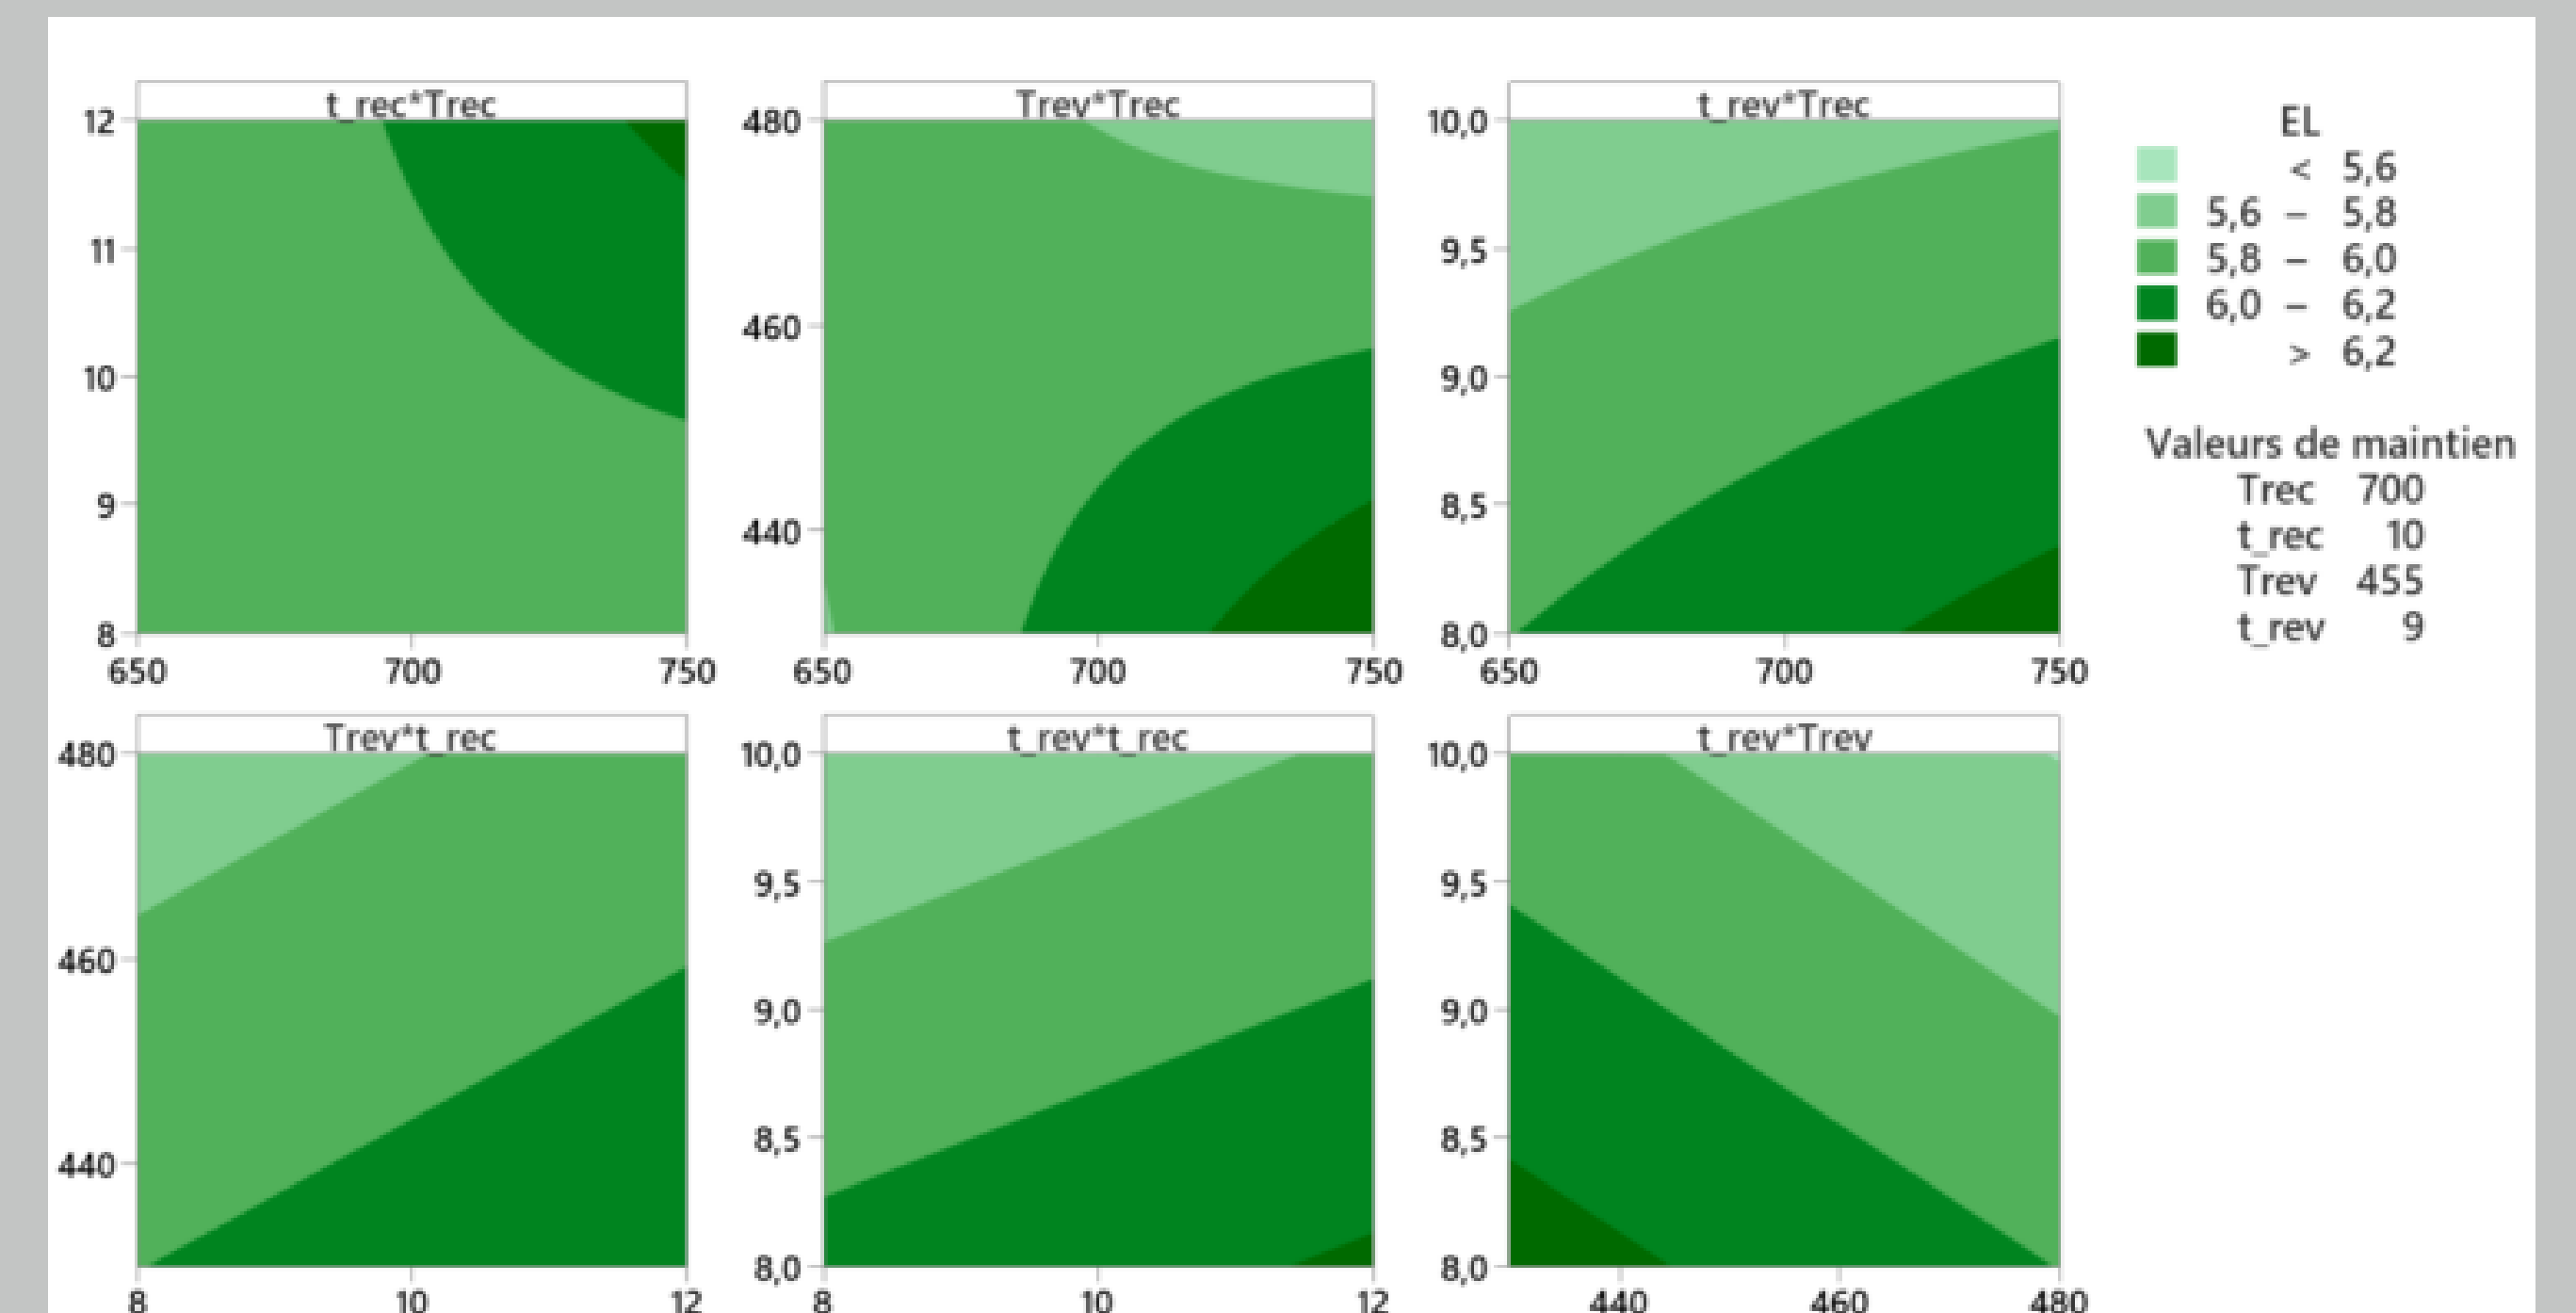


Figure 2: Contour plots of  $\epsilon_L$

Table 1: Optimized values of annealing temperature and duration, as well as tempering temperature and duration.

$$T_{annealing}=700^{\circ}\text{C}; t_{annealing}=10 \text{ min}; T_{tempering}=455^{\circ}\text{C}; t_{tempering}=9 \text{ min}$$

## Model response

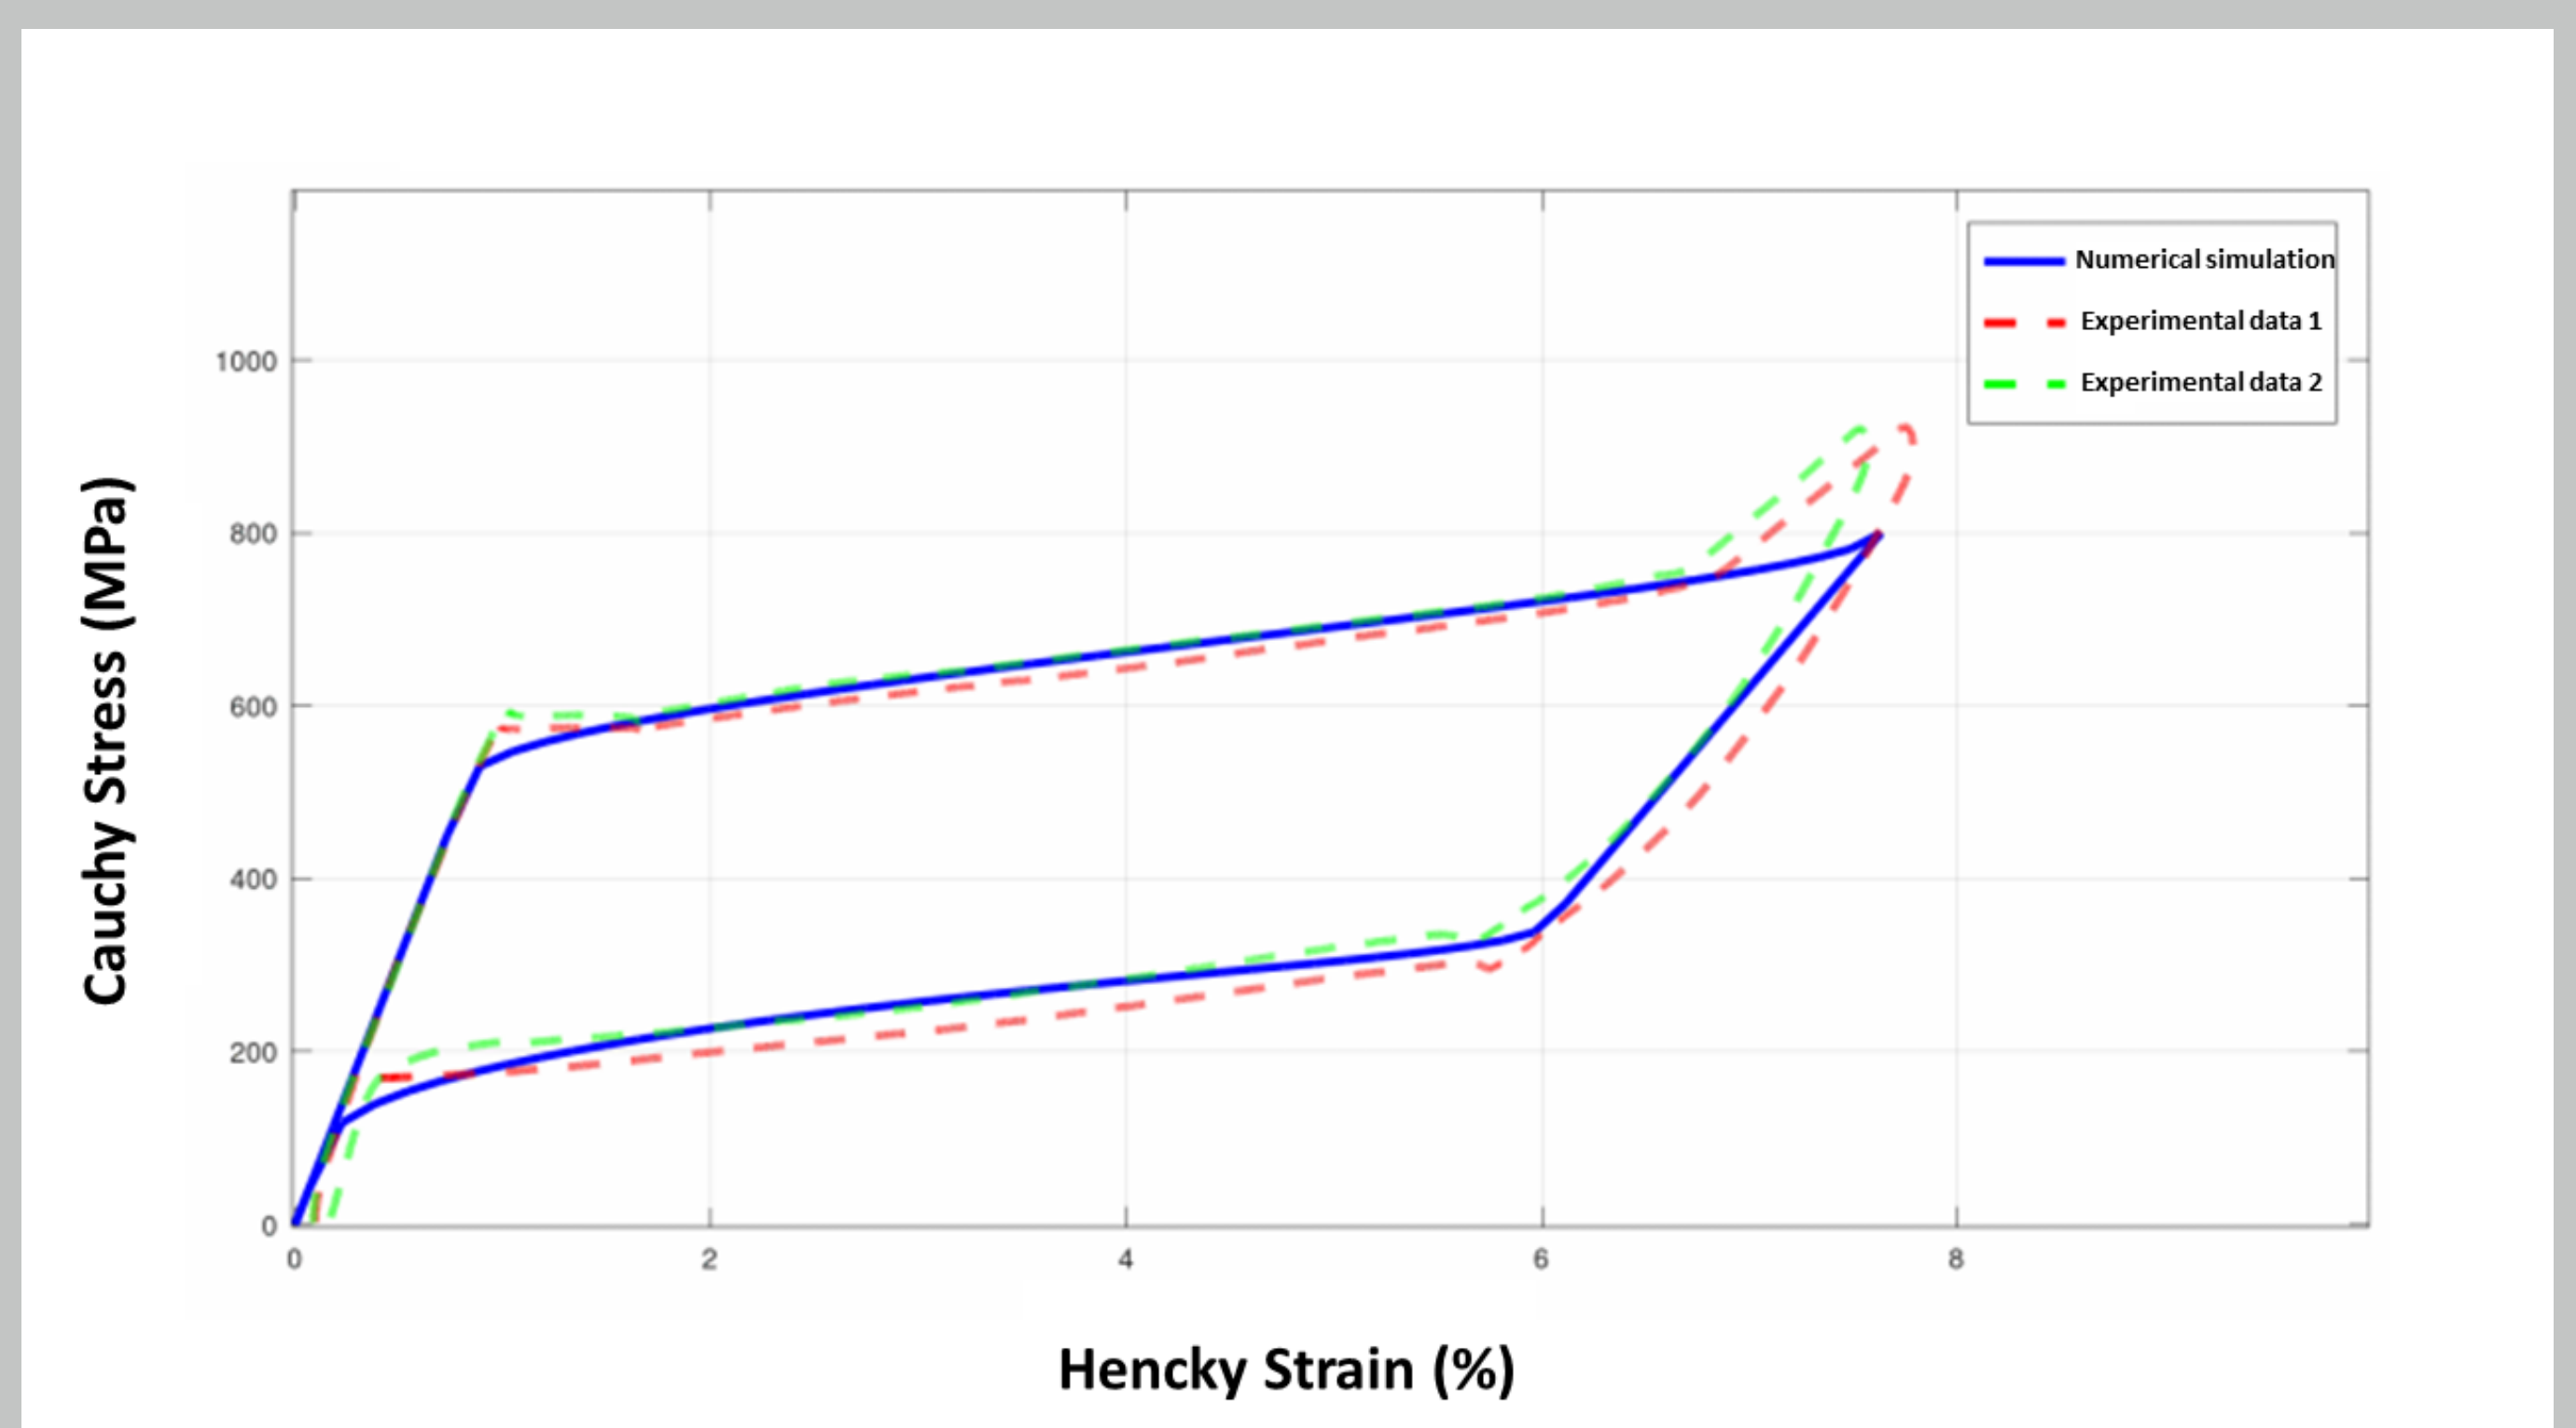


Figure 3: Experimental and Simulated Stress-Strain Behavior with Optimized Heat Treatment

Table 2: Model parameters for ASTM-F2063 nitinol [1]

Parameter	Value	Parameter	Value	Parameter	Value
$E_A$ (MPa)	61540	$E_M$ (MPa)	28230	$\nu_A$	0.33
$\nu_M$	0.33	$\epsilon_L$	0.05	$\sigma_S^{AM}$ (MPa)	540
$\sigma_f^{AM}$ (MPa)	800	$\sigma_S^{MA}$ (MPa)	350	$\sigma_f^{MA}$ (MPa)	100

## Heat Treatment Effects on the Mechanical Behavior of nitinol

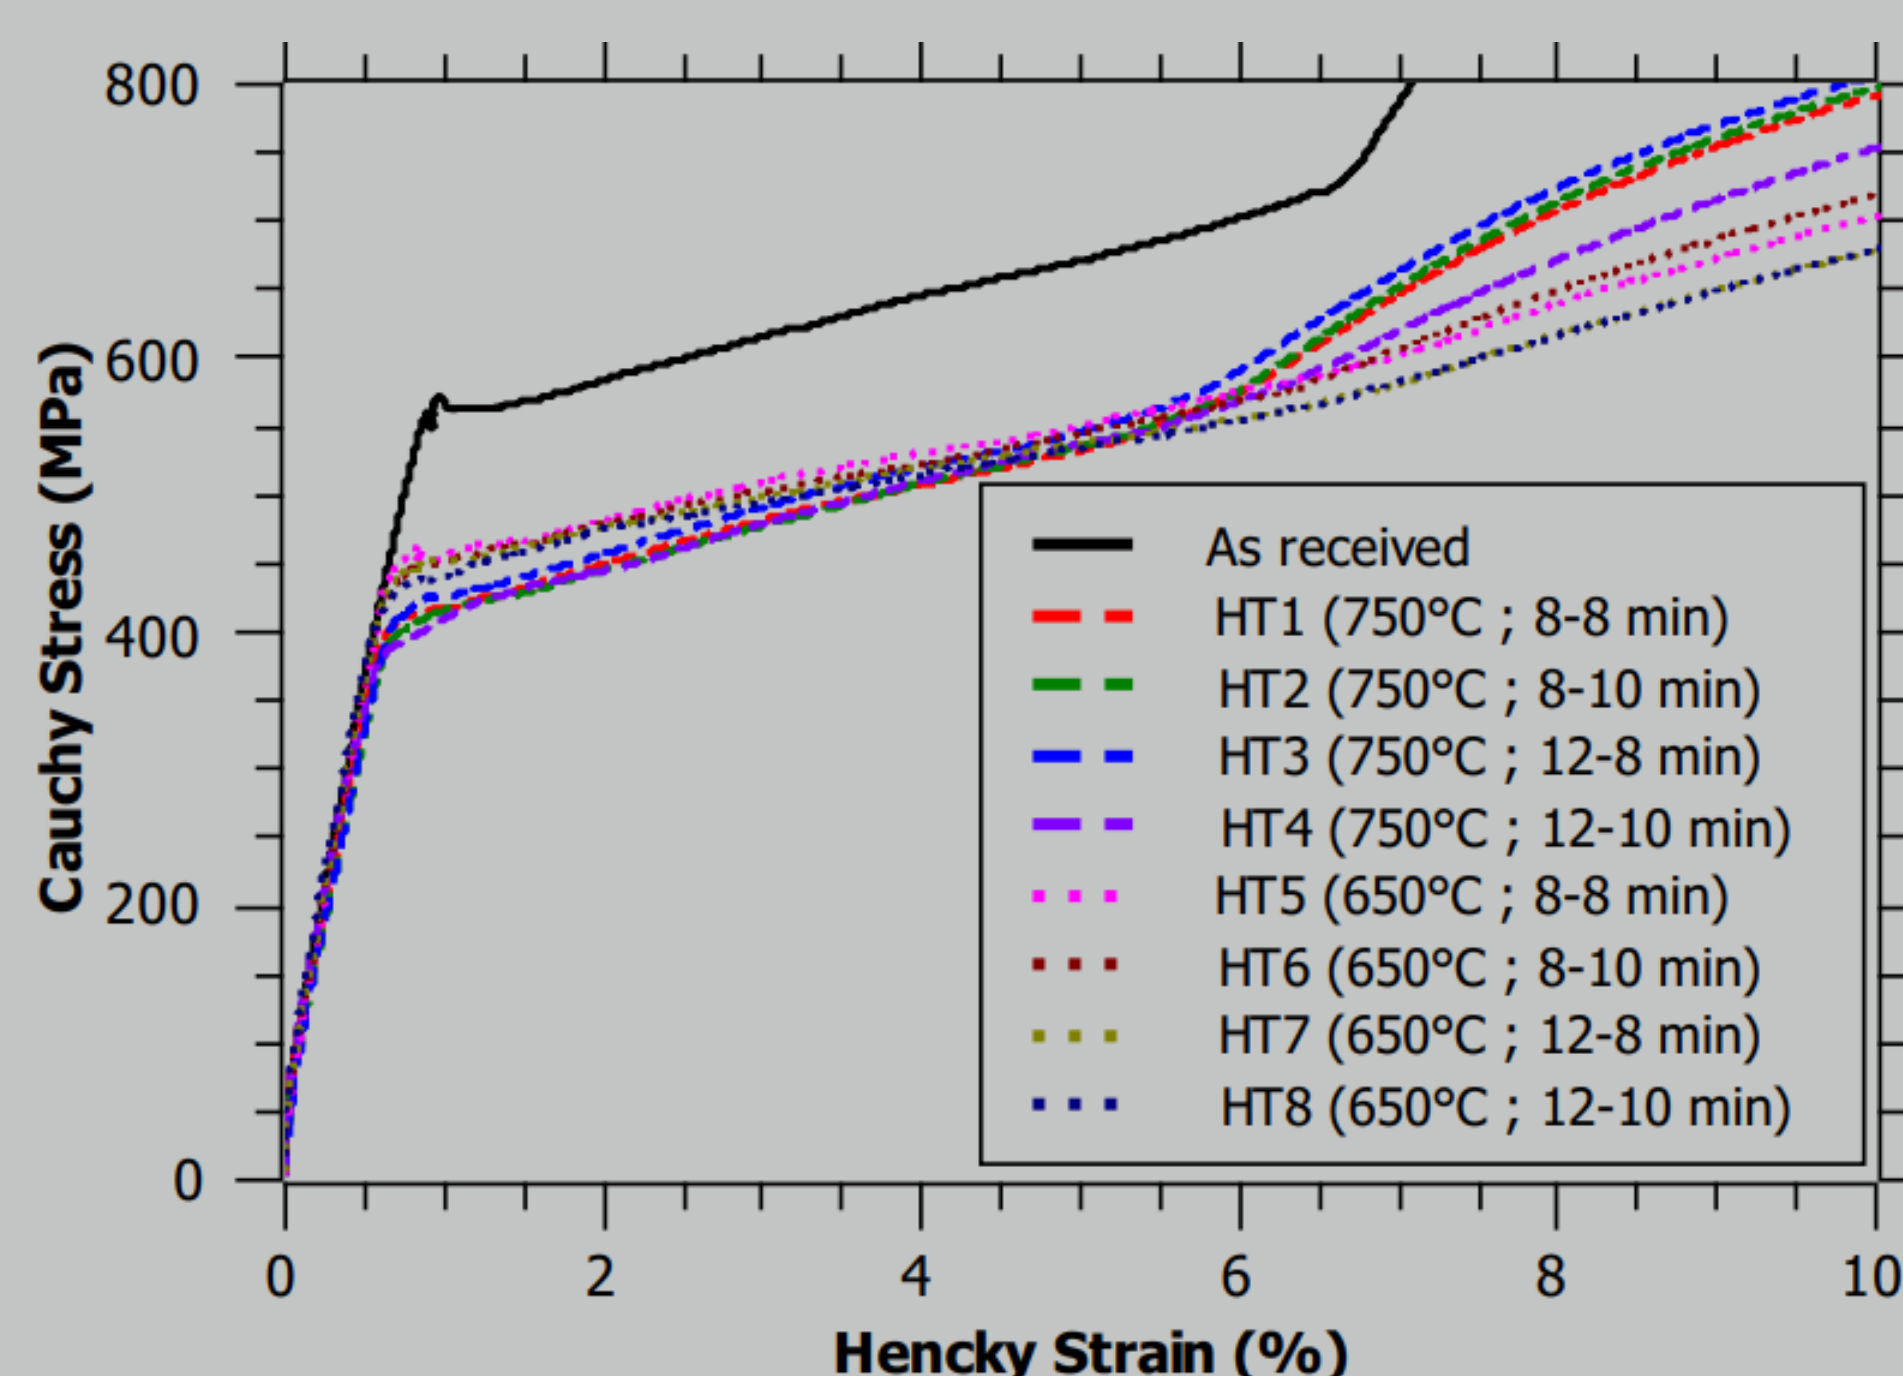


Figure 1: Comparative Tensile Test Curves of nitinol Samples with Varied Heat Treatments

## Acknowledgements

We are grateful to the FEMTO-ST research institute, the CNRS and the France Relance plan for the financial support of our research. Their generous funding allowed us to carry out our study and to obtain reliable and usable results.

## Conclusions

In this study, a Design of Experiments (DOE) approach was employed to optimize the behavior of medical nitinol ASTM-F2063 and identify model parameters for simulating stent response, specifically using the Auricchio model. Through careful experimentation and analysis, the following key findings have been obtained:

- Optimization of Nitinol Behavior: By systematically varying the heat treatment parameters, we were able to optimize the mechanical behavior of nitinol ASTM-F2063. The DOE study identified the optimal combination of annealing and tempering temperature and duration that maximizes the desired properties for stent applications.
- Model Parameter Identification: By correlating the experimental data with the simulation results using the Auricchio model [1], the model parameters that describe the behavior of nitinol has been defined.

## References

- [1] Ferdinando Auricchio and Robert L. Taylor. Shape-memory alloys: modelling and numerical simulations of the finite-strain superelastic behavior. *Computer Methods in Applied Mechanics and Engineering*, 143(1):175–194, 1997.