



**HAL**  
open science

## Deciphering simplified regional anticoagulation with citrate in intermittent hemodialysis: a clinical and computational study

Julien Aniort, Felix Richard, François Thouy, Louis Le Guen, Carole Philipponnet, Cyril Garrouste, Anne-Elisabeth Heng, Claire Dupuis, Mireille Adda, Durif Julie, et al.

### ► To cite this version:

Julien Aniort, Felix Richard, François Thouy, Louis Le Guen, Carole Philipponnet, et al.. Deciphering simplified regional anticoagulation with citrate in intermittent hemodialysis: a clinical and computational study. *Scientific Reports*, 2024, 14 (1), pp.19778. 10.1038/s41598-024-70708-9 . hal-04689240

**HAL Id: hal-04689240**

**<https://hal.science/hal-04689240v1>**

Submitted on 30 Jan 2025

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



Distributed under a Creative Commons Attribution 4.0 International License



OPEN

## Deciphering simplified regional anticoagulation with citrate in intermittent hemodialysis: a clinical and computational study

Julien Aniot<sup>1,2✉</sup>, Felix Richard<sup>1</sup>, François Thouy<sup>3</sup>, Louis Le Guen<sup>1</sup>, Carole Philipponnet<sup>1</sup>, Cyril Garrouste<sup>1</sup>, Anne Elisabeth Heng<sup>1,2</sup>, Claire Dupuis<sup>3</sup>, Mireille Adda<sup>4</sup>, Durif Julie<sup>5</sup>, Lebretonchel Elodie<sup>6</sup>, Laurent Chupin<sup>7</sup>, Damien Bouvier<sup>5</sup>, Bertrand Souweine<sup>3</sup> & Nicolae Cindea<sup>7</sup>

Regional citrate anticoagulation use in intermittent hemodialysis is limited by the increased risk of metabolic complications due to faster solute exchanges than with continuous renal replacement therapies. Several simplifications have been proposed. The objective of this study was to validate a mathematical model of hemodialysis anticoagulated with citrate that was then used to evaluate different prescription scenarios on anticoagulant effectiveness (free calcium concentration in dialysis filter) and calcium balance. A study was conducted in hemodialyzed patients with a citrate infusion into the arterial line and a 1.25 mmol/L calcium dialysate. Calcium and citrate concentrations were measured upstream and downstream of the citrate infusion site and in the venous line. The values measured in the venous lines were compared with those predicted by the model using Bland and Altman diagrams. The model was then used with 22 patients to make simulations. The model can predict the concentration of free calcium, bound to citrate or albumin, accurately. Irrespective of the prescription scenario a decrease in free calcium below 0.4 mmol/L was obtained only in a fraction of the dialysis filter. A zero or slightly negative calcium balance was observed, and should be taken into account in case of prolonged use.

**Keywords** Hemodialysis, Calcium, Citrate, Dialysate, Modeling, Anticoagulation

### Abbreviation

CRRT Continuous renal replacement therapy

The European ERA-EDTA guidelines for chronic hemodialysis<sup>1</sup> and international KDIGO guidelines for hemodialysis during acute kidney injury<sup>2</sup> have made recommendations for anticoagulation of the blood circuit in intermittent hemodialysis to the effect that heparin or low molecular weight heparin should be used in the absence of hemorrhagic risk and no anticoagulation should be used in the case of hemorrhagic risk. The absence of anticoagulation entails the risk of impairing dialysis efficacy and premature discontinuation because of clotting. Alternatives have been proposed. It is now well established that repetitive blood circuit flushing or pre-dilution are ineffective. Coating membranes with heparin or vitamin E provides better results but is less effective than anticoagulation with heparin<sup>3–5</sup>.

Citrate anticoagulation is a regional blood circuit anticoagulation technique currently used in routine practice for continuous renal replacement therapy (CRRT), where it is recommended regardless of the hemorrhagic

<sup>1</sup>Nephrology, Dialysis and Transplantation Department, CHU Clermont-Ferrand, Gabriel Montpied Hospital, CHU G. Montpied, 58 Rue Montalembert, 63000 Clermont-Ferrand, France. <sup>2</sup>INRAE UMR 1019, Human Nutrition Unit, Clermont Auvergne University, Clermont-Ferrand, France. <sup>3</sup>Intensive Care Unit, CHU Clermont-Ferrand, Gabriel Montpied Hospital, Clermont-Ferrand, France. <sup>4</sup>Clinical Research Department, CHU Clermont-Ferrand, Gabriel Montpied Hospital, Clermont-Ferrand, France. <sup>5</sup>Biochemistry Department, CHU Clermont-Ferrand, Gabriel Montpied Hospital, Clermont-Ferrand, France. <sup>6</sup>Biochemistry Department, CHU Lille, Lille, France. <sup>7</sup>Blaise Pascal Mathematics Laboratory, UMR 6620, Clermont Auvergne University, CNRS, Cezeaux Campus, Clermont-Ferrand, France. ✉email: janiort@chu-clermontferrand.fr

risk<sup>2</sup>. It is based on the property of citrate molecules to chelate calcium ions in plasma. Calcium is necessary for the cascade activation of clotting factors. In addition to its anticoagulant properties, citrate helps to reduce the inflammatory response induced by hemodialysis<sup>6</sup>. A concentrated solution of sodium citrate is infused into the arterial line upstream of the dialysis membrane. A recent meta-analysis confirmed the advantage of citrate over heparin showing that citrate anticoagulation can reduce the incidence of bleeding and transfusion requirements during CRRT and increase the duration of use of the dialysis filter<sup>7</sup>. However, this technique has the drawback of requiring close biological monitoring, especially with intermittent hemodialysis, in which solute exchanges are faster. An alternative technique has been proposed involving use of a calcium-free dialysate with or without citrate and reinfusion of a calcium-containing solution into the venous line. The amount of calcium ions lost in the dialysate is estimated as being equal to the product of the dialysance and the patient's free calcium. The calcium infusion rate is readjusted regularly during the session according to dialysance value<sup>8–11</sup>.

To simplify the procedure and guarantee a safe use in intermittent hemodialysis, a regional citrate anticoagulation technique using a dialysate containing calcium has been developed. It ensures that the patient's serum calcium level is maintained by establishing a balance between the calcium concentration of the dialysate and the patient's free serum calcium. In addition, the quantity of citrate returning to the patient and having to be metabolized in the liver is significantly reduced by elimination of the majority of citrate calcium complexes in the effluent dialysate. Evenopoe et al.<sup>12</sup> showed that this simplified technique was safe, effective and easier to implement than with a calcium-free dialysate. Fiaccadori et al.<sup>13</sup> showed that the use of a dialysate supplemented with calcium in patients treated with slow extended hemodialysis was an effective alternative to dialysate without calcium and compensation by post-filter calcium infusion. We recorded the results of its use in our department and found it was easy to implement, had stable dialysis efficacy and safety but could be associated with an increased risk of circuit clotting compared to heparin anticoagulation<sup>14</sup>. This manifest in premature stopping of dialysis and thus sub-optimal treatment to patients. Precise knowledge of the calcium and citrate concentrations in the dialyzer is essential to be able to optimize the technique. However, direct measurement is not possible in real practice.

In this context, the objectives of this study were to validate a mathematical model of intermittent hemodialysis using regional citrate anticoagulation and to use the model to study the impact of prescription parameters on anticoagulant effectiveness (reduction in free calcium in the blood circuit) and safety of use (patient calcium balance).

## Material and methods

### Population

A prospective study was conducted in the hemodialysis unit of the Clermont-Ferrand university hospital center, France, between January and December 2021. Patients aged over 18 years and treated with intermittent hemodialysis for renal failure were included. The non-inclusion criteria were severe hepatocellular insufficiency (prothrombin time < 50%, INR > 1.5 without anticoagulant), a hemoglobin level < 7 g/dL, and patients with psychiatric pathology or cognitive disorders. The study was carried out according to the Declaration of Helsinki, its protocol was approved by the Sud Ouest IV Research Ethics Committee (IORG009855) and registered at ClinicalTrials.gov (NCT04530175). All participants provided written informed consent.

### Citrate anticoagulation protocol

Patients were treated with AK200 Gambro or Nikkiso DBB07 dialysis machines. Regional anticoagulation with citrate was carried out according to the protocol previously described<sup>14</sup>. Briefly, a 4% citrate solution (136 mmol/L) was infused into the arterial line of the blood circuit with a flow rate proportional to the blood flow (citrate 4% flow rate (mL/hour) = 1.75 × blood flow rate (mL/min)) in order to achieve a citrate concentration of 0.40 mmol per 100 mL of blood flow<sup>14</sup>. A dialysate with a calcium concentration of 1.25 mmol/L was used. The total ultrafiltration volume takes into account the infused volume of citrate solution (ultrafiltration volume = net ultrafiltration volume + infused volume of citrate solution). The blood and dialysate flow rates, the sodium, potassium and bicarbonate contents of the dialysate, and the net ultrafiltration volume were left to the discretion of the prescribing physician.

### Measures

At H0, H1 and H4 a sample was taken in the arterial line upstream of the citrate injection site (patient), at H1 in the arterial line downstream of the citrate injection site (prefilter) and in the venous line (postfilter) (Supplementary Fig. S1). The samples were processed by a blood gas analyzer (GEM Premier 4000 Instrumental Laboratory®). Measurements were made of PO<sub>2</sub>, SaO<sub>2</sub>, PCO<sub>2</sub>, pH and bicarbonate, hematocrit, sodium, potassium and free calcium. At H1, blood samples were taken from the patient and prefilter sites. The tubes were sent to the biochemistry laboratory of Clermont-Ferrand University Hospital for determination of total calcium, phosphate, magnesium, urea and albumin. Dry tubes with separator were centrifuged and the serum was collected (within 4 h after collection) and stored at -20 °C. The frozen serum was sent to the biochemistry laboratory of Lille University Hospital for citrate measurement. Calcium balance  $\Delta Ca$  was calculated according to the following equations.

$$\Delta Ca = Ca_{totaloutlet} \times (1 - ht_{outlet}) \times Q_{bloodoutlet} - Ca_{totalinlet} \times (1 - ht_{inlet}) \times Q_{bloodinlet}$$

## Calculations

The dissociation constants of calcium-citrate and calcium-albumin binding site complexes were estimated by nonlinear regression from measurements taken in patients at the prefilter and postfilter sites. The equation used gave the total serum calcium as the sum of the free calcium and calcium complexed with citrate or albumin.

$$c_{BCa_{tot}} = c_{BCa_i} + \frac{c_{BCa_i}}{c_{BCa_i} + K_{dCit}} \cdot c_{BCit} + \frac{c_{BCa_i}}{c_{BCa_i} + K_{dalb}} \cdot c_{Balb}$$

The same equation was used to calculate the concentrations of the five species in solution (free calcium, calcium-citrate, and calcium-albumin binding site, free albumin binding site and free citrate)<sup>15</sup> at the prefilter site. The rate of the association and dissociation reactions of the calcium-citrate and calcium-albumin binding site complexes were retrieved from literature data and adapted so that the ratio of the rate constants corresponded to the finding of dissociation at equilibrium<sup>16</sup>.

## Modeling

The mathematical model used to calculate the calcium concentration during intermittent hemodialysis treatment has been described in detail elsewhere<sup>16</sup>. The model comprises two parts. The first describes the flow of blood and dialysate through a dialysis filter fiber and is made up of three coupled partial differential equations, two Navier–Stokes equations modeling the flow of blood and the flow of dialysate, combined with a Darcy law describing the porous flow through the membrane. The second part of the model is a reaction–convection–diffusion system that describes the spatial evolution of the concentrations of the five chemical species in a fiber from the dialysis filter. The fluid speeds calculated by the first part of the model intervene in the convective term of the reaction–convection–diffusion system. In order to take into account that the albumin do not cross the membrane we consider a Robin type boundary.

condition on the interface blood/porous membrane:

$$D_{alb} \frac{\partial c_{alb}}{\partial n} = v \cdot n \cdot c_{alb}$$

These conditions produce the increase of the albumin concentration in blood proportional to the ultrafiltration flow rate. We were particularly interested in the concentrations in the blood at the outlet of the dialysis filter and the values of these concentrations at the blood/membrane interface. To numerically simulate this model we developed a calculation code based on the finite element method using the FreeFEM Language<sup>17</sup>.

## Statistical analysis

To study the agreement between the measured value and the values calculated by the model for total and free calcium, the number of subjects was calculated from the hypothesis of nullity of the Lin concordance coefficient, which makes it possible to study the intensity of the concordance that might exist between quantitative parameters. Thus, to detect a concordance coefficient  $r$  statistically of at least 0.7, it was necessary to include 20 subjects for a bilateral risk of 5% and a power of 90%. In view of these elements, we decided to recruit 30 patients. Statistical analyses were performed with R (version 3.6.3) and Graphpad software (version 8.0.0). The qualitative variables were expressed as numbers and associated percentages and the quantitative variables by means ( $\pm$  standard deviation) and medians (with range). Values of quantitative variables were compared by Student's  $t$  test for paired data or repeated measures ANOVA followed by post-hoc Bonferroni test (normality of distribution assessed by the Shapiro–Wilk test). To study the agreement between the measured values and the values calculated by the model, the results were represented in the form of a Bland and Altman graph. Bias (average of differences) and dispersion index (95% confidence interval of difference between measured and calculated value) values were calculated.

## Results

### Patient characteristics

A total of 30 patients were included. One patient had zero dialysate flow at the time of sampling, and for 7 others laboratory analyses were missing. Hence, final analysis was made of 22 patients, of whom 5 had zero citrate flow at the time of sampling. Their data were not used to describe the variations in calcium and citrate concentrations according to the citrate anticoagulation protocol but retained in the evaluation of the model of exchanges in the dialysis filter. The characteristics of the study population are summarized in Table 1. For the 17 patients who received citrate infusion, citrate 4% flow was  $452 \pm 31.6$  mL/hour.

### Evolution of calcium and citrate concentrations in the blood circuit

The measurement of free calcium after one hour of citrate infusion at the different sampling sites of the circuit is shown in Fig. 1A. The free calcium at the patient sampling site was  $1.052 \pm 0.1159$  mmol/L: it decreased after pre-dialysis filter citrate infusion to  $0.1979 \pm 0.05782$  mmol/L and rose postfilter to  $0.8895 \pm 0.1137$  mmol/L. For each patient, free serum calcium was measured at the patient sampling site at different times of the dialysis session (H0, H1 and H4). The results are shown in Fig. 1B with  $1.038 \pm 0.081$  mmol/L at H0,  $1.035 \pm 0.110$  mmol/L at H1, and  $1.010 \pm 0.079$  mmol/L at H4. There was no clinically relevant variation in patient free serum calcium during a session. Measurements of citrate concentrations at H1 at the pre- and postfilter sites are shown in Fig. 1C. The prefilter citrate concentration was  $6369 \pm 1510$   $\mu$ mol/L and was only  $596.6 \pm 295.9$   $\mu$ mol/L postfilter. The relationship between free calcium and citrate concentration is shown in Fig. 1D. A decrease in free serum

Characteristics	n = 22
Men n (%)	17 (77.2)
Age (years)	62.9 ± 11.4
Dialysis vintage (months)	3.8 [0.5–45.7]
Comorbidities n (%)	
Cardiovascular disease	20 (90.9)
Respiratory disease	8 (36.4)
Hepatopathy	6 (27.3)
Cancer	7 (31.8)
Diabetes	9 (40.9)
Tobacco	4 (18.2)
Dyslipemia	10 (45.5)
Dialysis duration (min)	228/23.6
Vascular access n (%)	
Tunneled catheter	6 (27.3)
Non-tunneled cathéter	8 (36.4)
Arteriovenous fistula	8 (36.4)
Hémodialysis machine n (%)	
DBB07 Nikiso*	10 (45.5)
AK200 Gambro*	12 (55.5)
Blood flow (mL/min)	259 ± 19.7
Dialysate flow (mL/min)	500 ± 0
Ultrafiltration rate (mL/h)	706 ± 258
Filter surface (m <sup>2</sup> )	2.05 ± 0.11

**Table 1.** Patients characteristics.

calcium was observed with increasing citrate concentration. A citrate concentration of at least 3000  $\mu\text{mol/L}$  was required to achieve a free calcium level below 0.4  $\text{mmol/L}$ . Total calcium balance was  $-1.72 \pm 1.15$   $\text{mmol/hour}$ .


### Modeling

The dissociation constants of calcium-citrate ( $K_d$  calcium-citrate) and the calcium-albumin binding site complex ( $K_d$  calcium-albumin) were estimated to be  $4.034 \times 10^{-4} \pm 2.301 \times 10^{-5}$  and  $7.073 \times 10^{-3} \pm 6.156 \times 10^{-4}$ , respectively. The rate constants of the association or dissociation reactions of the calcium-citrate and calcium-albumin binding site complexes chosen are provided in supplemental data. The values of the concentrations of free calcium, free citrate, calcium-citrate, free albumin binding site and calcium-albumin binding site calculated from the measurements at the filter outlet and the values calculated by the model from the data at the dialysis filter inlet are shown in Table 2. The Bland and Altman diagrams comparing the concentration values measured and calculated by the model are presented in Fig. 2. The bias values and the corresponding 95% agreement interval are shown in Table 3.

### Simulations

The model was used to conduct several simulations for a putative patient (supplemental data), with varying blood, dialysate, and citrate infusion flow rates. The proportion of fiber length for which the ionized calcium is  $< 0.4$   $\text{mmol/L}$  reflects the effectiveness of blood anticoagulation in the dialysis filter<sup>18</sup>. This proportion increases when blood flow increases or dialysate flow decreases. The results are reported in Fig. 3A. Total, free serum calcium, and calcium balance are given in Figs. 3B,C and D. All three decrease as blood flow increases, dialysate flow decreases or citrate infusion increases. Total calcium balance was  $-1.37$   $\text{mmol/h}$  with a 250  $\text{mL/min}$  blood flow, a 500  $\text{mL/min}$  dialysate flow and a 5  $\text{mmol/L}$  blood citrate concentration.

Our model was also used to compute a dialysis session using a citrate dialysate without calcium, and then a dialysate with neither citrate nor calcium. The results are given in Supplementary Figs. S2A–D and S3A–D. Of note, free calcium was below 0.4  $\text{mmol/L}$  only in the last part of the filter. The losses of calcium ions in the dialysate are usually estimated to be equal to the product of dialysance (ionic<sup>8</sup> or dialysance measured by UV absorptiometry on the effluent dialysate<sup>9</sup> depending on the dialysis machine used) and the patient's free calcium. This estimation is based on two hypotheses. First, only free calcium and calcium complexed (mostly) with citrate can cross the membrane i.e. the release of calcium from albumin is negligible because it is thought to be too slow. This is equivalent to the situation of blood without albumin and a total serum calcium equal to the free calcium and calcium citrate. Secondly calcium citrate and free calcium have dialysance equal to that of small solutes like sodium or urea. However, literature data indicate a diffusibility of calcium citrate about twofold lower than that of calcium<sup>19</sup>. Using the model, we calculated the calcium balance for different blood and dialysate flow rates. For example, with a blood flow rate of 250  $\text{mL/min}$  and a dialysate flow rate of 500  $\text{mL/min}$  free calcium is

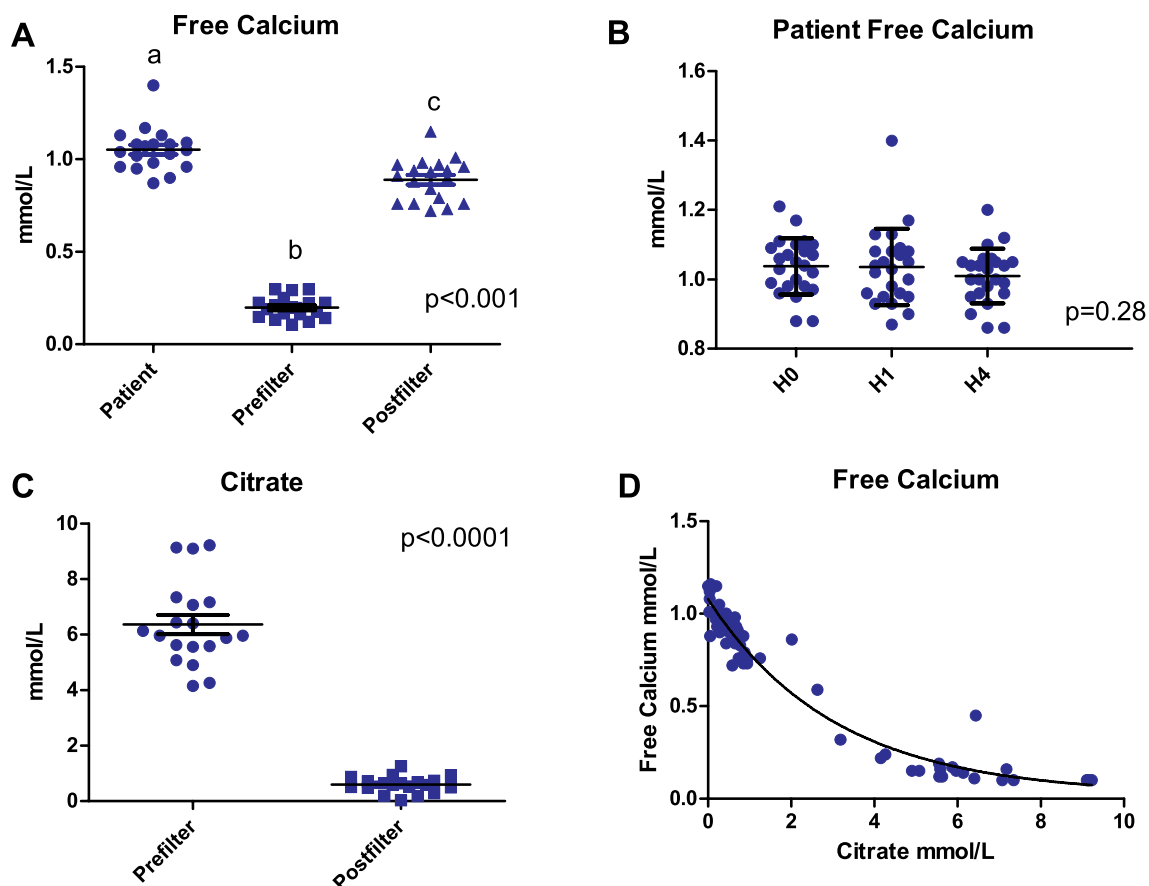

**Fig. 1.** (A) Free calcium measured in blood at H1 on the arterial line upstream of the citrate injection site (patient), on the arterial line downstream of the citrate injection site (prefilter) and on the venous line (postfilter). P-value of ANOVA for repeated measures. Values with different letters are significantly different with post-hoc Bonferroni test. (B) Patient free calcium measured at H0, H1 and H4. P-value of ANOVA for repeated measures. (C) Serum citrate concentration pre- and postfilter. P-value of paired T test. (D) Free calcium vs citrate concentration. Black line represents polynomial regression.

	Measured	Predicted
Free calcium (mmol/L)	$0.923 \pm 0.141$	$0.979 \pm 0.160$
Calcium-citrate (mmol/L)	$0.344 \pm 0.228$	$0.282 \pm 0.167$
Citrate (mmol/L)	$0.165 \pm 0.121$	$0.130 \pm 0.090$
Calcium-albumin binding site (mmol/L)	$0.619 \pm 0.143$	$0.640 \pm 0.145$
Albumin binding site (mmol/L)	$4.76 \pm 0.974$	$4.682 \pm 1.016$
Total calcium (mmol/L)	$1.89 \pm 0.210$	$1.97 \pm 0.108$


**Table 2.** Measured and predicted blood concentrations post-filter.

– 10.74 mmol/hour whereas it is – 19.9 mmol/hour when albumin and calcium-albumin are added to the model with a calcium-free dialysate containing 0.8 mmol/L citrate, and – 18.9 mmol/hour with a dialysate containing neither calcium nor citrate.

## Discussion

In this study we evaluated the impact on calcium exchanges of simplified regional citrate anticoagulation techniques in hemodialysis. The results obtained made it possible to validate modeling of calcium exchanges in the dialysis filter. The model was then used to determine the effects of the dialysis prescription parameters (i.e. dialysate, blood and citrate infusion flows) on anticoagulant effectiveness and calcium balance.

When using citrate infusion and a 1.25 mmol/L calcium-containing dialysate, the post-filter free calcium level does not decrease significantly compared to that measured pre-filter before citrate infusion. The diffusive exchange of calcium from the dialysate is sufficient to restore the patient's free calcium. Free calcium into the

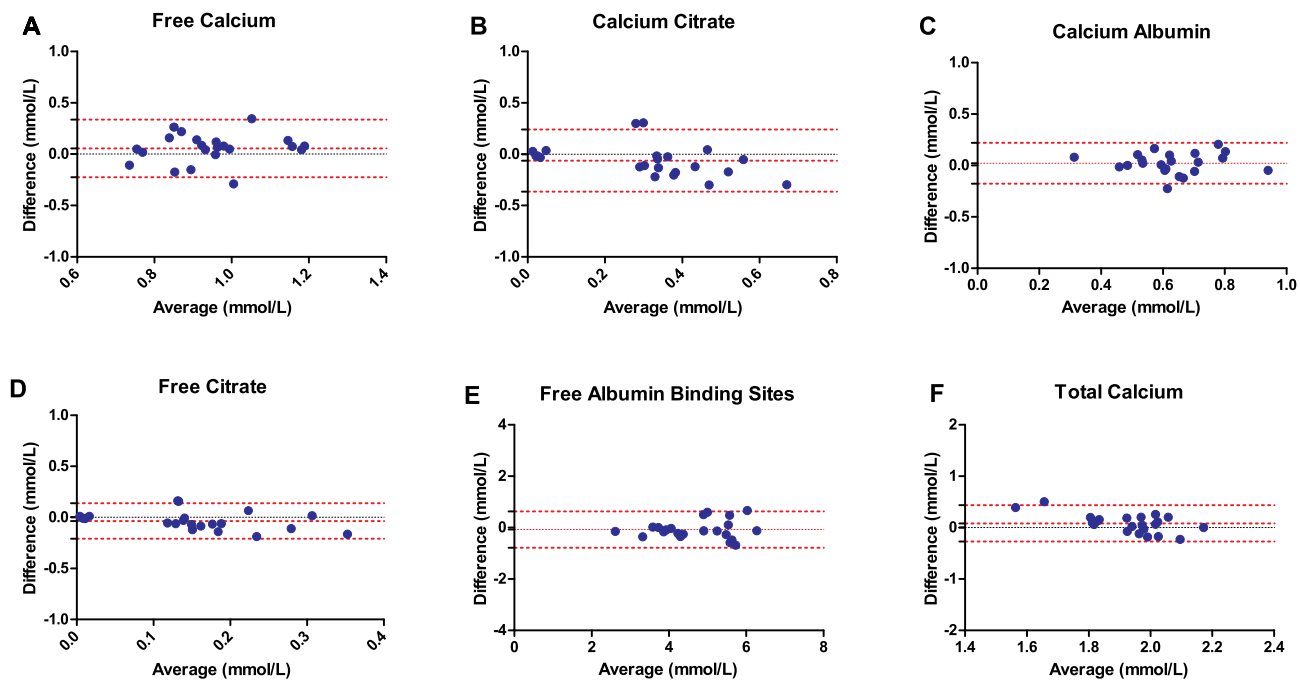

**Fig. 2.** Bland Altman diagram of postfilter values calculated with modeling, and measured values.

	Bias	95% Limits of agreement
Free calcium (mmol/L)	$0.056 \pm 0.143$	$-0.224-0.337$
Calcium-citrate (mmol/L)	$-0.062 \pm 0.154$	$-0.364-0.241$
Citrate (mmol/L)	$-0.035 \pm 0.089$	$-0.210-0.139$
Calcium-albumin binding site (mmol/L)	$0.021 \pm 0.101$	$-0.178-0.220$
Albumin binding site (mmol/L)	$-0.078 \pm 0.362$	$-0.788-0.631$
Total calcium (mmol/L)	$0.082 \pm 0.181$	$-0.273-0.437$


**Table 3.** Bias and limits of agreement.

arterial line after citrate infusion drops below 0.4 mmol/L. Thereafter no significant variation in the patient's free calcium level is observed. In addition, the total calcium balance is close to 0 mmol/min. The risk of hypocalcemia therefore seems to be low, as we showed in a previous study<sup>14</sup>. These results are comparable to those obtained by Evenopel et al.<sup>12</sup> and Fiaccadori et al.<sup>13</sup>. However, they provide no conclusive evidence on the long-term effects on mineral and bone disorders notably parathyroid hormone and bone turnover.

Pre- and post-filter citrate dosages indicated that more than 90% of the citrate is eliminated by diffusion and convection in the dialysate. This is a guarantee of patient safety since less than 10% of the infused citrate solution returns to the general blood circulation and is then metabolized by the liver. In order to obtain effective anticoagulation in the circuit (i.e. a free calcium level lower than 0.4 mmol/L), a pre-filter citrate concentration of at least 3000  $\mu\text{mol/L}$  is necessary, a figure that is consistent with the scarce data from the literature on the subject<sup>18</sup>.

Modeling makes it possible to predict fairly accurately the variations in concentration during the passage of blood through the dialysis filter. It enabled us to precisely study the impact of dialysis parameters (blood, dialysate and citrate infusion flow) on anticoagulant effectiveness and calcium balance. Thus, it appears that only the first half of the dialysis filter is effectively anticoagulated. In the second half and the venous bubble trap, the free calcium level is greater than 0.4 mmol/L. This could explain the occurrence of blood circuit coagulation episodes with this technique, which varies from 0.5 to 12%<sup>12-14</sup>. Calculations by modeling show that it is possible to increase the length of the anticoagulated dialysis filter effectively by increasing the blood flow or decreasing the dialysate flow (Fig. 3A). However, this leads to a decrease in free calcium (Fig. 3C) and an increase in citrate-calcium complexes in the blood at the outlet of the dialysis filter (as evidenced by a decrease in the free calcium/total calcium ratio, Fig. 3B,C). This can lead to a risk of metabolic alkalosis if the increased amount of citrate is normally metabolised in the liver into bicarbonate. On the contrary, in case of liver failure, citrate accumulation can cause hypocalcemia.

An alternative technique has been developed that involves use of a calcium-free dialysate with or without citrate and reinfusion of a calcium-containing solution into the venous line. The amount of calcium ions lost in the dialysate is estimated to be equal to the product of the dialysance and the patient's free calcium. The calcium infusion rate is readjusted regularly during the session according to dialysance value<sup>8-11</sup>. The model shows that: (i)

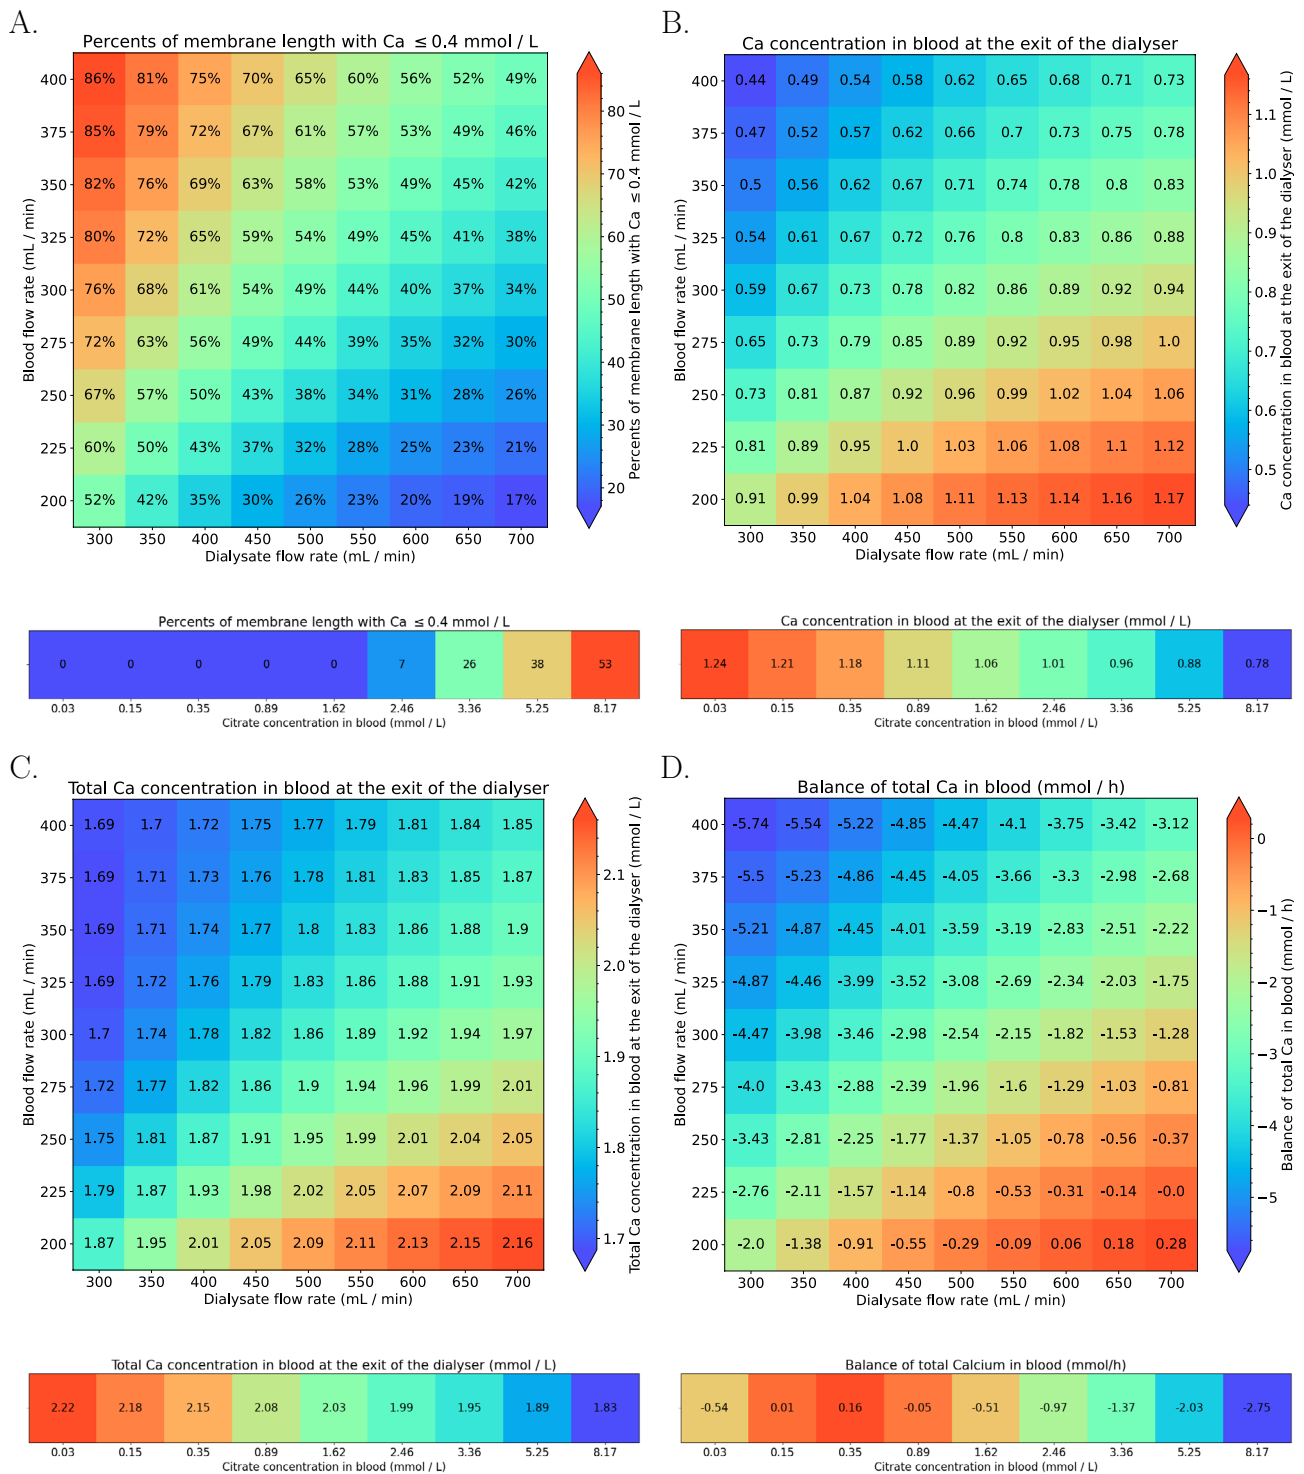

**Fig. 3.** Simulations of hemodialysis with blood citrate infusion and a dialysate containing calcium (1.25 mmol/L). Percentage of membrane length with free calcium concentration <0.4 mmol/L (A). Postfilter free calcium (B) and total calcium concentration (C) values. Calcium balance (D). Values are calculated for different dialysate and blood flows (prefilter citrate concentration 5 mmol/L) or different prefilter citrate concentrations (dialysate and blood flows set at 500 and 300 mL/min, respectively).

these techniques allow effective anticoagulation of the venous trap but do not ensure anticoagulation of the first half of the dialysis filter and as much as the first two thirds with a citrate-free dialysate; (ii) the addition of citrate to the dialysate reduces the calcium balance (it becomes more negative); and (iii) using the product of dialysance by free calcium concentration to estimate the calcium exchanges in the dialysis filter is an oversimplification that



leads to an underestimation of the quantity of calcium to infuse into the venous line (even more with a citrate dialysate). Taking into consideration blood calcium-albumin and albumin in the model increases calcium transfer to the dialysate. Thus, the amount of calcium delivered from albumin during the passage of blood through the dialysis filter should not be overlooked. These findings are in agreement with the results of Kozik-Jaromin et al.<sup>15</sup>, who showed that diffusible calcium accounts for 80% of total calcium and that total calcium is a better predictor of calcium balance than ionized calcium.

Our work has certain limitations. It was a single-center study with a small sample size, and certain patients had to be excluded from the analysis owing to errors or the absence of samples. However, the number of patients analyzed was greater than the minimum sample size calculated and sufficient to draw conclusions regarding the validity of the proposed model. Some patients were not administered citrate but we were able to use their measurements to validate the model in different situations. Finally, our model does not take into account the Gibbs-Donnan effect on calcium exchange through the dialysis membrane. A solution proposed by Muhawari et al.<sup>20</sup> is to use a 1-dimensional model and assume Gibbs-Donnan equilibrium is reached. In this case the concentration ratio of the ions on either side of the membrane can be provided as a function of the protein level according to an empirical relationship provided by Gotch et al.<sup>21</sup>. Unfortunately, this simplification is not applicable to our model. To take into account the Gibbs-Donnan effect while retaining the ability to compute solutes concentration distribution inside the dialysis filter it would be necessary to add other charged solutes, introduce electric migration to the advection–diffusion–reaction system and Poisson equation to calculate the electric field. This adds a level of complexity which does not seem necessary because the predicted results are sufficiently close to those observed in patients.

## Conclusion

Anticoagulation of extracorporeal blood circulation in hemodialysis is a significant concern, particularly in patients at high risk of bleeding. Simplified alternatives to conventional regional citrate anticoagulation have been proposed. In this study we show that it was possible to model the exchange of calcium and citrate in the dialysis filter quite accurately. Whatever the alternative techniques used (infusion of citrate and dialysate containing calcium, citrate dialysate without calcium, or dialysate without calcium) only part of the blood is effectively anticoagulated. Whether this provides clinical benefit compared to complete absence of anticoagulation remains unclear. In addition, the calcium balance is modified compared to standard hemodialysis. It is important to take these findings into account if we wish to use the techniques for patients undergoing chronic hemodialysis.

## Data availability

The datasets generated and/or analyzed during the current study are available from the corresponding author on reasonable request.

Received: 25 April 2024; Accepted: 20 August 2024

Published online: 26 August 2024

## References

1. European Best Practice Guidelines Expert Group on Hemodialysis. E.R.A. Section V. Chronic intermittent haemodialysis and prevention of clotting in the extracorporeal system. *Nephrol. Dial Transpl.* **17**(Suppl7), 63–71 (2002).
2. Palevsky, P. M. et al. KDOQI US commentary on the 2012 KDIGO clinical practice guideline for acute kidney injury. *Am. J. Kidney Dis.* **61**, 649–672 (2013).
3. Islam, M. S. et al. Vitamin E-coated and heparin-coated dialyzer membranes for heparin-free hemodialysis: A multicenter, randomized. *Crossover Trial. Am. J. Kidney Dis.* **68**, 752–762 (2016).
4. Laville, M. et al. Results of the HepZero study comparing heparin-grafted membrane and standard care show that heparin-grafted dialyzer is safe and easy to use for heparin-free dialysis. *Kidney Int.* **86**, 1260–1267 (2014).
5. Meijers, B. et al. A noninferiority trial comparing a heparin-grafted membrane plus citrate-containing dialysate versus regional citrate anticoagulation: Results of the CiTED study. *Nephrol. Dial Transpl.* **32**, 707–714 (2017).
6. Dellepiane, S. et al. Citrate anion improves chronic dialysis efficacy, reduces systemic inflammation and prevents Chemerin-mediated microvascular injury. *Sci. Rep.* **9**, 10622 (2019).
7. Zhang, W. et al. Safety and efficacy of regional citrate anticoagulation for continuous renal replacement therapy in liver failure patients: A systematic review and meta-analysis. *Crit. Care* **23**, 22 (2019).
8. Ridell, C. et al. Regional citrate anticoagulation during hemodialysis: A simplified procedure using Duocart biofiltration. *Blood Purif.* **23**, 473–480 (2005).
9. Scarfogliere, V. et al. Regional anticoagulation with calcium-free dialysate containing citrate in chronic haemodialysis patients. *Nephrol. Dial Transplant* **36**, 745–746 (2021).
10. Vigneron, C. et al. Efficacy and tolerance of sustained low-efficiency dialysis with calcium-free citrate-containing dialysate anticoagulation. *Clin. Kidney J.* **14**, 1025–1026 (2021).
11. Faguer, S. et al. Heparin-free prolonged intermittent hemodialysis using calcium-free citrate dialysate in critically ill patients. *Crit. Care Med.* **45**, 1887–1892 (2017).
12. Evenepoel, P. et al. Regional citrate anticoagulation for hemodialysis using a conventional calcium-containing dialysate. *Am. J. Kidney Dis.* **39**, 315–323 (2002).
13. Fiaccadori, E. et al. Efficacy and safety of a citrate-based protocol for sustained low-efficiency dialysis in AKI using standard dialysis equipment. *Clin. J. Am. Soc. Nephrol.* **8**, 1670–1678 (2013).
14. Leroy, C. et al. Comparison between regional citrate anticoagulation and heparin for intermittent hemodialysis in ICU patients: A propensity score-matched cohort study. *Ann. Intensive Care* **11**, 13 (2021).
15. Kozik-Jaromin, J., Nier, V., Heemann, U., Kreyman, B. & Bohler, J. Citrate pharmacokinetics and calcium levels during high-flux dialysis with regional citrate anticoagulation. *Nephrol. Dial Transpl.* **24**, 2244–2251 (2009).
16. Anfort, J., Chupin, L. & Cindea, N. Mathematical model of calcium exchange during haemodialysis using a citrate containing dialysate. *Math. Med. Biol.* **35**, 87–120 (2018).
17. Hecht, F. New development in freefem++. *J. Numer. Math.* **20**, 251–266 (2012).

18. Falkenhagen, D. T., Brandi, M. Correlation between activated clotting time and ionized calcium in regular dialysis treatment patients. *EDTA 2011 Poster* (2011).
19. Melia Rodrigo, M., Riberio, A. C., Verissimo, L. M., Estes, M. A. & Leait, D. G. Coupled diffusion in aqueous citric acid + calcium citrate solutions. *J. Chem. Thermodynam.* **131**, 314–321 (2019).
20. Maheshwari, V. *et al.* An in silico method to predict net calcium transfer during hemodialysis. *Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.* **2017**, 2740–2743 (2017).
21. Gotch, F. A., Lam, M. A., Prowitt, M. & Keen, M. Preliminary clinical results with sodium-volume modeling of hemodialysis therapy. *Proc. Clin. Dial Transplant Forum.* **10**, 12–17 (1980).

## Acknowledgements

We are indebted to Mr. Jeffrey Watts for assistance in the preparation of the manuscript.

## Author contributions

JA: conceptualization, analysis, interpretation, writing draft FR: data acquisition, writing draft FT: data acquisition, reviewing LL: data acquisition CP: reviewing CG: reviewing AEH: reviewing CD: reviewing MA: data acquisition DJ data acquisition LE: data acquisition LC: reviewing DB: reviewing BS: reviewing NC: computer programming, analysis, writing draft.

## Competing interests

The authors declare no competing interests.

## Additional information

**Supplementary Information** The online version contains supplementary material available at <https://doi.org/10.1038/s41598-024-70708-9>.

**Correspondence** and requests for materials should be addressed to J.A.

**Reprints and permissions information** is available at [www.nature.com/reprints](http://www.nature.com/reprints).

**Publisher's note** Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

**Open Access** This article is licensed under a Creative Commons Attribution-NonCommercial-NoDerivatives 4.0 International License, which permits any non-commercial use, sharing, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if you modified the licensed material. You do not have permission under this licence to share adapted material derived from this article or parts of it. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by-nc-nd/4.0/>.

© The Author(s) 2024