



HAL
open science

Fibronectin Conformations after Electrodeposition onto 316L Stainless-Steel Substrates Enhanced Early-stage Osteoblasts' Adhesion but Affected Their Behavior

Séverine Alfonsi, Pithursan Karunathan, Ayann Mamodaly Samdjee, Keerthana Balathandayutham, Sarah Lefevre, Anamar Miranda, Olivier Gallet, Damien Seyer, Mathilde Hindié

► To cite this version:

Séverine Alfonsi, Pithursan Karunathan, Ayann Mamodaly Samdjee, Keerthana Balathandayutham, Sarah Lefevre, et al.. Fibronectin Conformations after Electrodeposition onto 316L Stainless-Steel Substrates Enhanced Early-stage Osteoblasts' Adhesion but Affected Their Behavior. *Journal of Functional Biomaterials*, 2024. hal-04735743

HAL Id: hal-04735743

<https://hal.science/hal-04735743v1>

Submitted on 14 Oct 2024

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Fibronectin Conformations after Electrodeposition onto 316L Stainless-Steel Substrates Enhanced Early-stage Osteoblasts' Adhesion but Affected Their Behavior

Séverine Alfonsi¹, Pithursan Karunathan¹⁻², Ayann Mamodaly Samdjee¹⁻², Keerthana Balathandayutham¹⁻², Sarah Lefevre¹⁻², Anamar Miranda², Olivier Gallet², Damien Seyer², Mathilde Hindié^{2*}

Affiliations : 1 CY Cergy Paris Université, LPPI, F-95000 Cergy, France

2 CY Cergy Paris Université, ERRMECe, F-95000 Cergy, France

* Corresponding author

The implantation of metallic orthopedic prostheses is increasingly common due to an aging population and accidents. There is a real societal need to implement new metal implants that combine durability, good mechanical properties, excellent biocompatibility as well as affordable costs. Since the functionalization of low-cost 316L stainless-steel substrates through the successive electrodeposition of a polypyrrole film (PPy) and a calcium phosphate deposit doped with silicon was previously carried out by our labs, we have also developed a bio-functional coating by electrodepositing or oxidating of fibronectin (Fn) coating. Fn is an extracellular matrix glycoprotein involved in cell adhesion and differentiation. Impacts of either electrodeposition or oxidation on the structure and functionality of Fn were studied and validated by the resulting pre-osteoblast behavior. Compared to oxidation, electrodeposition seems to largely modify Fn conformation, resulting in changes to the accessibility of the molecular probes tested (antibodies directed against Fn whole molecule and Fn cell-binding domain). Electrodeposition reduced pre-osteoblasts' ability to remodel Fn coating on supports because of a partial modification of Fn conformation, which reduced accessibility to the cell-binding domain. However, the N-terminal extremity of Fn was not modified by electrodeposition as demonstrated by *Staphylococcus aureus* attachment after 3h of culture on a specific domain localized

in this region. Electrodeposited Fn seems more favorable to pre-osteoblast early-stage behavior than during a longer culture of 24h and 48h. The electrodeposition of matrix proteins could be improved to maintain their bio-activity and to develop this promising, fast technique to bio-functionalize metallic implants.

KEYWORDS: 316L stainless steel, polypyrrole, electrodeposition, bio-functionalization, fibronectin coatings, STRO-1⁺ A pre-osteoblasts

Implantable materials, such as metallic orthopedic prostheses, continue to be increasingly used due to both an aging population and traumatology. Orthopedic prostheses, 70% of which are made from metals [1], constitute a flourishing market of \$ 115 billion which is still growing [2]. Metallic materials are first used as bone implants due to their physical and mechanical properties and inert nature [3]. The three most implanted metallic biomaterials are titanium alloys (Ti), cobalt-chromium alloys, and medical-grade stainless steel (316L SS). 316L SS plates, screws, and pins are extensively used as bone fracture fixation devices due their mechanical properties and low cost [4]. However, corrosion is the main reason for 316L SS implants' failure when they come into contact with biological fluid [5]. The release of metal ions induced by corrosion causes aseptic loosening, osteolysis, adverse local tissue reactions, or inflammation of the area around metal implants [6]. Despite its high cost, the biomedical-grade titanium (Ti) is widely used in biomedical implants such as joint replacements, bone plates, and dental implants [7] thanks to its biocompatibility and resistance to corrosion. However, release of Ti oxide from Ti alloys induces allergy and exposure to toxic Ti nanoparticles which have been proven by *in vitro* studies [8].

Nevertheless, bacterial infections constitute another major cause of metallic prosthesis implantation failure. In periprosthetic infections, *Staphylococcus aureus* bacteria are frequently involved because of their high adaptation to the human physiology and their ability to form biofilms that are tolerant to antibiotics [9].

Several physical and chemical techniques have been developed to protect 316L SS against corrosion such as trimethylsilane plasma nanocoatings [10], surface modification with deposition of a polycaprolactone film [11], nanosecond laser treatment of 316L SS surface [12], or sol-gel spin coating [13], but these techniques prevent the deposition of biodegradable coatings [14]. In this study, the approach used to prevent the 316L SS support from corroding is the electrodeposition of a conductive polymer film, which is a well-known approach [15]. Polypyrrole (PPy), polyaniline (PA), and poly (3,4-ethylene-dioxythiophene) (PEDOT) are three of the conductive polymers most used for the protection

of active metals such 316L SS from corrosion [16]. Furthermore, Martins *et al.* demonstrated that electrodeposition maintains the chemical composition and thickness of the coating, so coating depositions are reproducible [17]. Electrodepositions are reproducible even on supports with a complex geometry or on porous surfaces. Besides, only inexpensive equipment is needed to perform these depositions [18].

The conducting polymer chosen for this study was PPy because of its high resistance to corrosion and delamination [19], its easy synthesis, high conductivity, and good biocompatibility [20,21]. PPy-based materials were described with levels of immunogenicity that are comparable to other FDA-approved biomaterials [22]. Still, PPy coating improvements were necessary to increase their biocompatibility and adherent cells' adhesion. Inorganic components were incorporated in PPy coatings, such as hydroxyapatite nanoparticles or zinc oxide particles, to improve biocompatibility with the bone matrix [23,24]. However, the absence of PPy functional groups such as carboxyl groups [25] able to interact with human body biomolecules blocks the further adsorption of exogenous biological molecules such as matrix proteins [26]. Several approaches have recently been developed to improve PPy biocompatibility such as RGD peptide covalent grafting via cysteine residues [27].

Cellular matrix (ECM) proteins, such as fibronectin (Fn) or collagen, are important for early-stage adhesion, migration, and differentiation, and they are used to improve implants' bio-activity [28,29]. Thus, the bio-functionalization of implants with Fn was shown to stimulate adhesion of cells such as osteoblasts [30]. ECM proteins immobilized on supports facilitate the indirect formation of bone tissue. These proteins create ECM adhesion sites, allowing osteoblastic cells to attach and initiate the osseointegration process [31].

Different methods were employed to bio-functionalize implants with Fn such as adsorption[32], grafting [33], or laser-assisted printing [34]. The choice of the most appropriate technique depends on the physico-chemical properties of the implant on which functionalization is performed [35]. Since the biological inertia of the PPy surface reduces cell affinity and bioactivity [36], an alternative method of

protein bio-functionalization was employed to improve the bioactivity of our implants coated with a PPy film: Fn electrodeposition.

The aim of this present work was to optimally functionalize 316L SS supports through successive electrodepositions of a PPy film and of Fn. The coatings' physico-chemical properties were characterized and the effects of electrodeposition on Fn bioactivity were analyzed.

The response of the STRO-1+ A pre-osteoblasts cultured on our supports was also studied on early-stage culture as well as longer ones in order to investigate the effect of electro-coating of Fn on cell bioactivity and morphology.

2.1. Support preparation

2.1.1. Steel plate treatment

Medical-grade 316L SS plates (Arcelor) were cut using blue-laser technologies (CMS, France) with a L3030 laser cutting machine (Trumpf) to obtain supports with a precise size of 30 x 5 x 1 mm.

Before each electrochemical experience, substrates were polished with abrasive paper using grain sizes 800 Si-C and a Struers LaboPol-1 polisher. The supports were then cleaned by immersion for 15 minutes, at room temperature, in an ultrasonic cleaner sequentially containing acetone, ethanol, and ultra-pure water. They were also air-dried.

2.1.2. PPy coating on 316L SS

The electrochemical polymerization of Py on the 316L SS plates was performed using a three-electrode potentiostat/galvanostat (VSP 150, Bio-logic Scientific Instrument). The 316L SS support was used as working electrode, a saturated calomel electrode (SCE) as reference, and a steel grid as counter-

electrode. The electrolytic solution used contained 0.2 M freshly distilled pyrrole (Thermo Scientific) and 0.5 M salicylate sodium (Sigma-Aldrich).

The applied potential was scanned between -0.5 and 1.1V/SCE for 15 cycles at a fixed scan rate of 50 mV/s, and then rinsed with deionized water to remove unused monomer molecules prior to drying in the air. Each PPy layer formed on supports has a surface of 1,3 cm².

2.2. Surface characterization

2.2.1. Profilometric analysis

The roughness and thickness of surface deposits were determined by profilometry (DEKTAK 150). The mean of three measures was calculated for over five different areas onto each support.

2.2.2. Measure of the surface wettability

This measurement was performed using a Theta Flow goniometer (Biolin Scientific). The goniometer helps measure the contact angle formed by a 5µl drop of water deposited on the surface of a support. The surface angle contact was determined by measuring five different areas per support and it was performed on 3 different supports for each type.

2.3. Support bio-functionalization

2.3.1. Fn adsorption

Supports covered with a PPy film were immersed in an Eppendorf tube®, containing Fn diluted at 10 µg/mL in adsorption buffer (HEPES 10 mM, NaCl 150 mM, and CaCl₂ 15 mM, Sigma-Aldrich), for 10 minutes at 37°C. Substrates were then rinsed with adsorption buffer and stored at 4°C.

2.3.2. Fn oxidation

Adsorbed Fn on supports is oxidized by applying an electric current through chronoamperometry. The electrochemical assembly is the same as the one used previously for PPy electrodeposition. Oxidation consists of applying a potential of +0.25 V/EOC for 10 minutes with adsorption buffer used as electrolyte. The substrate is then rinsed twice with adsorption buffer and stored at 4°C.

2.3.3. Fn electrodeposition on support

Fn was directly electrodeposited onto the supports through chronoamperometry using the same 3-electrode assembly. Electrodes were immersed in 20 mL of adsorption buffer containing Fn at a concentration of 10 µg/mL. The same parameters used for oxidation were applied, at a potential of +0.25 V/EOC for 10 minutes. The support is then rinsed and stored at 4°C as described previously.

2.4. Study of Fn behavior on each type of support

2.4.1. Immunostaining of Fn-deposited coatings on supports

The three types of samples were treated with a blocking buffer prepared with Phosphate Buffered Saline (PBS) containing 5% of bovine serum albumin (BSA) (Sigma-Aldrich), for 30 min at room temperature, to block non-specific binding sites. The supports were then incubated for 1 hour at room temperature with a 1/1000 dilution of anti-Fn rabbit polyclonal antibody (F3648, Sigma) in saturation buffer. After being rinsed with 0.1% (w/v) PBS-BSA buffer (three times for 5 minutes), supports were incubated for 1 hour with an Alexa Fluor 488 coupled anti-rabbit antibody at 1/200 in saturation buffer. After rinsing, observations and image capture were conducted using a Confocal Laser Scanning Microscope (CSLM) LSM 900 (Zeiss). Image post-processing was done using the Fiji® software.

2.4.2. Quantification of Fn present on supports

A desorption of Fn present on support was first performed to enable protein assays. Fn-coated supports were desorbed with 500 μL of adsorption buffer containing 1% SDS (v/v), three times for 5 minutes, in an ultrasonic bath. 150 μL of the desorbed Fn solution from each sample were transferred into a 96-well plate with 150 μL of working solution from a QuantiPro[®] BCA Assay kit (Sigma-Aldrich). The plate is then incubated for 1 hour at 60°C. After allowing the samples to cool down, the absorbance of each well was read at 562 nm using a Xenius spectrophotometer (SAFAS).

With the help of a calibration curve obtained by measuring the absorbance for a known protein concentration range for Fn (linear curve in concentration range studied), it was possible to determine the amount of protein in solution after desorption.

2.4.3. Enzyme-linked immunosorbent assay (ELISA)

The accessibility of the Fn cell-binding domain was tested using ELISA with specific antibodies. Samples with either adsorbed, oxidized, or electrodeposited Fn were blocked for 1 h at room temperature with Tris buffer saline (TBS) containing 1% BSA (w/v) and 0.1% Tween20 (v/v) (blocking buffer). Incubation with a monoclonal antibody against the Fn cell-binding domain (sc18825 mouse IgG Santa Cruz) 1/1000 diluted in blocking buffer was then performed. After 60 min of incubation at room temperature samples were washed three times with Tween[®] 0.1%-TBS (T-TBS). Then secondary antibody anti mouse IgG-peroxidase (A4416 Sigma-Aldrich) 1/5000 diluted in blocking buffer was incubated for 1 h at room temperature. Three washes with T-TBS were done and remaining antibodies were revealed with a tetramethylbenzidine substrate for 5 min. The reaction was stopped by sulfuric acid 0.5 M and measurements were done at 405 nm using a Xenius micro-plate reader (SAFAS).

2.5. Cellular influence of supports

The samples were first sterilized for 1 h at room temperature in sterile PBS with 100 units/mL of penicillin (Gibco) and 0.1 mg/mL of streptomycin (Gibco). The supports were rinsed twice with sterile PBS and then dried for 30 minutes at 37°C before cell culture.

2.5.1. Human cell adhesion on supports

F/STRO-1+A (STRO) osteoblast progenitor cells were kindly provided by Dr. P. Marie (Inserm U1132, Paris Diderot University, France). They were cultured at 37°C in Iscove's modified Dulbecco's medium (IMDM) (Gibco) containing 10% (v/v) fetal bovine serum (FBS), 2 mM Glutamax® (Invitrogen), 100 units/mL of penicillin (Gibco), and 0.1 mg/mL of streptomycin (Gibco). Cells were incubated at 37°C in a humidified atmosphere (95% relative humidity) with 5% CO₂ until pre-confluence.

2.5.2. Bacteria adhesion on supports

The reference *Staphylococcus aureus* CIP4.83 strains were purchased from the "Collection de l'Institut Pasteur Paris". Bacteria were grown in Tryptic Soy broth (TSB, BD™ Biosciences, San Jose, CA, USA) for 24h at 37°C.

The bacterial suspension was quantified with a spectrophotometer (ThermoSpectronic® Genesys 20) at a wavelength of 600 nm. The bacterial suspension was diluted in PBS to obtain 10⁵ CFU/mL. Supports were put in a tube containing 500 µL of bacterial suspension, and incubated at 37°C in constant agitation during 3h. The supports were then rinsed twice with 0.9% (w/v) NaCl solution (SW) and placed in an Eppendorf® tube with 500 µL of SW to be treated by sonication for 10 min. The Mix of

bacteria and SW was preserved. This sonication treatment was renewed twice. The total supernatant obtained was diluted (serially diluted 1:10) and 100 μL of each suspension were deposited on a TS agar plate and incubated at 37°C for 24h. A count of the colonies obtained was performed to determine the quantity of adherent bacteria on each type of supports.

2.5.3.Mitochondrial activity

Pre-confluent STRO cells were treated with trypsin/EDTA, harvested through centrifugation, and the cell pellet was re-suspended in IMDM containing 10% FCS and 1% Glutamax[®]. 50 μL of cell suspension was seeding on each substrate (corresponding to 20,000 cells/cm²). Culture was performed for 24 or 48 hours in a humidified atmosphere of 5% CO₂, at 37°C. After incubation time, each support was transferred in an Eppendorf tube with 500 μL of culture medium and 50 μL of AlamarBlue[™] reactive. Tubes were incubated for 3 hours at 37°C, and 100 μL of media from each tube were transferred to a 96-well black plate in order to read fluorescence with a Xenius spectrofluorometer (SAFAS) using a fluorescence excitation wavelength of 560 nm and an emission of 590 nm. The measurements of mitochondrial activity were renewed in three independent experiments in duplicate.

2.5.4.Cell proliferation

To determine cell proliferation, previous samples were fixed for 15 min with 4% paraformaldehyde (Sigma-Aldrich) solution in PBS. Cells were then labeled for 30 min with a solution containing 10 $\mu\text{g}/\text{mL}$ of 4',6-diamidino-2-phenylindole dihydrochloride (DAPI, Sigma-Aldrich). Cellularized supports were examined using a Leica fluorescence microscope (10X objective). For each sample, 3 independent fields were analyzed. Data are representative of three different experiments performed in duplicate. Image post-processing was performed using the Fiji[®] software.

2.5.5. Cell morphology

Pre-osteoblasts were seeding on sterile supports as describe previously, and they were grown for 3h, 24h, or 48h. Cells were first fixed with a 4% paraformaldehyde solution for 10 minutes, and rinsed with PBS. Cells were then permeabilized with a 0.2% (v/v) PBS-Triton solution for 5 minutes and the supports were rinsed with PBS. Each support was placed for 30 minutes in blocking buffer, PBS-BSA 5% (v/m). Supports were incubated during 1 hour at room temperature with either a primary antibody anti-Fn rabbit (F3648, Sigma) diluted at 1/200th in blocking buffer, or a primary antibody anti- α 5 integrin (MAB 33231 Invitrogen) diluted at 1/100th, or a primary antibody anti-Fn extra domain A (EDA) (BML-FG6010, Enzo) 1/100th diluted in blocking buffer. They were then rinsed with PBS-BSA 0.1% (v/m) buffer and incubated for 1 hour with a secondary antibody (anti-IgG rabbit AlexaFluor 488 diluted at 1/400th, or anti-IgG mouse AlexaFluor 488 diluted at 1/400th) with DAPI (10 μ g/mL) and AlexaFluor 568 coupled phalloidin (1/400th diluted). After rinsing, a lamella was fixed on each sample with Prolong Gold[®]. Observations and image capture were conducted using a CLSM, LSM 900 (Zeiss) with objectives (x20, or x63). For each sample, 3 independent fields were analyzed. Post-treatment images were taken using the Fiji[®] software.

2.6. Statistical analysis

Data were analyzed using the InStat3[®] statistical software (GraphPad Software). The statistical significance between groups was assessed, after the normality test was passed, using one-way analysis of variance (ANOVA), followed by Student–Newman–Keuls multiple comparison tests for protein assays, mitochondrial activity tests, and cell proliferation or Dunn test for ELISA. Experimental results are expressed as means \pm standard deviation at a significance level of $P < 0.001$, $P < 0.05$, or $P < 0.01$.

3. Results and discussion

3.1. Bio-functionalization and characterization of supports

3.1.1. Electrodeposition of PPy coatings

After applying the potential between -0.5 and + 1.1V/ECS with a scanning speed of 50mV/s for 15 cycles, a black smooth and adherent film of PPy was obtained on 316L SS supports. Uniformity of PPy film was controlled by optical microscopy observations (Appendix A).

In order to analyze the PPy films formed on the supports, a profilometry study was performed to determine their thickness and roughness. PPy films had a thickness of $4.98 \mu\text{m} \pm 0.15$ and a low roughness of $0.27 \mu\text{m} \pm 0.05$. In this study, films obtained were thicker ($4.9\mu\text{m}$ versus $2.2 \mu\text{m}$) than those obtained by Hamdaoui S *et al.* [37]. Those results are consistent because the Py solution used was twice more concentrated than the one previously used in the lab.

3.1.2. Surface wettability of supports

Support water contact angle was measured before and after PPy film deposition. 316L SS substrates presented a wettability of $100 \pm 3^\circ$ so they were considered as hydrophobic, whereas the substrates covered by PPy had more hydrophilic wettability of $79 \pm 4^\circ$. Hydrophobic surfaces induce a conformational change in Fn by reducing accessibility to the cell-binding domain (CBD) [29,38] and preventing cell adhesion [39]. Hence wettability values measured for PPy supports were more favorable to the adsorption of matrix proteins such as Fn or vitronectin and improve the subsequent adhesion of cells cultivated on their surface.

3.1.3.Support functionalization with Fn

Three different methods were employed to deposit Fn on supports covered by a PPy film:

- AD: Simple adsorption of Fn
- OX: Oxidation of precoated Fn
- ED: Electrodeposition of Fn

A potential of +0.25 V/EOC for 10 minutes was applied on supports coated by Fn to prepare Ox supports. Chronoamperometry with the same potential used for oxidation was employed to induce the electrodeposition of Fn on PPy films. These functionalization of Fn through electro-oxidation or electro-deposition was compared to a simple adsorption of Fn. The presence and morphology of Fn on supports were determined by Confocal laser scanning microscopy (CSLM).

3.2. Study of the bioactivity of Fn deposited on each type of supports

3.2.1.Quantity of Fn on substrates

The quantity of Fn present on the three types of supports was determined by BCA assay after protein desorption with 1%SDS solution. Controls were performed to confirm the total desorption of proteins by this treatment (Appendix B). In Figure 1, results of protein quantification show a mean amount of $2.9 \pm 1.7 \mu\text{g}$ proteins adsorbed on AD supports, $3.3 \mu\text{g} \pm 2.1\mu\text{g}$ proteins on OX supports, and $5.2 \pm 2.1 \mu\text{g}$ proteins on ED supports. Compared to AD supports, a significant increase of 78% was measured on ED supports after protein assays. No significant differences were detected between AD and OX supports. The quantity of deposited Fn by electrodeposition seems to be strongly higher than the one after simple adsorption and it is confirmed by statistical analysis. Different results were observed with

pronectin, a synthetic protein, electrodeposited on titanium supports [40], but the electrodeposition of macromolecules depends on their isoelectric points [41]. The Fn (with a pHi = 5.5) is negatively charged in adsorption buffer at pH 7.5 so it may interact more easily with PPy films that are positively charged [42]. Our hypothesis is that the deposition of Fn was enhanced on ED supports by their surface charge and the potential applied for electrochemical deposition.

The Fn was stained with an anti-Fn polyclonal antibody and an Alexa Fluor® 488 coupled secondary antibody (green). CSLM images of Fn are shown in Figure 2: on AD substrates a homogenous coating of Fn is observed, whereas on OX supports Fn microspheres are observed. A totally different organization is visualized on ED supports, which present long Fn fibers organized along fractal structures (Figure 2). The morphology of Fn observed on AD supports is similar to the ones described after Fn coating on supports such as glass coverslips [43] or titanium substrate [34]. Fn aggregates observed on OX substrates are comparable to the ones described by Bascetin R *et al.* [44] after high-temperature treatment of Fn; this indicates denaturation of Fn and aggregation patterns during the oxidation step on OX supports.

3.2.2. Biological conformation of Fn

The bioactivity of Fn on the supports is indirectly determined by Fn adhesion capacity due to the preservation or not of the cell-binding domain in the structural conformation of Fn. Fn is a ≈ 450 -kDa dimeric glycoprotein with a modular structure [45]. In Figure 3, a schematic representation of a Fn monomer shows the organization of its specific domain such as CBD. Thank to ELISA tests, targeting Fn CBD, only non denaturated Fn could be detected. Antibodies used are directed against the conformational cell-binding domain of Fn. Absorbance measured is proportional to the quantity of cell-binding domain available. The strongest signal was detected on AD supports (Figure 4), meaning that CBD of Fn (domains III9 and III10) is more accessible when Fn is absorbed. Compared to AD supports, accessibility to CBD of Fn is lower on OX and ED supports. If data measured are normalized with the quantity of Fn measured on supports and compared to AD supports, it appears that Fn-CBD is respectively 19% and 42% less accessible on OX supports and ED supports. These decreases can be explained by a conformational change in Fn resulting from oxidation or EPD. Similar results were

described with formation of Fn aggregates after thermal and mechanical denaturation. This treatment induced a modification of conformational organization that decreased Fn CBD accessibility [44].

3.3. Effects of supports on pre-osteoblast early-stage behavior

3.3.1. Cell morphology

The morphology of pre-osteoblasts was observed via Confocal Laser Scanning Microscopy (CLSM). Cells were cultured for 3h on the three types of supports, before being fixed. Fn filaments were stained with a polyclonal antibody directed against Fn (green), nuclei by DAPI (blue) as DNA probe, and actin cytoskeleton by Alexa Fluor® 568 phalloidin (red). Pre-osteoblast CSLM images are shown in Figure 5: on AD supports, cells were evenly spread out and had a clearly distinguishable actin cytoskeleton (Figure 5a). Cells were attached onto all types of supports but the typical aspect of the osteoblasts' morphology was observed mostly on AD supports. A comparable number of cells was observed, for all the supports. Pre-osteoblasts present a more elongated morphology on OX supports (Figure 5b) and are less spread out, while they are more rounded on ED supports (Figure 5c). A previous study showed similar results, where cells cultured on Fn aggregates were less spread out than the ones cultured on native Fn [46]. Pre-osteoblasts cultured on ED didn't follow the Fn fiber and were the least spread out, which could be due to the reduced accessibility of Fn CBD. This phenomenon was also described with HUVEC cells cultured on self-assembled monolayers which decreased Fn CBD access [29].

3.3.2. $\alpha 5$ integrins and cellular Fn organization

The expression and organization of $\alpha 5$ integrins in pre-osteoblasts cultured for 3h on supports was analyzed after immunostaining and observations by CSLM. Fn was stained with a polyclonal antibody against Fn (green), and $\alpha 5$ integrins monoclonal antibody targeting $\alpha 5$ integrins (magenta). Nuclei

were labelled with DAPI (blue) and actin cytoskeleton with Alexa Fluor® 568 phalloidin (cyan). Pre-osteoblasts were cultured on the three types of supports, $\alpha 5$ integrins were observed in pre-osteoblasts each time but their organization was not the same for all supports. On AD supports, $\alpha 5$ integrins were around the nucleus and along the cell membrane (Figure 6g). Focal adhesion began to be organized on AD supports as we observed in previous work [32]. On OX supports, $\alpha 5$ integrins remained in the cytoplasm along the nucleus. Since $\alpha 5$ integrins specifically bind to Fn [47] at the CBD site (Figure 3), they probably are not able to bind to oxidized Fn with a CBD site that is less accessible. On ED supports, $\alpha 5$ integrins showed round the nucleus and a little in the cytoplasm (Figures 6c – 6i). A long Fn fiber was also observed on ED supports (Figure 6c), but no $\alpha 5$ integrin staining was detected along this structure. These results are consistent with ELISA tests results, demonstrating that Fn CBD is less accessible on Fn fiber produced by electrodeposition treatment which induces less cell attachment.

The expression of Fn extra domain A (EDA) which is specific to cellular Fn was followed by immunological staining in pre-osteoblasts cultured on supports for 3h. After culture and fixation cells were stained, Fibronectin, EDA Fn, nuclei, and actin cytoskeleton were stained with a polyclonal antibody against Fn (green), a monoclonal antibody targeting EDA fragment of Fn (red), DAPI (blue), and Alexa Fluor® 568 phalloidin (cyan) respectively. EDA Fn was observed in pre-osteoblasts cultured on the three types of supports. However, EDA Fn was secreted only by cell cultures on AD supports (Figure 7a). EDA Fn was detected only in the cytoplasm for cells cultivated on OX and ED supports. We previously described a synthesis of EDA Fn by STRO-1+ A cultured on plasmatic Fn coating and a cell remodeling of this coating [32]. EDA Fn is an insoluble Fn, known to participate in cell matrix remodeling [48]. Only pre-osteoblasts cultured on AD supports have the ability to reorganize the Fn coating using Fn coating and EDA Fn jointly. So, oxidation and electrodeposition modified the resulting Fn coating but also reduced EDA Fn secretion. We hypothesize that the important diminution of Fn CBD, and the reduction of EDA Fn secretion, consequently inhibited Fn coating remodeling by pre-osteoblasts.

3.4. Early-stage bacterial behavior on supports

All types of supports were deep in a *Staphylococcus aureus* bacteria suspension and incubated for 3h at 37°C. Adherent bacteria were detached by sonication, bacteria obtained were diluted, seeded on agar plate, and grown for 24h at 37°C to count the number of colonies formed on each support. No significant differences between each support were observed as shown in Figure 8. Comparable quantities of UFC were counted on AD, OX, and ED supports; however, more *S. aureus* seems to have adhered on supports coated only with a PPy film. Hence, Fn deposition methods didn't appear to affect *S. aureus* adhesion on supports. These results seem to demonstrate that the *S. aureus* binding domain of Fn was not modified by either oxidation or electrodeposition.

Furthermore, at physiological pH, Fn is negatively charged [28]. PBS buffer used for bacteria culture has a physiological pH, which maintains Fn negative charge. On the other site, *S. aureus* presents a global negative surface charge [49]. So, negatively charged *S. aureus* bacteria could interact more with the positive charge in the PPy structure than with the negative surface charge of Fn [50].

3.5. Pre-osteoblast behavior after culture for 48h on supports

For longer pre-osteoblast cultures we focused on AD and ED supports which induced more specific cell responses as compared to OX supports which induce a lack of cell attachment.

3.5.1. Cell morphology

The morphology of pre-osteoblasts cultured for 24h and 48h on both types of supports was studied after cell fixation and immunological staining as previously described. Fibronectin was labelled in green; nuclei and actin filaments were stained in blue and red respectively. Pre-osteoblast CSLM images acquired are shown in Figure 9: on AD supports, cells had a clearly distinguishable actin

cytoskeleton but they were less spread out than after 3h culture and they had an elongated morphology (Figure 9a-b). On AD supports, pre-osteoblasts remodeled the Fn coating to produce fibril (arrow on Figure 9b). Cell cultivated on ED supports were also elongated but with a smaller area than on AD supports (Figure 9c-d). Pre-osteoblasts were grouped as clusters on ED (Figure 9c) or appeared entrapped in large Fn electrodeposited fibers (Figure 9d). On both ED supports, cells were less numerous than on AD supports. An elongated morphology and aligned actin fibers of pre-osteoblasts cultured on AD supports for 24h are typical of those observed for osteoblasts cultured on a Fn coating [51]. The lower quantity of cells observed on ED supports may be due to their inability to remodel the Fn matrix.

3.5.2. Mitochondrial activity

Cells were cultured for 24h and 48h on both support types and an Alamarblue™ assay was performed to determine their mitochondrial activity; results obtained are presented in Figure 10. After 24h of culture mean mitochondrial activity was higher on ED supports, but a significant augmentation of mitochondrial activity was observed on AD supports at t=48h. On the other hand, mitochondrial activity seemed to decrease on ED supports after 48h of culture. These results may be due to a lower quantity of cells remaining on ED supports as observed on Figure 9d. Muhonen V *et al.* observed similar results with Fn coating on Nitinol supports [52]. The martensite Nitinol structure reduced the remodeling of Fn and induced a lower mitochondrial activity of murine pre-osteoblasts MC3T3-E1 after 48h culture compared to control.

3.5.3. Proliferation of pre-osteoblasts

Cells seeded on AD and ED substrates up to 48h were fixed and their nuclei were stained by DAPI. Photos of three independent fields were taken and the number of nuclei was counted. Results obtained are presented in Figure 11. A significant augmentation of the nuclei number was observed between 24h and 48h on AD supports, whereas this number remained stable for ED supports. So, pre-osteoblasts proliferated on AD substrates, whereas they did not on ED supports. These results are consistent with osteoblast morphology observations. Fibers formed by electrodeposition are not natural fibers and present less CBD accessibility as previously presented. It is why, as denatured fibers, they appear unable to stimulate cell attachment and further proliferation [53]. Furthermore, Fn remodeling is important for matrix organization and cell proliferation [54], which is not possible when Fn is electrodeposited. These difficulties for cells to adhere could induce a specific type of apoptosis in pre-osteoblasts named anoikis. This phenomenon could explain the reduction of mitochondrial activity on ED supports after 48h of culture [55].

4. Conclusion

A new approach to bio-functionalizing 316L SS coated with a film of PPy was developed in our lab by electrodepositing Fn. In parallel, Fn adsorption and oxidation of Fn adsorbed were also performed for comparison purposes.

Fn was successfully electrodeposited on supports, and presented typical reproducible fractal fibrillar structures, whereas oxidized Fn formed aggregates. The amount of Fn electrodeposited on 316L SS supports was higher than the deposit performed by adsorption with or without electro-oxidation. Effects of these different modes of deposition on the structure and functionality of Fn were studied using antibody conformational ELISA, which demonstrated a strong diminution of CBD accessibility on ED supports.

The early-stage culture of STRO-1⁺A human pre-osteoblasts on supports revealed adhesion and spreading on all types of support, suggesting the absence of toxicity. However, Fn coating remodeling was inhibited on ED and OX supports, mainly due to the inhibition of $\alpha 5$ integrin binding to electrodeposited or oxidized Fn.

The culture of STRO-1⁺A human pre-osteoblasts for 24h and 48h demonstrated a good proliferation and mitochondrial activity on AD supports, whereas they were strongly inhibited on ED supports, probably due to the difficulty to remodel Fn matrix as observed previously [52].

In this study, an easy, fast, and reproducible way to bio-functionalize 316L SS supports was developed using electrodeposition. It appeared that the Fn structure was structurally modified around its cell binding site, whereas the N-ter remained functional. This approach seemed more efficient in improving early-stage pre-osteoblast culture. However, even if the quantity of Fn present on ED supports was higher, it did not have any significant effect on *S. aureus* adhesion, so it would not increase the risk of contamination by *S. aureus* bacteria. Complementary experiments with another matrix protein such

as type I collagen could be performed to develop the long-term efficiency of this technique for bio-functionalizing metallic implants. This promising technique could also enable the simultaneous deposition of several biomolecules, such as an ECM protein and an anti-bacterial peptide, to improve implants' properties.

Figure captions

Figure 1: Surface protein quantities after 1% SDS rinses for the Fn initially adsorbed (AD), oxidized (OX), or electrodeposited (ED) on PPy-coated 316L SS supports. Values are means \pm standard deviations. (Data are representative of three independent experiments performed in triplicate; significant differences were determined using a one-way ANOVA analysis, $**P < 0.01$, $***P < 0.001$.)

Figure 2: Images of Fn adsorbed (AD), oxidized (OX), or electrodeposited (ED) on PPy-coated 316L SS supports. Fn was immunostained to be observed by CSLM. Scale bar: 50 μm . (Data are representative of two different experiments.)

Figure 3: Schematic representation of fibronectin monomer. Binding sites for *Staphylococcus aureus* bacteria and the integrin $\alpha 5\beta 1$ /cell-binding domain are reported. The extra domain A (EDA), which is involved in matrix remodeling, and the extra domain B (EDB), which has an important role during embryogenesis, are also indicated.

Figure 4: ELISA test of Fn adsorbed (AD), oxidized (OX), or electrodeposited (ED) on PPy-coated 316L SS substrates using monoclonal antibodies specific to the assessment of cell-binding domain accessibility. Values are means \pm standard deviations ($n = 3$, $* P < 0.05$).

Figure 5: Images of STRO-1+ A cells cultured on Fn adsorbed (AD), oxidized (OX), or electrodeposited (ED) on supports for 3h. Fn, nucleus, and actin cytoskeleton are stained in green, blue, and red respectively. Scale bar: 50 μm .

Figure 6: Cytoskeletal structure and cellular $\alpha 5$ integrin expression of STRO1+A pre-osteoblasts cultured for 3h on supports functionalized by Fn adsorbed (AD), oxidized (OX), or electrodeposited (ED). Fn, actin cytoskeleton, $\alpha 5$ integrin, and nuclei are stained in green, cyan, magenta, and blue respectively. Scale bar: 20 μm .

Figure 7: Cytoskeletal structure and Fn extra domain A (EDA) synthesis of STRO1+A pre-osteoblasts cultured for 3h on supports functionalized by Fn adsorbed (AD), oxidized (OX), or electrodeposited (ED). Fn, actin cytoskeleton, EDA Fn, and nuclei are stained in green, cyan, red, and blue respectively. Scale bar: 20 μm .

Figure 8: Bacterial attachment on bio-functionalized supports. Number of *Staphylococcus aureus* CIP4.83 bacteria adhering on Fn adsorbed (AD), oxidized (OX), or electrodeposited (ED), on a polypyrrole (PPy) coating, or on a stainless-steel (SS) substrate. The incubation time was 3h.

Figure 9: Images of STRO-1+ A cells cultured on Fn adsorbed (AD), oxidized (OX), or electrodeposited (ED) on supports for 24h and 48h. Fn, nucleus, and actin cytoskeleton are stained in green, blue, and red respectively. Scale bar: 50 μm .

Figure 10: Mitochondrial activity of STRO-1+A pre-osteoblasts cultured on Fn adsorbed (AD), oxidized (OX), or electrodeposited (ED) on supports for 24h and 48h. The box represents the data, with the horizontal line indicating the median value. (ANOVA test was performed, $n=3$, $***P < 0.001$.)

Figure 11: Proliferation of STRO-1+A pre-osteoblasts cultured on Fn, adsorbed (AD), oxidized (OX), or electrodeposited (ED) on supports for 24h and 48h. For each plot, the line within the box represents the median. (ANOVA test was done, $n=3$, $*P < 0.05$, $**P < 0.01$.)

Figure 1:

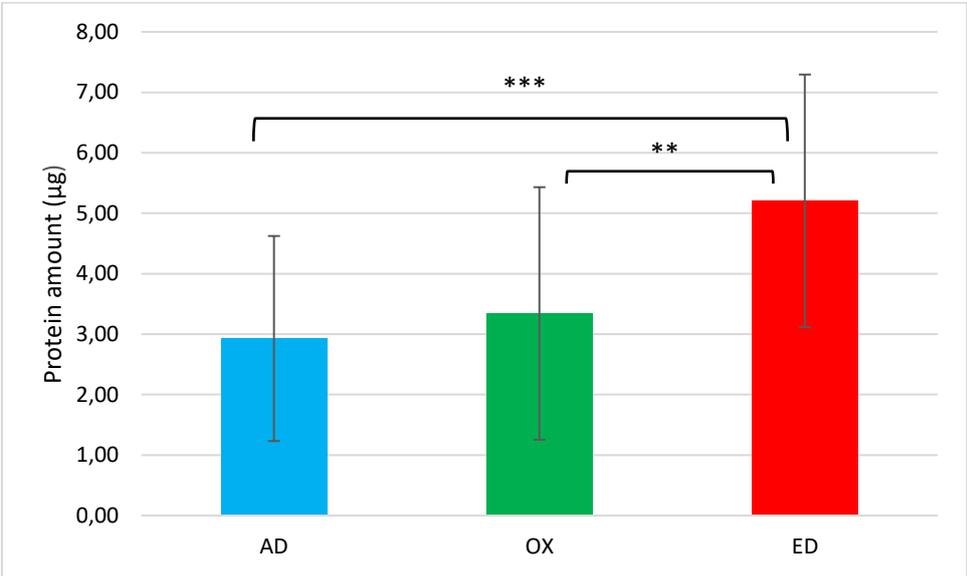


Figure 2:

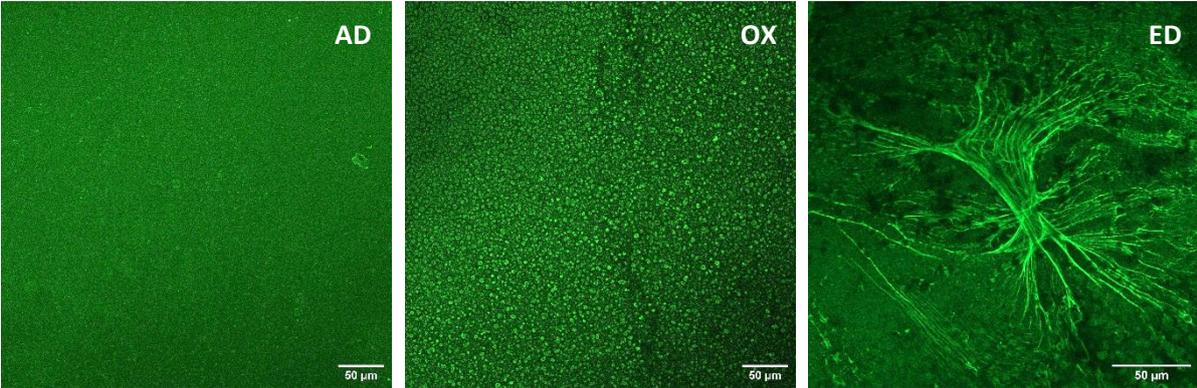


Figure 3:

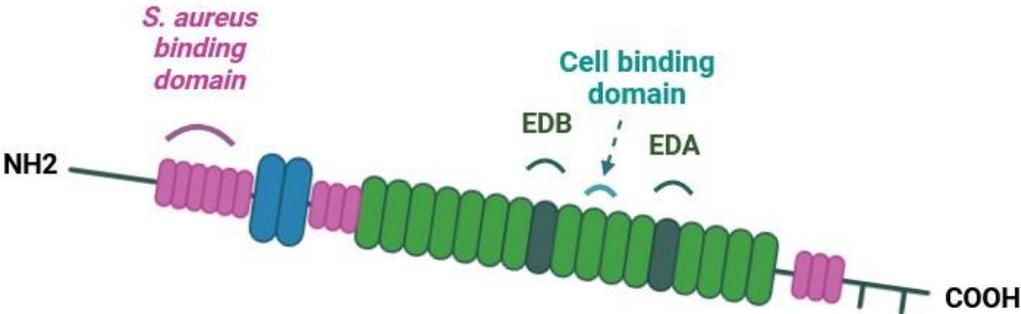


Figure 4:

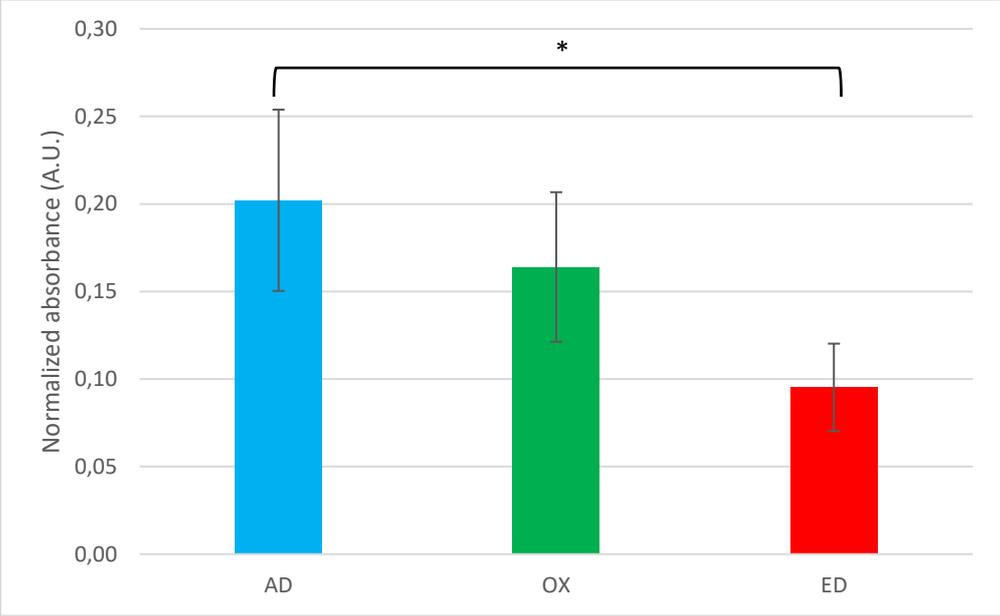


Figure 5 :

Fibronectin / actin / nuclei

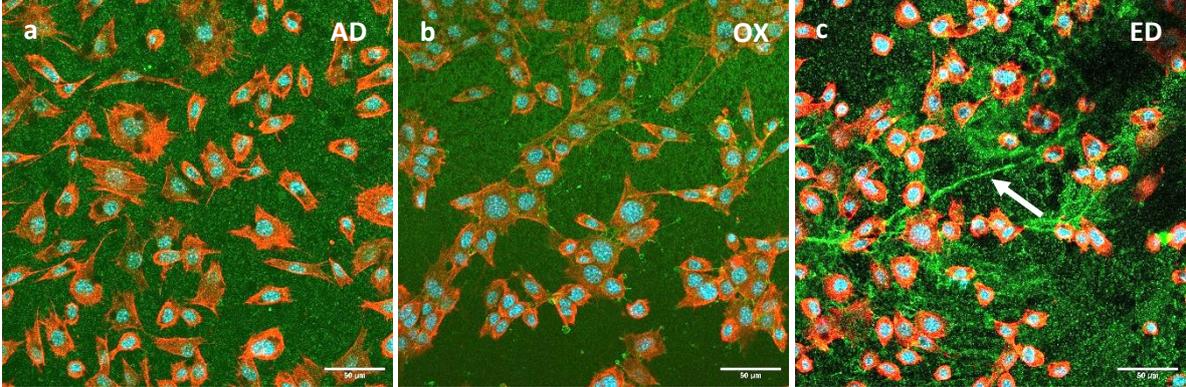


Figure 6:

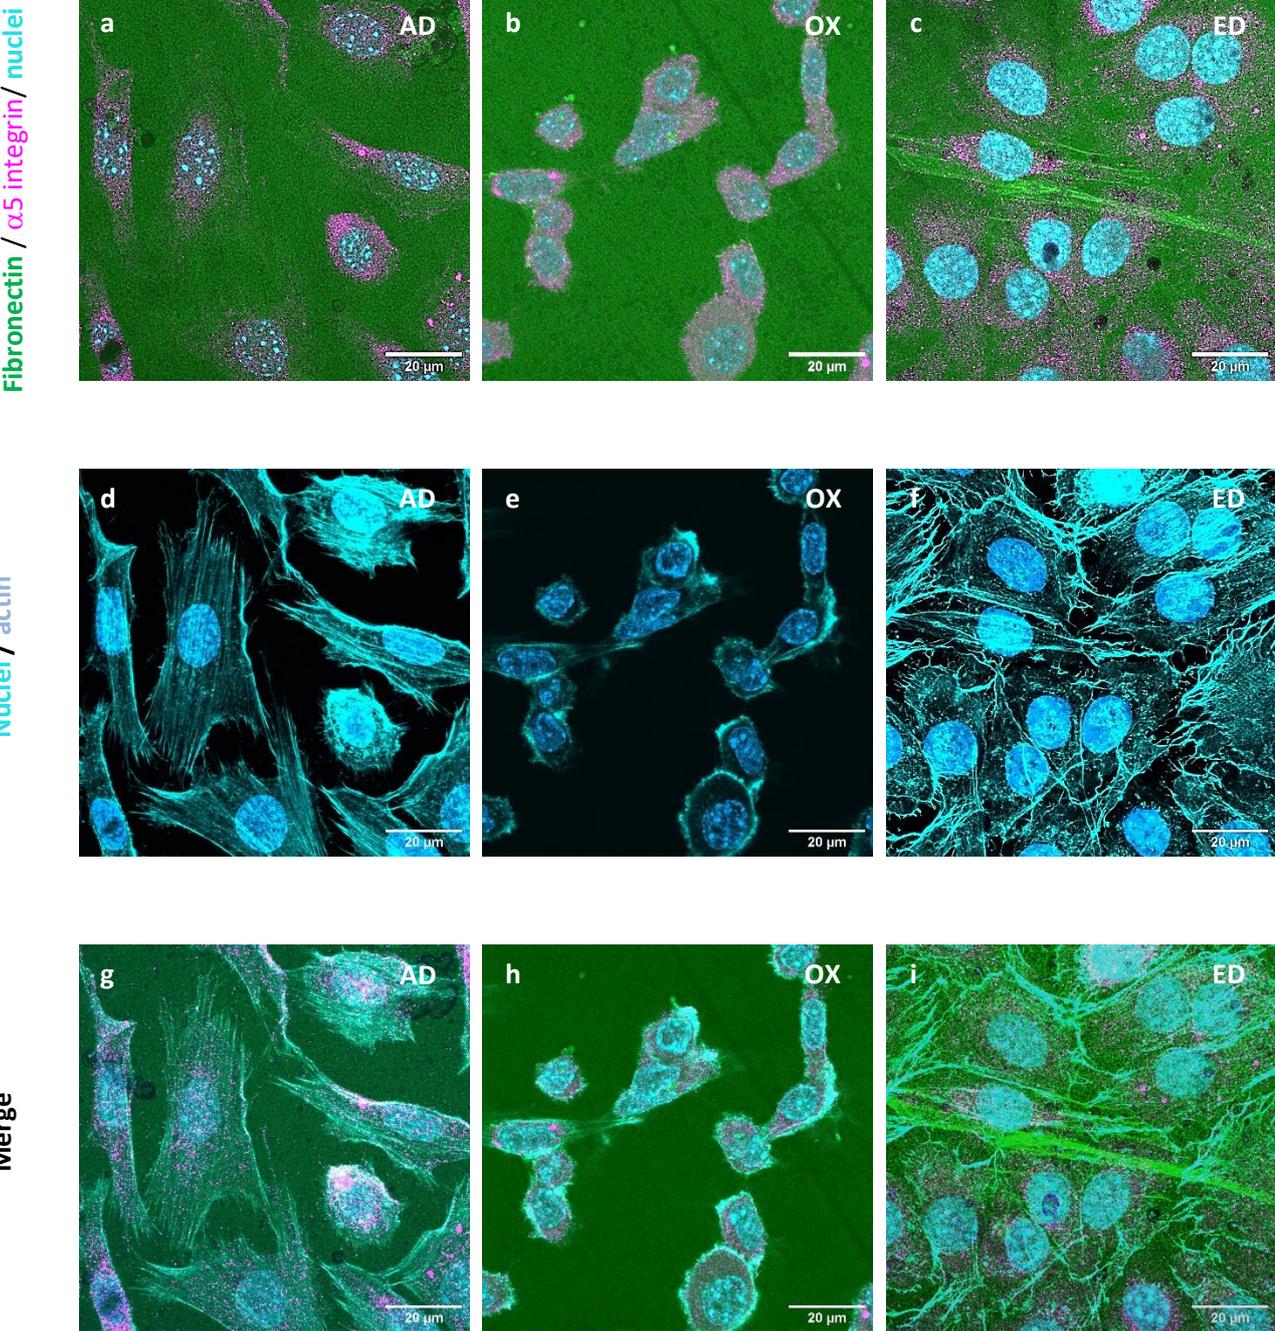


Figure 7 :

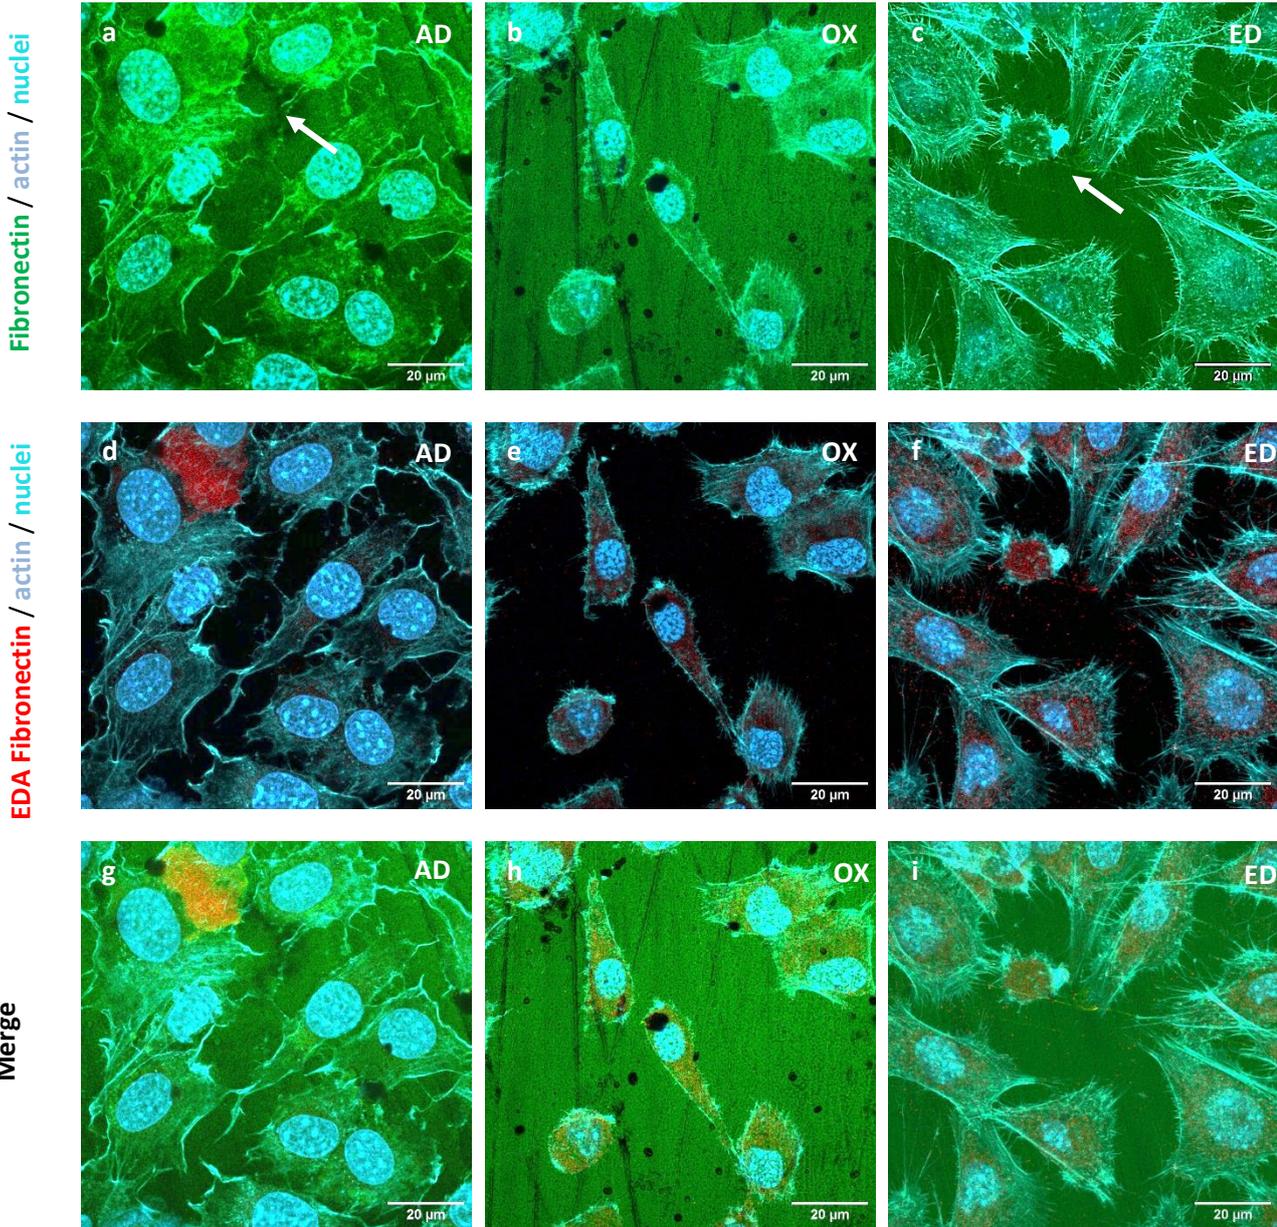


Figure 8:

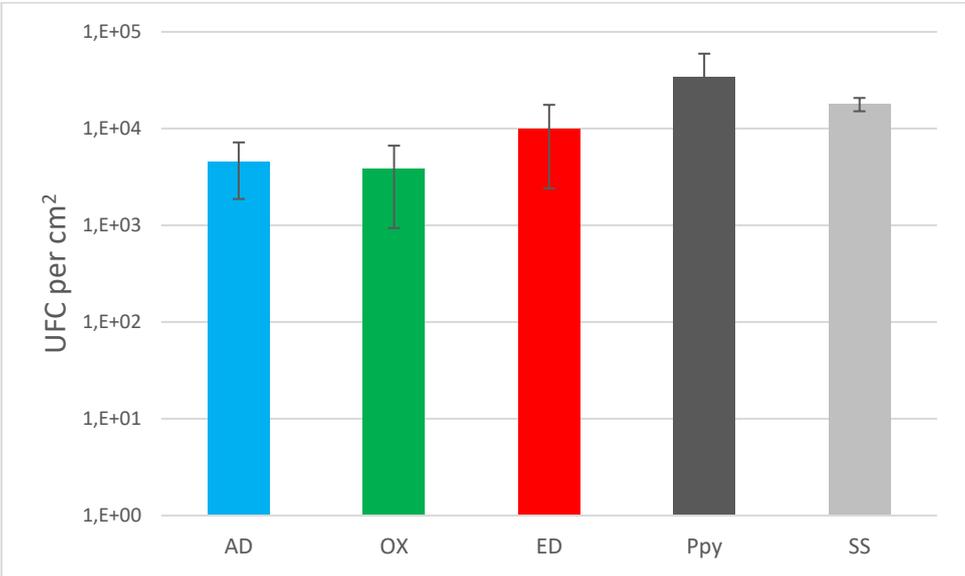


Figure 9:

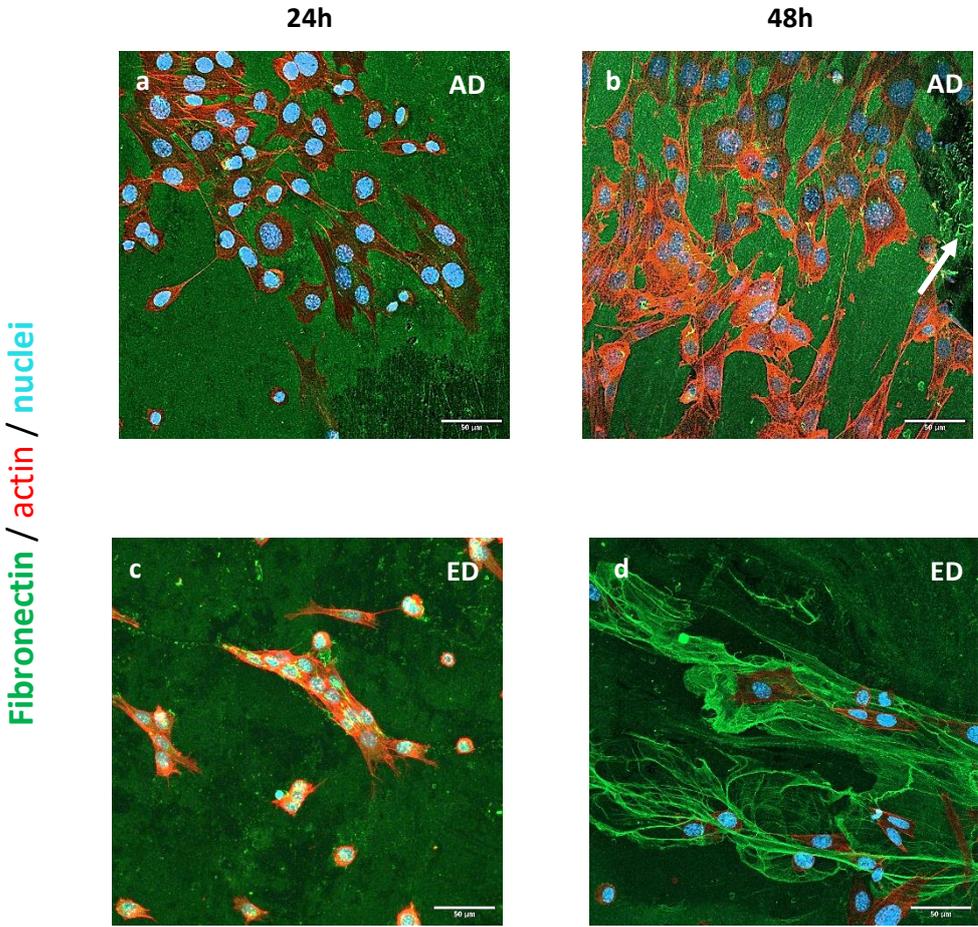


Figure 10:


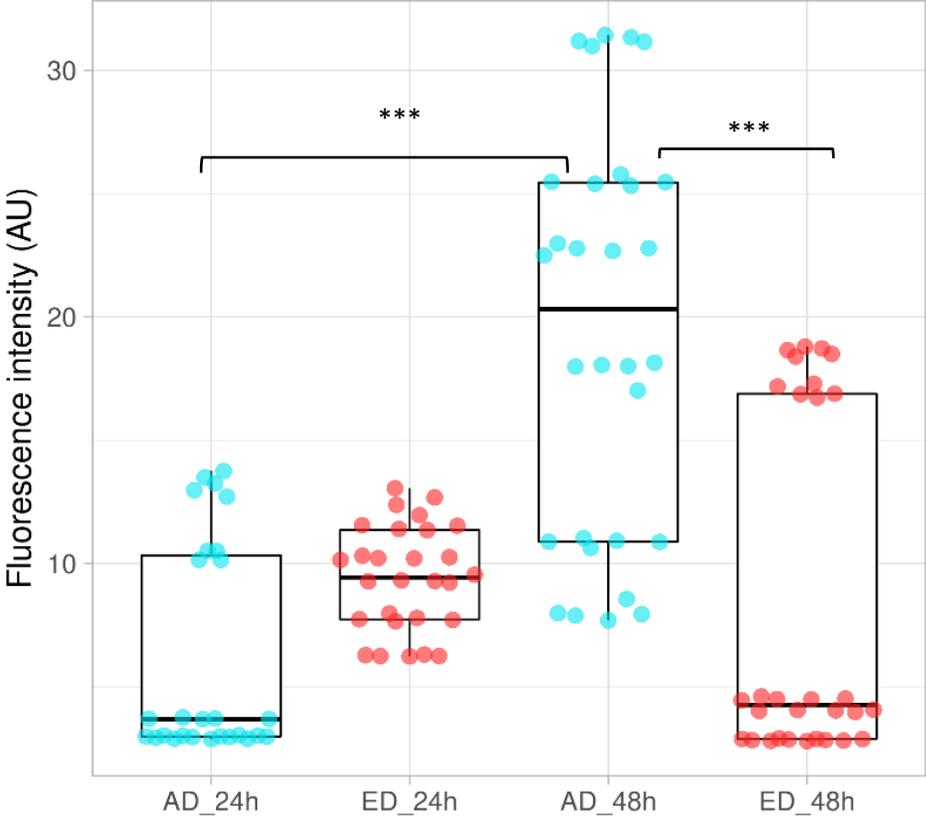


Figure 11:

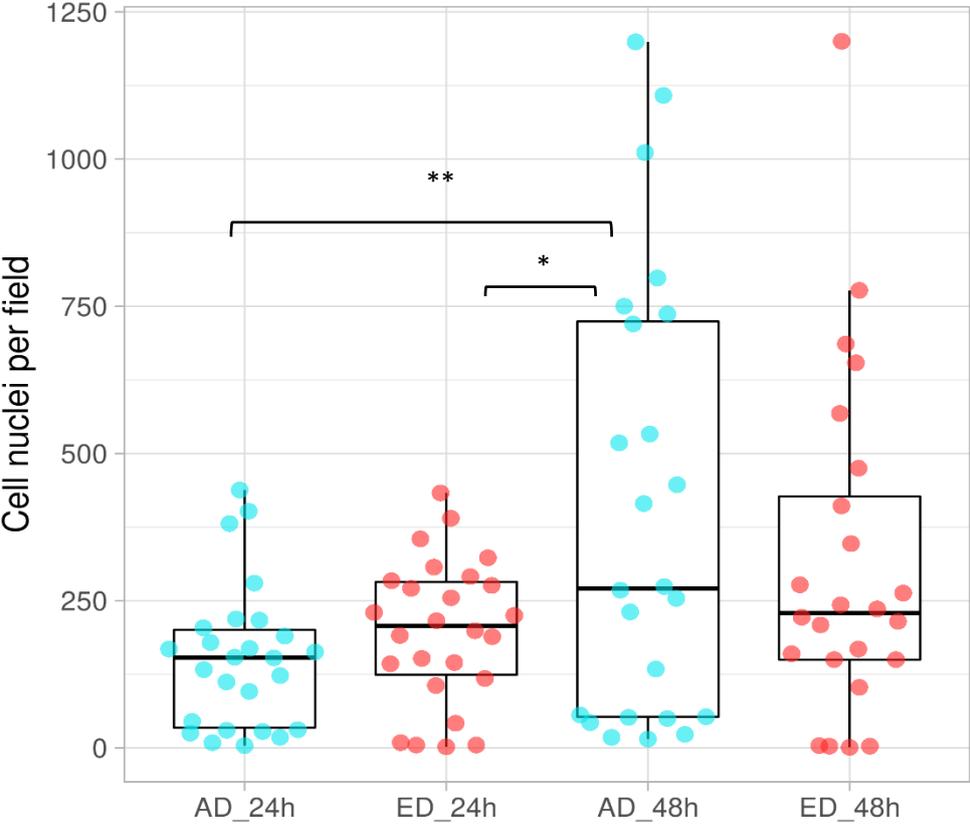

References :

1. Niinomi, M.; Nakai, M.; Hieda, J. Development of new metallic alloys for biomedical applications. *Acta Biomater* **2012**, *8*, 3888-3903, doi:10.1016/j.actbio.2012.06.037.
2. G, C. *Bio-implants Market- Global Opportunity Analysis and Industry Forecast, 2013-2020*; 2014.
3. Nikolova, M.P.; Apostolova, M.D. Advances in Multifunctional Bioactive Coatings for Metallic Bone Implants. *Materials* **2022**, *16*, 183, doi:10.3390/ma16010183.
4. Agarwal, R.; García, A.J. Biomaterial strategies for engineering implants for enhanced osseointegration and bone repair. *Adv Drug Deliv Rev* **2015**, *94*, 53-62, doi:10.1016/j.addr.2015.03.013.
5. Herting, G.; Wallinder, I.O.; Leygraf, C. Metal release rate from AISI 316L stainless steel and pure Fe, Cr and Ni into a synthetic biological medium--a comparison. *J Environ Monit* **2008**, *10*, 1092-1098, doi:10.1039/b805075a.
6. Eslami, M.; Speranza, G.; Fedel, M.; Andersson, N.E.; Deflorian, F.; Omanovic, S.; Zanella, C. Electropolymerization and Possible Corrosion Protection Effect of Polypyrrole Coatings on AA1050 (UNS A91050) in NaCl Solutions. *Corrosion* **2019**, *75*, 745-755, doi:10.5006/3124.
7. Davis, R.; Singh, A.; Jackson, M.J.; Coelho, R.T.; Prakash, D.; Charalambous, C.P.; Ahmed, W.; da Silva, L.R.R.; Lawrence, A.A. A comprehensive review on metallic implant biomaterials and their subtractive manufacturing. *International Journal of Advanced Manufacturing Technology* **2022**, *120*, 1473-1530, doi:10.1007/s00170-022-08770-8.
8. Fage, S.W.; Muris, J.; Jakobsen, S.S.; Thyssen, J.P. Titanium: a review on exposure, release, penetration, allergy, epidemiology, and clinical reactivity. *Contact Dermatitis* **2016**, *74*, 323-345, doi:10.1111/cod.12565.
9. Lamret, F.; Colin, M.; Mongaret, C.; Gangloff, S.C.; Reffuveille, F. Antibiotic Tolerance of. *Antibiotics (Basel)* **2020**, *9*, doi:10.3390/antibiotics9090547.
10. Eric Jones, J.; Chen, M.; Yu, Q. Corrosion resistance improvement for 316L stainless steel coronary artery stents by trimethylsilane plasma nanocoatings. *J Biomed Mater Res B Appl Biomater* **2014**, *102*, 1363-1374, doi:10.1002/jbm.b.33115.
11. Chang, S.-H.; Hsiao, Y.-C. Surface and Protein Adsorption Properties of 316L Stainless Steel Modified with Polycaprolactone Film. *Polymers* **2017**, *9*, 545, doi:10.3390/polym9100545.
12. Lu, Y.; Guan, Y.C.; Li, Y.; Yang, L.J.; Wang, M.L.; Wang, Y. Nanosecond laser fabrication of superhydrophobic surface on 316L stainless steel and corrosion protection application. *Colloids and Surfaces a-Physicochemical and Engineering Aspects* **2020**, *604*, doi:10.1016/j.colsurfa.2020.125259.
13. Salahinejad, E.; Hadianfard, M.J.; Macdonald, D.D.; Mozafari, M.; Vashaei, D.; Tayebi, L. A new double-layer sol-gel coating to improve the corrosion resistance of a medical-grade stainless steel in a simulated body fluid. *Materials Letters* **2013**, *97*, 162-165, doi:10.1016/j.matlet.2013.01.111.

14. Goldmann, W.H. Biosensitive and antibacterial coatings on metallic material for medical applications. *Cell Biol Int* **2021**, *45*, 1624-1632, doi:10.1002/cbin.11604.
15. Zhang, L.L.; Liu, S.J.; Han, H.C.; Zhou, Y.; Hu, S.C.; He, C.; Yan, Q.X. Studies on the formation process and anti-corrosion performance of polypyrrole film deposited on the surface of Q235 steel by an electrochemical method. *Surface & Coatings Technology* **2018**, *341*, 95-102, doi:10.1016/j.surfcoat.2017.12.034.
16. Garcia-Cabezón, C.; Salvo-Comino, C.; Garcia-Hernandez, C.; Rodríguez-Mendez, M.L.; Martín-Pedrosa, F. Nanocomposites of conductive polymers and nanoparticles deposited on porous material as a strategy to improve its corrosion resistance. *Surface and Coatings Technology* **2020**, *403*, 126395, doi:10.1016/j.surfcoat.2020.126395.
17. Martins, N.C.T.; Silva, T.M.E.; Montemor, M.F.; Fernandes, J.C.S.; Ferreira, M.G.S. Electrodeposition and characterization of polypyrrole films on aluminium alloy 6061-T6. *Electrochimica Acta* **2008**, *53*, 4754-4763, doi:10.1016/j.electacta.2008.01.059.
18. Gopi, D.; Ramya, S.; Rajeswari, D.; Kavitha, L. Corrosion protection performance of porous strontium hydroxyapatite coating on polypyrrole coated 316L stainless steel. *Colloids Surf B Biointerfaces* **2013**, *107*, 130-136, doi:10.1016/j.colsurfb.2013.01.065.
19. Gonzalez, M.B.; Saidman, S.B. Electrodeposition of polypyrrole on 316L stainless steel for corrosion prevention. *Corrosion Science* **2011**, *53*, 276-282, doi:10.1016/j.corsci.2010.09.021.
20. Vaitkuvienė, A.; Ratautaite, V.; Mikoliūnaite, L.; Kaseta, V.; Ramanauskaite, G.; Biziuleviciene, G.; Ramanaviciene, A.; Ramanavicius, A. Some biocompatibility aspects of conducting polymer polypyrrole evaluated with bone marrow-derived stem cells. *Colloids and Surfaces a-Physicochemical and Engineering Aspects* **2014**, *442*, 152-156, doi:10.1016/j.colsurfa.2013.06.030.
21. Balint, R.; Cassidy, N.J.; Cartmell, S.H. Conductive polymers: Towards a smart biomaterial for tissue engineering. *Acta Biomaterialia* **2014**, *10*, 2341-2353, doi:10.1016/j.actbio.2014.02.015.
22. Liang, Y.; Goh, J.C.H. Polypyrrole-Incorporated Conducting Constructs for Tissue Engineering Applications: A Review. *Bioelectricity* **2020**, *2*, 101-119, doi:10.1089/bioe.2020.0010.
23. Chakraborty, R.; Manna, J.S.; Saha, P. Development and relative comparison of polypyrrole-calcium phosphate composite coatings with differential concentration of chlorophyll functionalized polymer particle achieved through pulsed electro deposition. *Surface & Coatings Technology* **2019**, *363*, 221-235, doi:10.1016/j.surfcoat.2019.02.025.
24. Maimaiti, B.; Zhang, N.; Yan, L.; Luo, J.; Xie, C.; Wang, Y.; Ma, C.; Ye, T. Stable ZnO-doped hydroxyapatite nanocoating for anti-infection and osteogenic on titanium. *Colloids and surfaces. B, Biointerfaces* **2019**, *186*, 110731, doi:10.1016/j.colsurfb.2019.110731.
25. Landim, V.P.A.; Foguel, M.V.; Prado, C.M.; Sotomayor, M.P.T.; Vieira, I.C.; Silva, B.V.M.; Dutra, R.F. A Polypyrrole/Nanoclay Hybrid Film for Ultra-Sensitive Cardiac Troponin T Electrochemical Immunosensor. *Biosensors (Basel)* **2022**, *12*, doi:10.3390/bios12070545.
26. Molino, P.J.; Wallace, G.G.; Hanks, T.W. Hydrophobic conducting polymer films from post deposition thiol exposure. *Synthetic Metals* **2012**, *162*, 1464-1470, doi:10.1016/j.synthmet.2012.06.013.

27. De Giglio, E.; Sabbatini, L.; Colucci, S.; Zambonin, G. Synthesis, analytical characterization, and osteoblast adhesion properties on RGD-grafted polypyrrole coatings on titanium substrates. *Journal of Biomaterials Science-Polymer Edition* **2000**, *11*, 1073-1083, doi:10.1163/156856200743580.
28. Gossart, A.; Battiston, K.G.; Gand, A.; Pauthe, E.; Santerre, J.P. Mono vs multilayer fibronectin coatings on polar/hydrophobic/ionic polyurethanes: Altering surface interactions with human monocytes. *Acta Biomaterialia* **2018**, *66*, 129-140, doi:10.1016/j.actbio.2017.11.013.
29. Tzoneva, R.; Faucheux, N.; Groth, T. Wettability of substrata controls cell-substrate and cell-cell adhesions. *Biochimica Et Biophysica Acta-General Subjects* **2007**, *1770*, 1538-1547, doi:10.1016/j.bbagen.2007.07.008.
30. Hindié, M.; Degat, M.C.; Gaudière, F.; Gallet, O.; Van Tassel, P.R.; Pauthe, E. Pre-osteoblasts on poly(L-lactic acid) and silicon oxide: Influence of fibronectin and albumin adsorption. *Acta Biomater* **2011**, *7*, 387-394, doi:10.1016/j.actbio.2010.08.001.
31. Lu, H.H.; Subramony, S.D.; Boushell, M.K.; Zhang, X. Tissue engineering strategies for the regeneration of orthopedic interfaces. *Ann Biomed Eng* **2010**, *38*, 2142-2154, doi:10.1007/s10439-010-0046-y.
32. Hindié, M.; Camand, E.; Agniel, R.; Carreiras, F.; Pauthe, E.; Van Tassel, P. Effects of human fibronectin and human serum albumin sequential adsorption on preosteoblastic cell adhesion. *Biointerphases* **2014**, *9*, doi:10.1116/1.4867598.
33. Ba, O.M.; Hindie, M.; Marmey, P.; Gallet, O.; Anselme, K.; Ponche, A.; Duncan, A.C. Protein covalent immobilization via its scarce thiol versus abundant amine groups: Effect on orientation, cell binding domain exposure and conformational lability. *Colloids Surf B Biointerphases* **2015**, *134*, 73-80, doi:10.1016/j.colsurfb.2015.06.009.
34. Grigorescu, S.; Hindie, M.; Axente, E.; Carreiras, F.; Anselme, K.; Werckmann, J.; Mihailescu, I.N.; Gallet, O. Fabrication of functional fibronectin patterns by nanosecond excimer laser direct write for tissue engineering applications. *Journal of Materials Science-Materials in Medicine* **2013**, *24*, 1809-1821, doi:10.1007/s10856-013-4927-0.
35. Wang, R.; Neoh, K.G.; Shi, Z.; Kang, E.T.; Tambyah, P.A.; Chiong, E. Inhibition of Escherichia coli and Proteus mirabilis adhesion and biofilm formation on medical grade silicone surface. *Biotechnol Bioeng* **2012**, *109*, 336-345, doi:10.1002/bit.23342.
36. He, Y.; Dai, L.F.; Zhang, X.M.; Sun, Y.N.; Shi, W.; Ge, D.T. The Bioactive Polypyrrole/Polydopamine Nanowire Coating with Enhanced Osteogenic Differentiation Ability with Electrical Stimulation. *Coatings* **2020**, *10*, doi:10.3390/coatings10121189.
37. Hamdaoui, S.; Lambert, A.; Khireddine, H.; Agniel, R.; Cousture, A.; Coulon, R.; Gallet, O.; Alfonsi, S.; Hindie, M. An efficient and inexpensive method for functionalizing metallic biomaterials used in orthopedic applications. *Colloid and Interface Science Communications* **2020**, *37*, doi:10.1016/j.colcom.2020.100282.
38. Stephansson, S.N.; Byers, B.A.; García, A.J. Enhanced expression of the osteoblastic phenotype on substrates that modulate fibronectin conformation and integrin receptor binding. *Biomaterials* **2002**, *23*, 2527-2534, doi:10.1016/s0142-9612(01)00387-8.

39. Bacakova, L.; Filova, E.; Parizek, M.; Ruml, T.; Svorcik, V. Modulation of cell adhesion, proliferation and differentiation on materials designed for body implants. *Biotechnol Adv* **2011**, *29*, 739-767, doi:10.1016/j.biotechadv.2011.06.004.
40. Kawabata, S.; Asano, K.; Miyazawa, A.; Satoh, T.; Tabata, Y. Electrodeposition of pronectin for titanium to augment gingival epithelium adhesion. *J Tissue Eng Regen Med* **2013**, *7*, 348-352, doi:10.1002/term.527.
41. Sikkema, R.; Baker, K.; Zhitomirsky, I. Electrophoretic deposition of polymers and proteins for biomedical applications. *Advances in Colloid and Interface Science* **2020**, *284*, doi:10.1016/j.cis.2020.102272.
42. Wong, J.Y.; Langer, R.; Ingber, D.E. CELL-INTERACTIONS WITH FIBRONECTIN-COATED ELECTRICALLY CONDUCTING POLYPYRROLE THIN-FILMS. In Proceedings of the Symposium on Biomaterials for Drug and Cell Delivery, Boston, Ma, Nov 29-Dec 01, 1993; pp. 141-145.
43. Hindie, M.; Wu, D.N.; Anselme, K.; Gallet, O.; Di Martino, P. Effects of Fibronectin Coating on Bacterial and Osteoblast Progenitor Cells Adherence in a Co-culture Assay. In *Advances in Microbiology, Infectious Diseases and Public Health, Vol 7*, Donelli, G., Ed.; Advances in Experimental Medicine and Biology; 2017; Volume 973, pp. 17-30.
44. Bascetin, R.; Admane, K.; Agniel, R.; Boudou, T.; Doussineau, T.; Antoine, R.; Gallet, O.; Leroy-Dudal, J.; Vendrely, C. Amyloid-like aggregates formation by blood plasma fibronectin. *Int J Biol Macromol* **2017**, *97*, 733-743, doi:10.1016/j.ijbiomac.2017.01.061.
45. Agniel, R.; Vendrely, C.; Poulouin, L.; Bascetin, R.; Benachour, H.; Gallet, O.; Leroy-Dudal, J. Lectins as probes for assessing the accessibility of N-linked glycans in relation to the conformational changes of fibronectin. *J Mol Recognit* **2015**, *28*, 731-741, doi:10.1002/jmr.2487.
46. Bascetin, R.; Blay, L.; Kellouche, S.; Carreiras, F.; Picot, C.R.; Briand, M.; Agniel, R.; Gallet, O.; Vendrely, C.; Leroy-Dudal, J. Fibronectin amyloid-like aggregation alters its extracellular matrix incorporation and promotes a single and sparsed cell migration. *Experimental Cell Research* **2018**, *371*, 104-121, doi:10.1016/j.yexcr.2018.07.047.
47. Hynes, R.O. Integrins: Bidirectional, allosteric signaling machines. *Cell* **2002**, *110*, 673-687, doi:10.1016/s0092-8674(02)00971-6.
48. Lemanska-Perek, A.; Adamik, B. Fibronectin and its soluble EDA-FN isoform as biomarkers for inflammation and sepsis. *Advances in Clinical and Experimental Medicine* **2019**, *28*, 1561-1567, doi:10.17219/acem/104531.
49. Borges, M.H.R.; Nagay, B.E.; Costa, R.C.; Mathew, M.T.; Bara, V.A.R.; Souza, J.G.S. Recent advances of polypyrrole conducting polymer film for biomedical application: Toward a viable platform for cell-microbial interactions. *Advances in Colloid and Interface Science* **2023**, *314*, doi:10.1016/j.cis.2023.102860.
50. Zhang, X.; Bai, R.B. Surface electric properties of polypyrrole in aqueous solutions. *Langmuir* **2003**, *19*, 10703-10709, doi:10.1021/la034893v.
51. Demais, V.; Audrain, C.; Mabilieu, G.; Chappard, D.; Baslé, M.F. Diversity of bone matrix adhesion proteins modulates osteoblast attachment and organization of actin cytoskeleton. *Morphologie* **2014**, *98*, 53-64, doi:10.1016/j.morpho.2014.02.003.

52. Muhonen, V.; Fauveaux, C.; Olivera, G.; Vigneron, P.; Danilov, A.; Nagel, M.D.; Tuukkanen, J. Fibronectin modulates osteoblast behavior on Nitinol. *Journal of Biomedical Materials Research Part A* **2009**, *88A*, 787-796, doi:10.1002/jbm.a.31953.
53. Dalton, C.J.; Lemmon, C.A. Fibronectin: Molecular Structure, Fibrillar Structure and Mechanochemical Signaling. *Cells* **2021**, *10*, doi:10.3390/cells10092443.
54. Sevilla, C.A.; Dalecki, D.; Hocking, D.C. Regional fibronectin and collagen fibril co-assembly directs cell proliferation and microtissue morphology. *PLoS One* **2013**, *8*, e77316, doi:10.1371/journal.pone.0077316.
55. Kamarajan, P.; Kapila, Y.L. An altered fibronectin matrix induces anoikis of human squamous cell carcinoma cells by suppressing integrin alpha v levels and phosphorylation of FAK and ERK. *Apoptosis* **2007**, *12*, 2221-2231, doi:10.1007/s10495-007-0138-9.


Author Contributions:

Conceptualization S.A., P.S., A.M.S., D.S., and M.H.; methodology, S.A., P.S., A.M.S., K.S., S.L., and A.M.; writing—original draft preparation, M.H.; writing—review and editing, M.H., S.A, D.S. and O.G.; supervision, M.H., S.A and D.S.; funding acquisition, M.H.

Acknowledgments


Ms Balathandayutham and Mr Karunathan acknowledge CY I-Mat for their grant.

Appendix A

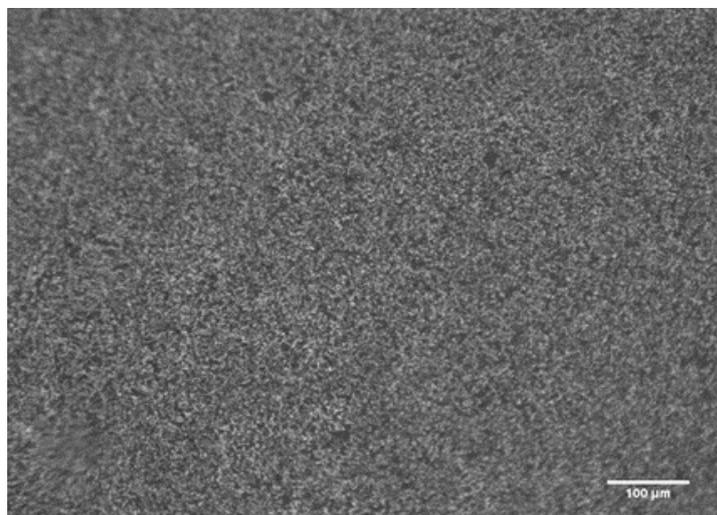

Observation of PPy coating on support with an optical microscope

Appendix B

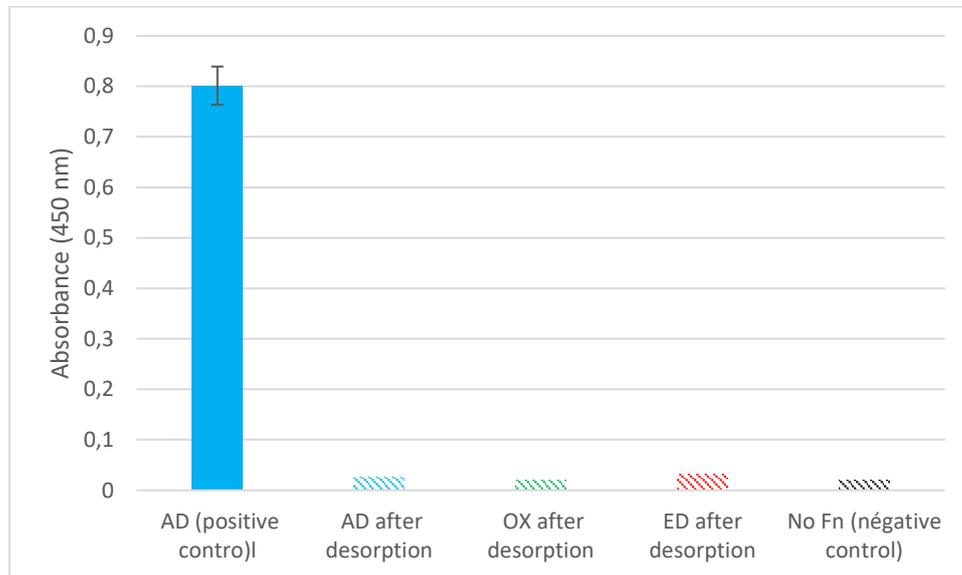

ELISA test of Fn adsorbed (AD), oxidized (OX), or electrodeposited (ED) on PPy-coated 316L SS substrates after desorption using a polyclonal antibody targeting Fn. Positive control was done with Fn adsorbed (AD) without desorption, and negative control was done with substrate without Fn coating.